

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
 Data File : BF128265.D
 Acq On : 16 May 2022 13:40
 Operator : CG\JU
 Sample : N2833-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TWP02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	544	547	560	rBV	724867	715177	23.36%	5.110%
2	6.510	715	718	734	rBV	490915	446765	14.60%	3.192%
3	6.881	778	781	785	rBV	562873	492058	16.08%	3.516%
4	7.451	873	878	881	rBV	1673621	1663708	54.35%	11.886%
5	8.169	995	1000	1003	rBV	714937	629055	20.55%	4.494%
6	9.245	1177	1183	1186	rBV	3241836	2870057	93.76%	20.505%
7	9.928	1293	1299	1302	rBV	786246	735919	24.04%	5.258%
8	10.716	1429	1433	1447	rBV	1565185	1386318	45.29%	9.905%
9	11.416	1548	1552	1556	rBV	970973	811146	26.50%	5.795%
10	13.004	1817	1822	1825	rBV	3413088	3060944	100.00%	21.869%
11	13.910	1971	1976	1986	rBV	20135	46307	1.51%	0.331%
12	14.063	1998	2002	2006	rBV	683176	599872	19.60%	4.286%
13	14.151	2013	2017	2024	rBV	34712	40269	1.32%	0.288%
14	15.557	2250	2256	2265	rVB	380323	499206	16.31%	3.567%




Sum of corrected areas: 13996801

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
Data File : BF128265.D
Acq On : 16 May 2022 13:40
Operator : CG\JU
Sample : N2833-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

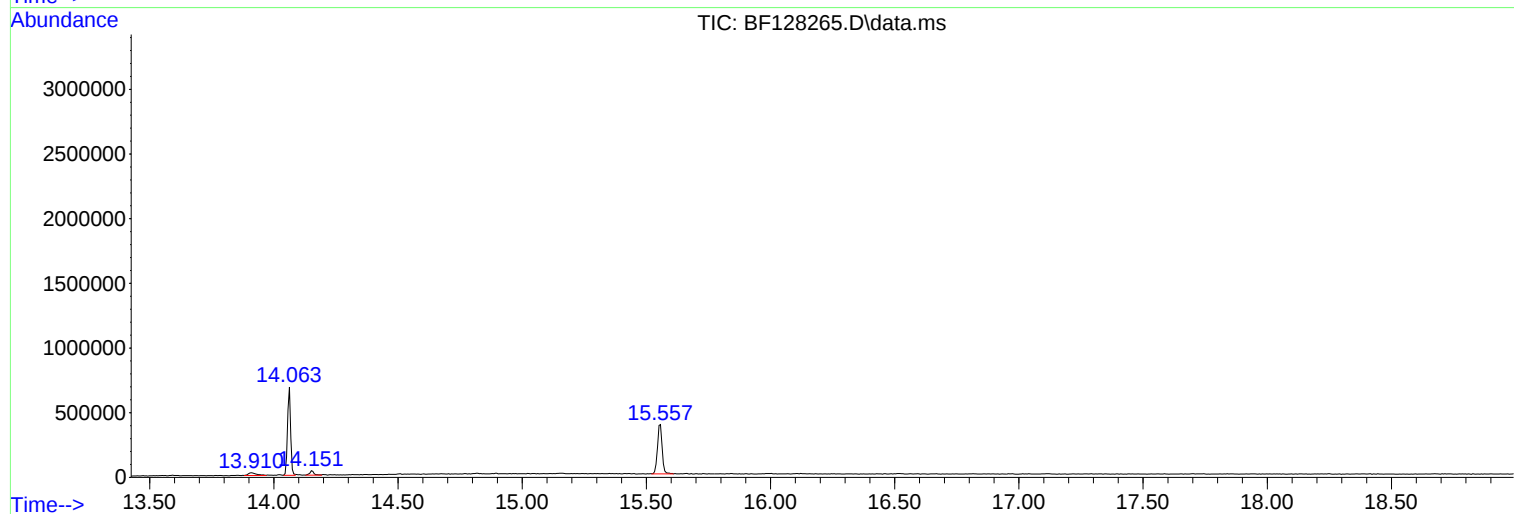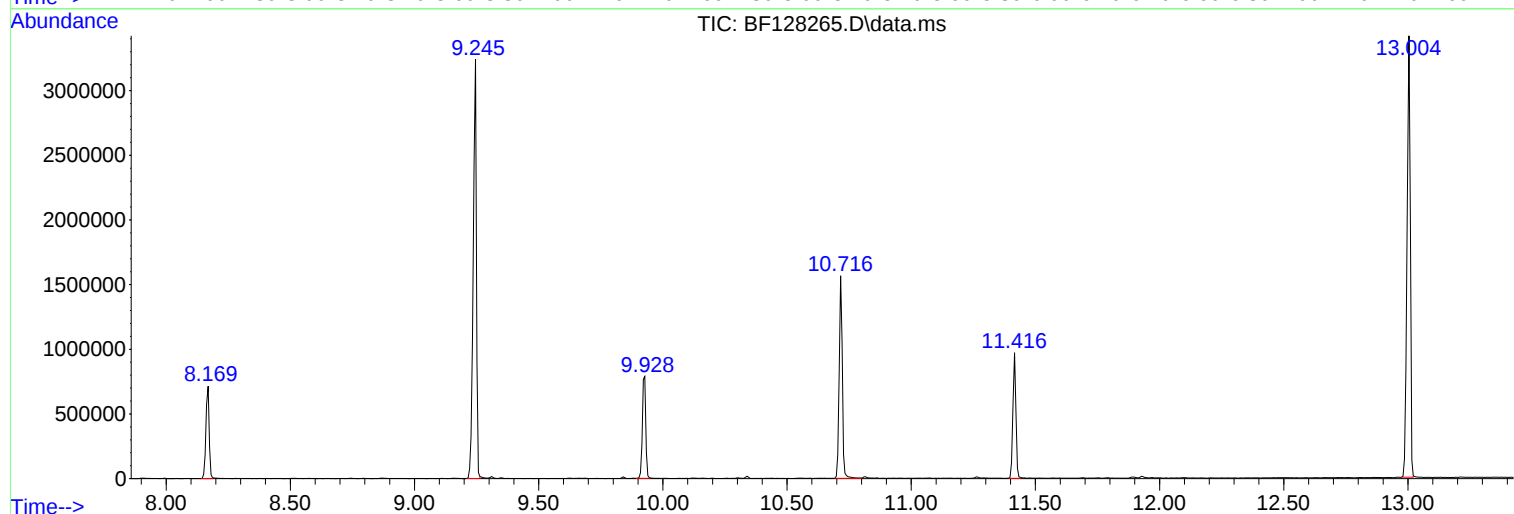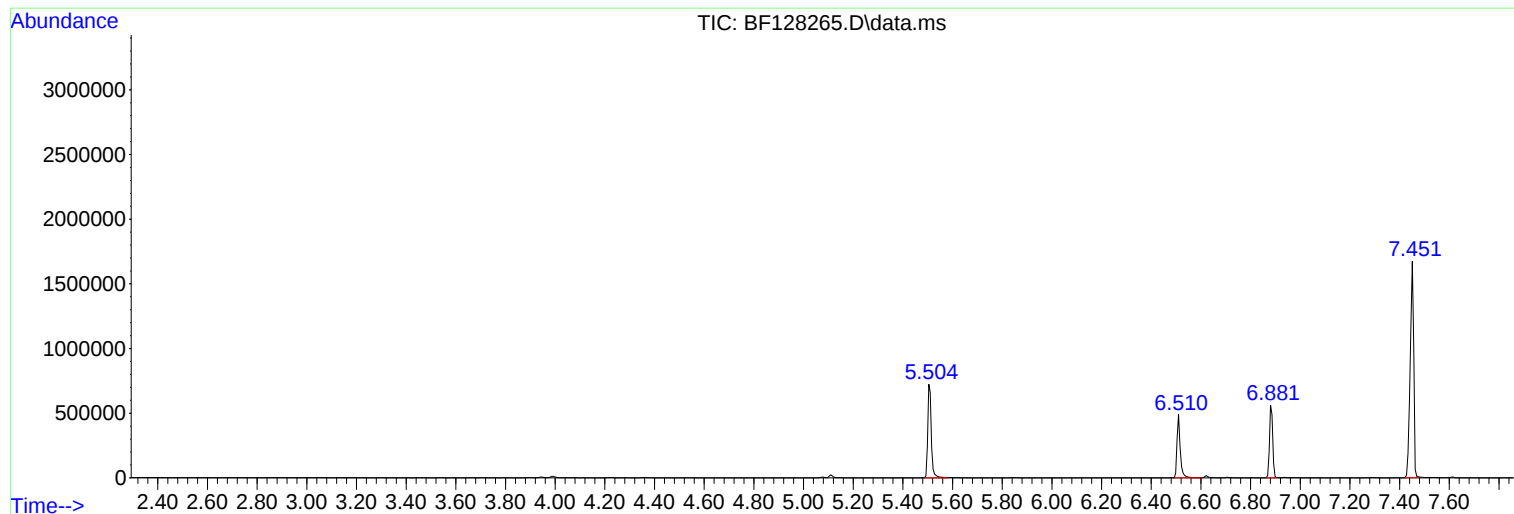

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
Data File : BF128265.D
Acq On : 16 May 2022 13:40
Operator : CG\JU
Sample : N2833-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
Data File : BF128265.D
Acq On : 16 May 2022 13:40
Operator : CG\JU
Sample : N2833-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------