

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
 Data File : BF128266.D
 Acq On : 16 May 2022 14:10
 Operator : CG\JU
 Sample : N2833-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TWP03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128266.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.104	476	479	487	rVB	26483	30545	1.19%	0.245%
2	5.504	544	547	562	rBV	850501	756506	29.41%	6.057%
3	6.510	715	718	732	rBV	592711	506989	19.71%	4.059%
4	6.881	778	781	785	rBV	525742	441303	17.15%	3.533%
5	7.451	873	878	881	rBV	1582841	1414020	54.97%	11.322%
6	8.169	996	1000	1003	rBV	606584	563535	21.91%	4.512%
7	9.245	1178	1183	1186	rBV	2704852	2510627	97.59%	20.102%
8	9.922	1294	1298	1302	rBV	761026	656431	25.52%	5.256%
9	10.716	1429	1433	1447	rBV	1387769	1183652	46.01%	9.477%
10	11.416	1548	1552	1560	rBV	847185	694650	27.00%	5.562%
11	13.004	1817	1822	1825	rBV	2849287	2572559	100.00%	20.598%
12	13.910	1970	1976	1985	rBV6	22412	59771	2.32%	0.479%
13	14.063	1998	2002	2010	rBV	617064	566717	22.03%	4.538%
14	14.151	2014	2017	2022	rVB	29623	31966	1.24%	0.256%
15	15.557	2250	2256	2264	rVB	383518	500267	19.45%	4.005%




Sum of corrected areas: 12489538

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
Data File : BF128266.D
Acq On : 16 May 2022 14:10
Operator : CG\JU
Sample : N2833-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

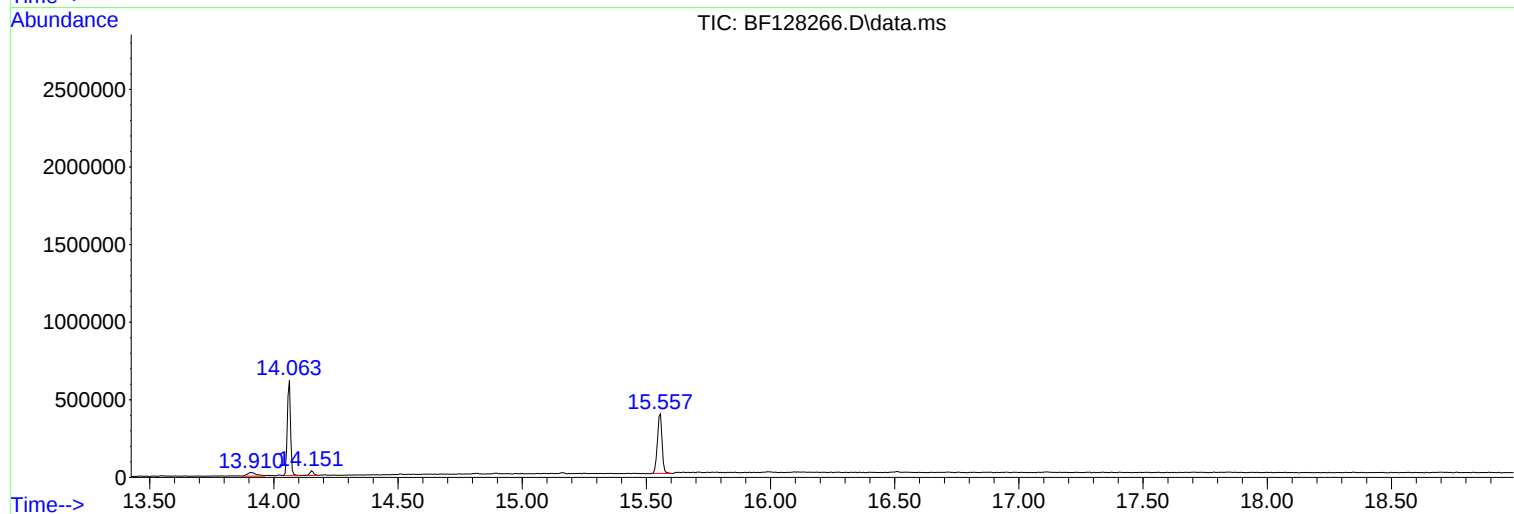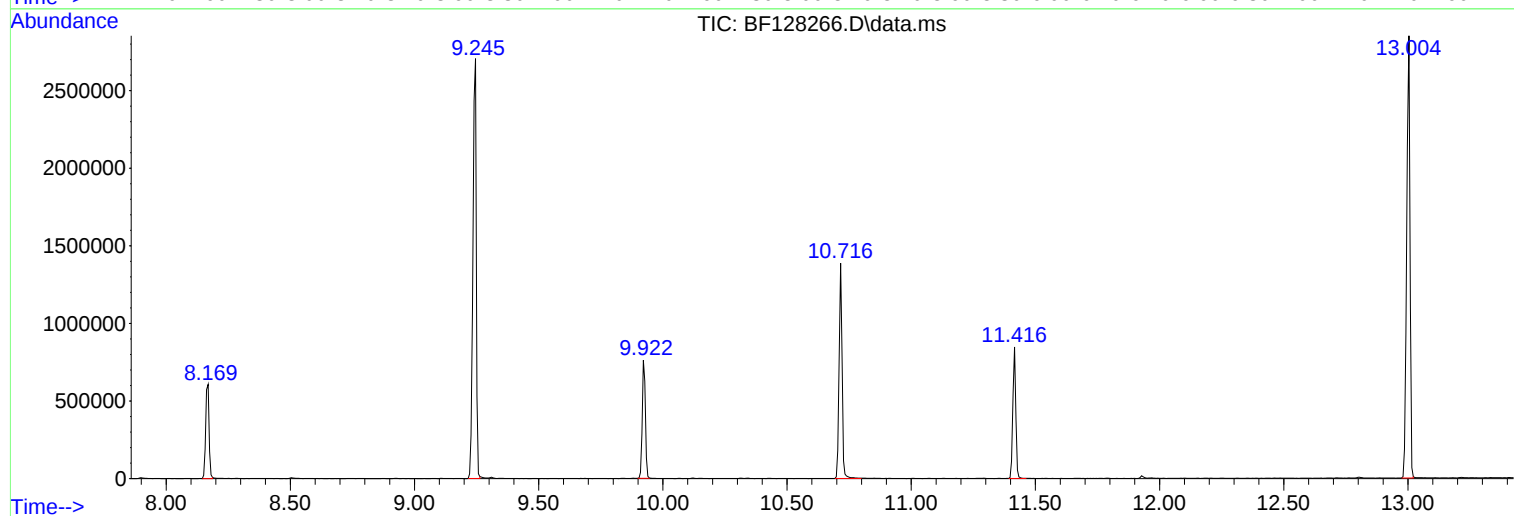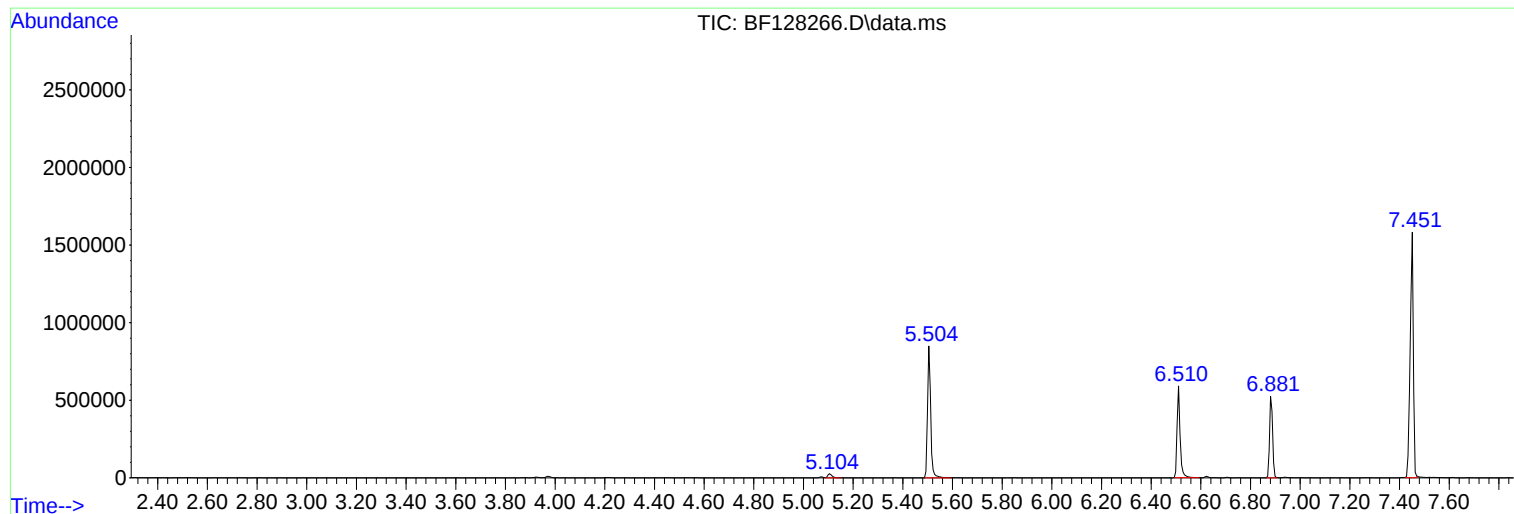

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
Data File : BF128266.D
Acq On : 16 May 2022 14:10
Operator : CG\JU
Sample : N2833-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP03










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentafluoropropionic acid, ... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.910	2.11 ng	59771	Chrysene-d12	14.063

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pentafluoropropionic acid, tetra...	360	C17H29F5O2	006222-06-6	93
2			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	93
3			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	93
4			1-Heptacosanol	396	C27H56O	002004-39-9	87
5			1-Hexacosene	364	C26H52	018835-33-1	81

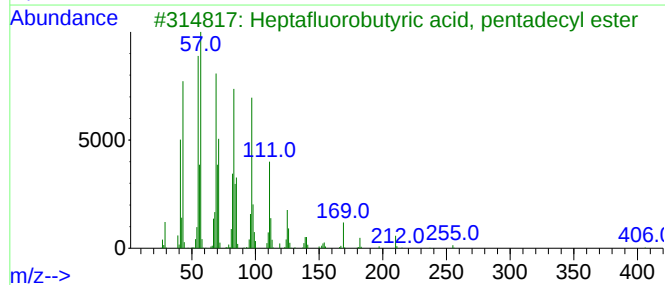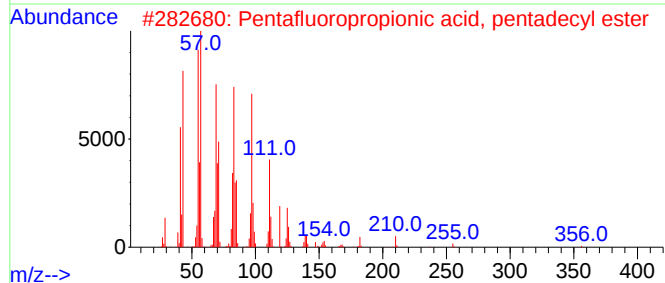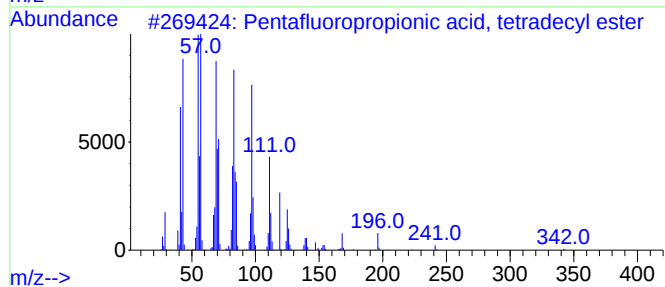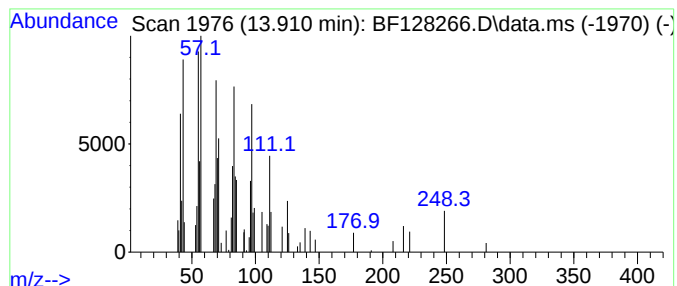

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
Data File : BF128266.D
Acq On : 16 May 2022 14:10
Operator : CG\JU
Sample : N2833-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentafluoroprop...	13.910	2.1	ng	59771	5	14.063	566717	20.0