
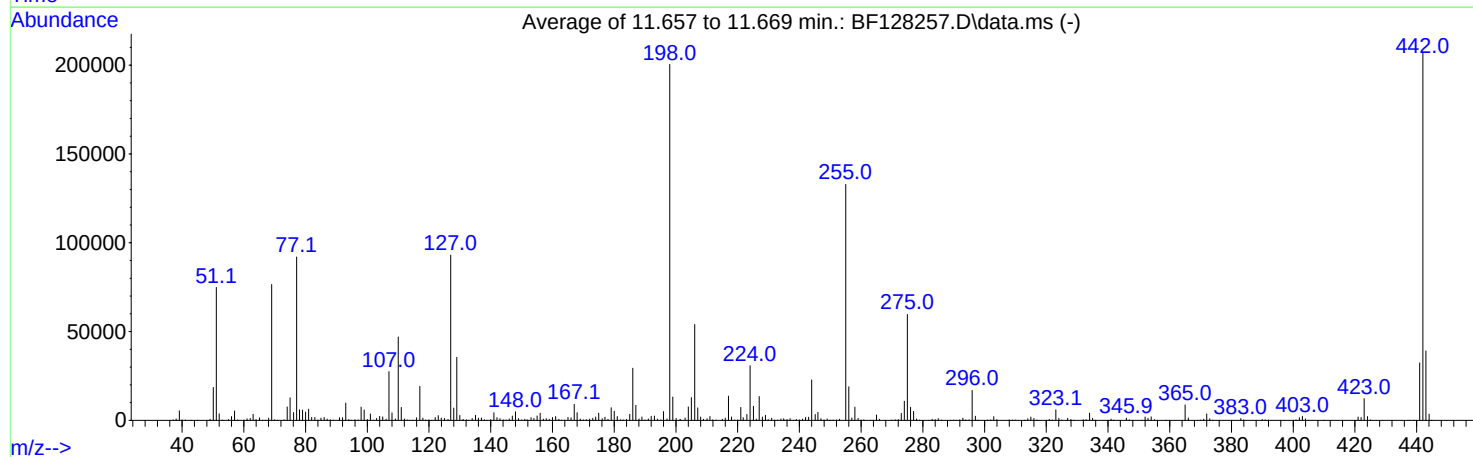


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
 Data File : BF128257.D
 Acq On : 16 May 2022 09:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 14 00:51:21 2022

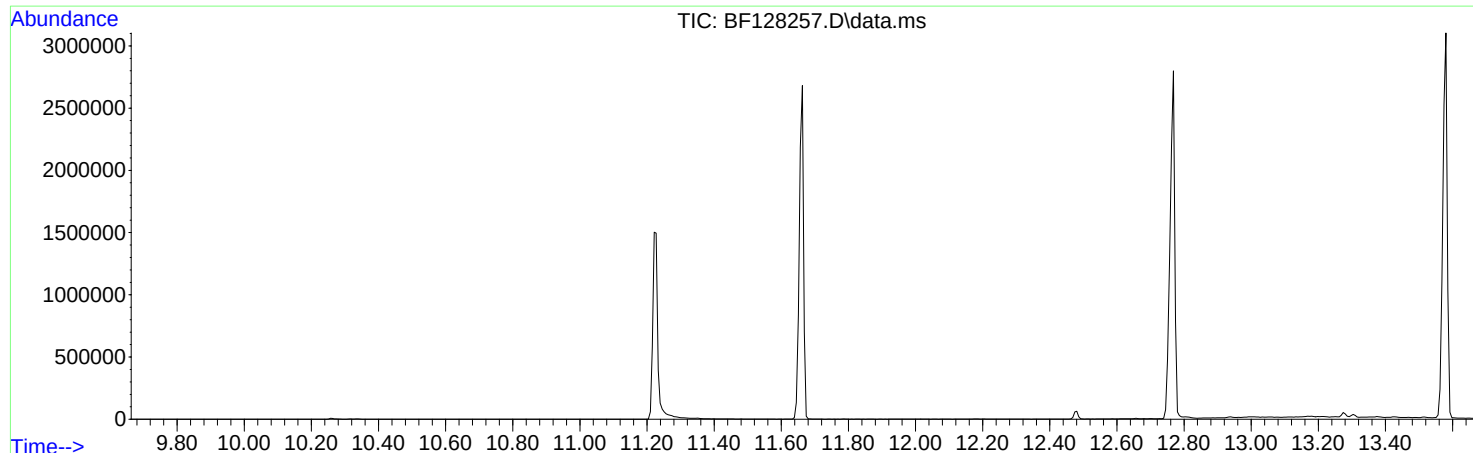




AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	74848	PASS
68	69	0.00	2	1.7	1307	PASS
69	198	0.00	100	38.1	76460	PASS
70	69	0.00	2	0.5	396	PASS
127	198	10	80	46.4	93093	PASS
197	198	0.00	2	0.4	776	PASS
198	198	100	100	100.0	200424	PASS
199	198	5	9	6.6	13173	PASS
275	198	10	60	29.8	59683	PASS
365	198	1	100	4.4	8773	PASS
441	198	0.01	100	16.2	32381	PASS
442	442	50	100	100.0	207125	PASS
443	442	15	24	18.9	39069	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
Data File : BF128257.D
Acq On : 16 May 2022 09:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 16 18:37:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 14 00:51:21 2022
Response via : Initial Calibration

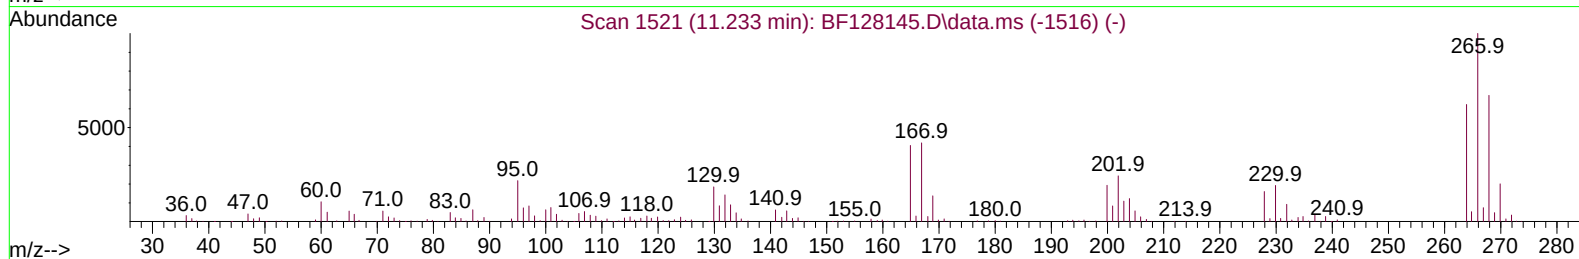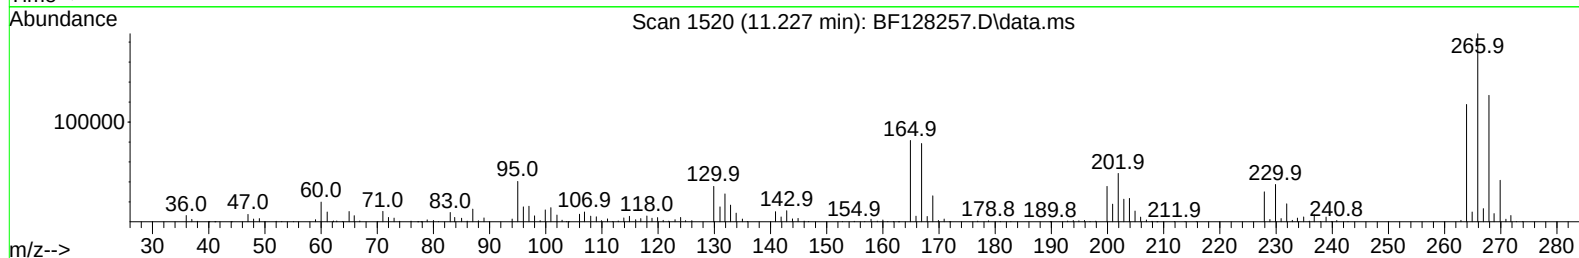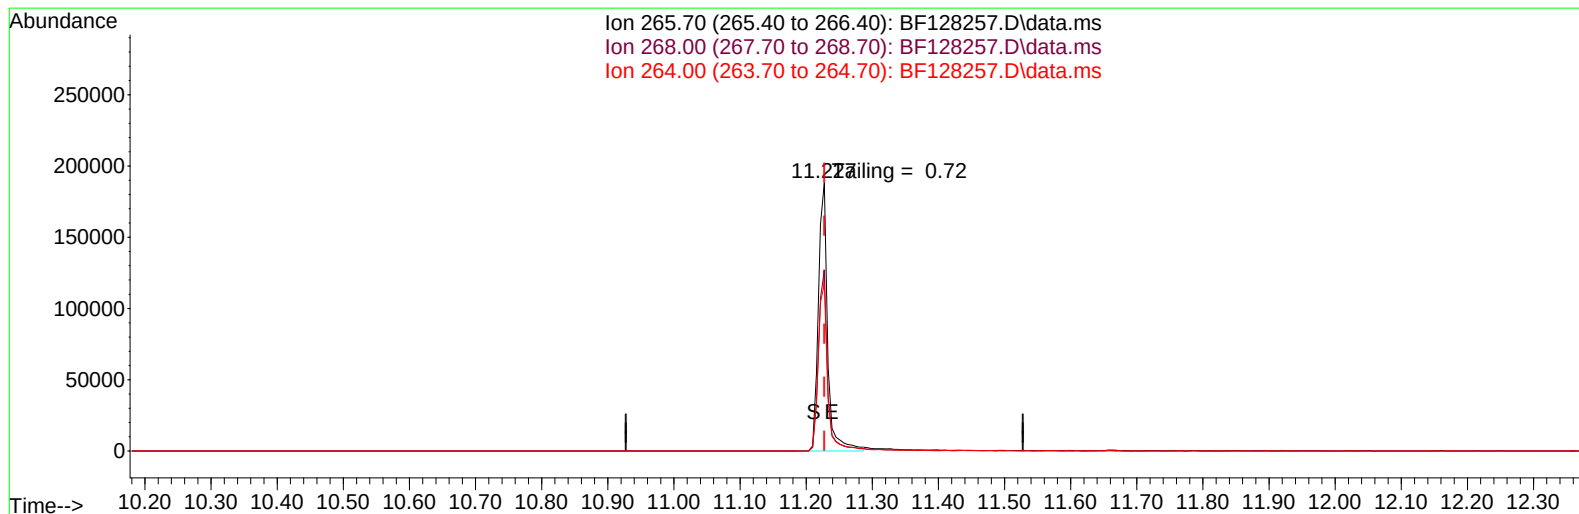

TIC: BF128257.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 336994.85 ng




response 190555

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.27
264.00	66.40	62.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
 Data File : BF128257.D
 Acq On : 16 May 2022 09:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 16 18:37:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 14 00:51:21 2022
 Response via : Initial Calibration

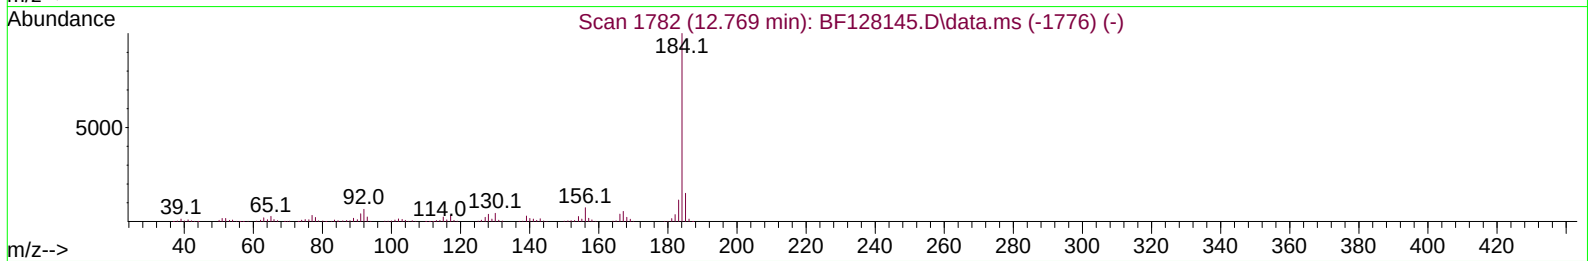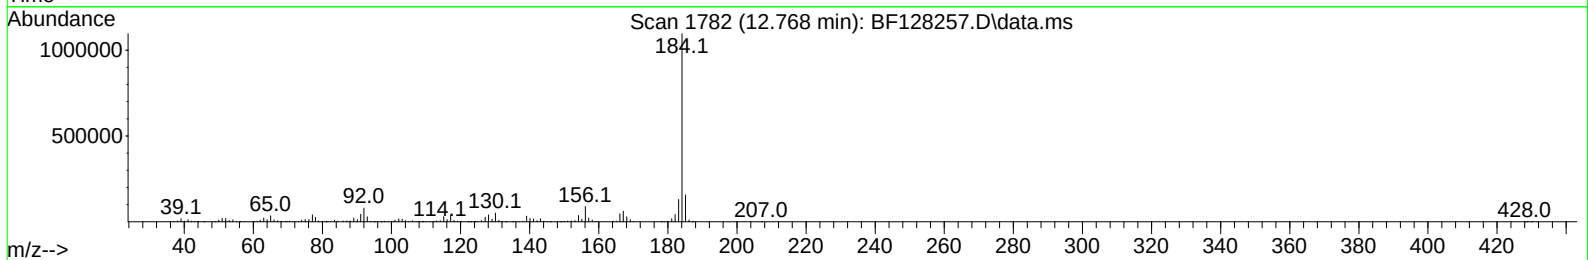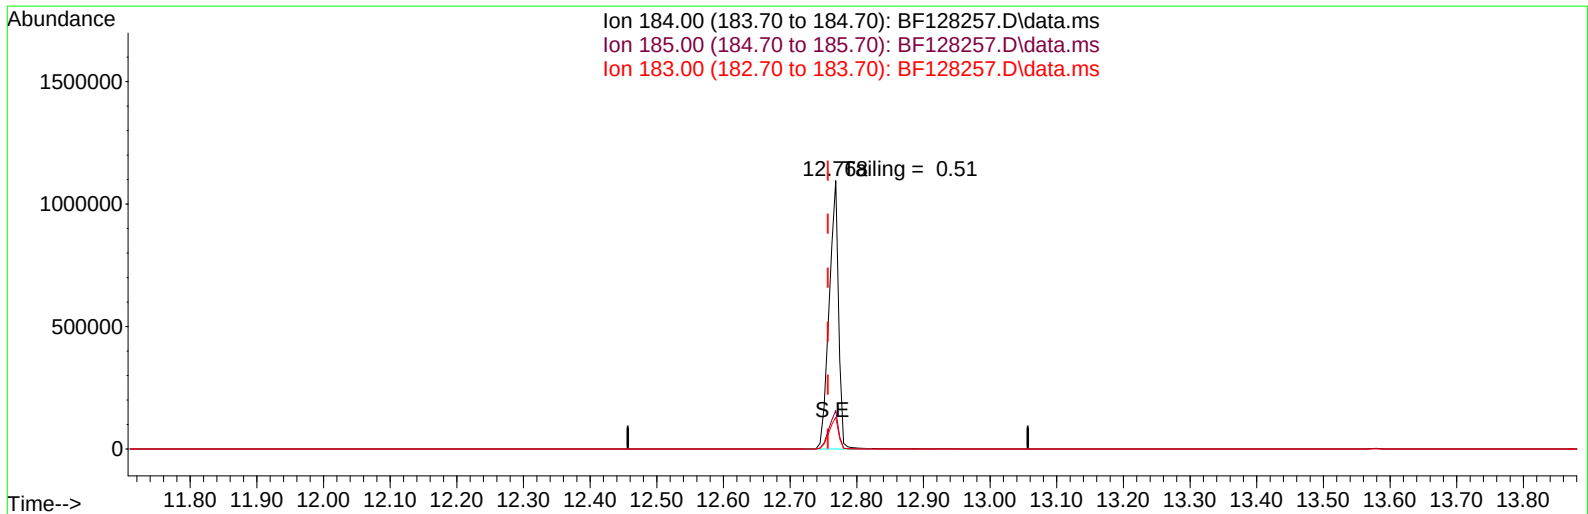

TIC: BF128257.D\data.ms

(77) Benzidine**12.768min (+ 0.012) 102623.33 ng****response 1073539**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.31
183.00	11.20	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/16/2022	BNA_F	<u>BF128257.D</u>
Compound Name	Response	Retention Time
DDT	548340	13.58
DDD	6271	13.27
DDE	888	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7159	555499	1.29

Instrument :
BNA_F
ClientSampleId :
DFTPP