
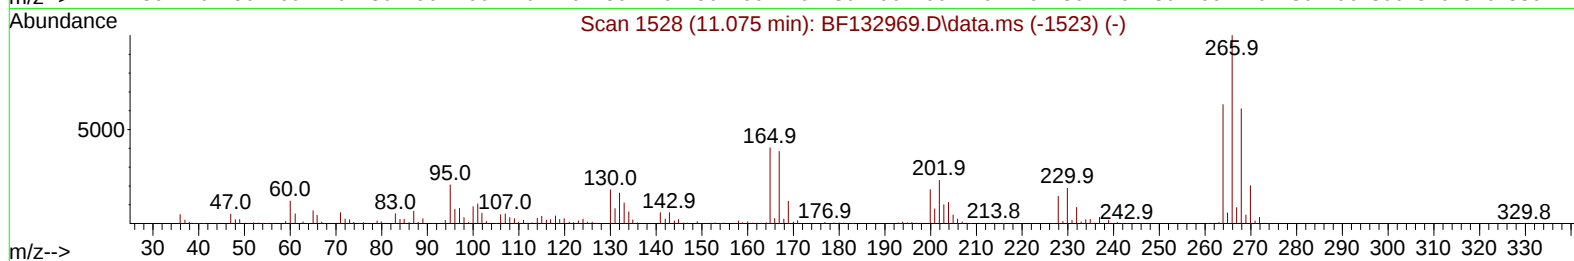
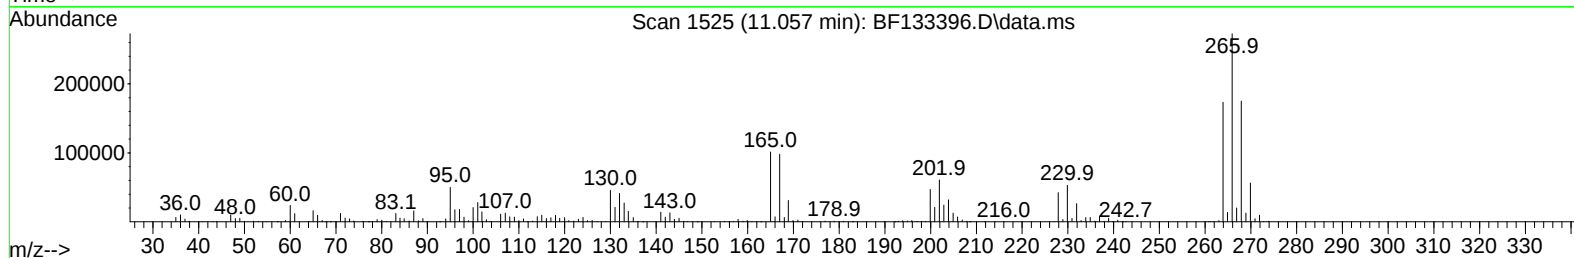


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051623\
Data File : BF133396.D
Acq On : 16 May 2023 11:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 16:14:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 16 14:39:29 2023
Response via : Initial Calibration

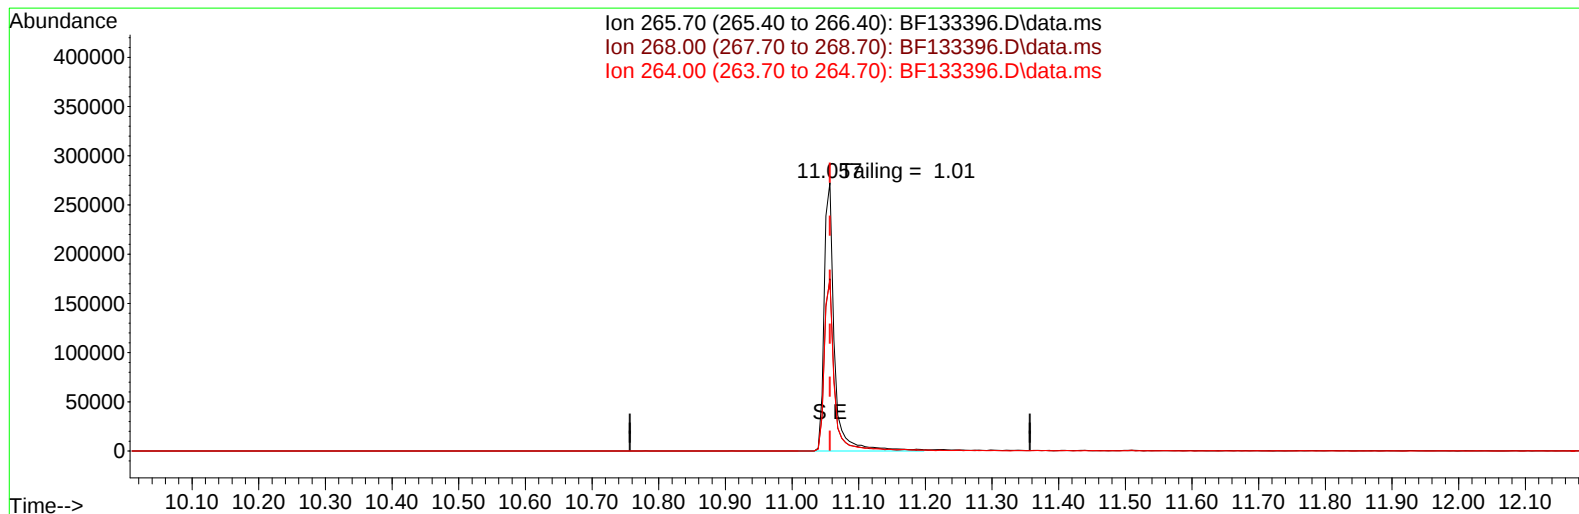

TIC: BF133396.D\data.ms

(70) Pentachlorophenol (C)




11.057min (-0.000) 144336.21 ng

response 289027

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.16
264.00	63.30	63.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051623\
Data File : BF133396.D
Acq On : 16 May 2023 11:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 16:14:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 16 14:39:29 2023
Response via : Initial Calibration

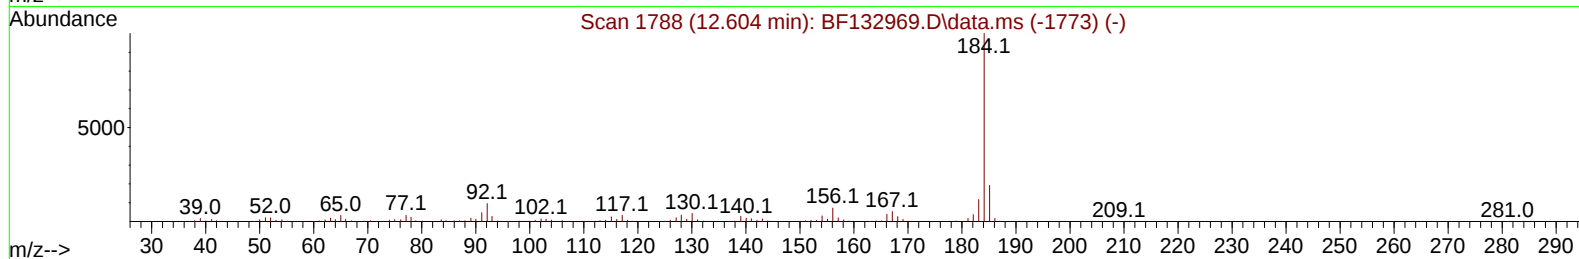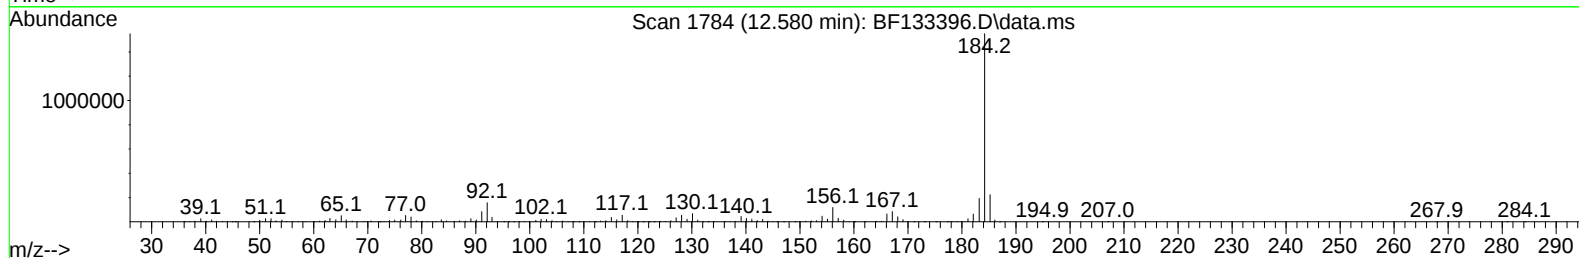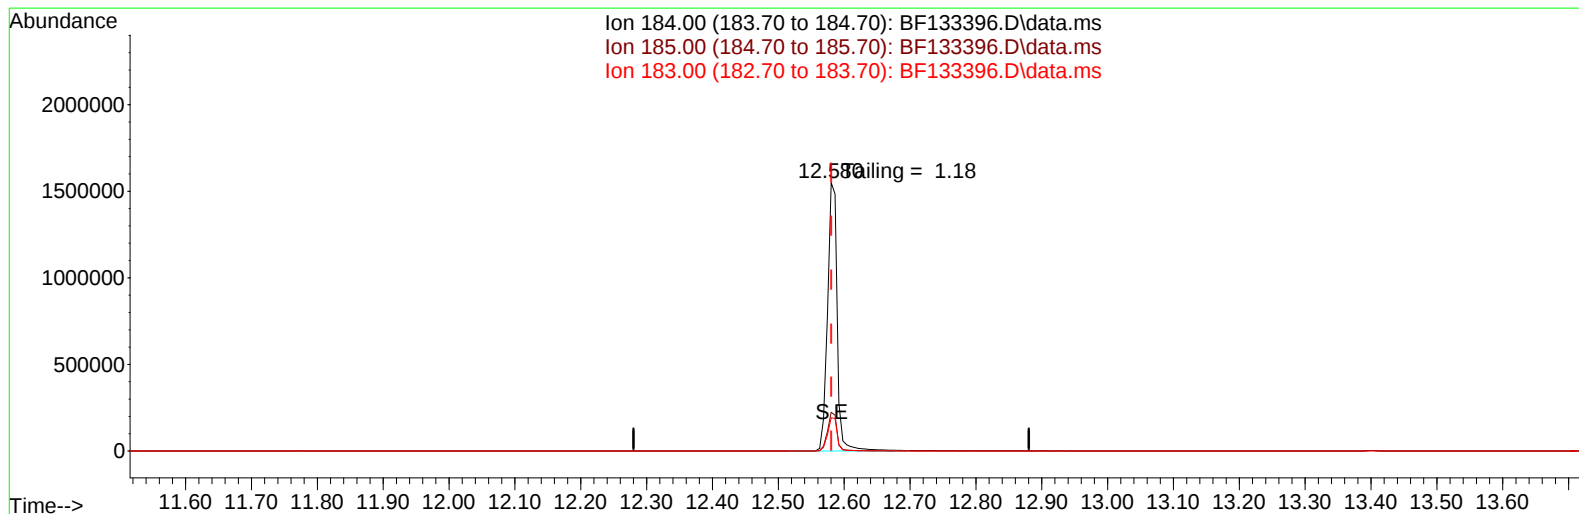

TIC: BF133396.D\data.ms

(77) Benzidine**12.580min (-0.000) 85949.78 ng****response 1600255**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.42#
183.00	11.70	12.43
0.00	0.00	0.00