
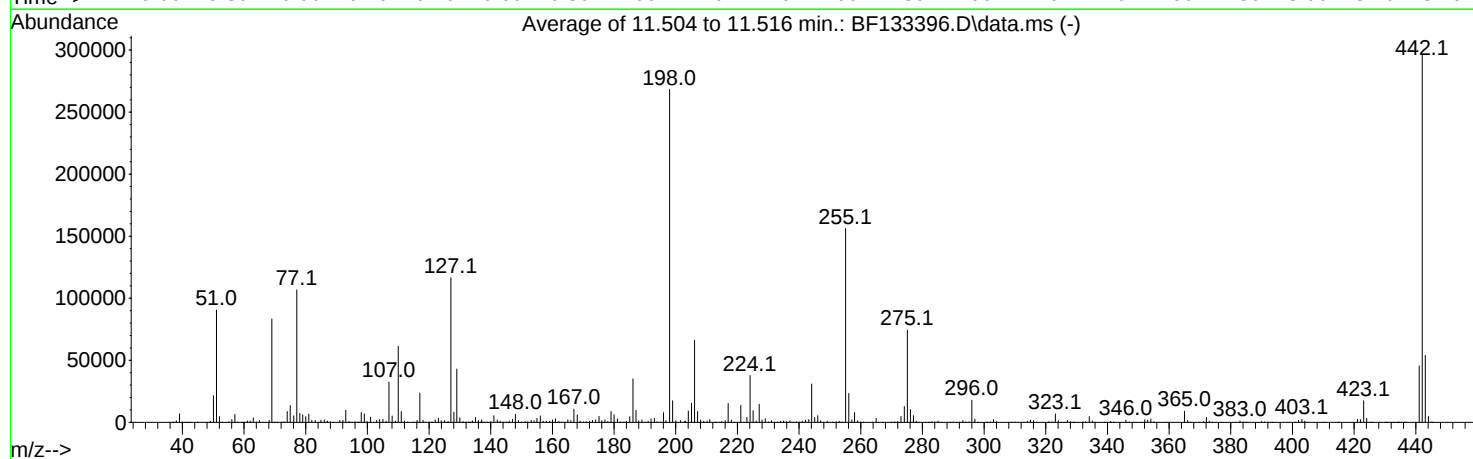


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051623\
 Data File : BF133396.D
 Acq On : 16 May 2023 11:07
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 16 14:39:29 2023

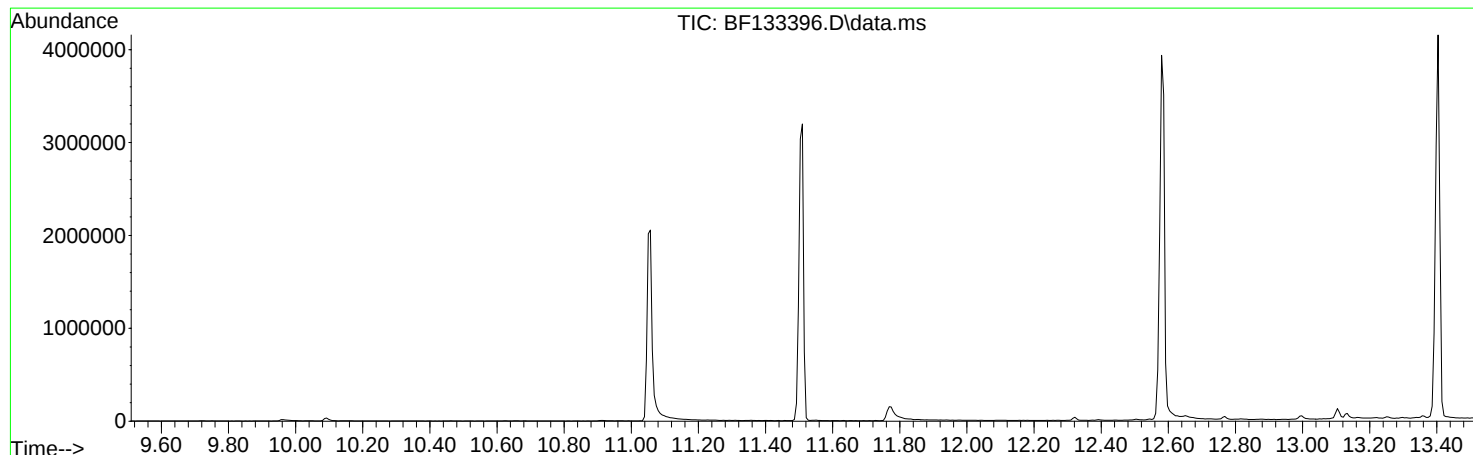

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	90535	PASS
68	69	0.00	2	2.0	1653	PASS
69	198	0.00	100	31.0	83233	PASS
70	69	0.00	2	0.5	394	PASS
127	198	10	80	43.5	116619	PASS
197	198	0.00	2	0.5	1364	PASS
198	198	100	100	100.0	268269	PASS
199	198	5	9	6.5	17415	PASS
275	198	10	60	27.7	74301	PASS
365	198	1	100	3.4	9026	PASS
441	198	0.01	100	17.0	45571	PASS
442	442	50	100	100.0	296427	PASS
443	442	15	24	18.2	54040	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/16/2023	BNA_F	<u>BF133396.D</u>
Compound Name	Response	Retention Time
DDT	733413	13.404
DDD	28980	13.104
DDE	3310	12.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32290	765703	4.22

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051623\
 Data File : BF133396.D
 Acq On : 16 May 2023 11:07
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 16 16:14:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 16 14:39:29 2023
 Response via : Initial Calibration

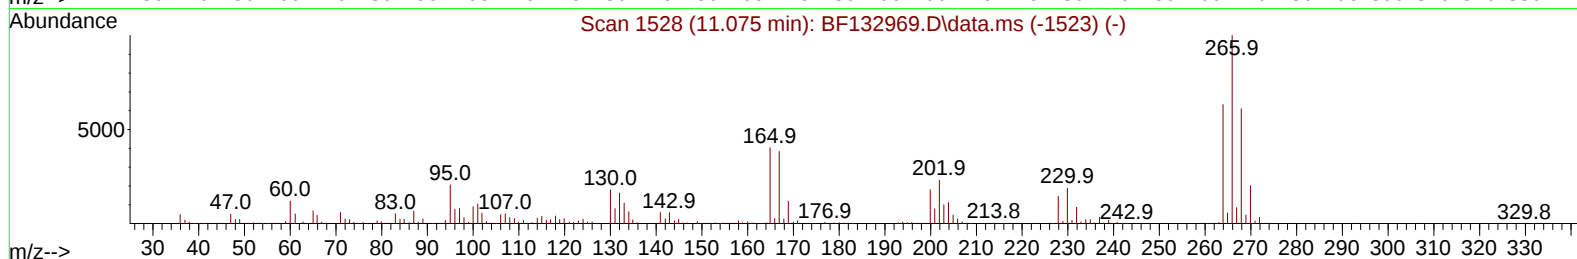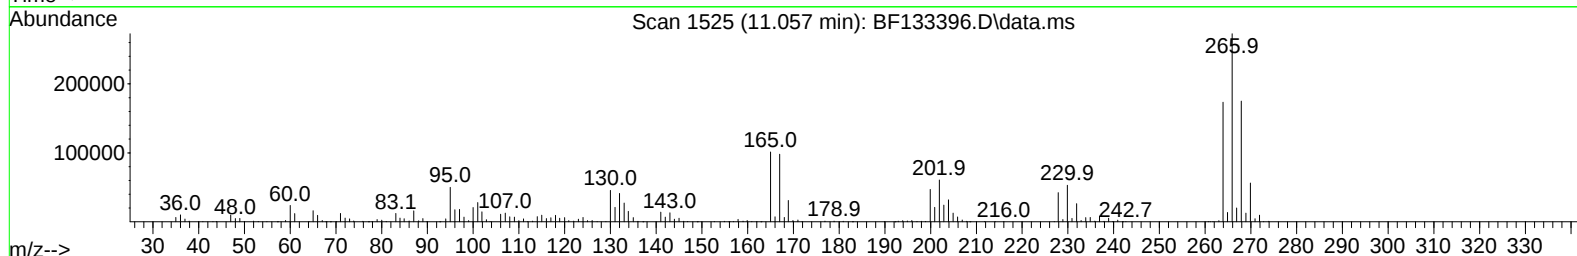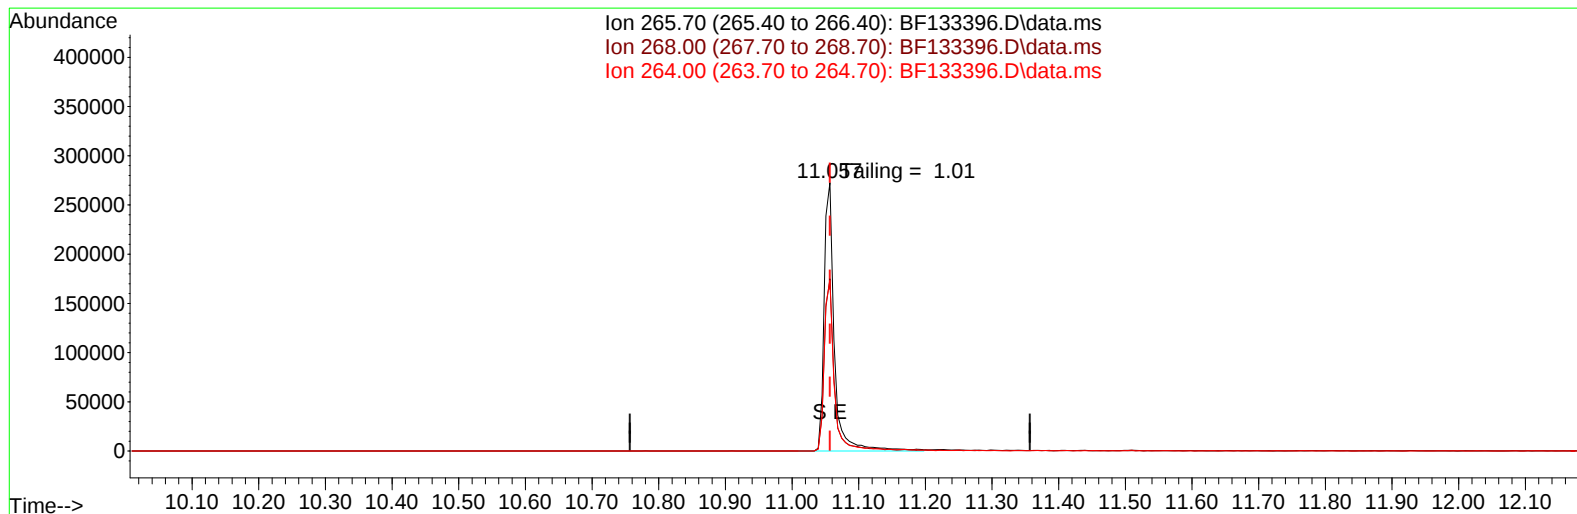

TIC: BF133396.D\data.ms

(70) Pentachlorophenol (C)

11.057min (-0.000) 144336.21 ng




response 289027

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.16
264.00	63.30	63.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051623\
Data File : BF133396.D
Acq On : 16 May 2023 11:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 16 16:14:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 16 14:39:29 2023
Response via : Initial Calibration

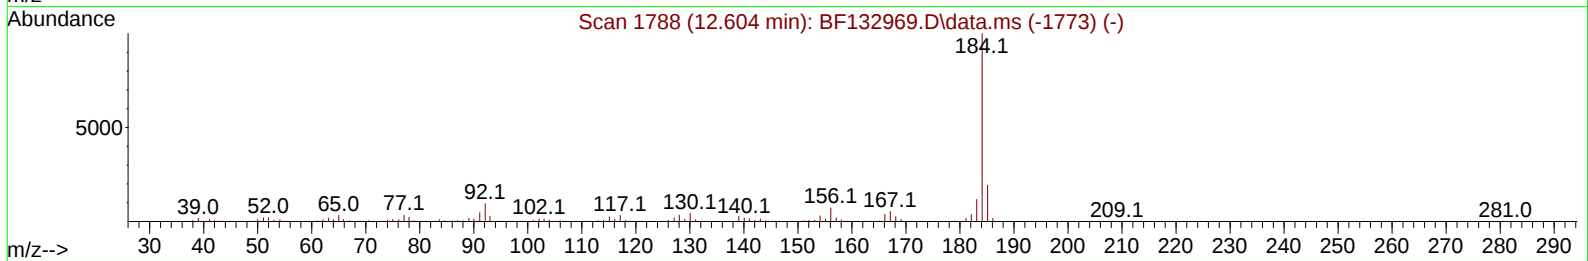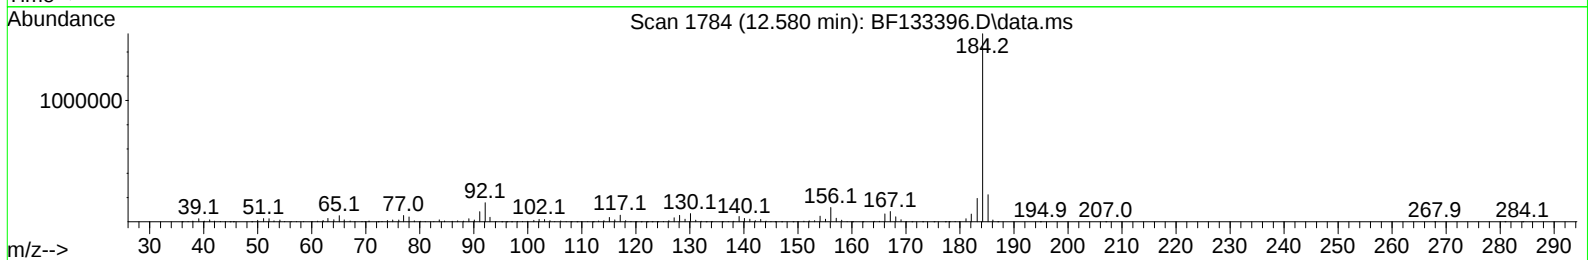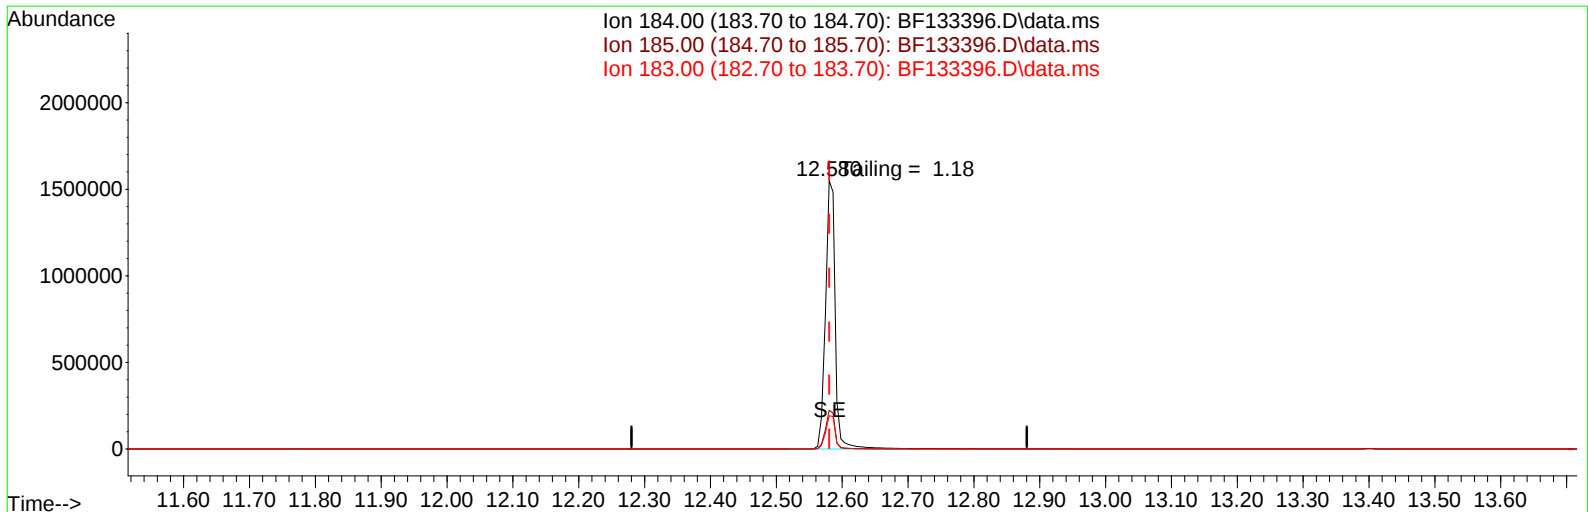

TIC: BF133396.D\data.ms

(77) Benzidine

12.580min (-0.000) 85949.78 ng

response 1600255

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.42#
183.00	11.70	12.43
0.00	0.00	0.00