
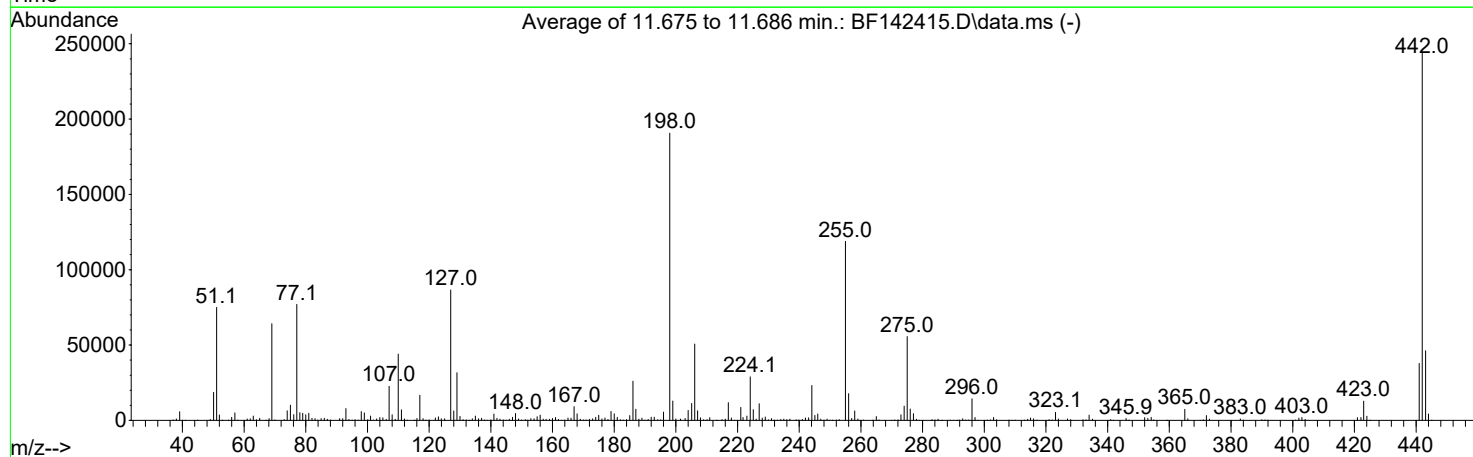


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051625\
Data File : BF142415.D
Acq On : 16 May 2025 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 05 18:41:44 2025

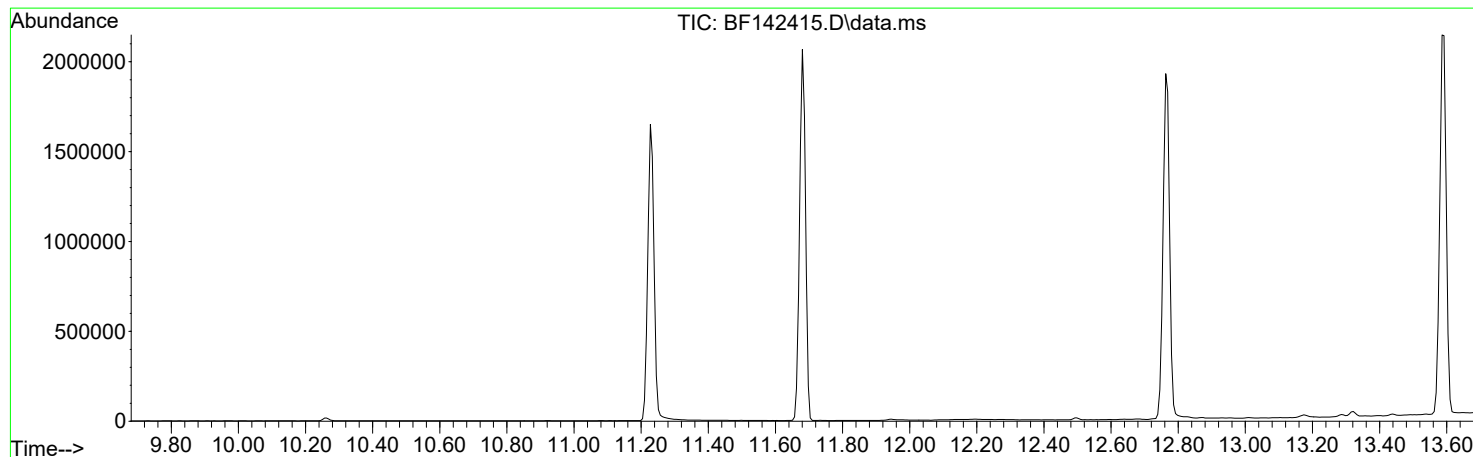

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	74965	PASS
68	69	0.00	2	1.8	1180	PASS
69	198	0.00	100	33.6	64124	PASS
70	69	0.00	2	0.5	327	PASS
127	198	10	80	45.4	86573	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	190699	PASS
199	198	5	9	6.8	12901	PASS
275	198	10	60	29.2	55699	PASS
365	198	1	100	3.9	7361	PASS
441	198	0.01	100	19.8	37803	PASS
442	442	50	100	100.0	244203	PASS
443	442	15	24	18.9	46171	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/16/2025	BNA_F	<u>BF142415.D</u>
Compound Name	Response	Retention Time
DDT	577011	13.592
DDD	9476	13.322
DDE	405	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9881	586892	1.68

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051625\
Data File : BF142415.D
Acq On : 16 May 2025 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 16 12:07:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

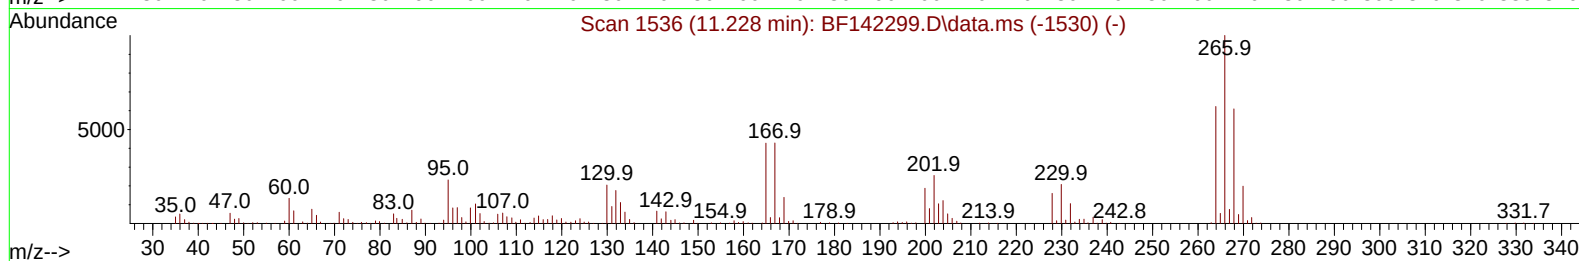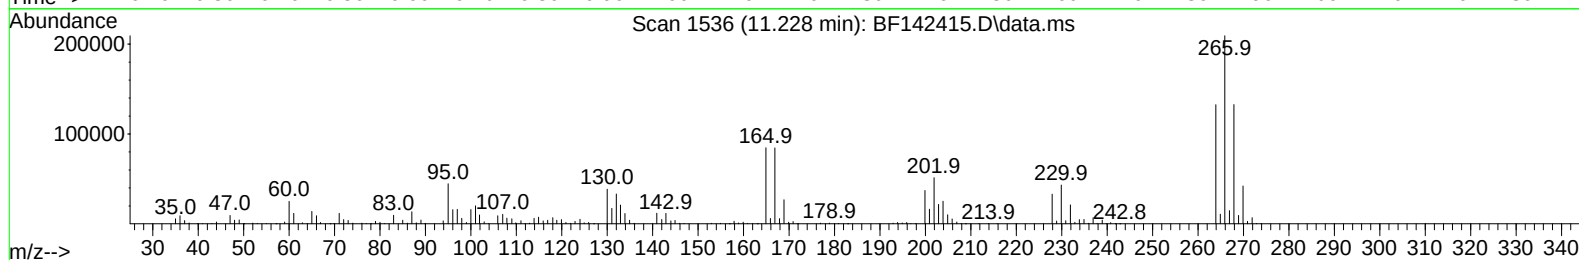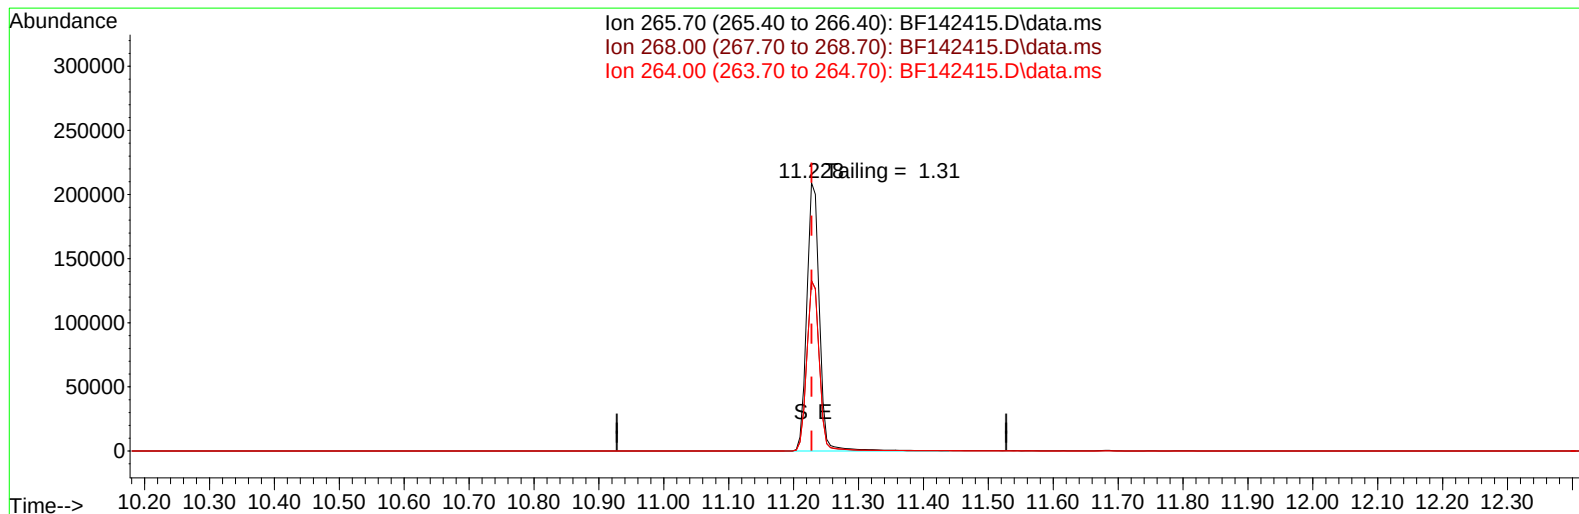

TIC: BF142415.D\data.ms

(70) Pentachlorophenol (C)

11.228min (-0.000) 104520.37 ng




response 282413

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.90	63.46
264.00	62.20	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051625\
Data File : BF142415.D
Acq On : 16 May 2025 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 16 12:07:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

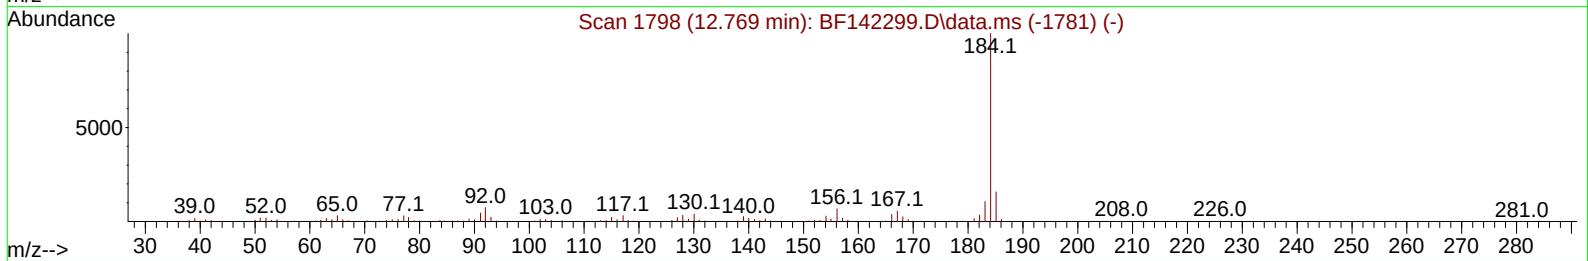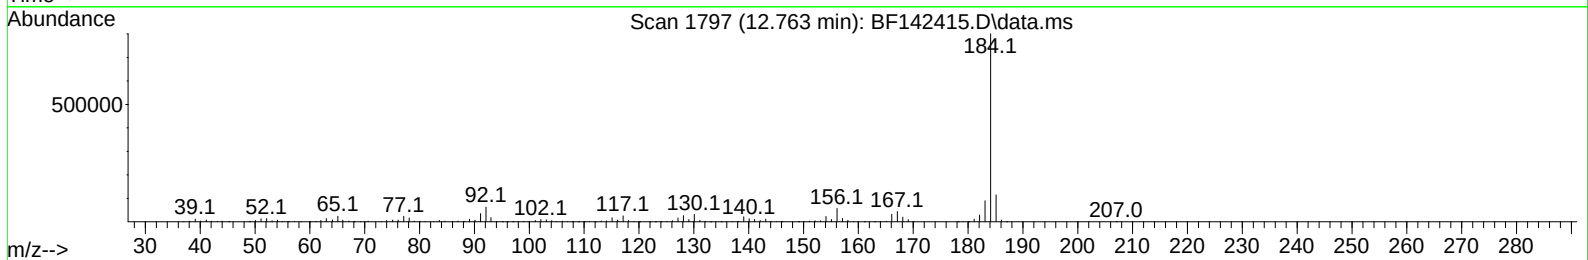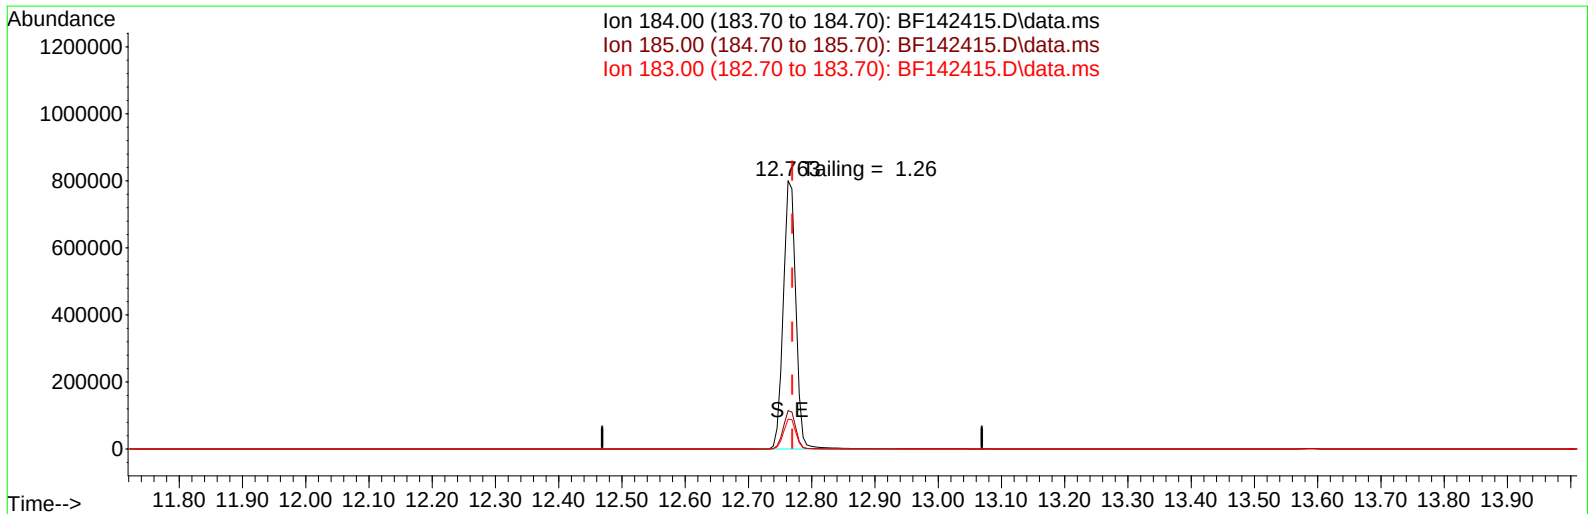

TIC: BF142415.D\data.ms

(77) Benzidine

12.763min (-0.006) 92267.44 ng

response 1111692

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.34
183.00	10.70	11.15
0.00	0.00	0.00