


Benzaldehyde

Response Ratio

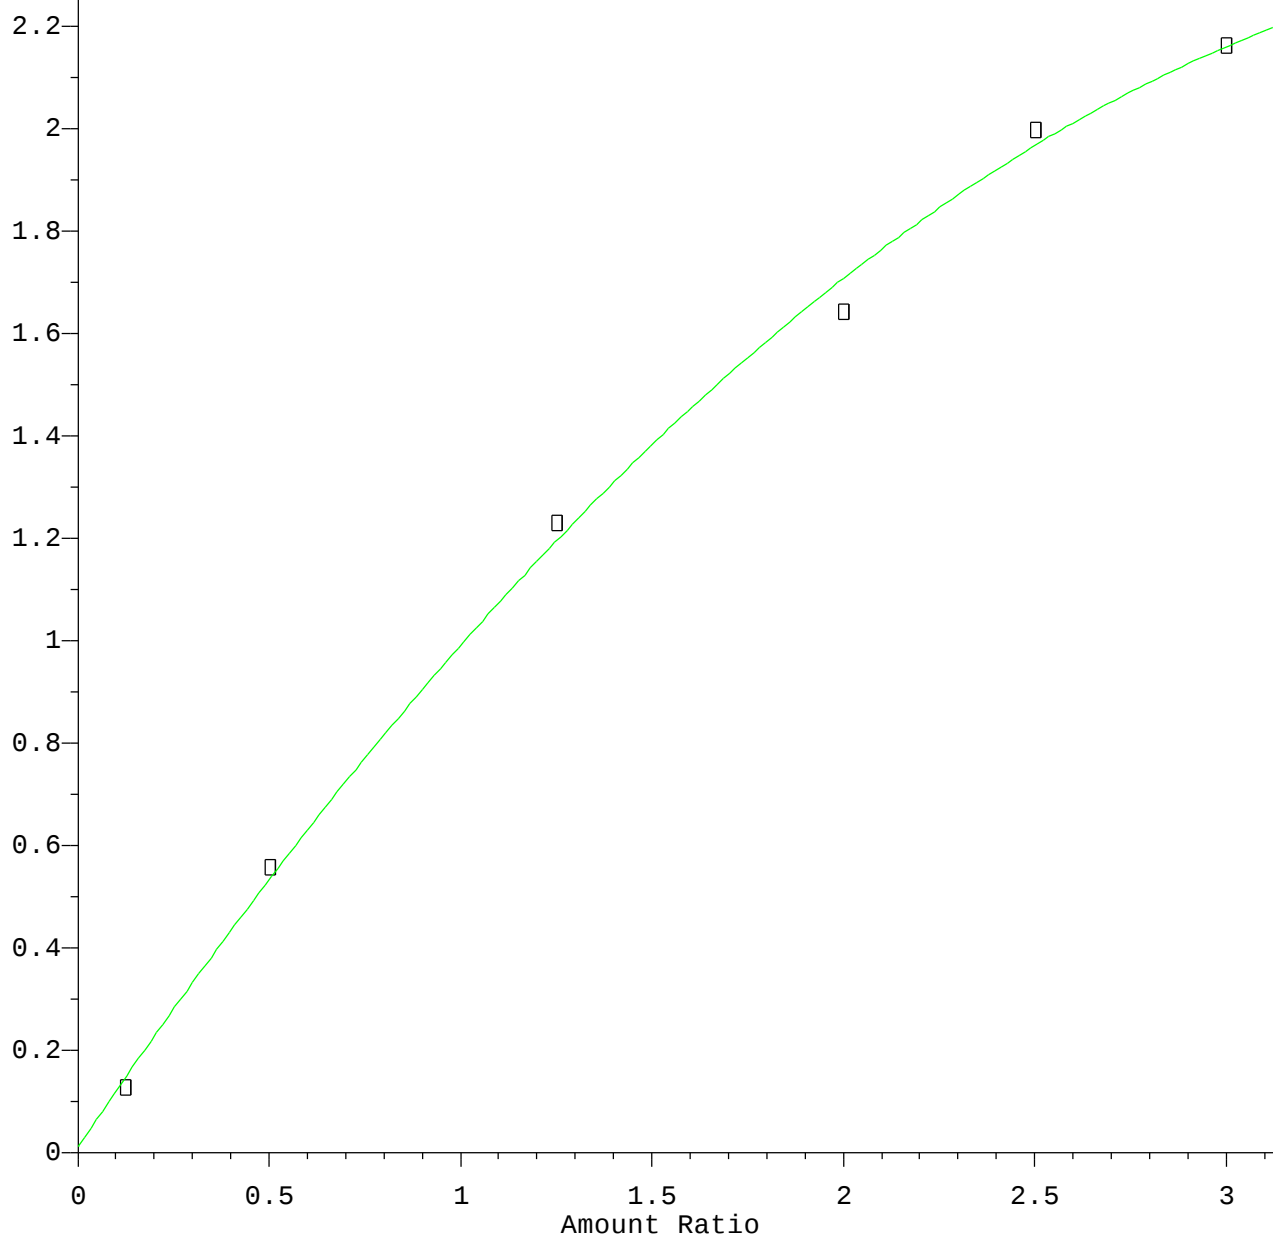


$R = -1.32e-001 A^2 + 1.11e+000 A + 1.18e-002$
Coef of Det (r^2) = 0.998 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Calibration Table Last Updated: Tue May 17 16:55:01 2016


Hexachlorocyclopentadiene

Response Ratio

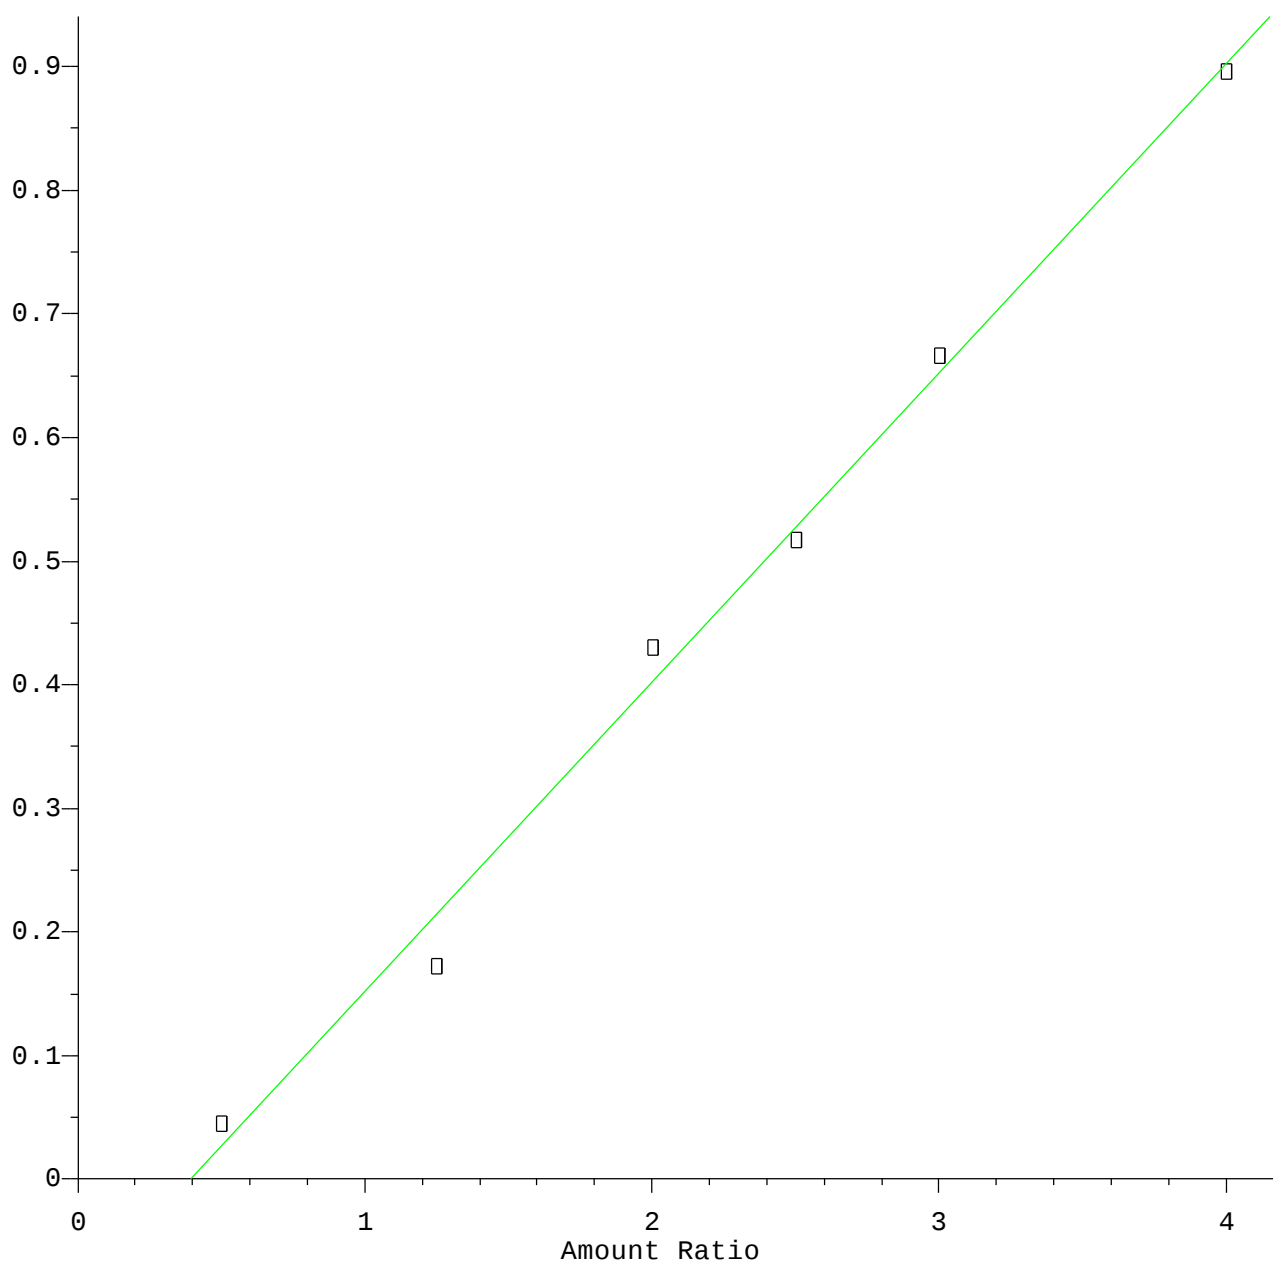


Resp Ratio = $2.50 \times 10^{-1} \times \text{Amt} - 9.82 \times 10^{-2}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Calibration Table Last Updated: Tue May 17 16:55:01 2016

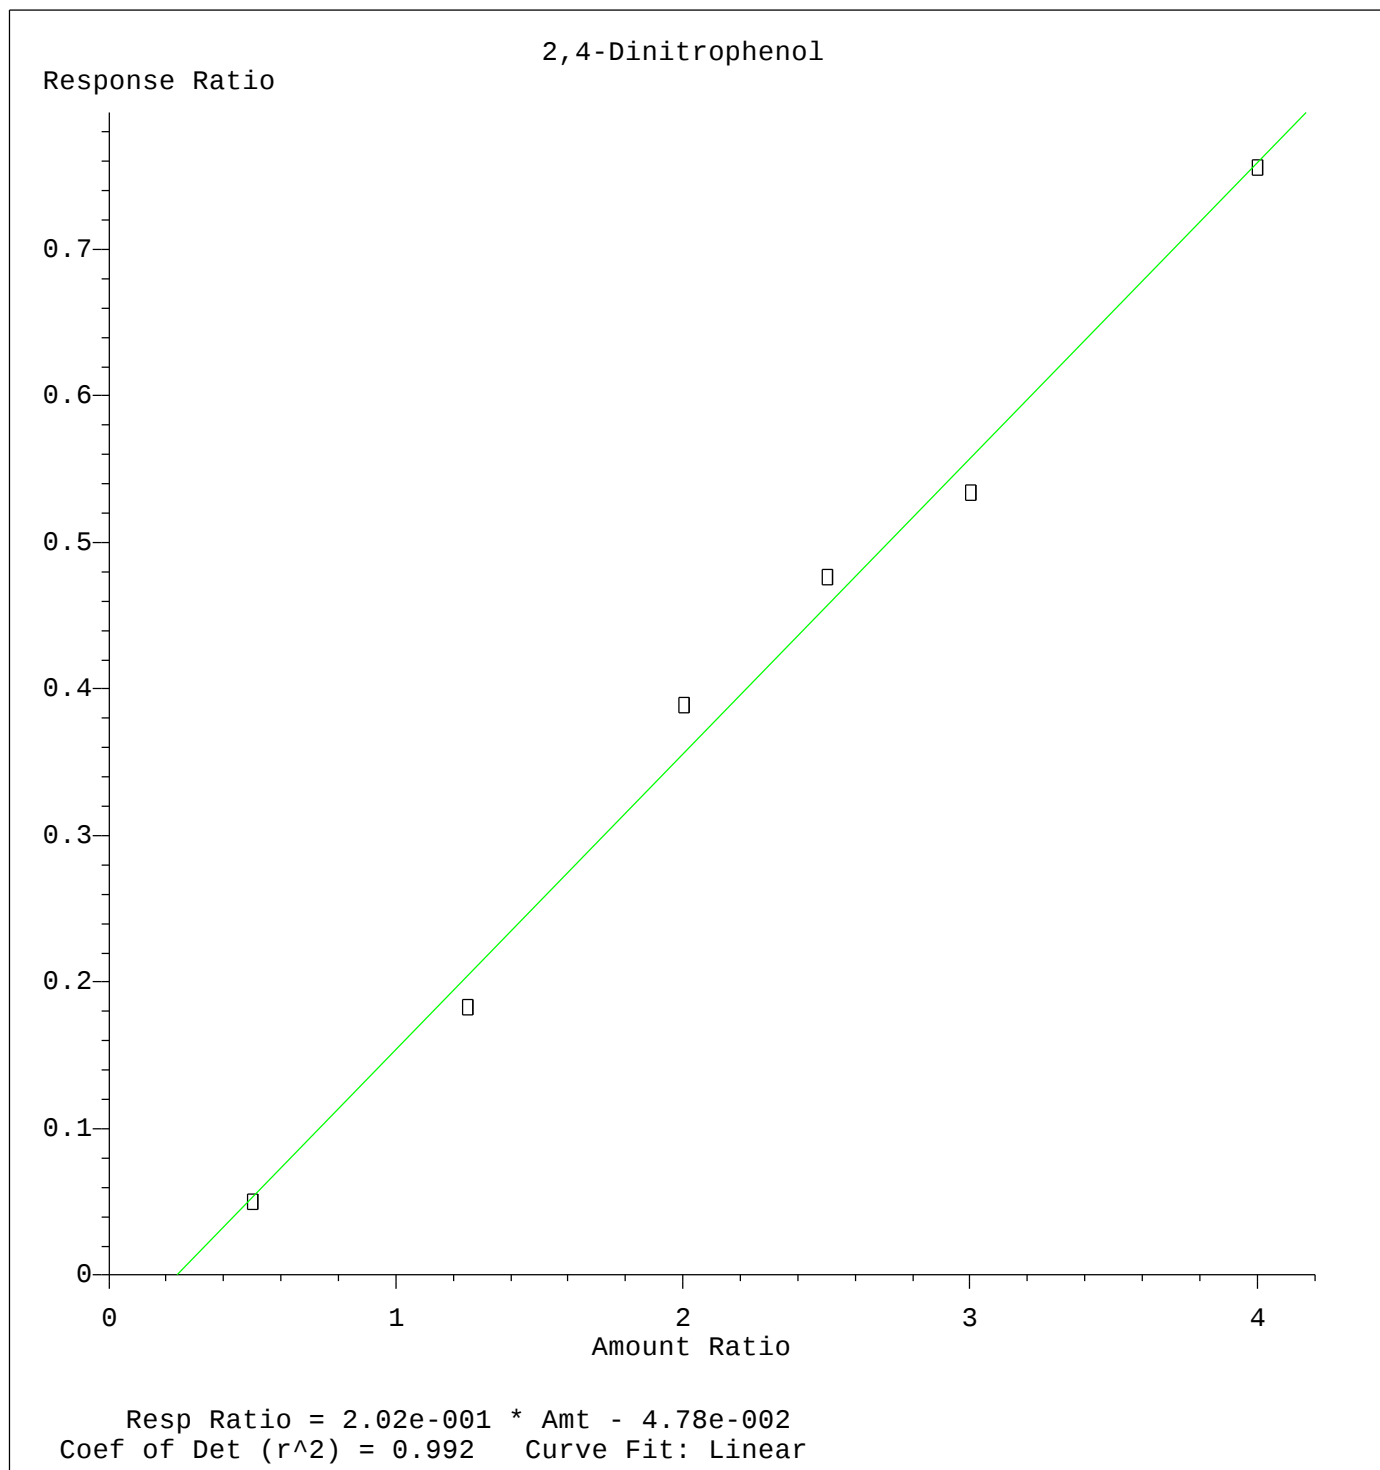

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Calibration Table Last Updated: Tue May 17 16:55:01 2016

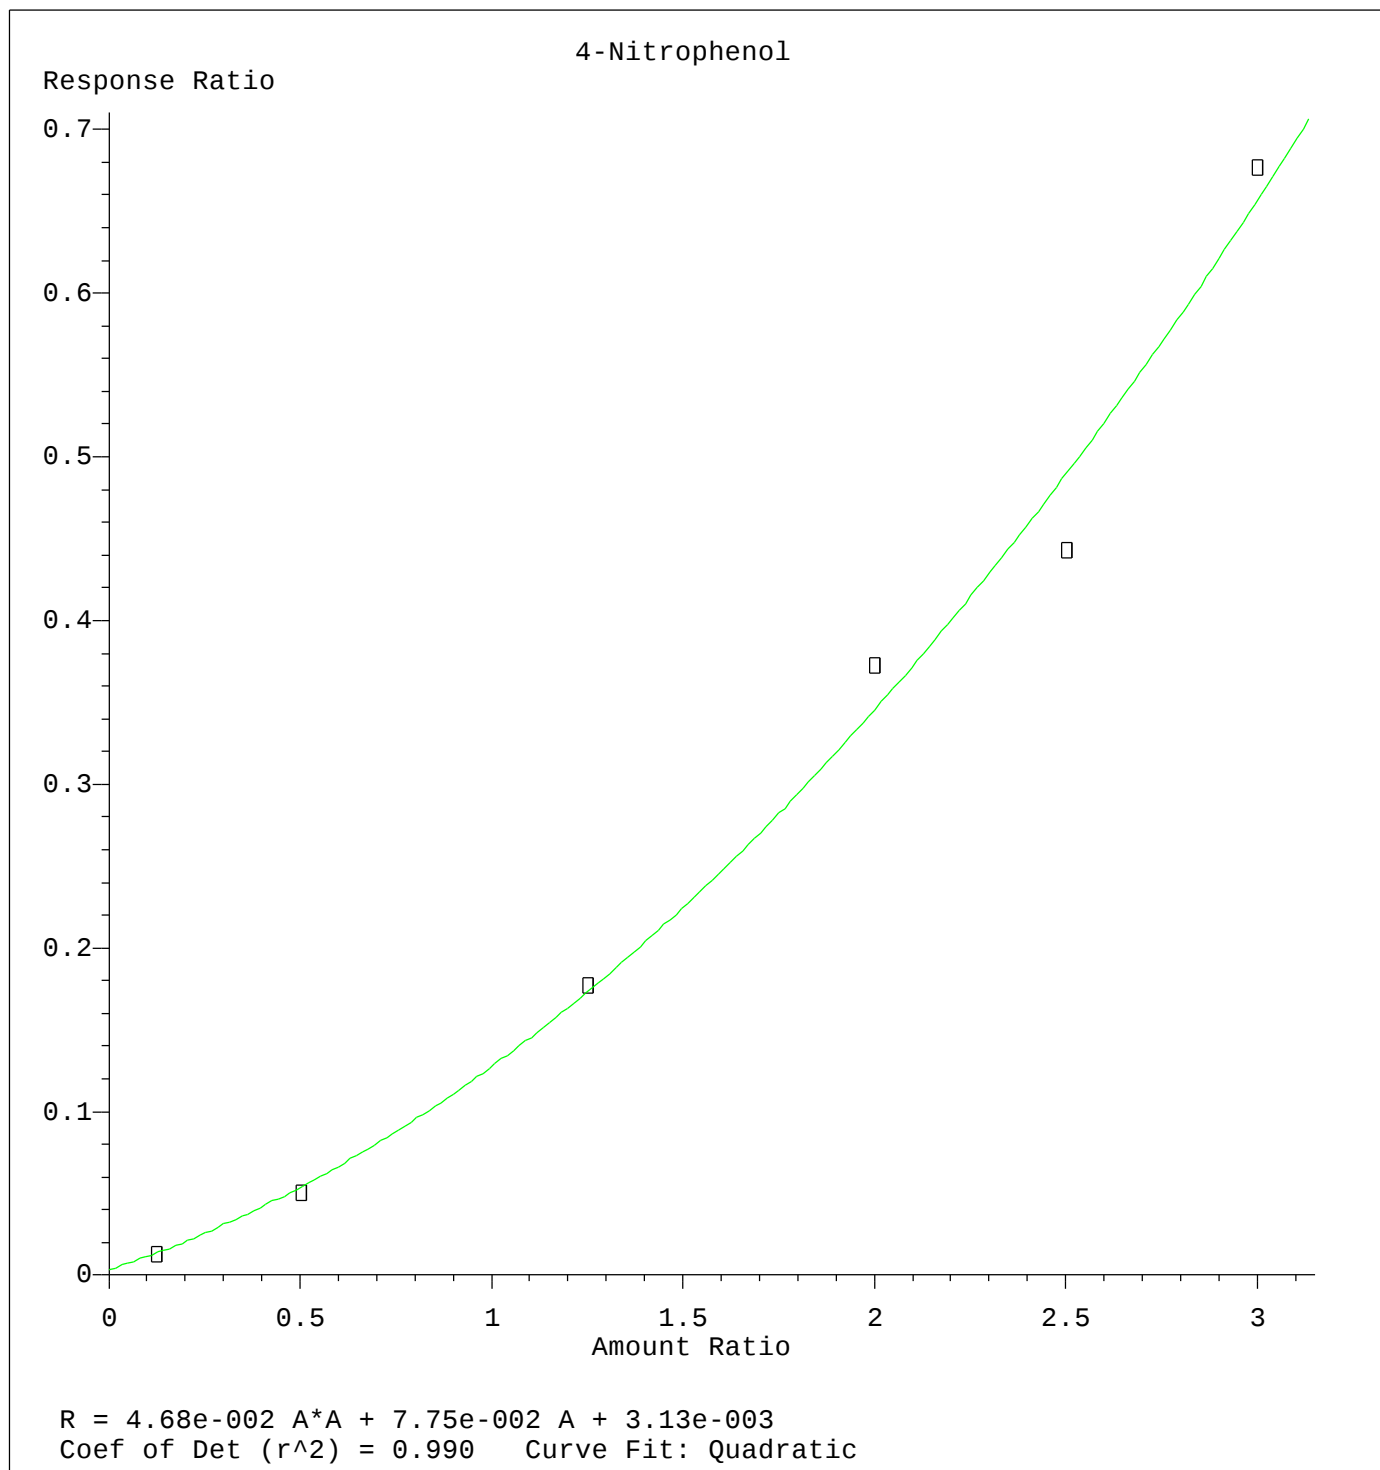

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Calibration Table Last Updated: Tue May 17 16:55:01 2016

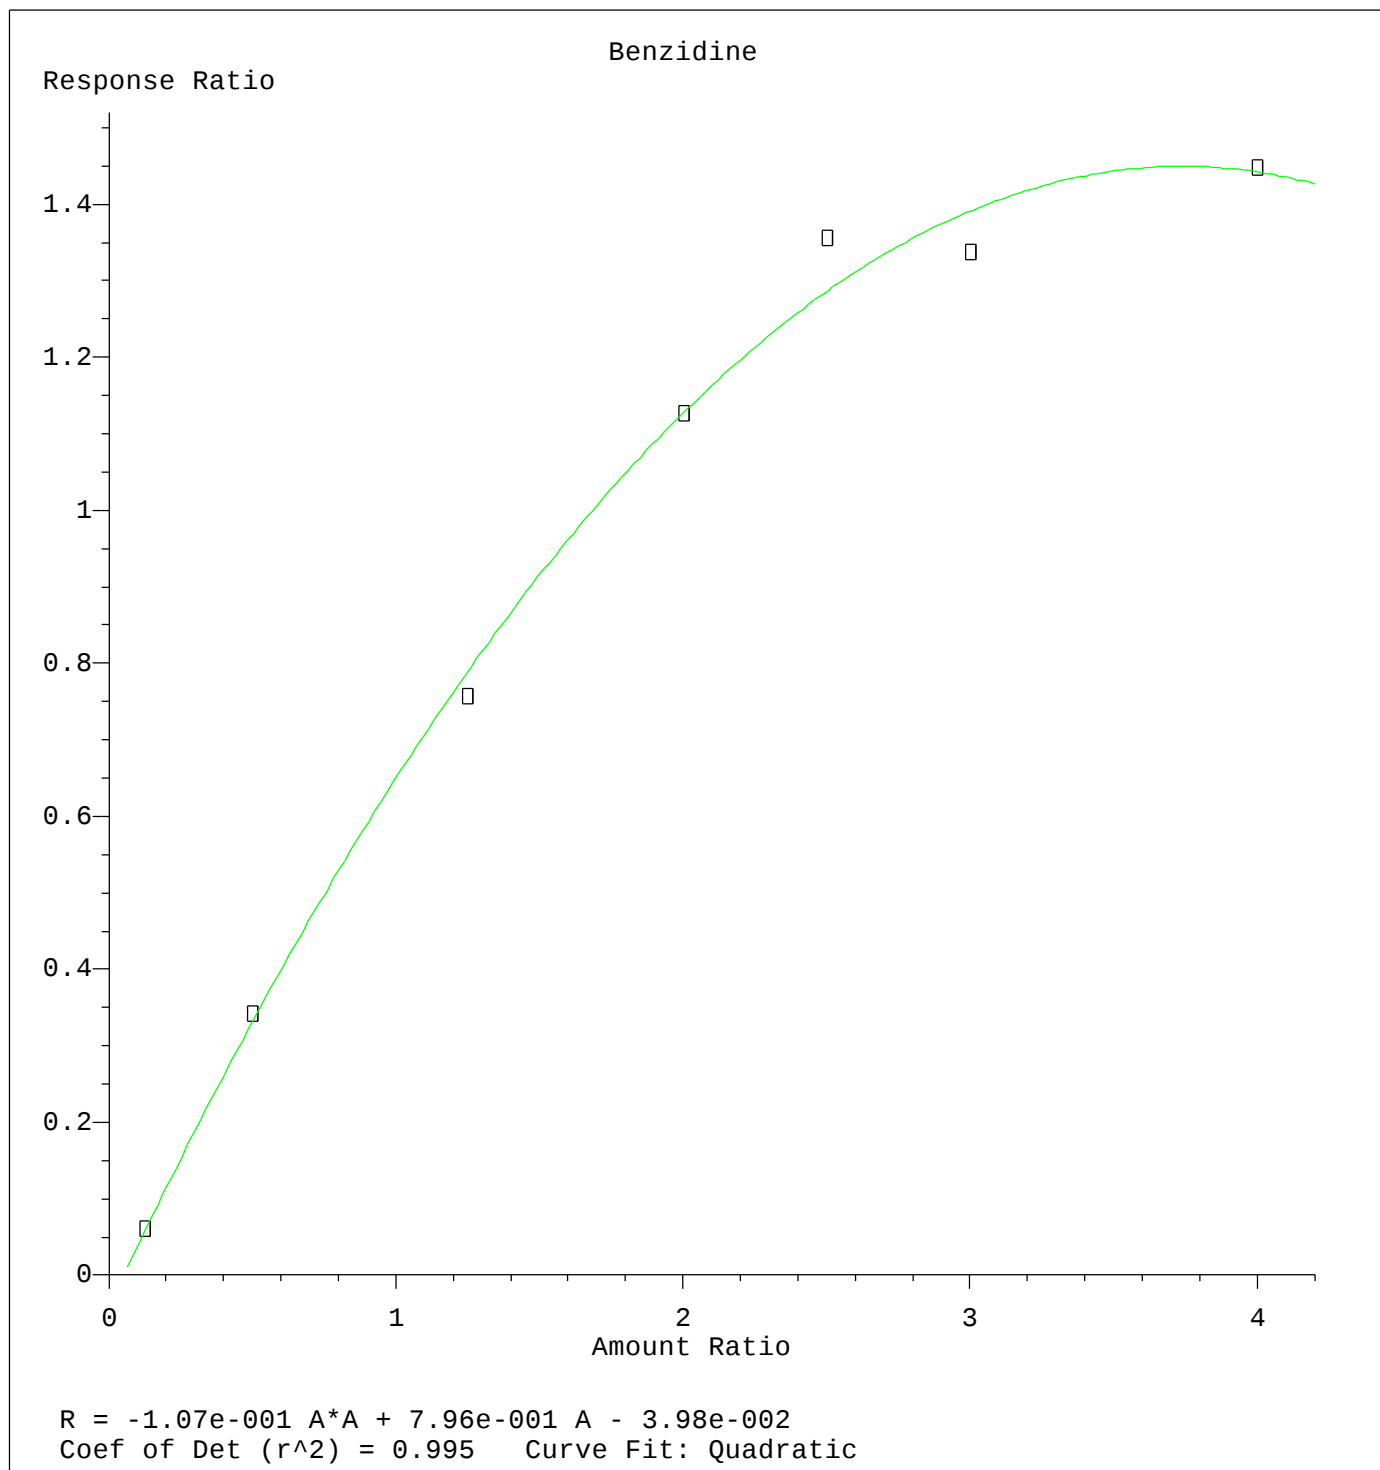

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Calibration Table Last Updated: Tue May 17 16:55:01 2016