
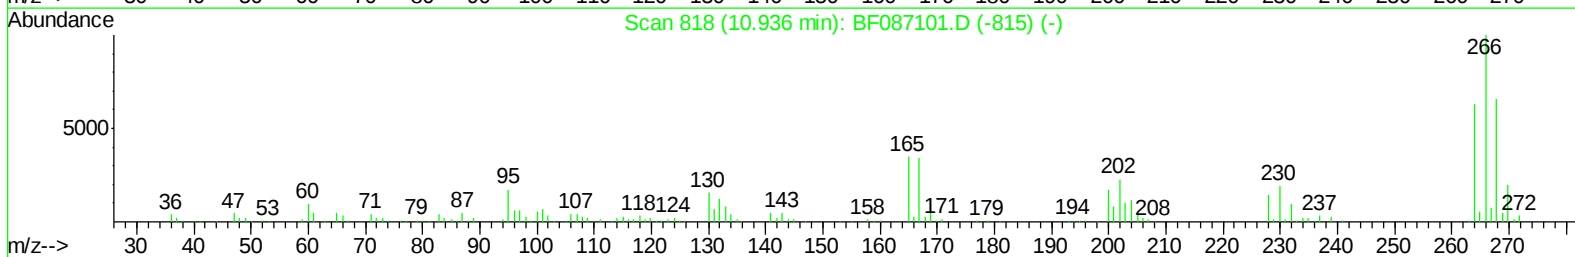
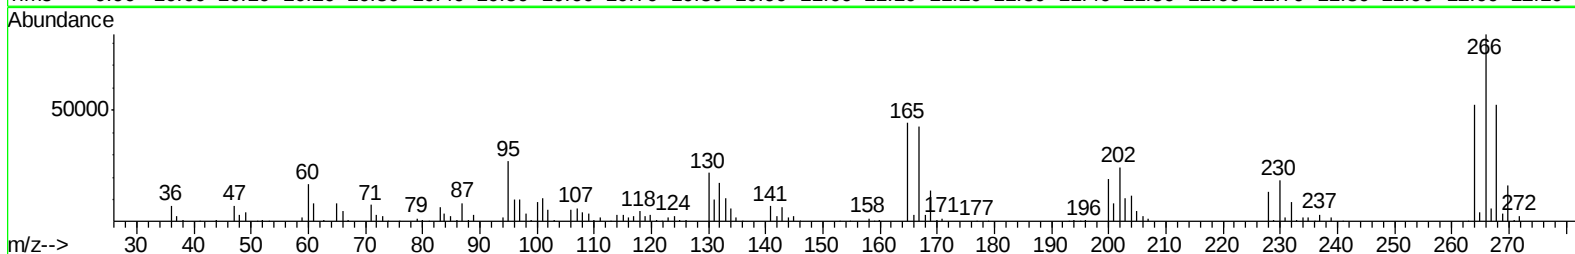


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051716\
Data File : BF087096.D
Acq On : 17 May 2016 11:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 18:55:37 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 16:55:01 2016
Response via : Initial Calibration

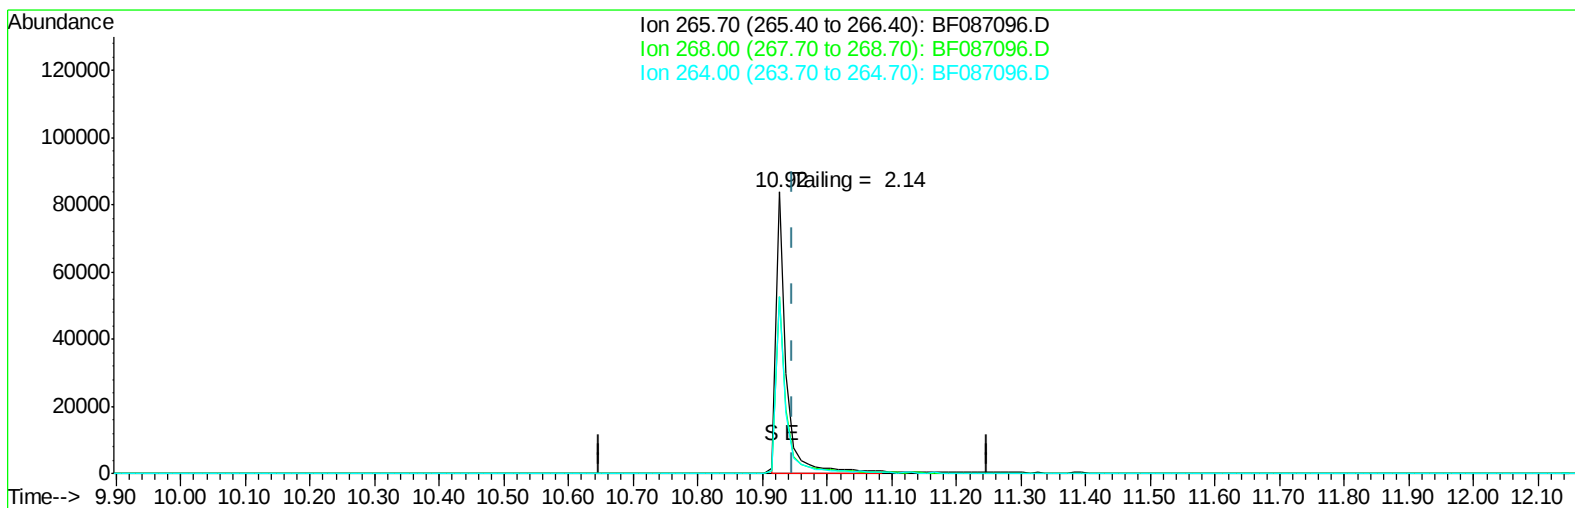

TIC: BF087096.D

(69) Pentachlorophenol (C)




10.925min (-0.023) 0.00ng

response 99192

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.62
264.00	66.10	62.82
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051716\
Data File : BF087096.D
Acq On : 17 May 2016 11:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 18:55:37 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 16:55:01 2016
Response via : Initial Calibration

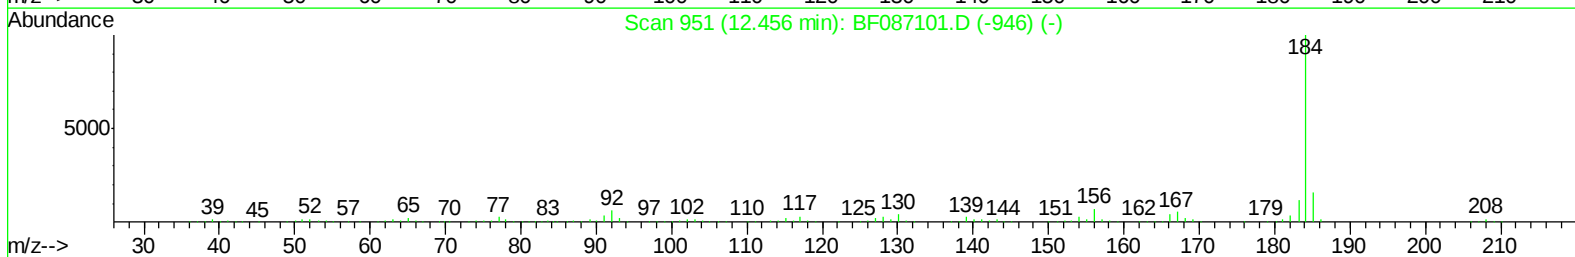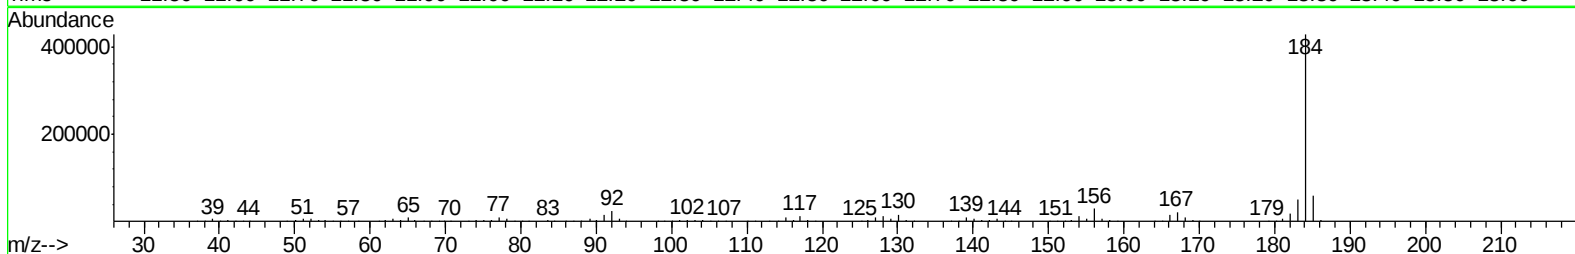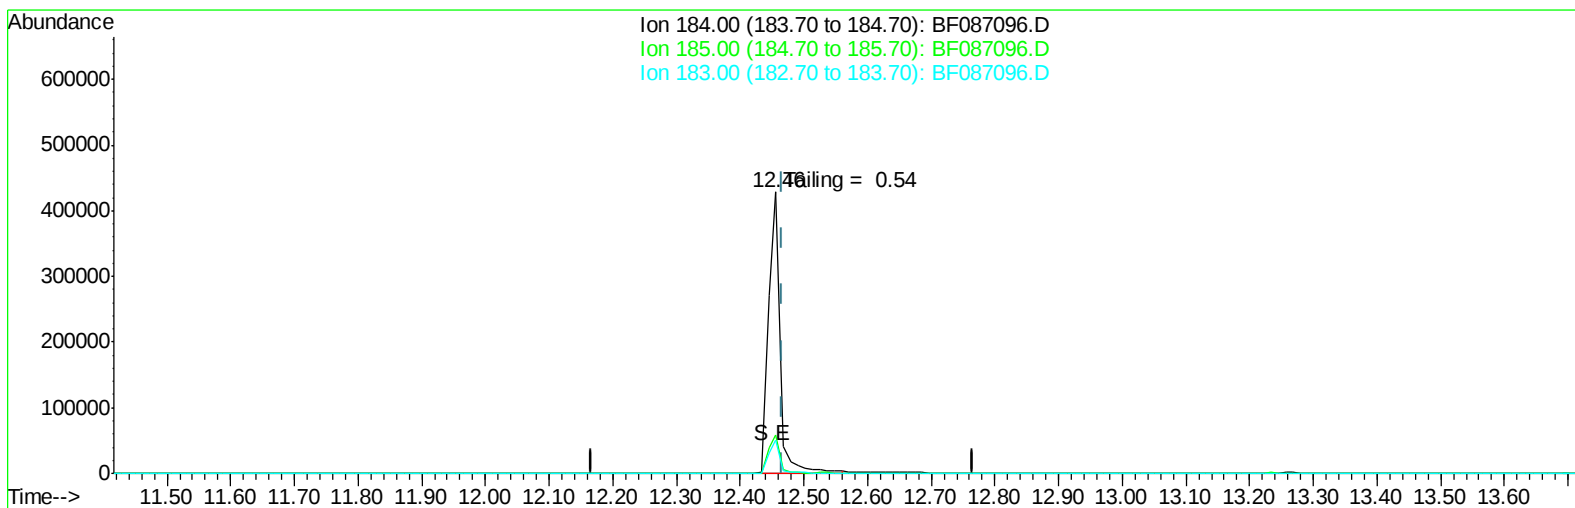

TIC: BF087096.D

(76) Benzidine

12.457min (-0.010) 0.00ng

response 565663

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	13.58#
183.00	12.20	12.06
0.00	0.00	0.00