


Data Path : Z:\HPCHEM1\BNA F\Data\BF051716\
 Data File : BF087096.D
 Acq On : 17 May 2016 11:40
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 17 16:55:01 2016

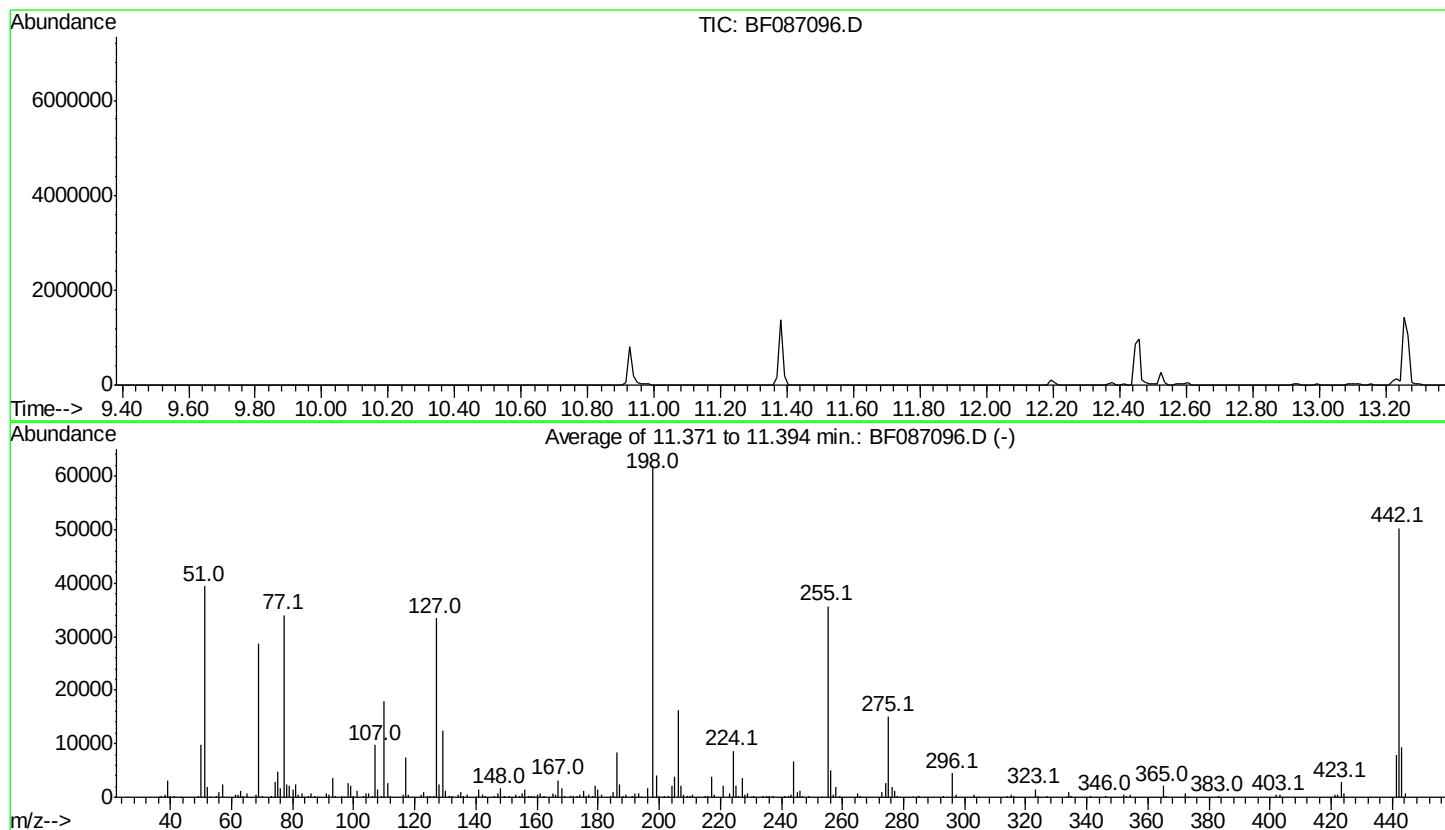

AutoFind: Scans 856, 857, 858; Background Corrected with Scan 853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.7	39436	PASS
68	69	0.00	2	2.0	566	PASS
69	198	0.00	100	46.3	28657	PASS
70	69	0.00	2	0.5	136	PASS
127	198	10	80	54.0	33441	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61949	PASS
199	198	5	9	6.7	4135	PASS
275	198	10	60	24.3	15049	PASS
365	198	1	100	3.4	2131	PASS
441	442	0.01	24	15.9	7995	PASS
442	198	50	100	81.1	50261	PASS
443	442	15	24	18.7	9397	PASS