


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051716\
 Data File : BF087117.D
 Acq On : 17 May 2016 22:27
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 17 16:55:01 2016

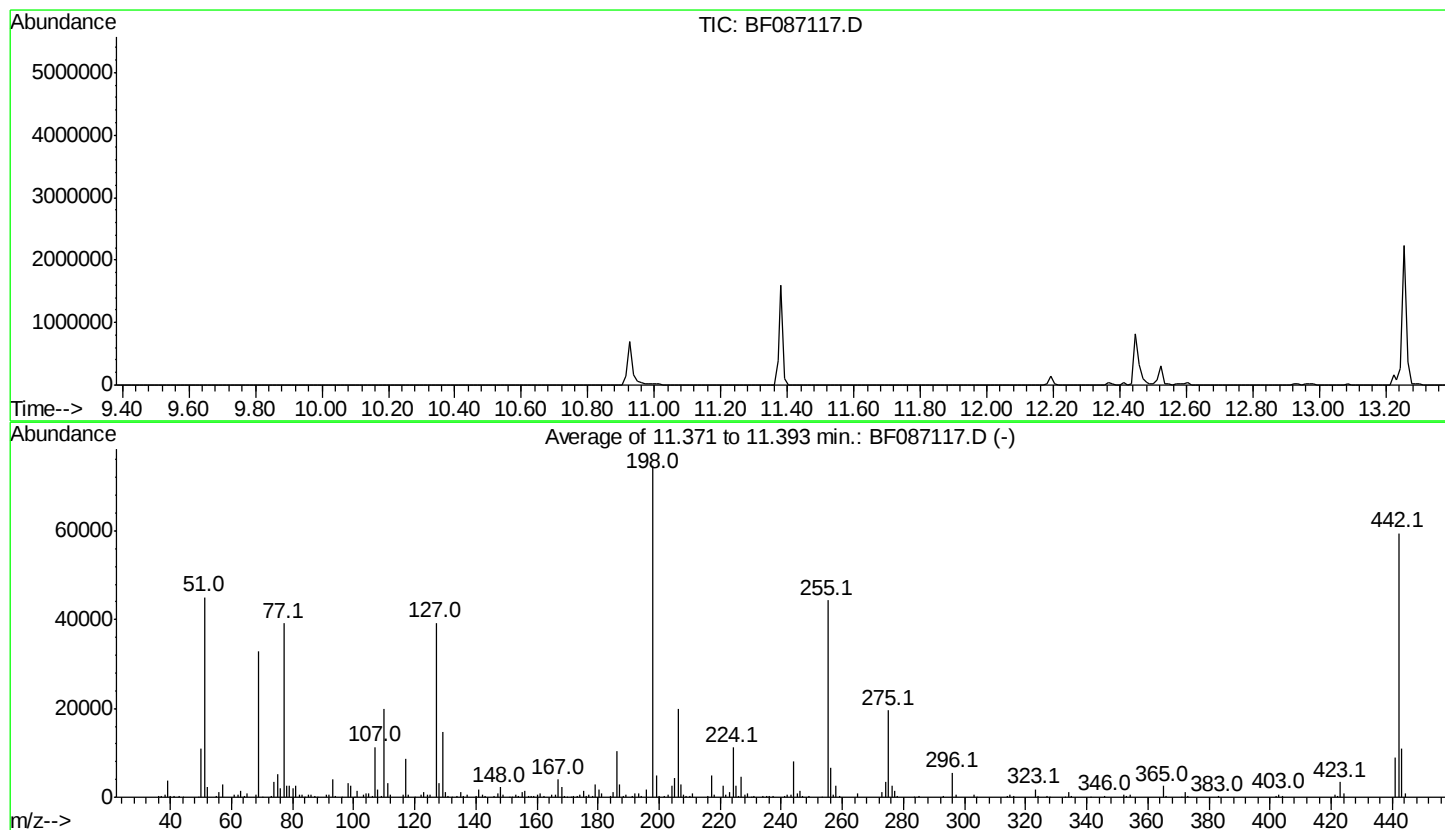

AutoFind: Scans 856, 857, 858; Background Corrected with Scan 852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.3	45041	PASS
68	69	0.00	2	1.6	533	PASS
69	198	0.00	100	43.8	32753	PASS
70	69	0.00	2	0.4	119	PASS
127	198	10	80	52.7	39334	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74705	PASS
199	198	5	9	6.8	5049	PASS
275	198	10	60	26.2	19546	PASS
365	198	1	100	3.5	2582	PASS
441	442	0.01	24	15.3	9075	PASS
442	198	50	100	79.6	59467	PASS
443	442	15	24	18.5	10978	PASS