

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051717\
 Data File : BF095203.D
 Acq On : 18 May 2017 00:57
 Operator : SJ/MA
 Sample : I3172-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: May 18 04:14:03 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 17:24:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	92446	20.00	ng	0.04
21) Naphthalene-d8	9.79	136	368715	20.00	ng	0.04
38) Acenaphthene-d10	12.62	164	164089	20.00	ng	0.04
63) Phenanthrene-d10	15.02	188	261780	20.00	ng	0.04
75) Chrysene-d12	18.69	240	175635	20.00	ng	0.04
86) Perylene-d12	20.37	264	173137	20.00	ng	0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.74	112	791258	142.70	ng	0.06
7) Phenol-d6	7.32	99	1035435	155.63	ng	0.04
23) Nitrobenzene-d5	8.67	82	588525	100.65	ng	0.04
41) 2,4,6-Tribromophenol	13.92	330	176798	131.56	ng	0.04
44) 2-Fluorobiphenyl	11.56	172	1031872	90.51	ng	0.03
78) Terphenyl-d14	17.34	244	649490	81.45	ng	0.03
Target Compounds						Qvalue
10) Phenol	7.34	94	27453	3.92	ng	84
15) Benzyl Alcohol	8.01	79	8568	2.00	ng	# 47
19) n-Nitroso-di-n-propylamine	8.67	70	74246	16.50	ng	# 75
49) Dimethylphthalate	12.25	163	192060	14.26	ng	99
51) Acenaphthene	12.67	154	42004	4.02	ng	98
54) Dibenzofuran	12.97	168	42522	2.94	ng	# 96
55) 4-Nitrophenol	12.97	139	14785	8.35	ng	# 25
57) Fluorene	13.52	166	76188	6.07	ng	99
70) Phenanthrene	15.06	178	857177	56.99	ng	98
71) Anthracene	15.14	178	314593	20.48	ng	97
72) Carbazole	15.44	167	28064	2.01	ng	93
74) Fluoranthene	16.81	202	1287134	83.42	ng	99
77) Pvrene	17.11	202	1115985	84.96	ng	97
80) Benzo(a)anthracene	18.68	228	540372	52.86	ng	100
82) Chrysene	18.73	228	469698	47.52	ng	97
85) Indeno(1,2,3-cd)pyrene	21.70	276	164226	20.46	ng	91
87) Benzo(b)fluoranthene	19.97	252	789772	73.82	ng	# 97
88) Benzo(k)fluoranthene	19.97	252	789772	76.53	ng	99
89) Benzo(a)pvrene	20.31	252	398813	40.40	ng	97
90) Dibenzo(a,h)anthracene	21.53	278	27924	3.42	ng	94
91) Benzo(g,h,i)perylene	22.09	276	159564	19.94	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051717\
Data File : BF095203.D
Acq On : 18 May 2017 00:57
Operator : SJ/MA
Sample : I3172-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: May 18 04:14:03 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

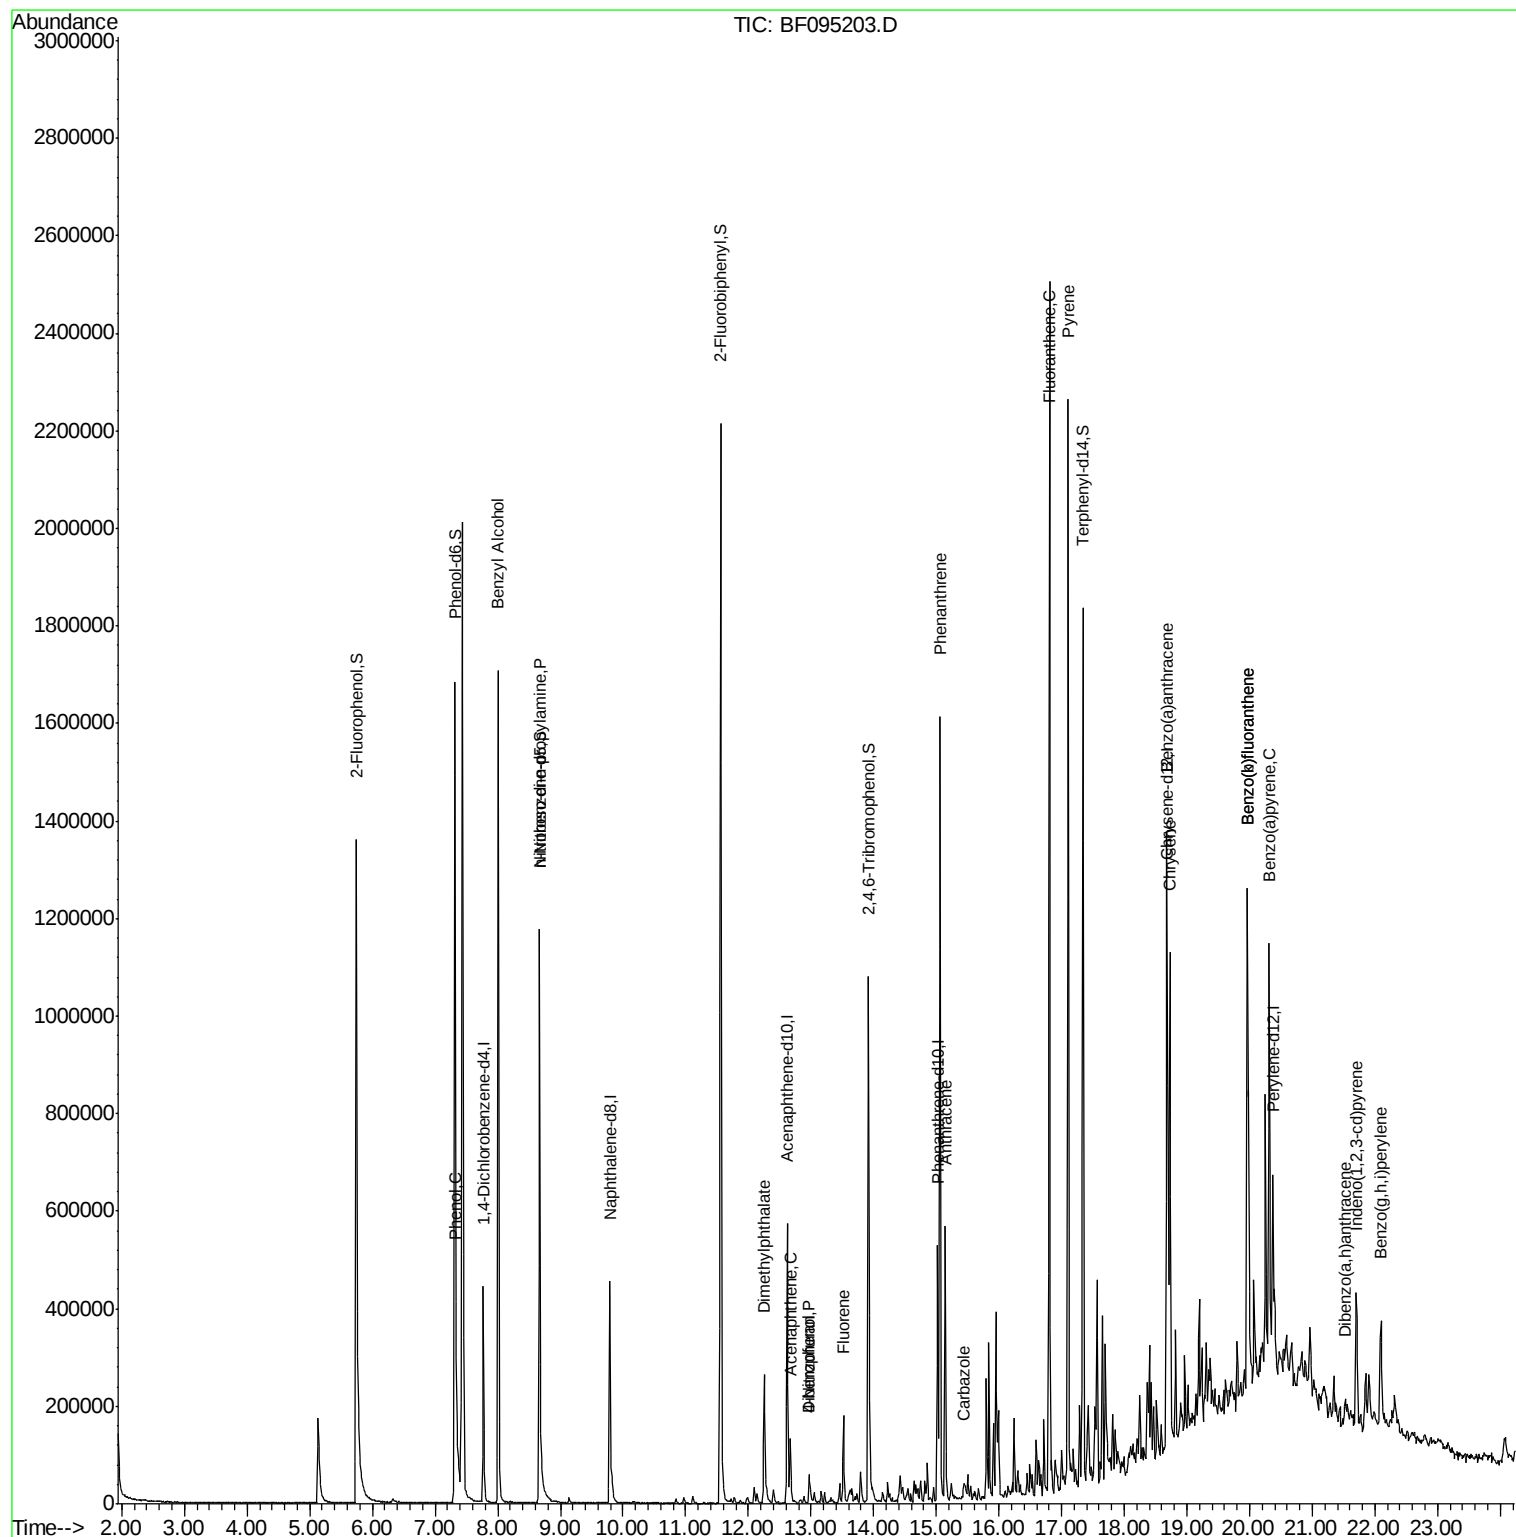

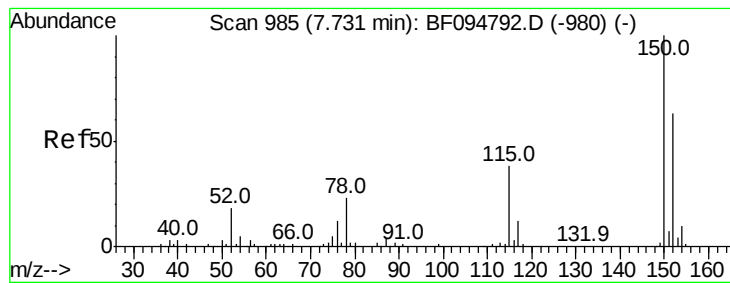


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.77 min Scan# 992
 Delta R.T. 0.04 min
 Lab File: BF095203.D
 Acq: 18 May 2017 00:57

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:152 Resp: 92446
 Ion Ratio Lower Upper
 152 100
 150 160.9 126.2 189.2
 115 61.2 52.2 78.2

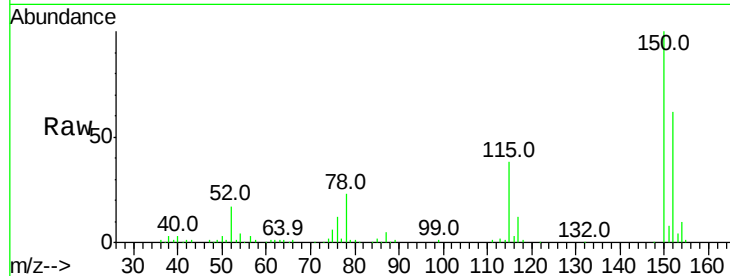


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

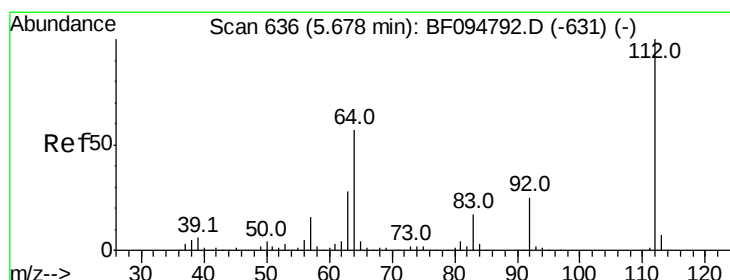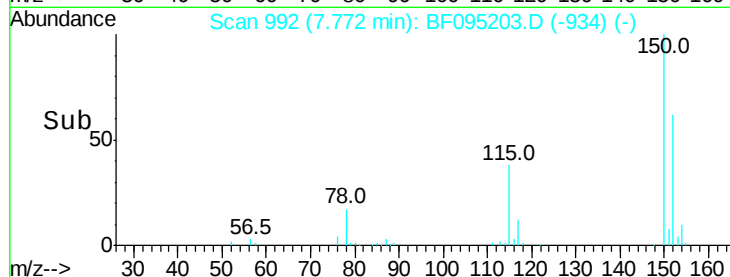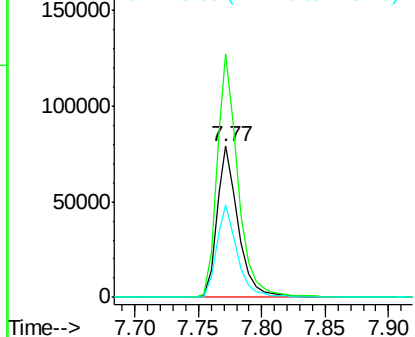



#5

2-Fluorophenol
 Concen: 142.70 ng
 RT: 5.74 min Scan# 647
 Delta R.T. 0.06 min
 Lab File: BF095203.D
 Acq: 18 May 2017 00:57

Tgt Ion:112 Resp: 791258
 Ion Ratio Lower Upper
 112 100
 64 53.6 46.0 69.0
 63 25.7 23.4 35.0

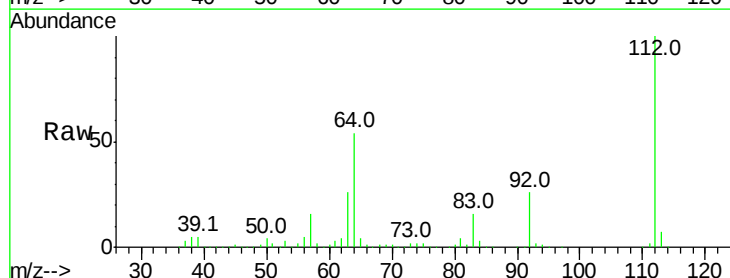

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

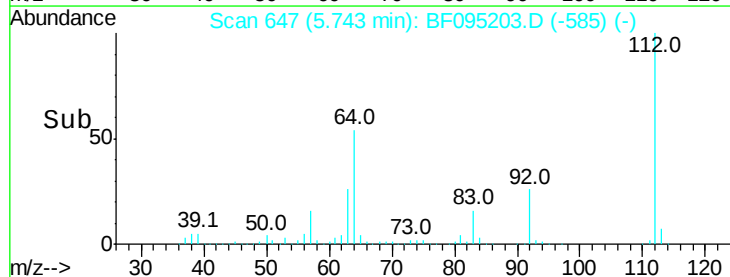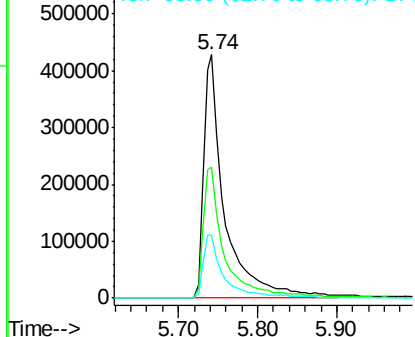



#7

Phenol-d6

Concen: 155.63 ng

RT: 7.32 min Scan# 915

Delta R.T. 0.04 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57


Instrument :

BNA_F

ClientSampled :

Tot Ion: 99 Resp: 1035435




Ion	Ratio	Lower	Upper
99	100		
42	15.4	13.5	20.3
71	31.8	24.5	36.7



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

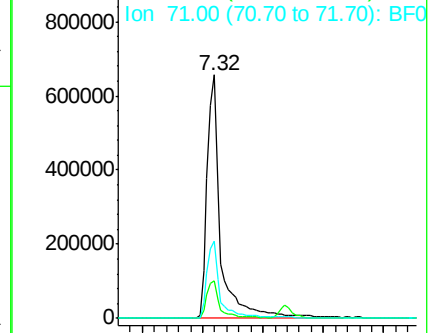

#10

Phenol

Concen: 3.92 ng

RT: 7.34 min Scan# 918


Delta R.T. 0.04 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57

Tgt Ion: 94 Resp: 27453



Ion	Ratio	Lower	Upper
94	100		
65	25.5	9.9	49.9
66	56.8	23.1	63.1




Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

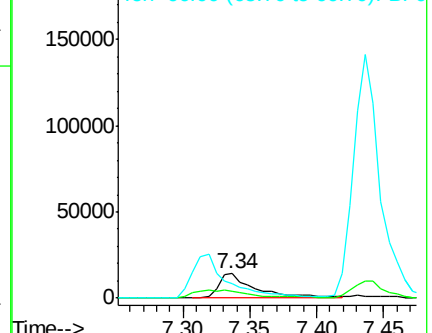



#15

Benzyl Alcohol

Concen: 2.00 ng

RT: 8.01 min Scan# 1032

Delta R.T. -0.01 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57

Instrument :

BNA_F

ClientSampled :





Tot Ion: 79 Resp: 8568

Ion Ratio Lower Upper

79 100

108 33.7 63.4 95.0#

77 104.1 49.2 73.8#

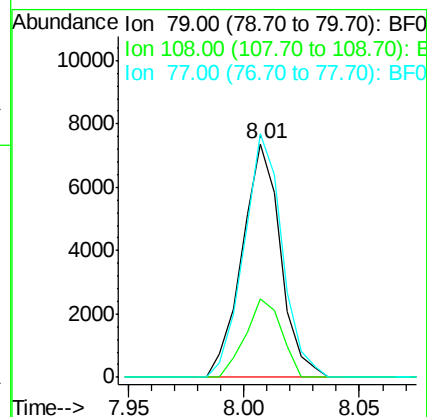

#19

n-Nitroso-di-n-propylamine

Concen: 16.50 ng

RT: 8.67 min Scan# 1145

Delta R.T. 0.23 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57

Tgt Ion: 70 Resp: 74246




Ion Ratio Lower Upper


70 100

42 43.6 47.2 70.8#

101 0.0 7.2 10.8#

130 2.1 15.9 23.9#

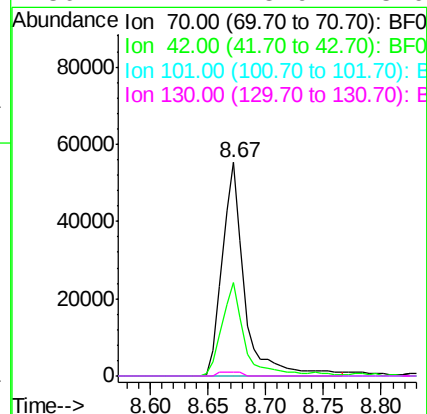



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.79 min Scan# 1335

Delta R.T. 0.04 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 368715



Ion Ratio Lower Upper

136 100

137 10.0 8.5 12.7

54 6.6 4.9 7.3

68 5.4 4.1 6.1





Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

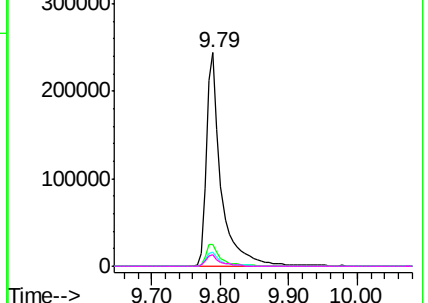

#23

Nitrobenzene-d5

Concen: 100.65 ng

RT: 8.67 min Scan# 1145

Delta R.T. 0.04 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57



Tgt Ion: 82 Resp: 588525

Ion Ratio Lower Upper

82 100

128 46.9 34.0 51.0


54 46.8 42.2 63.2




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

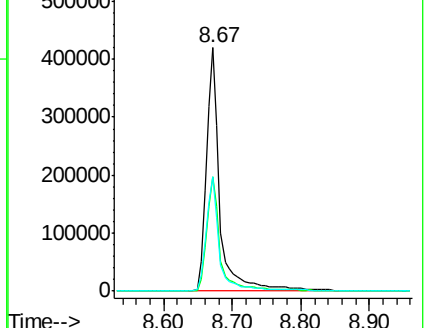



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 12.62 min Scan# 1816

Delta R.T. 0.04 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 164089

Ion Ratio Lower Upper

164 100

162 103.5 82.6 123.8




160 45.1 36.2 54.2



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

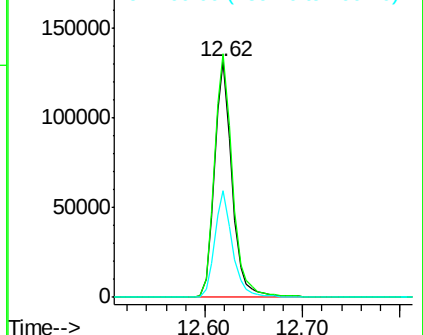

#41

2,4,6-Tribromophenol

Concen: 131.56 ng

RT: 13.92 min Scan# 2037

Delta R.T. 0.04 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57


Tgt Ion:330 Resp: 176798

Ion Ratio Lower Upper

330 100

332 97.4 76.6 115.0



141 40.4 31.4 47.2




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

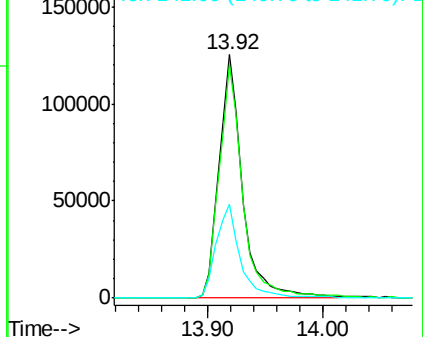




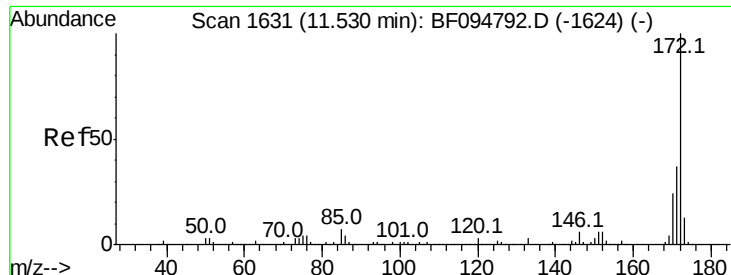


#44
 2-Fluorobiphenyl
 Concen: 90.51 ng
 RT: 11.56 min Scan# 1636
 Delta R.T. 0.03 min
 Lab File: BF095203.D
 Acq: 18 May 2017 00:57

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:172 Resp: 1031872




Ion	Ratio	Lower	Upper
172	100		
171	36.3	29.6	44.4
170	23.1	19.8	29.8

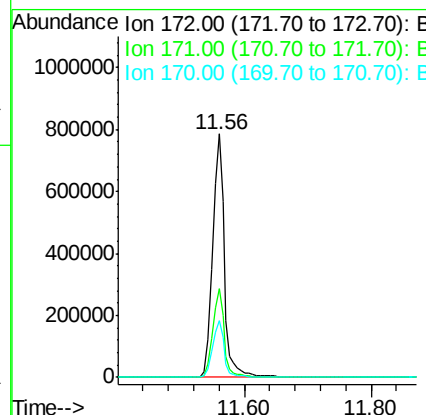


#49
 Dimethylphthalate
 Concen: 14.26 ng
 RT: 12.25 min Scan# 1754
 Delta R.T. 0.02 min
 Lab File: BF095203.D
 Acq: 18 May 2017 00:57

Tgt Ion:163 Resp: 192060

Ion	Ratio	Lower	Upper
163	100		
194	3.4	2.6	4.0
164	10.2	8.4	12.6

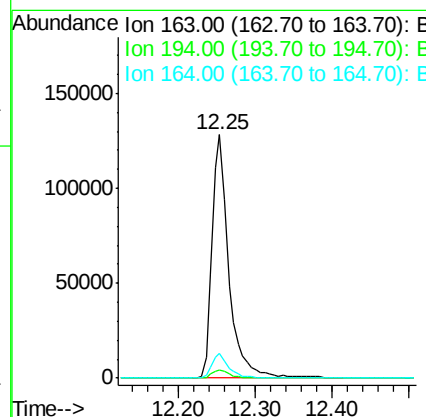



#51

Acenaphthene

Concen: 4.02 ng

RT: 12.67 min Scan# 1825

Delta R.T. 0.03 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57

Instrument :

BNA_F

ClientSampleId :


Tot Ion:154 Resp: 42004

Ion Ratio Lower Upper

154 100

153 110.8 90.5 135.7




152 54.9 43.6 65.4



Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

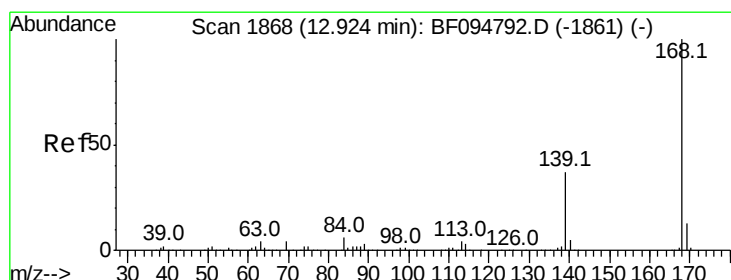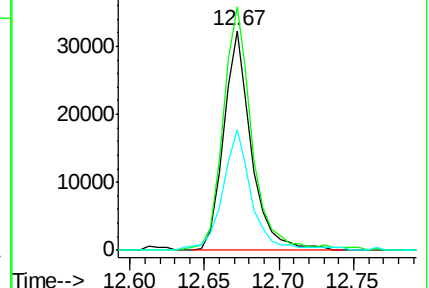

#54

Dibenzofuran

Concen: 2.94 ng

RT: 12.97 min Scan# 1876

Delta R.T. 0.05 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57


Tgt Ion:168 Resp: 42522

Ion Ratio Lower Upper

168 100

139 36.3 30.6 45.8



169 16.3 10.8 16.2#

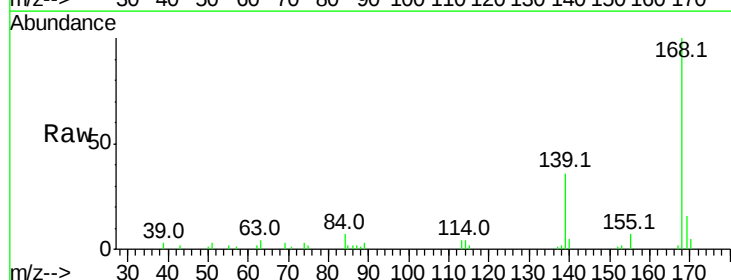


Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E

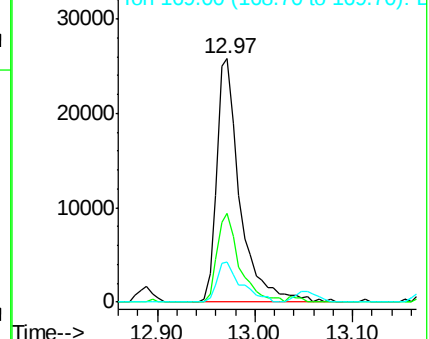







#55
4-Nitrophenol
Concen: 8.35 ng
RT: 12.97 min Scan# 1876
Delta R.T. 0.01 min
Lab File: BF095203.D
Acq: 18 May 2017 00:57

Instrument :
BNA_F
ClientSampleId :

Tot Ion:139 Resp: 14785
Ion Ratio Lower Upper
139 100
109 0.0 34.1 74.1#
65 0.0 31.4 71.4#




Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): BF0


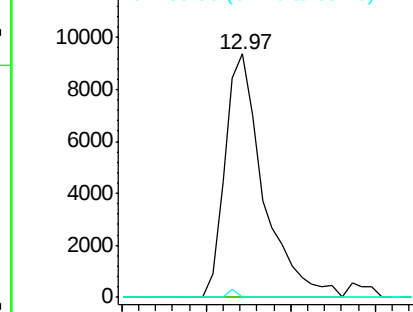



#57
Fluorene
Concen: 6.07 ng
RT: 13.52 min Scan# 1969
Delta R.T. 0.04 min
Lab File: BF095203.D
Acq: 18 May 2017 00:57

Tgt Ion:166 Resp: 76188
Ion Ratio Lower Upper
166 100
165 97.8 78.8 118.2
167 13.1 10.6 16.0



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

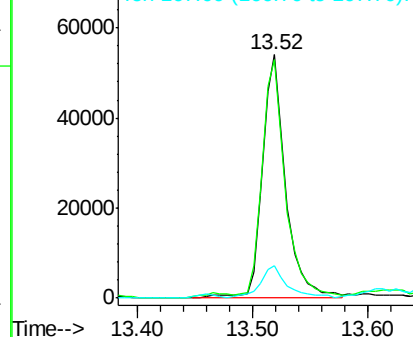


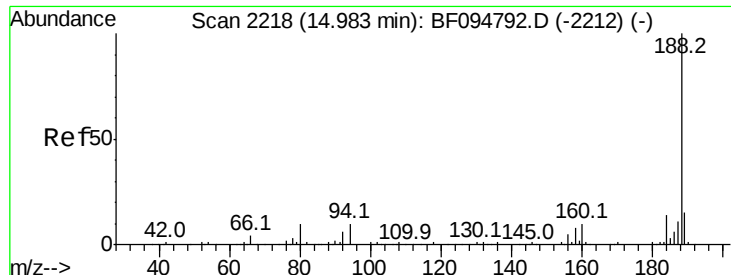




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 15.02 min Scan# 2224
 Delta R.T. 0.04 min
 Lab File: BF095203.D
 Acq: 18 May 2017 00:57

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:188 Resp: 261780
 Ion Ratio Lower Upper
 188 100
 94 10.1 9.4 14.2
 80 12.0 10.2 15.2




Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

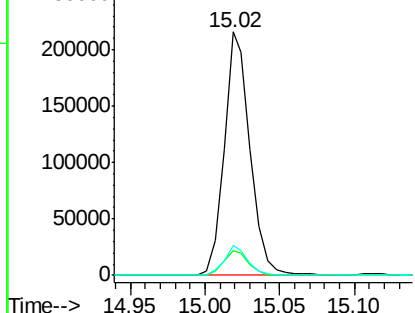




#70
 Phenanthrene
 Concen: 56.99 ng
 RT: 15.06 min Scan# 2231
 Delta R.T. 0.04 min
 Lab File: BF095203.D
 Acq: 18 May 2017 00:57

Tgt Ion:178 Resp: 857177
 Ion Ratio Lower Upper
 178 100
 176 19.0 16.2 24.4
 179 15.6 12.6 19.0



Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E

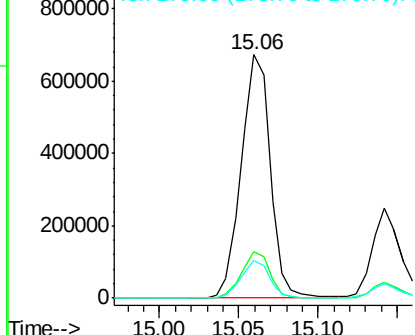







#71
 Anthracene
 Concen: 20.48 ng
 RT: 15.14 min Scan# 2245
 Delta R.T. 0.04 min
 Lab File: BF095203.D
 Acq: 18 May 2017 00:57

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:178 Resp: 314593
 Ion Ratio Lower Upper
 178 100
 176 17.3 15.8 23.8
 179 15.9 12.7 19.1




Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E

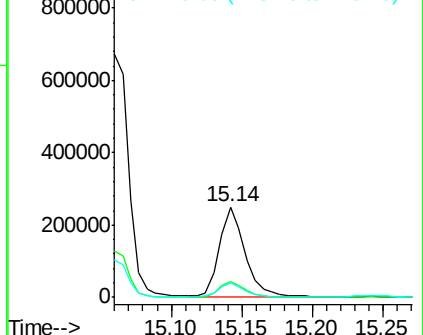




#72
 Carbazole
 Concen: 2.01 ng
 RT: 15.44 min Scan# 2295
 Delta R.T. 0.05 min
 Lab File: BF095203.D
 Acq: 18 May 2017 00:57

Tgt Ion:167 Resp: 28064
 Ion Ratio Lower Upper
 167 100
 166 18.8 18.1 27.1
 139 12.3 11.7 17.5



Abundance Ion 167.00 (166.70 to 167.70): E
 Ion 166.00 (165.70 to 166.70): E
 Ion 139.00 (138.70 to 139.70): E

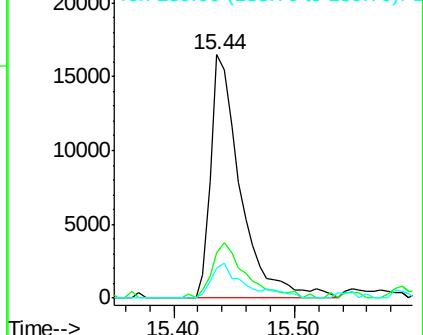







#74
 Fluoranthene
 Concen: 83.42 ng
 RT: 16.81 min Scan# 2528
 Delta R.T. 0.04 min
 Lab File: BF095203.D
 Acq: 18 May 2017 00:57

Instrument :
 BNA_F
 ClientSampleID :

Tot Ion:202 Resp: 1287134
 Ion Ratio Lower Upper
 202 100
 101 14.0 0.0 33.2
 203 17.7 0.0 38.1




Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 203.00 (202.70 to 203.70): E


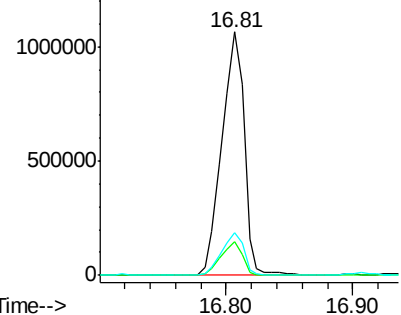



#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 18.69 min Scan# 2849
 Delta R.T. 0.04 min
 Lab File: BF095203.D
 Acq: 18 May 2017 00:57

Tgt Ion:240 Resp: 175635
 Ion Ratio Lower Upper
 240 100
 120 14.1 5.8 8.8#
 236 24.9 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

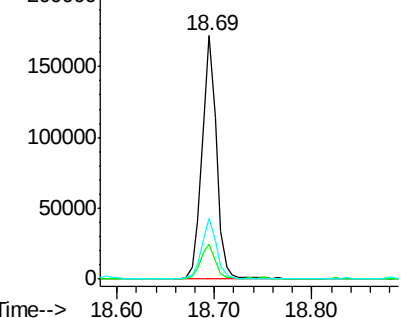



#77

Pvrene

Concen: 84.96 ng

RT: 17.11 min Scan# 2579

Delta R.T. 0.04 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57


Instrument :

BNA_F

ClientSampled :

Tot Ion:202 Resp: 1115985

Ion	Ratio	Lower	Upper
202	100		
200	21.7	17.6	26.4
203	20.3	14.4	21.6






Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

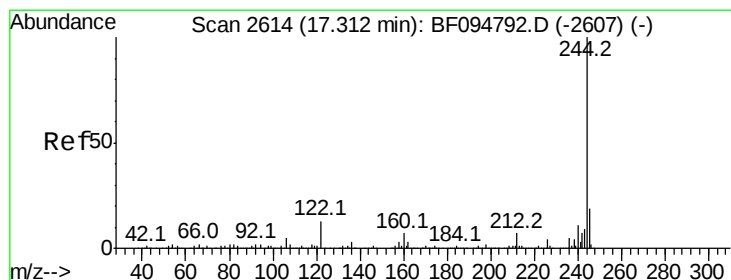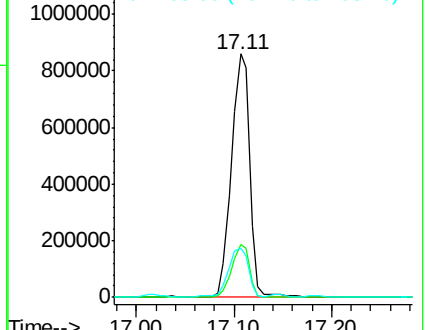

#78

Terphenyl-d14

Concen: 81.45 ng

RT: 17.34 min Scan# 2619


Delta R.T. 0.03 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57

Tgt Ion:244 Resp: 649490

Ion	Ratio	Lower	Upper
244	100		
212	7.2	6.0	9.0
122	14.4	10.3	15.5


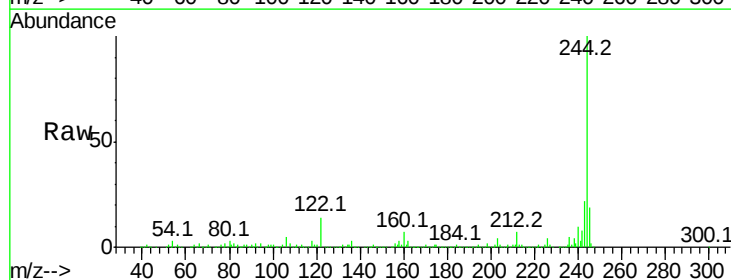



Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E




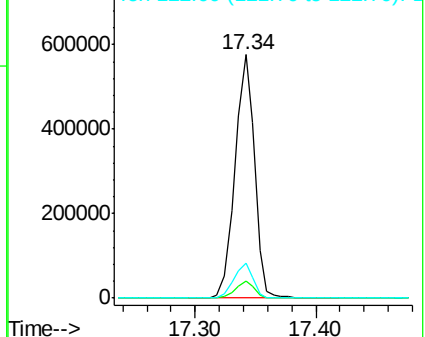




#80
Benzo(a)anthracene
Concen: 52.86 ng
RT: 18.68 min Scan# 2847
Delta R.T. 0.05 min
Lab File: BF095203.D
Acq: 18 May 2017 00:57




Instrument :
BNA_F
ClientSampleId :


Tot Ion:228 Resp: 540372
Ion Ratio Lower Upper
228 100
226 28.2 22.6 33.8
229 20.7 16.3 24.5

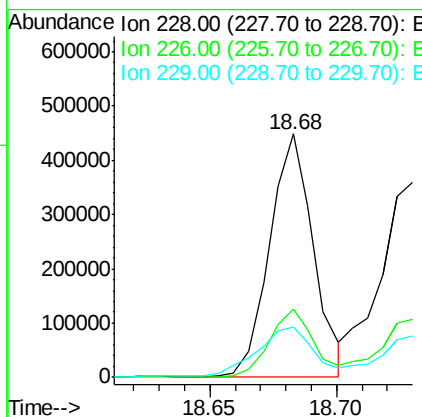

#82
Chrysene
Concen: 47.52 ng
RT: 18.73 min Scan# 2855
Delta R.T. 0.04 min
Lab File: BF095203.D
Acq: 18 May 2017 00:57

Tgt Ion:228 Resp: 469698
Ion Ratio Lower Upper
228 100
226 29.6 24.9 37.3
229 21.1 15.8 23.6

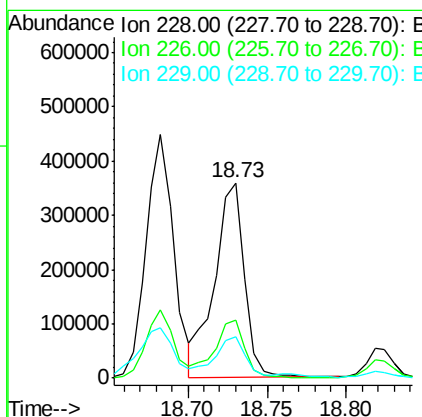







#85
 Indeno(1,2,3-cd)pyrene
 Concen: 20.46 ng
 RT: 21.70 min Scan# 3360
 Delta R.T. 0.09 min
 Lab File: BF095203.D
 Acq: 18 May 2017 00:57

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:276 Resp: 164226
 Ion Ratio Lower Upper
 276 100
 138 28.5 27.8 41.6
 277 22.6 20.2 30.4




Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E

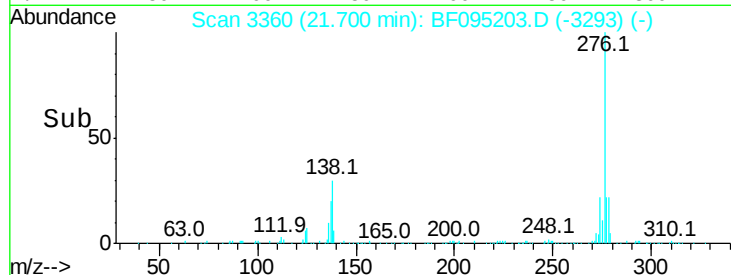
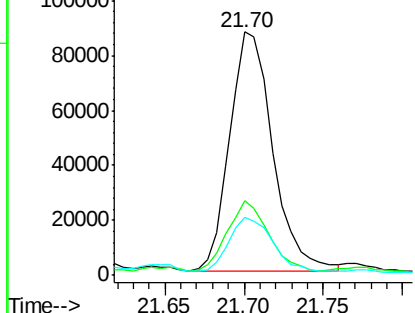



#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 20.37 min Scan# 3134
 Delta R.T. 0.06 min
 Lab File: BF095203.D
 Acq: 18 May 2017 00:57

Tgt Ion:264 Resp: 173137
 Ion Ratio Lower Upper
 264 100
 260 22.8 19.5 29.3
 265 21.7 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E




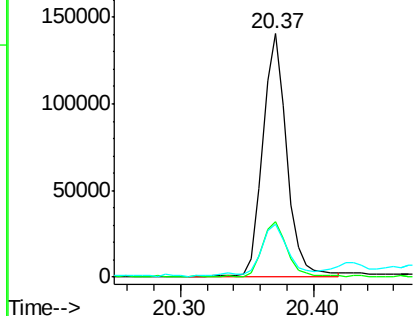




#87
Benzo(b)fluoranthene
Concen: 73.82 ng
RT: 19.97 min Scan# 3065
Delta R.T. 0.05 min
Lab File: BF095203.D
Acq: 18 May 2017 00:57




Instrument :
BNA_F
ClientSampleId :


Tot Ion:252 Resp: 789772
Ion Ratio Lower Upper
252 100
253 22.4 18.1 27.1
125 15.7 9.8 14.8#

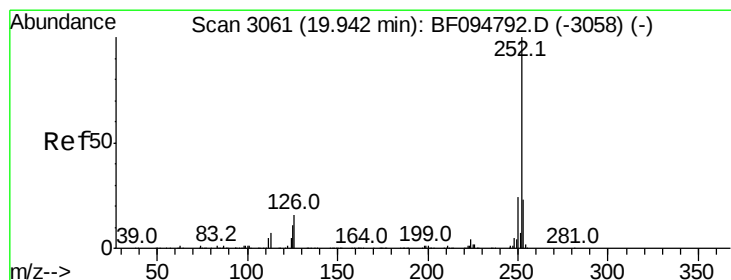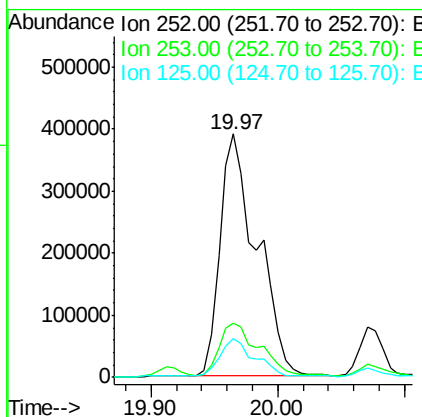

#88
Benzo(k)fluoranthene
Concen: 76.53 ng
RT: 19.97 min Scan# 3065
Delta R.T. 0.02 min
Lab File: BF095203.D
Acq: 18 May 2017 00:57

Tgt Ion:252 Resp: 789772
Ion Ratio Lower Upper
252 100
253 22.4 18.4 27.6
125 15.7 13.1 19.7



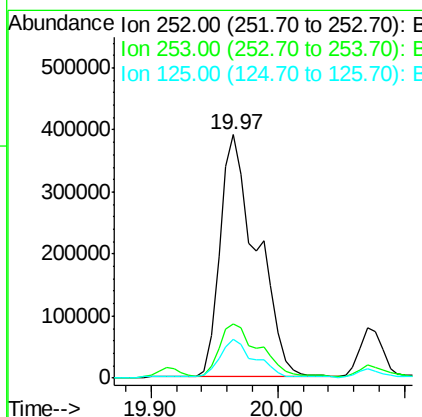
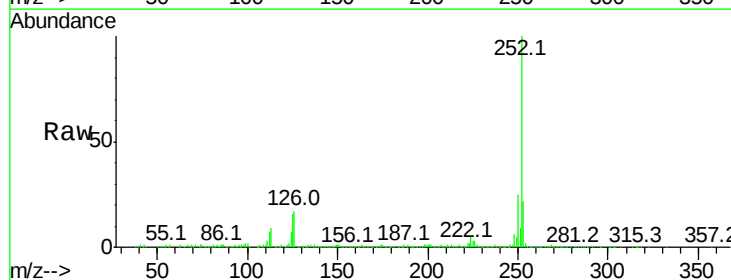




#89
Benzo(a)pyrene
Concen: 40.40 ng
RT: 20.31 min Scan# 3124
Delta R.T. 0.05 min
Lab File: BF095203.D
Acq: 18 May 2017 00:57




Instrument :
BNA_F
ClientSampled :


Tot Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.5	26.3
125	15.8	11.0	16.4

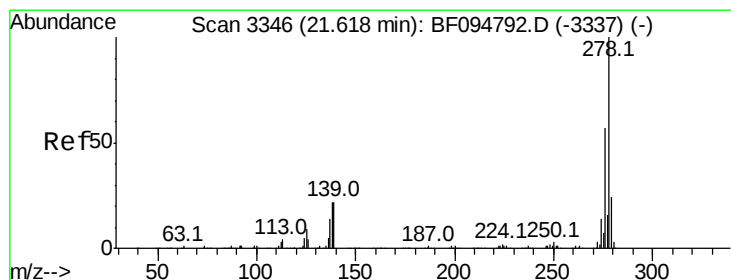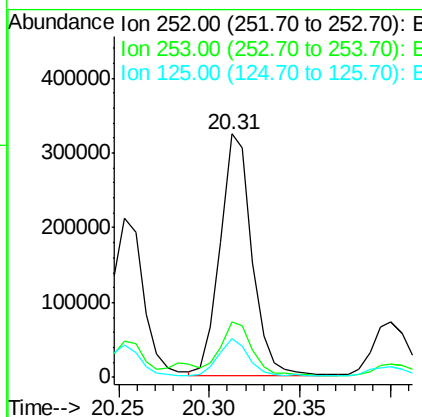

#90
Dibenzo(a,h)anthracene
Concen: 3.42 ng
RT: 21.53 min Scan# 3331
Delta R.T. -0.09 min
Lab File: BF095203.D
Acq: 18 May 2017 00:57

Tgt Ion	Ratio	Lower	Upper
278	100		
139	24.8	16.6	24.8
279	25.6	19.3	28.9

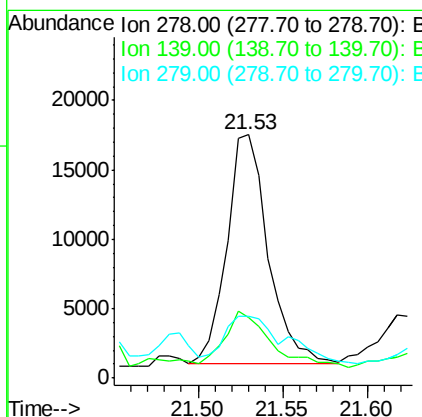

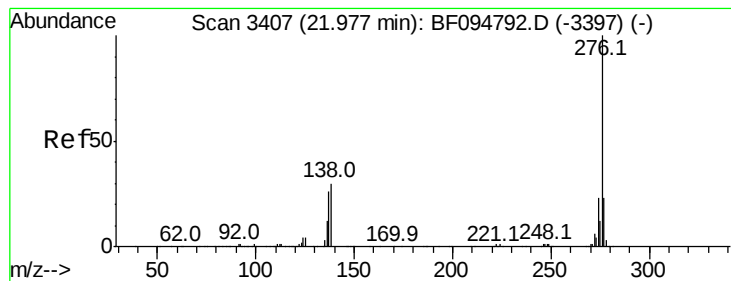

#91

Benzo(a,h,i)perylene

Concen: 19.94 ng

RT: 22.09 min Scan# 3427

Delta R.T. 0.12 min

Lab File: BF095203.D

Acq: 18 May 2017 00:57

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 276 Resp: 159564

Ion Ratio Lower Upper

276 100

277 25.9 18.6 28.0

138 29.1 25.4 38.0

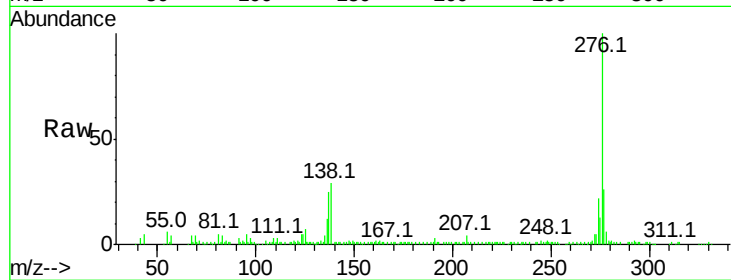

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

