
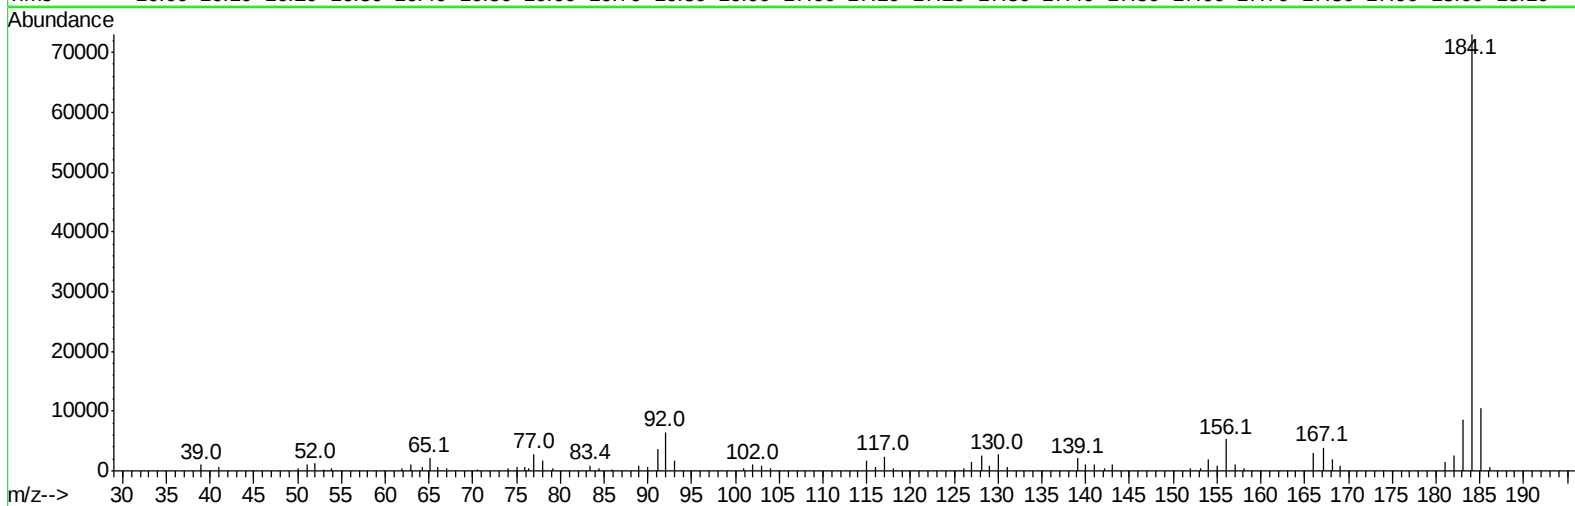


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051717\
Data File : BF095187.D
Acq On : 17 May 2017 16:08
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 08:04:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

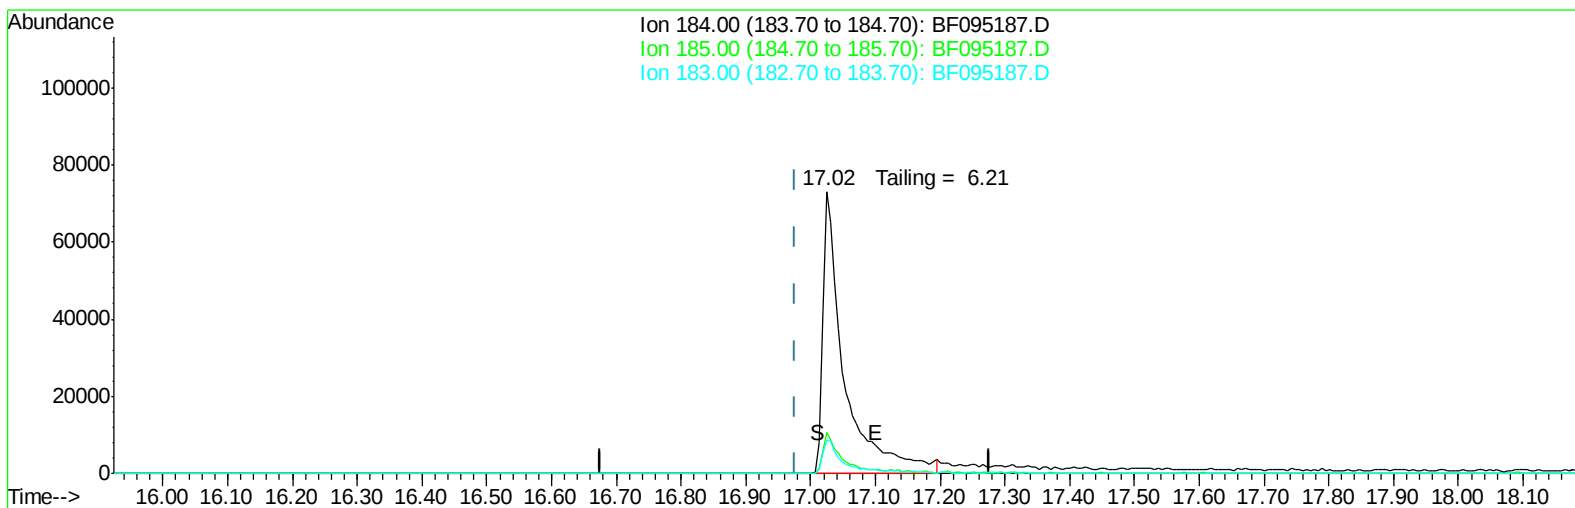

TIC: BF095187.D

(76) Benzidine



17.024min (+0.047) 0.00ng

response 166337

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.43#
183.00	12.20	11.70
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051717\
Data File : BF095187.D
Acq On : 17 May 2017 16:08
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 08:04:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

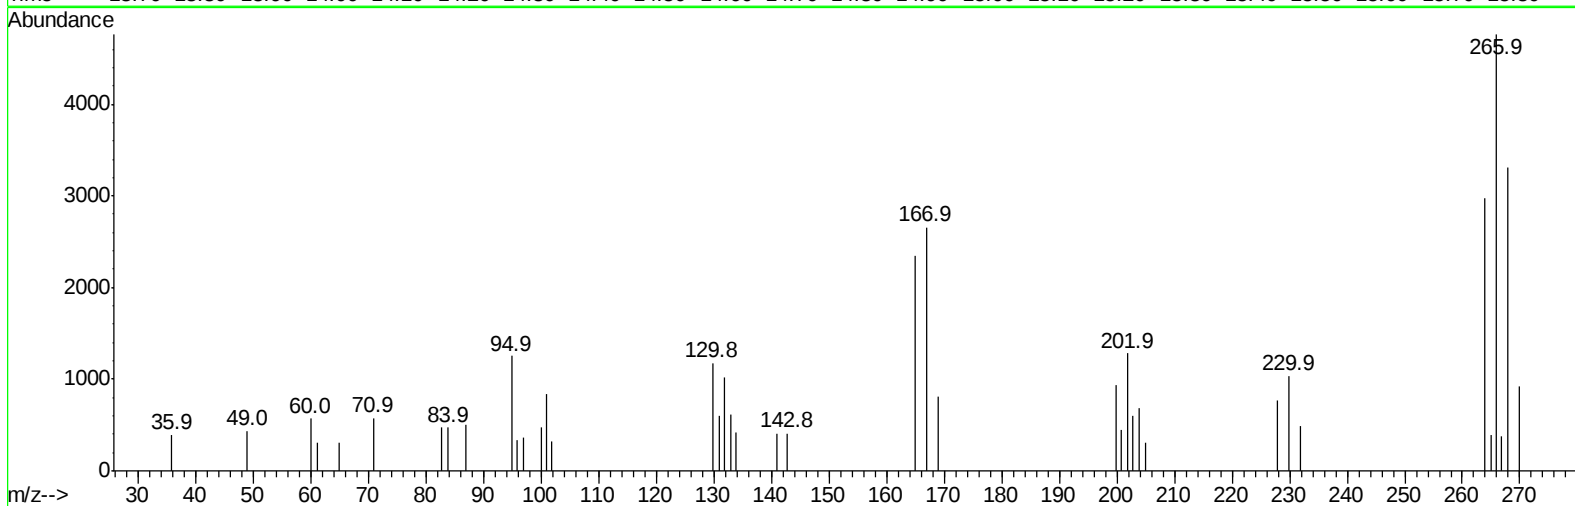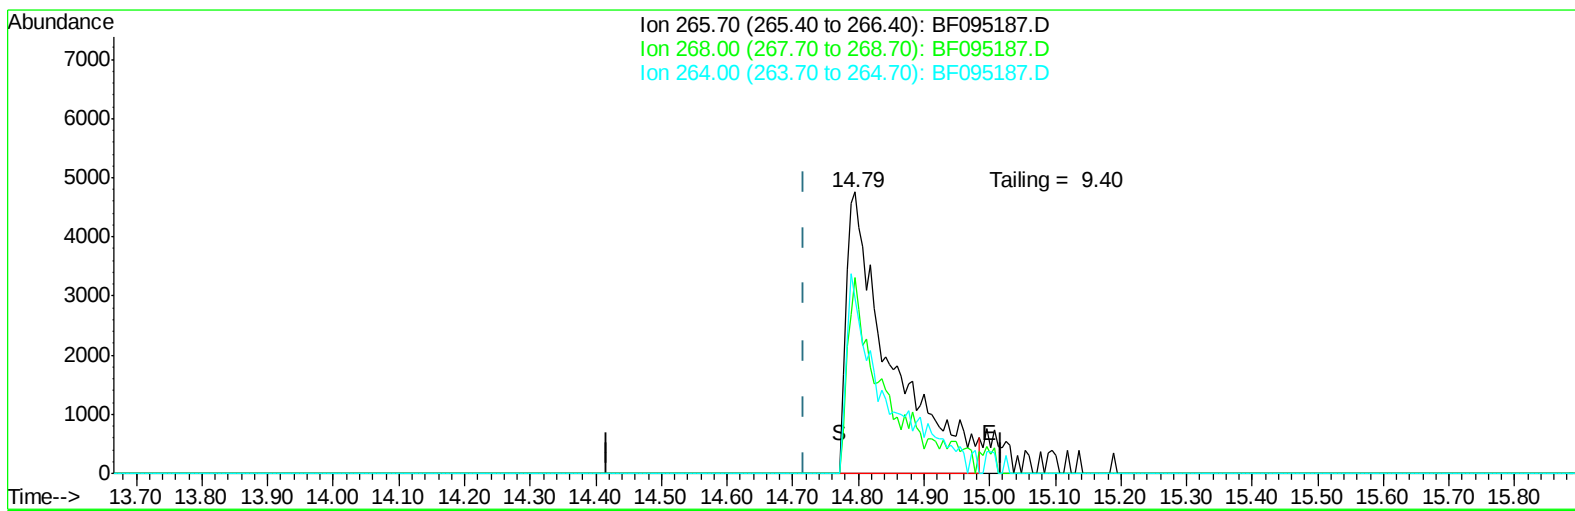

TIC: BF095187.D

(69) Pentachlorophenol (C)

14.795min (+0.077) 0.00ng m

response 22381

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	69.40
264.00	64.60	62.40
0.00	0.00	0.00