
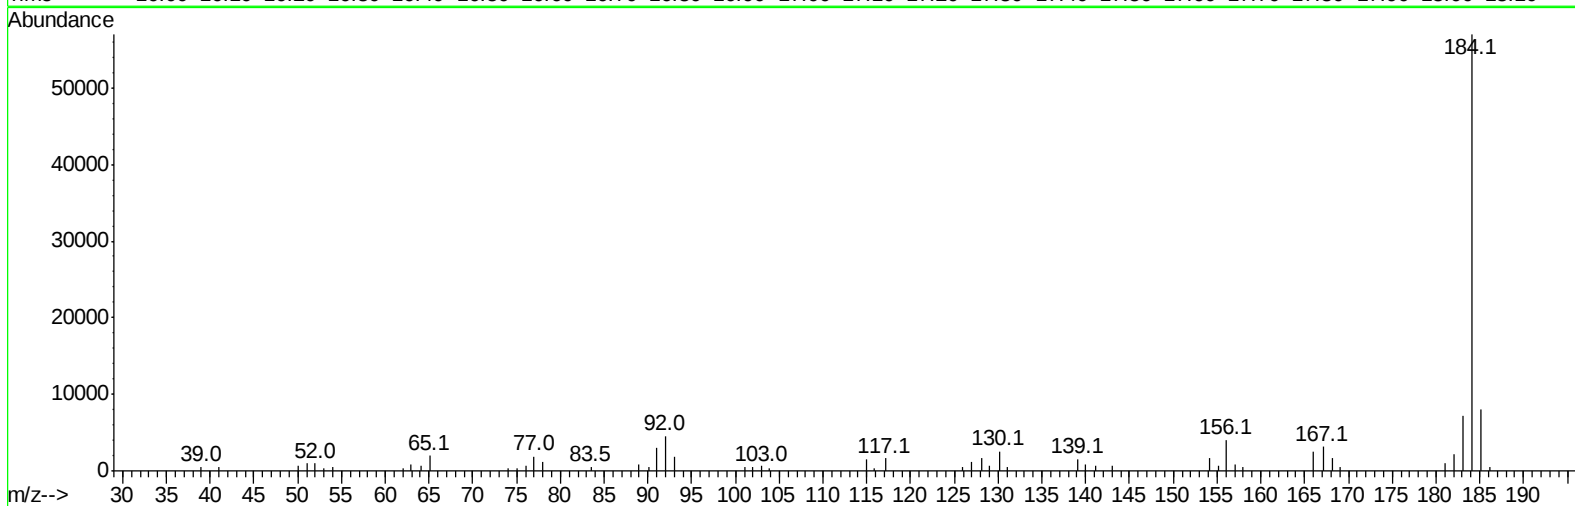


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051717\
Data File : BF095209.D
Acq On : 18 May 2017 4:26
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 08:07:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

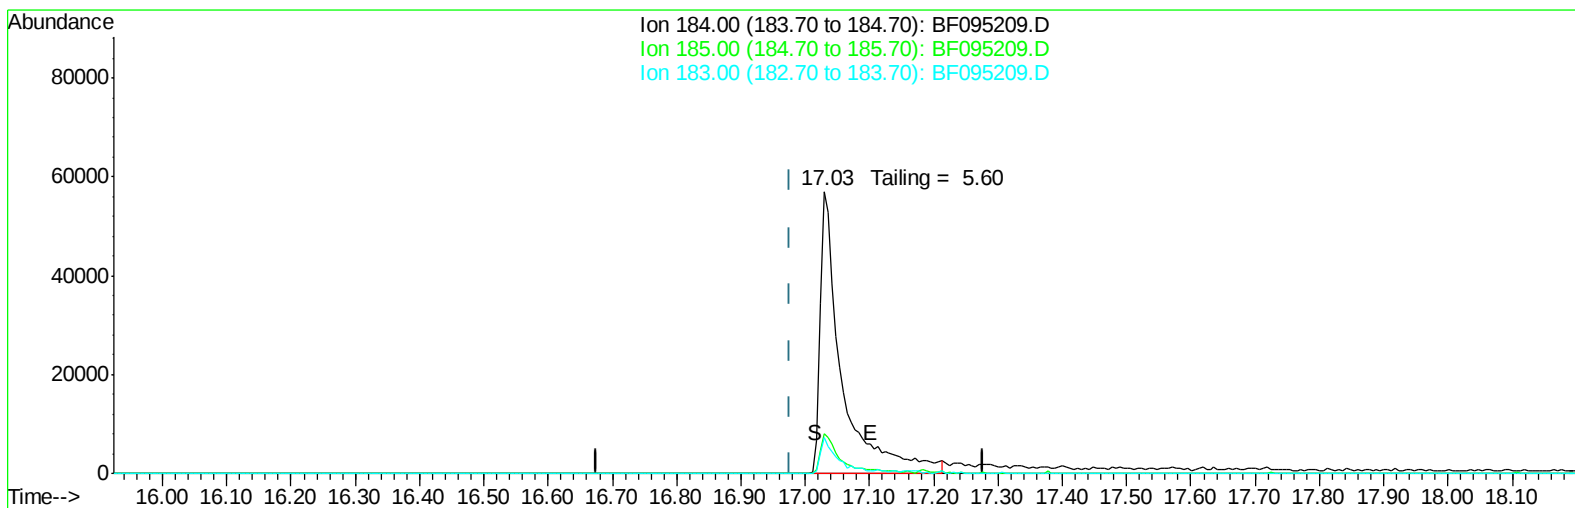

TIC: BF095209.D

(76) Benzidine



17.030min (+0.053) 0.00ng

response 130670

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.15#
183.00	12.20	12.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051717\
Data File : BF095209.D
Acq On : 18 May 2017 4:26
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 08:07:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

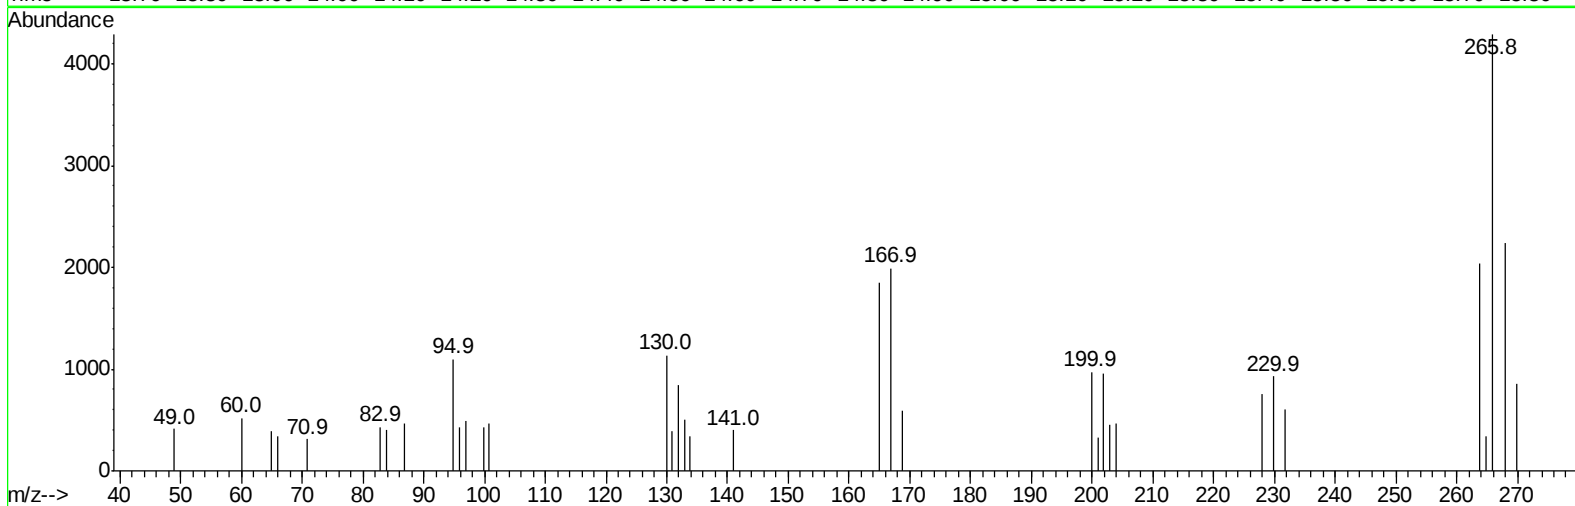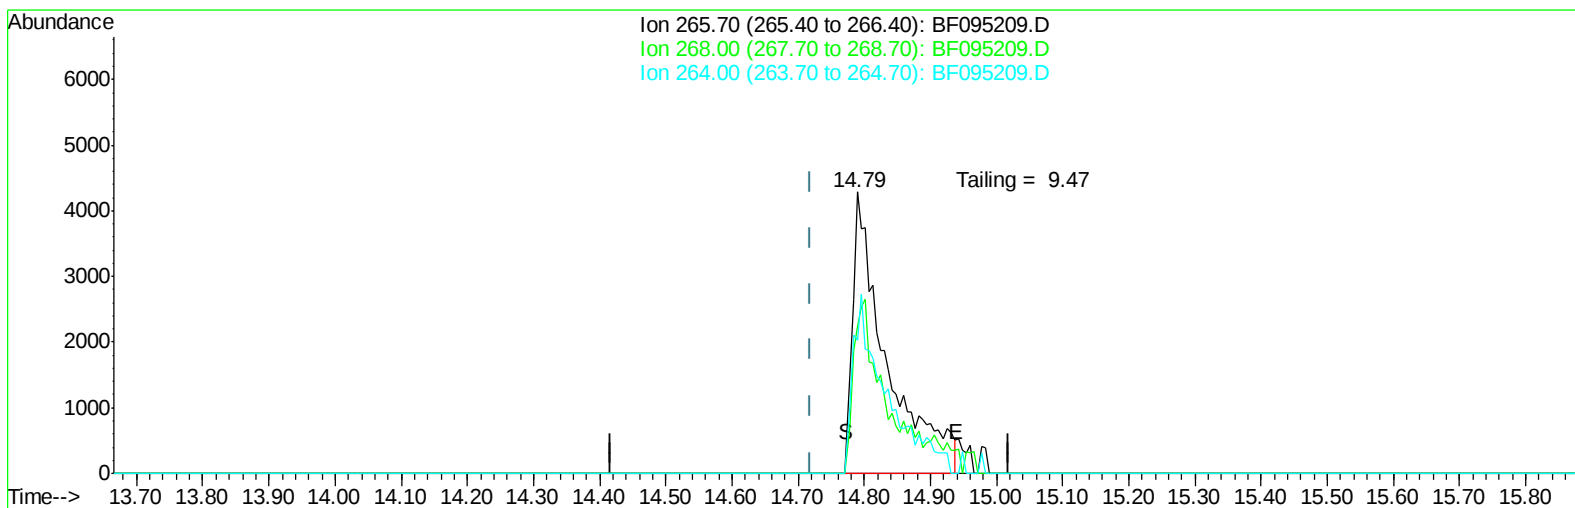

TIC: BF095209.D

(69) Pentachlorophenol (C)

14.789min (+0.071) 0.00ng

response 12798

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	52.06
264.00	64.60	47.38#
0.00	0.00	0.00