

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051717\
 Data File : BF095206.D
 Acq On : 18 May 2017 2:34
 Operator : SJ/MA
 Sample : I3184-05 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMPOSITE1

Quant Time: May 18 07:12:08 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 17:24:51 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	80094	20.00	ng	0.04
21) Naphthalene-d8	9.79	136	325273	20.00	ng	0.04
38) Acenaphthene-d10	12.62	164	132089	20.00	ng	0.04
63) Phenanthrene-d10	15.02	188	202809	20.00	ng	0.04
75) Chrysene-d12	18.69	240	191871	20.00	ng	0.04
86) Perylene-d12	20.37	264	129628	20.00	ng	0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.79	112	67973	14.15	ng	0.11
7) Phenol-d6	7.35	99	84474	14.66	ng	0.08
23) Nitrobenzene-d5	8.69	82	53184	10.31	ng	0.05
41) 2,4,6-Tribromophenol	13.94	330	14038	12.98	ng	0.05
44) 2-Fluorobiphenyl	11.56	172	121190	13.21	ng	0.03
78) Terphenyl-d14	17.34	244	86150	9.89	ng	0.03


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051717\
Data File : BF095206.D
Acq On : 18 May 2017 2:34
Operator : SJ/MA
Sample : I3184-05 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMPOSITE1

Quant Time: May 18 07:12:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

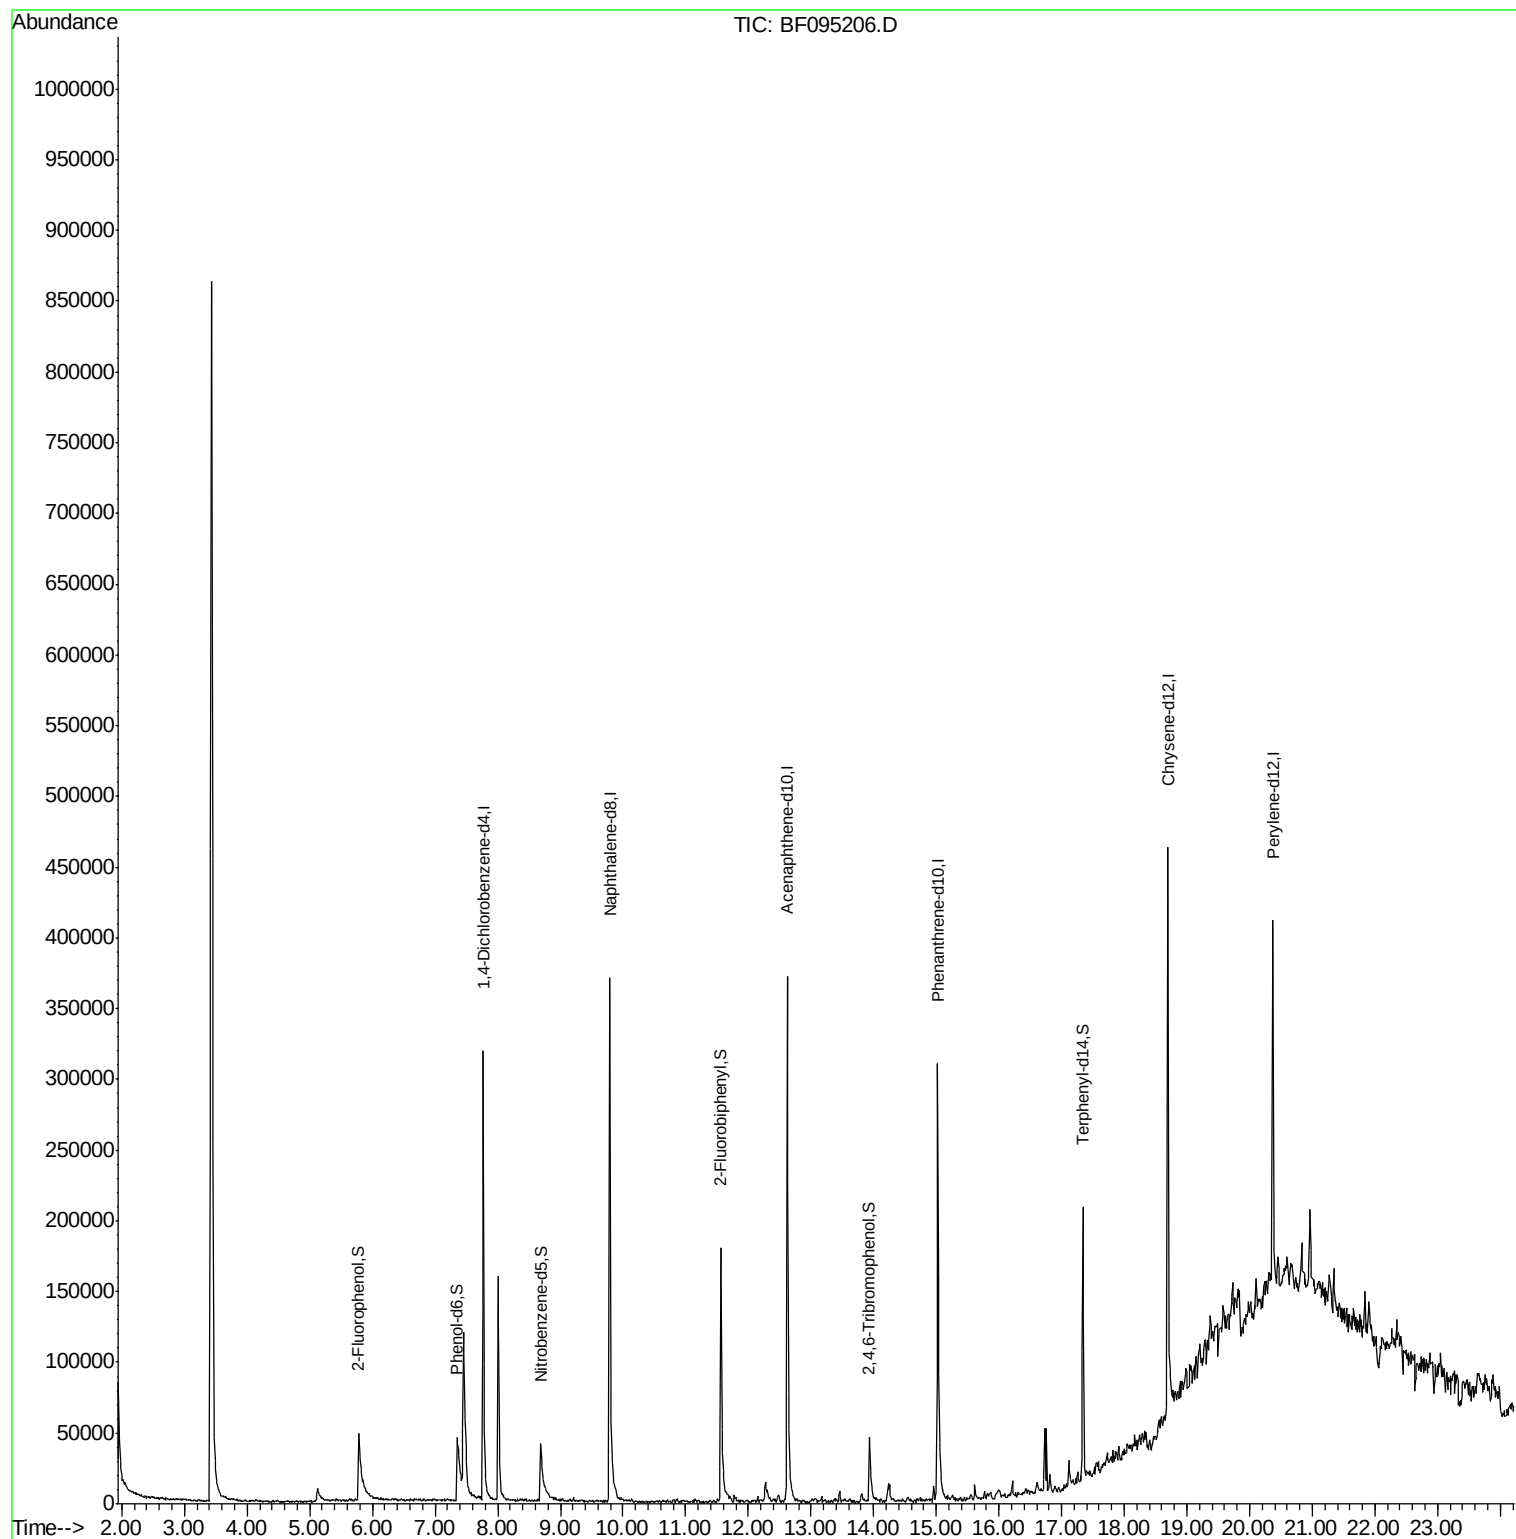

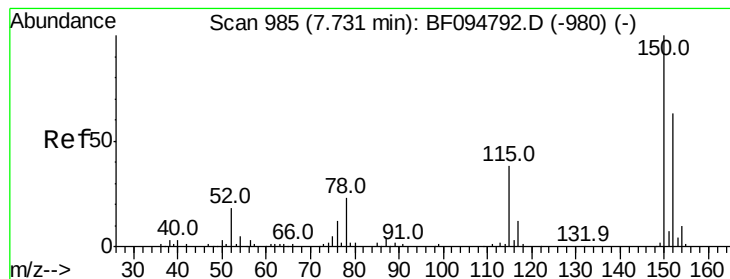


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.77 min Scan# 992
 Delta R.T. 0.04 min
 Lab File: BF095206.D
 Acq: 18 May 2017 2:34

Instrument :
 BNA_F
 ClientSampleId :
 COMPOSITE1

Tot Ion:152 Resp: 80094
 Ion Ratio Lower Upper
 152 100
 150 152.2 126.2 189.2
 115 55.9 52.2 78.2

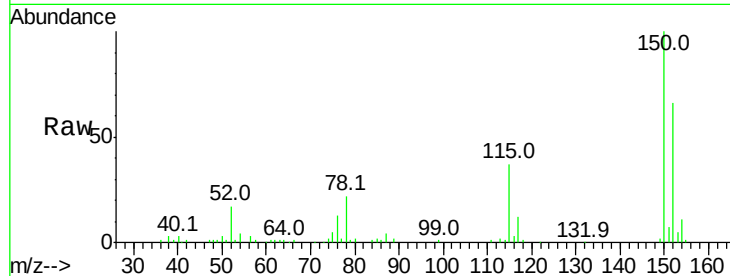


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

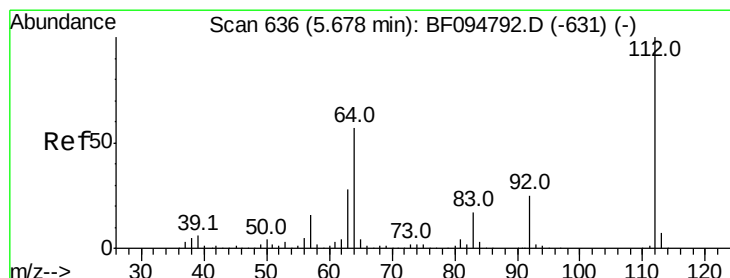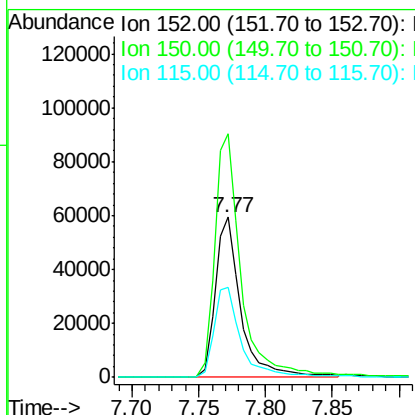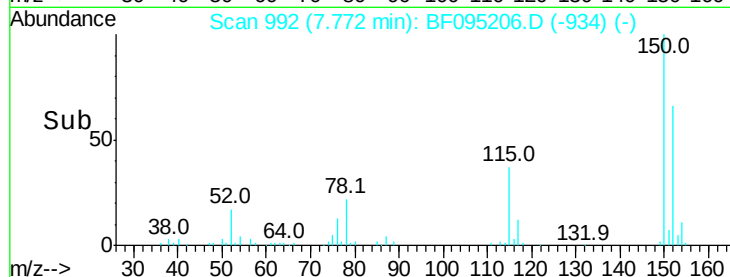



#5


2-Fluorophenol
 Concen: 14.15 ng
 RT: 5.79 min Scan# 655
 Delta R.T. 0.11 min
 Lab File: BF095206.D
 Acq: 18 May 2017 2:34

Tgt Ion:112 Resp: 67973
 Ion Ratio Lower Upper
 112 100
 64 49.4 46.0 69.0
 63 25.1 23.4 35.0

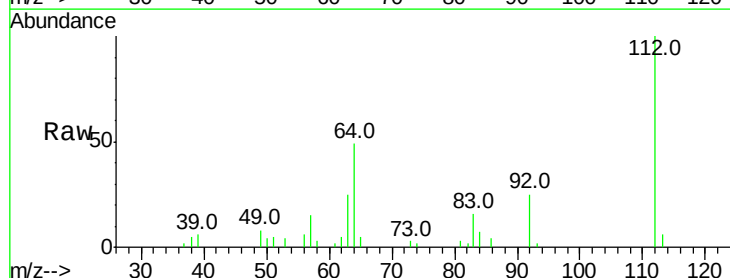

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

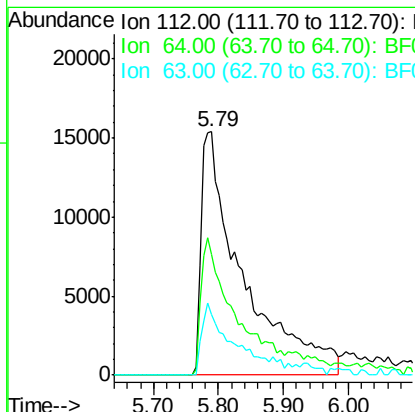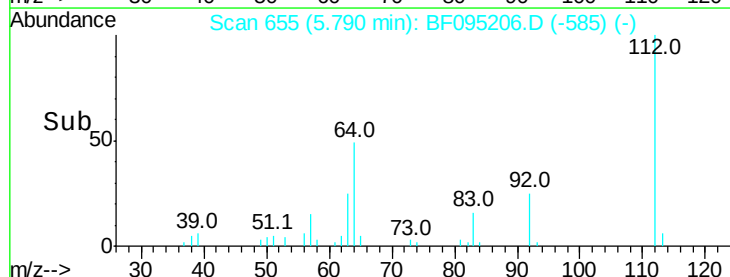

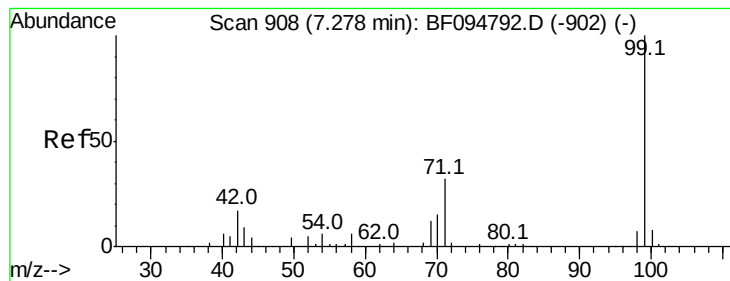

#7

Phenol-d6

Concen: 14.66 ng

RT: 7.35 min Scan# 921

Delta R.T. 0.08 min

Lab File: BF095206.D

Acq: 18 May 2017 2:34

Instrument :

BNA_F

ClientSampleId :

COMPOSITE1


Tot Ion: 99 Resp: 84474

Ion Ratio Lower Upper

99 100

42 18.2 13.5 20.3




71 30.8 24.5 36.7

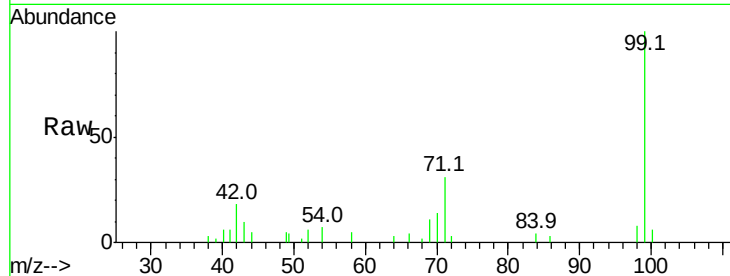

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

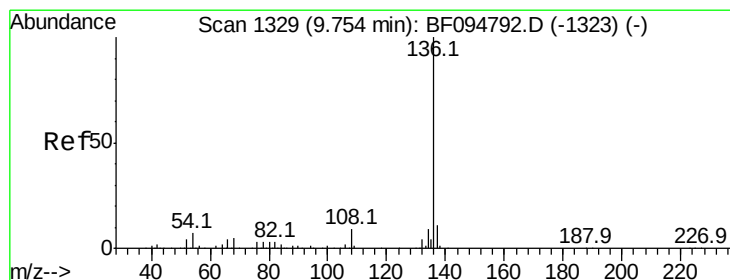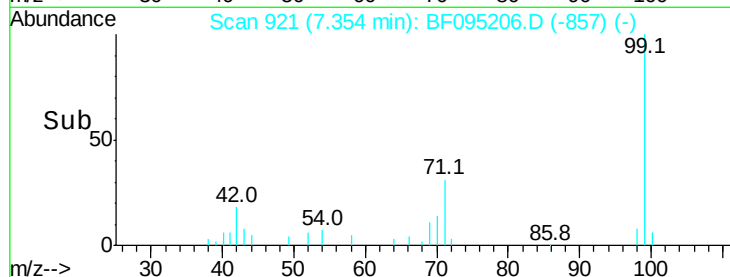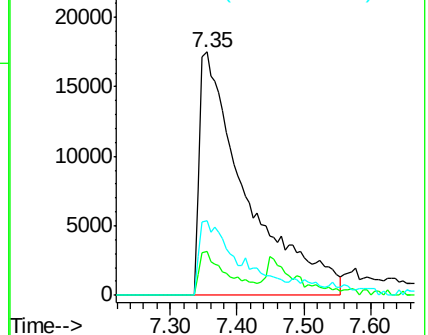

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.79 min Scan# 1335

Delta R.T. 0.04 min

Lab File: BF095206.D

Acq: 18 May 2017 2:34

Tgt Ion: 136 Resp: 325273


Ion Ratio Lower Upper

136 100

137 10.8 8.5 12.7

54 6.4 4.9 7.3

68 5.2 4.1 6.1


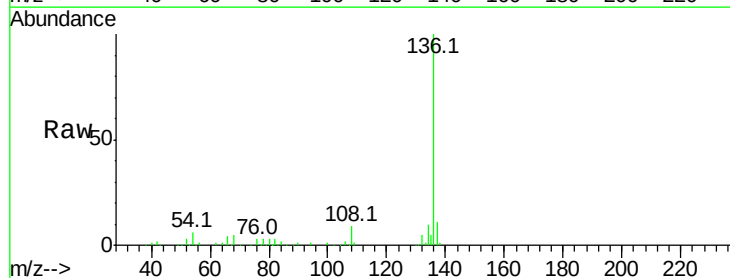



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



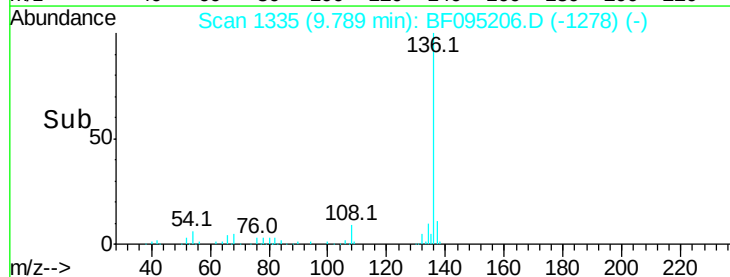
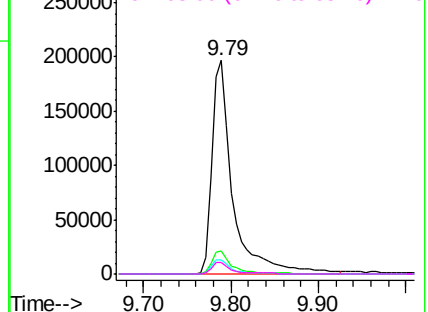


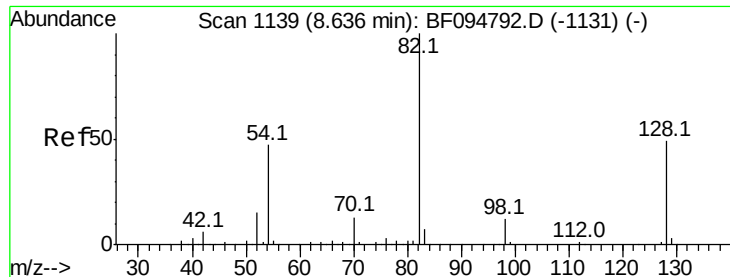

#23
 Nitrobenzene-d5
 Concen: 10.31 ng
 RT: 8.69 min Scan# 1148
 Delta R.T. 0.05 min
 Lab File: BF095206.D
 Acq: 18 May 2017 2:34




Instrument :
 BNA_F
 ClientSampleId :
 COMPOSITE1


Tot Ion: 82 Resp: 53184
 Ion Ratio Lower Upper
 82 100
 128 46.2 34.0 51.0
 54 42.4 42.2 63.2

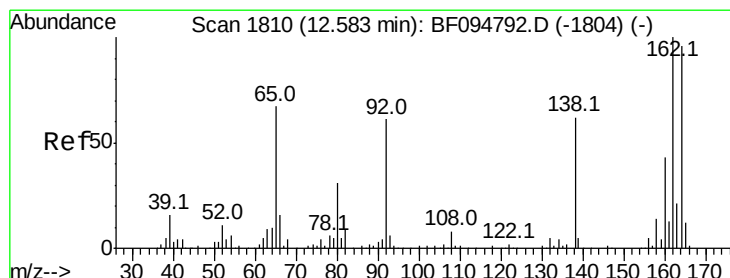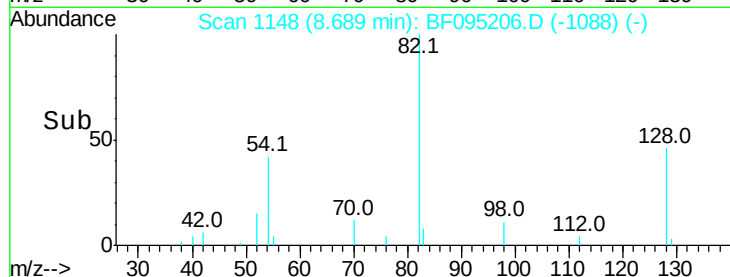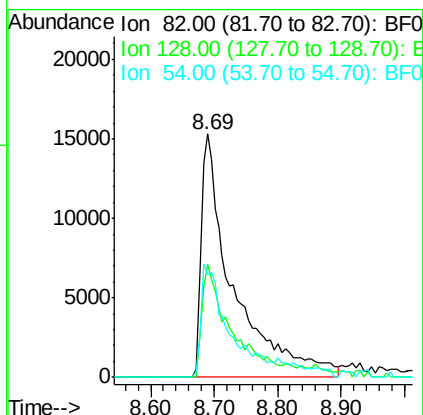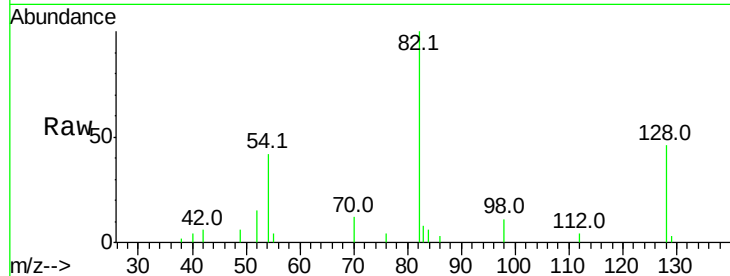

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.62 min Scan# 1816
 Delta R.T. 0.04 min
 Lab File: BF095206.D
 Acq: 18 May 2017 2:34

Tgt Ion:164 Resp: 132089
 Ion Ratio Lower Upper
 164 100
 162 105.6 82.6 123.8
 160 44.2 36.2 54.2

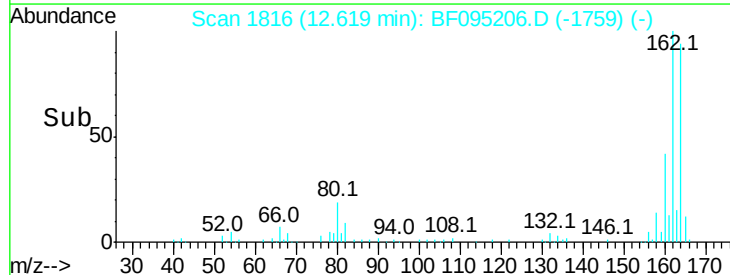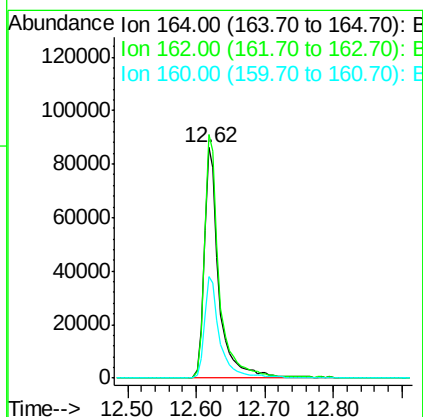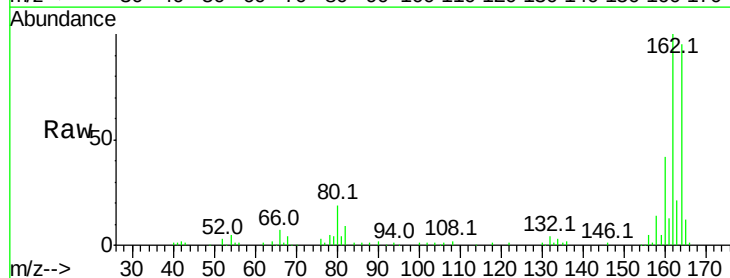

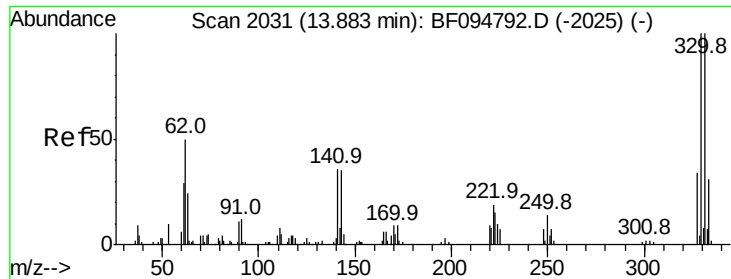

#41

2,4,6-Tribromophenol

Concen: 12.98 ng

RT: 13.94 min Scan# 2040

Delta R.T. 0.05 min

Lab File: BF095206.D

Acq: 18 May 2017 2:34

Instrument :

BNA_F

ClientSampleId :

COMPOSITE1


Tot Ion:330 Resp: 14038

Ion Ratio Lower Upper

330 100

332 93.3 76.6 115.0




141 38.4 31.4 47.2

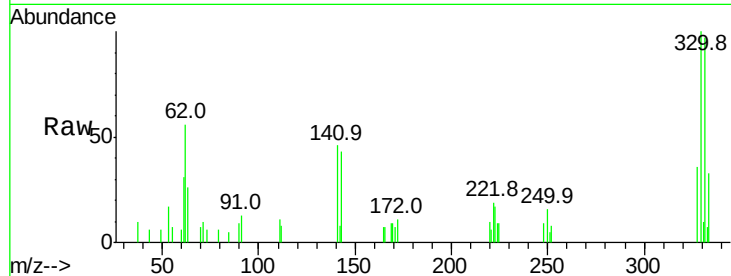

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

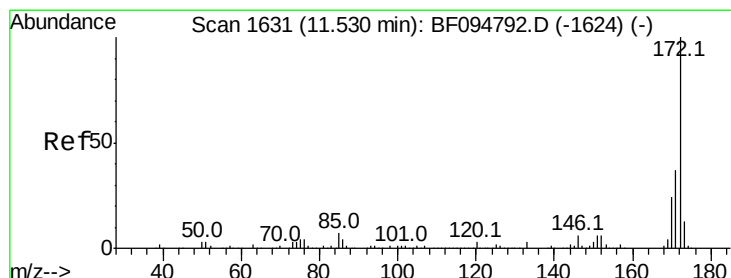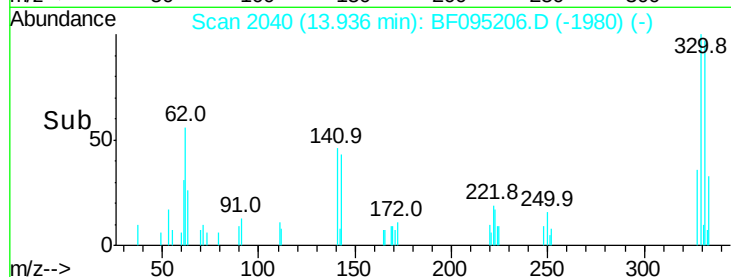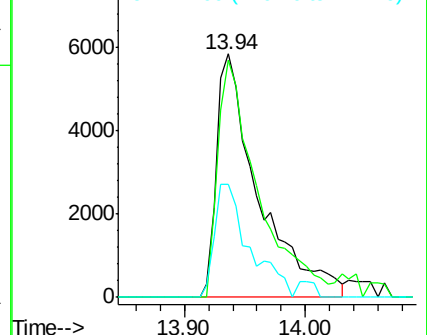

#44

2-Fluorobiphenyl

Concen: 13.21 ng

RT: 11.56 min Scan# 1636

Delta R.T. 0.03 min

Lab File: BF095206.D

Acq: 18 May 2017 2:34


Tgt Ion:172 Resp: 121190

Ion Ratio Lower Upper

172 100

171 33.9 29.6 44.4



170 20.9 19.8 29.8

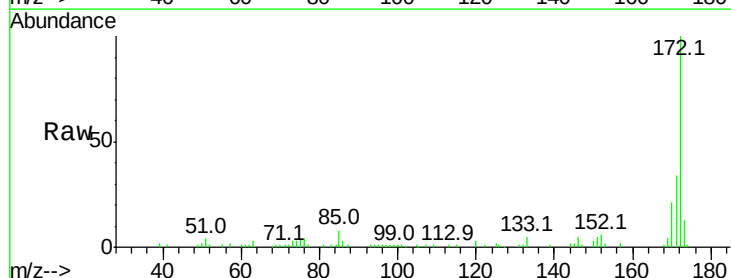


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



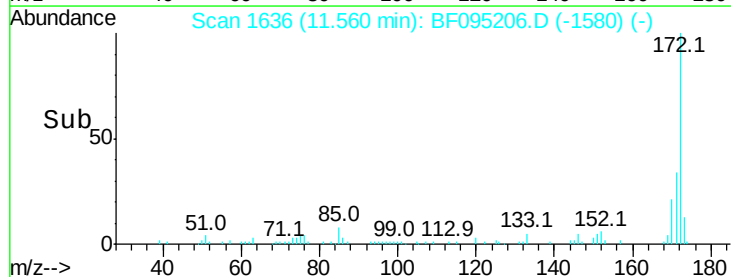
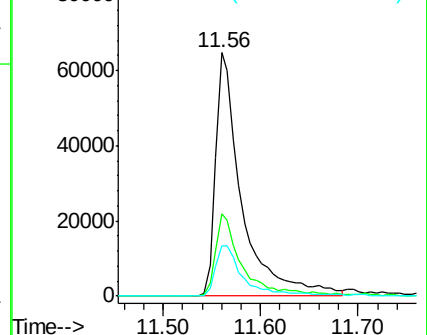


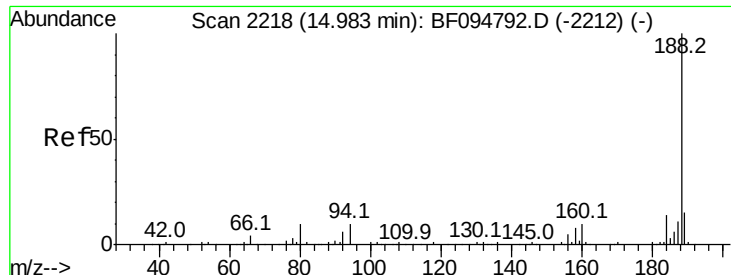

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 15.02 min Scan# 2225
 Delta R.T. 0.04 min
 Lab File: BF095206.D
 Acq: 18 May 2017 2:34




Instrument :
 BNA_F
 ClientSampleId :
 COMPOSITE1


Tot Ion	Ratio	Lower	Upper
188	100		
94	10.2	9.4	14.2
80	11.9	10.2	15.2

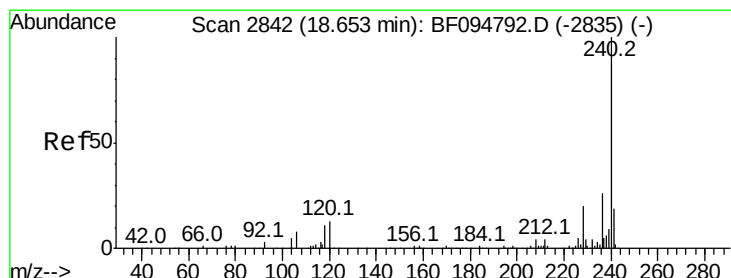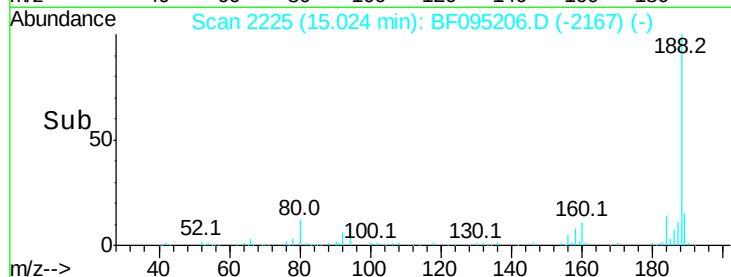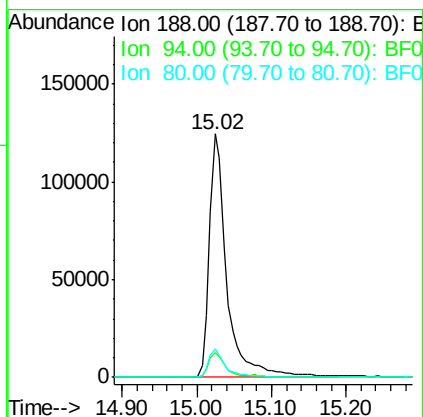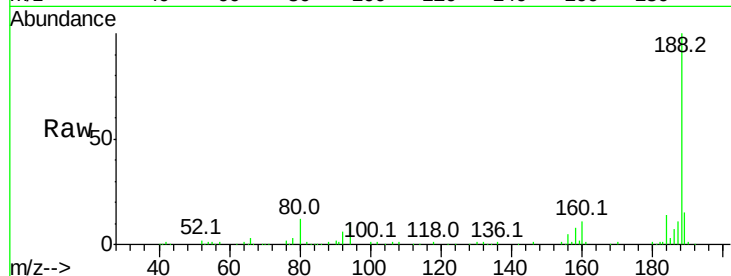

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 18.69 min Scan# 2849
 Delta R.T. 0.04 min
 Lab File: BF095206.D
 Acq: 18 May 2017 2:34

Tgt Ion	Ratio	Lower	Upper
240	100		
120	14.0	5.8	8.8#
236	25.3	20.5	30.7

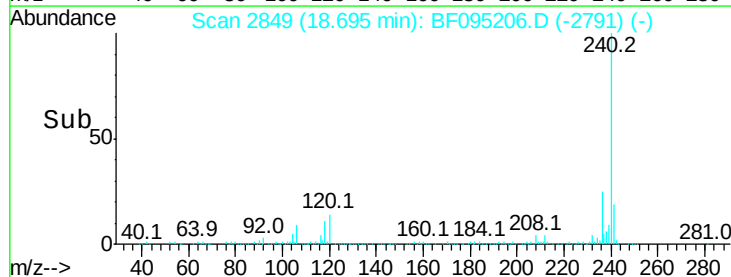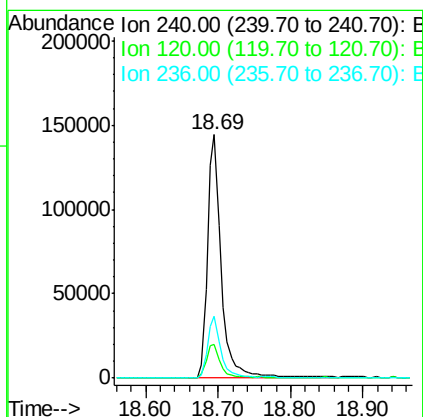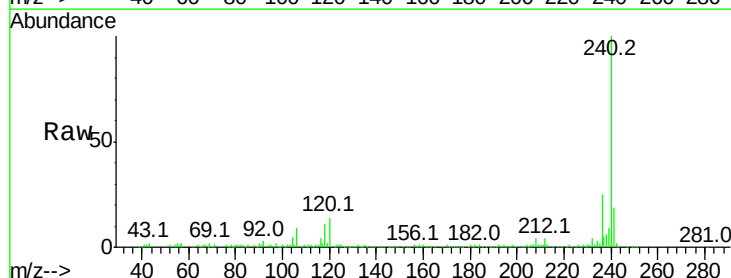

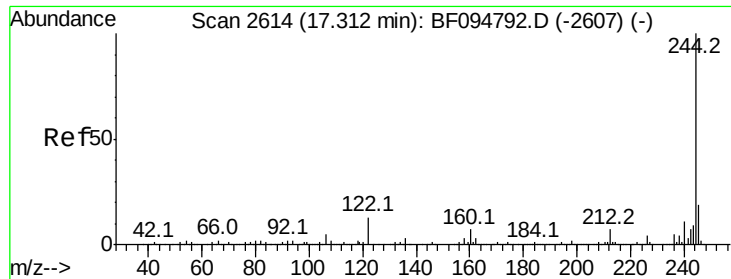

#78

Terphenyl-d14

Concen: 9.89 ng

RT: 17.34 min Scan# 2619

Delta R.T. 0.03 min

Lab File: BF095206.D

Acq: 18 May 2017 2:34

Instrument :

BNA_F

ClientSampleId :

COMPOSITE1


Tot Ion:244 Resp: 86150

Ion Ratio Lower Upper

244 100

212 6.9 6.0 9.0



122 12.1 10.3 15.5

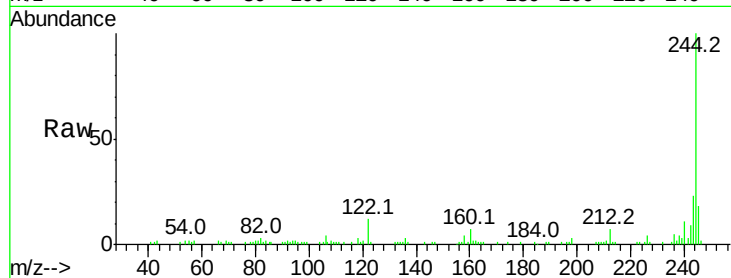


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

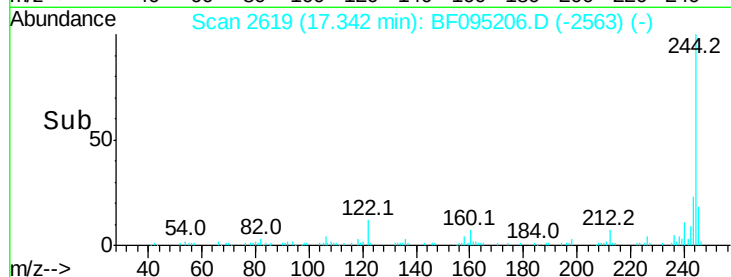

Time-->

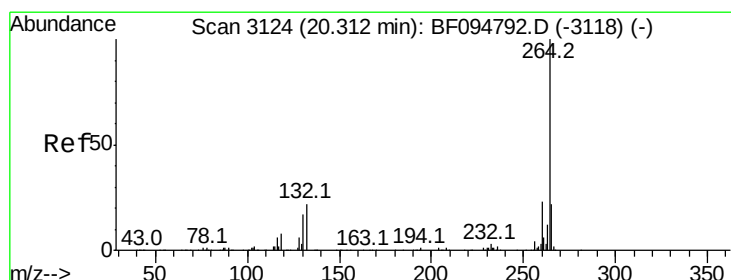

#86

Perylene-d12

Concen: 20.00 ng

RT: 20.37 min Scan# 3134

Delta R.T. 0.06 min

Lab File: BF095206.D

Acq: 18 May 2017 2:34


Tgt Ion:264 Resp: 129628

Ion Ratio Lower Upper

264 100

260 22.5 19.5 29.3



265 21.0 17.2 25.8

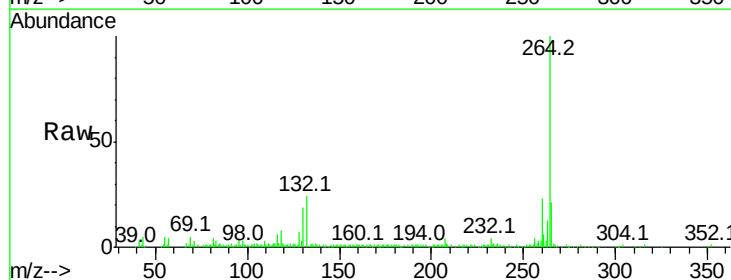

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

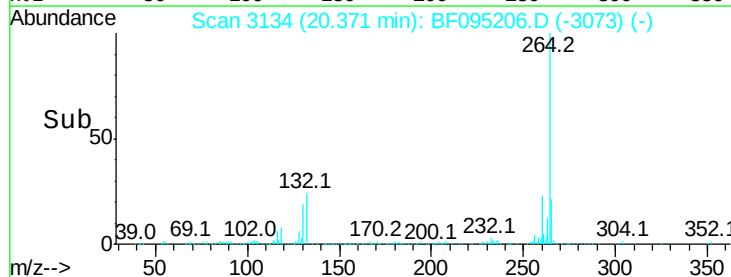

Time-->