

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051717\
 Data File : BF095206.D
 Acq On : 18 May 2017 2:34
 Operator : SJ/MA
 Sample : I3184-05 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMPOSITE1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.437	246	255	280	rBV	862308	1848439	100.00%	27.254%
2	5.125	538	542	555	rBV3	8372	21795	1.18%	0.321%
3	5.784	650	654	674	rBV	47263	162211	8.78%	2.392%
4	7.354	917	921	934	rBV	45194	154588	8.36%	2.279%
5	7.454	934	938	953	rVB	114090	282449	15.28%	4.164%
6	7.772	988	992	1010	rBV	317495	439852	23.80%	6.485%
7	8.007	1028	1032	1054	rVB	158008	234015	12.66%	3.450%
8	8.689	1144	1148	1168	rBV2	40023	125460	6.79%	1.850%
9	9.789	1330	1335	1356	rBV	368481	595976	32.24%	8.787%
10	11.560	1632	1636	1650	rBV	178180	297586	16.10%	4.388%
11	12.272	1752	1757	1761	rBV2	13783	26084	1.41%	0.385%
12	12.619	1812	1816	1837	rBV2	370745	592832	32.07%	8.741%
13	13.930	2036	2039	2052	rBV3	45491	93747	5.07%	1.382%
14	15.024	2217	2225	2241	rVV	308019	502041	27.16%	7.402%
15	16.724	2510	2514	2517	rBV2	43360	46429	2.51%	0.685%
16	16.760	2517	2520	2524	rVV2	43994	48425	2.62%	0.714%
17	16.812	2524	2529	2535	rVB	12760	18678	1.01%	0.275%
18	17.112	2577	2580	2588	rBV	16767	24245	1.31%	0.357%
19	17.342	2614	2619	2626	rBV	192958	254211	13.75%	3.748%
20	18.695	2844	2849	2861	rBV	402721	591149	31.98%	8.716%
21	19.142	2923	2925	2929	rBV5	16261	22316	1.21%	0.329%
22	19.324	2954	2956	2959	rBV3	17547	24404	1.32%	0.360%
23	19.518	2985	2989	2991	rBV5	19192	33522	1.81%	0.494%
24	20.371	3130	3134	3143	rVB	256842	341919	18.50%	5.041%


Sum of corrected areas: 6782373

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051717\
Data File : BF095206.D
Acq On : 18 May 2017 2:34
Operator : SJ/MA
Sample : I3184-05 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMPOSITE1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

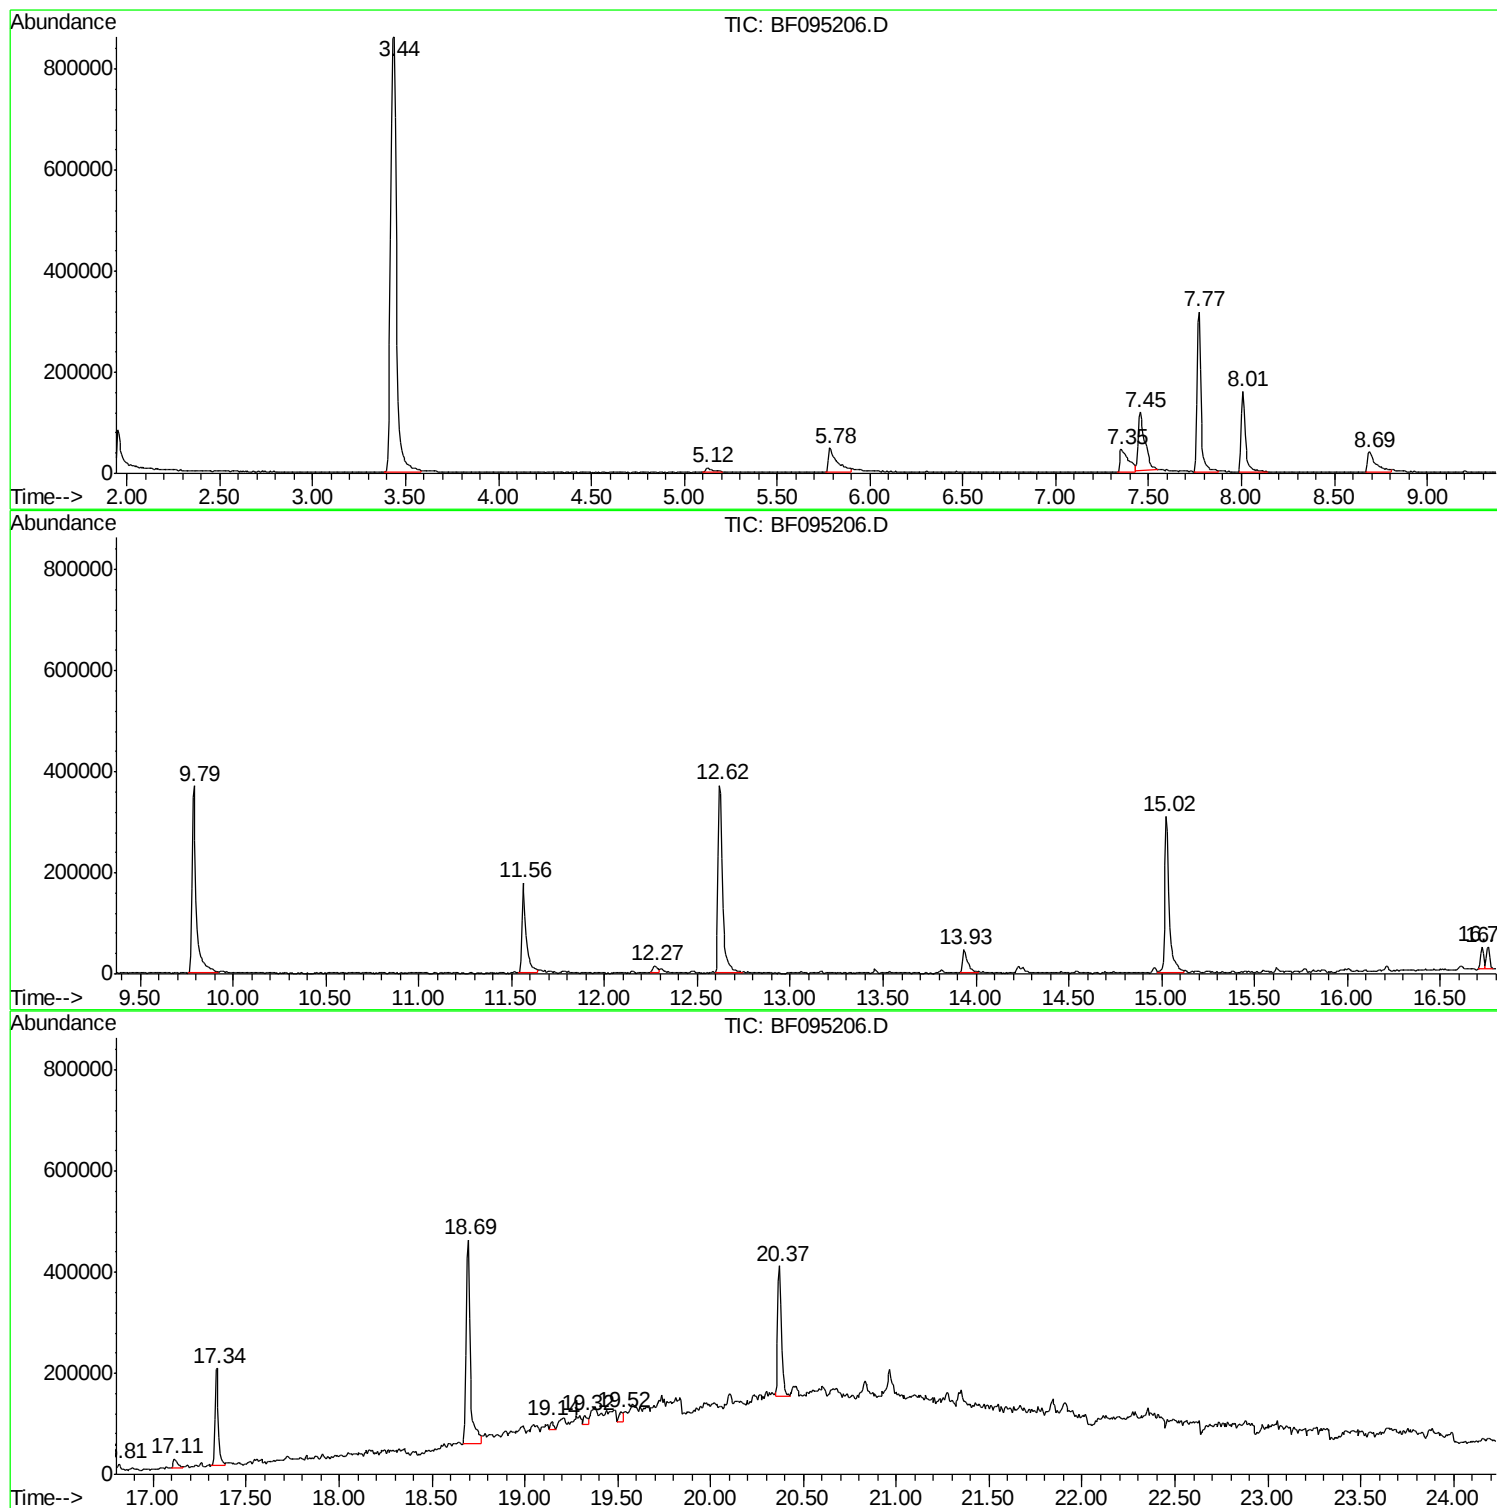

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051717\
Data File : BF095206.D
Acq On : 18 May 2017 2:34
Operator : SJ/MA
Sample : I3184-05 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMPOSITE1










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.45 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.45	12.84 ng	282449	1,4-Dichlorobenzene-d4	7.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
2		N-(-phenylisopropyl)benzalimine	223	C16H17N	1000379-01-3	12
3		Benzeneethanamine, .alpha.-methv...	223	C16H17N	002980-02-1	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
5		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	10

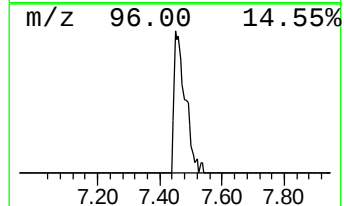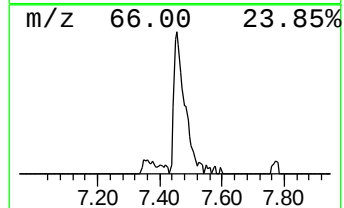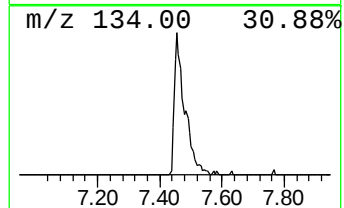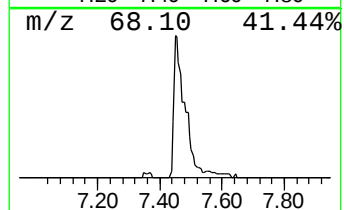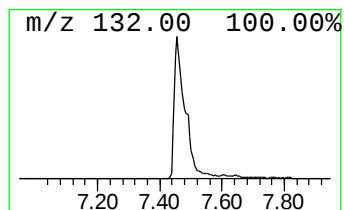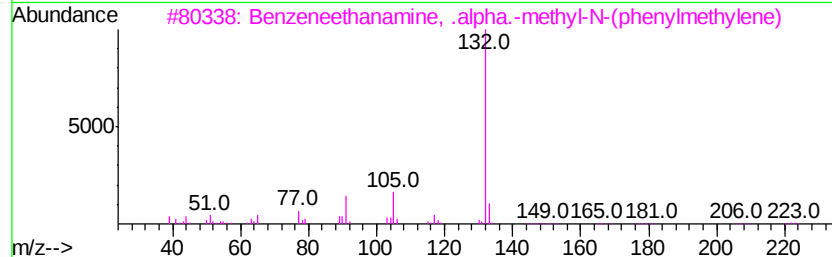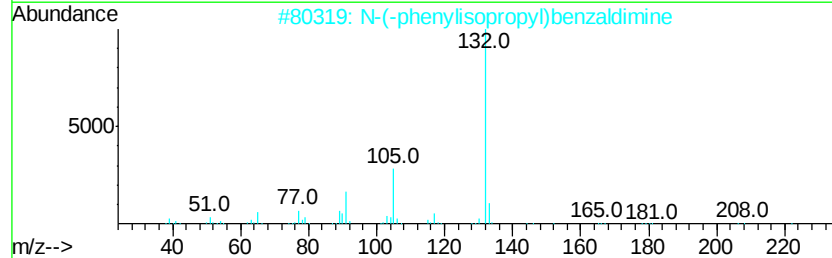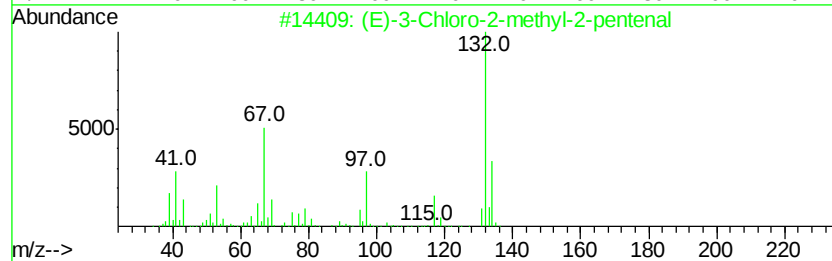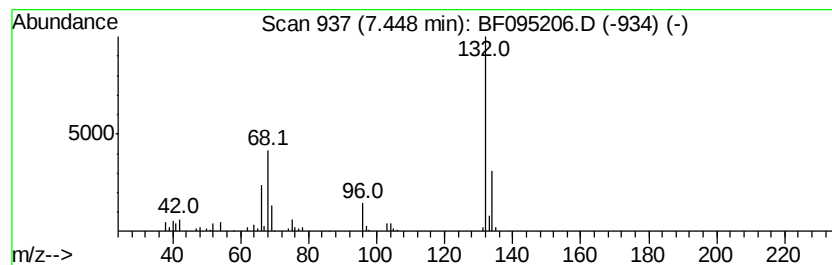

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051717\
Data File : BF095206.D
Acq On : 18 May 2017 2:34
Operator : SJ/MA
Sample : I3184-05 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMPOSITE1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.45	7.45	12.8	ng	282449	1	7.77	439852	20.0