


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051719\
 Data File : BF114339.D
 Acq On : 17 May 2019 10:08
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 20 04:47:40 2019

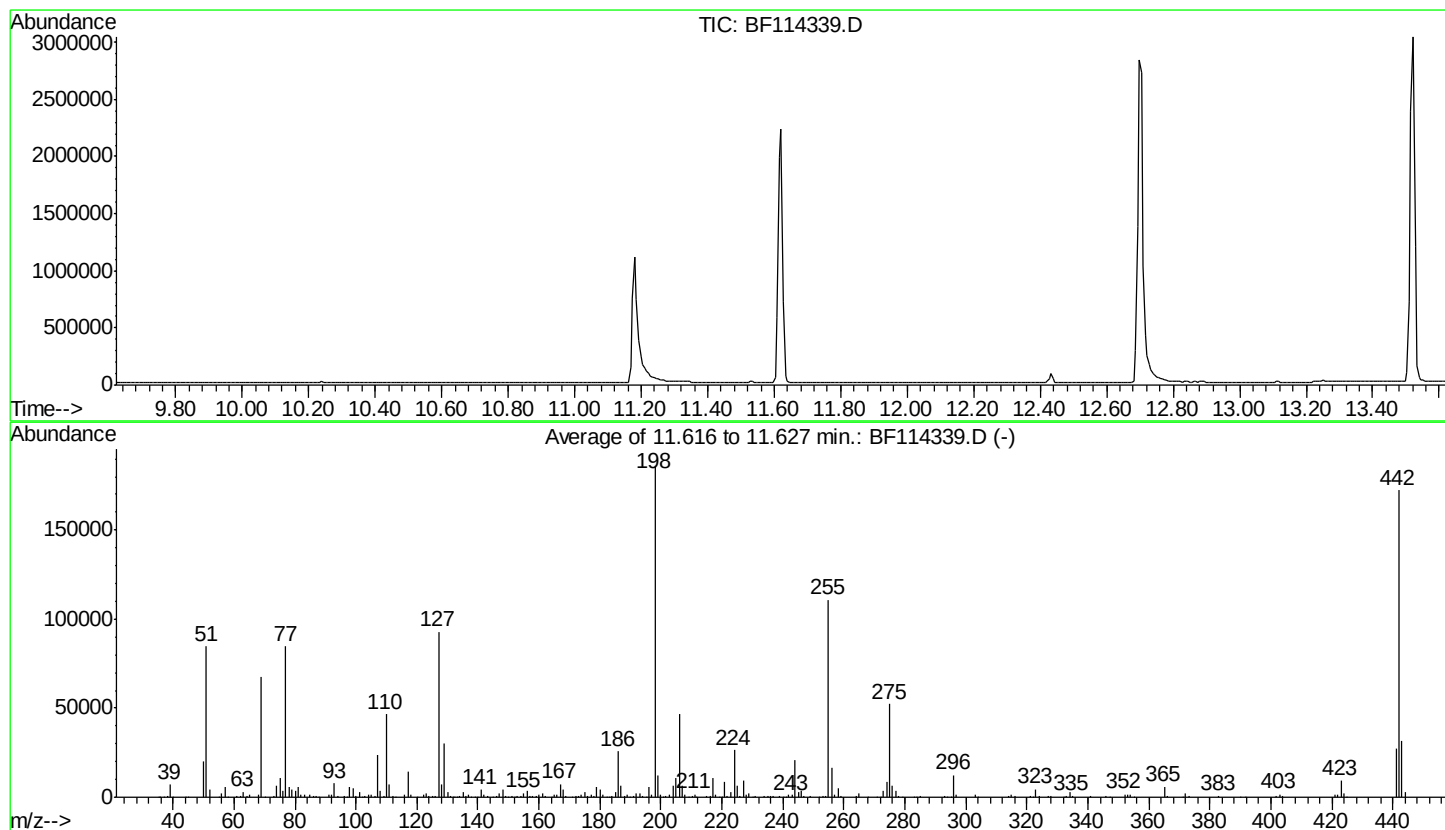

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	84798	PASS
68	69	0.00	2	1.8	1236	PASS
69	198	0.00	100	36.4	67794	PASS
70	69	0.00	2	0.5	346	PASS
127	198	10	80	50.0	93040	PASS
197	198	0.00	2	0.7	1321	PASS
198	198	100	100	100.0	186160	PASS
199	198	5	9	6.8	12579	PASS
275	198	10	60	28.2	52410	PASS
365	198	1	100	3.3	6106	PASS
441	198	0.01	100	14.7	27346	PASS
442	198	50	100	92.6	172453	PASS
443	442	15	24	18.5	31930	PASS