


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051719\
Data File : BF114363.D
Acq On : 17 May 2019 22:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 20 04:47:40 2019

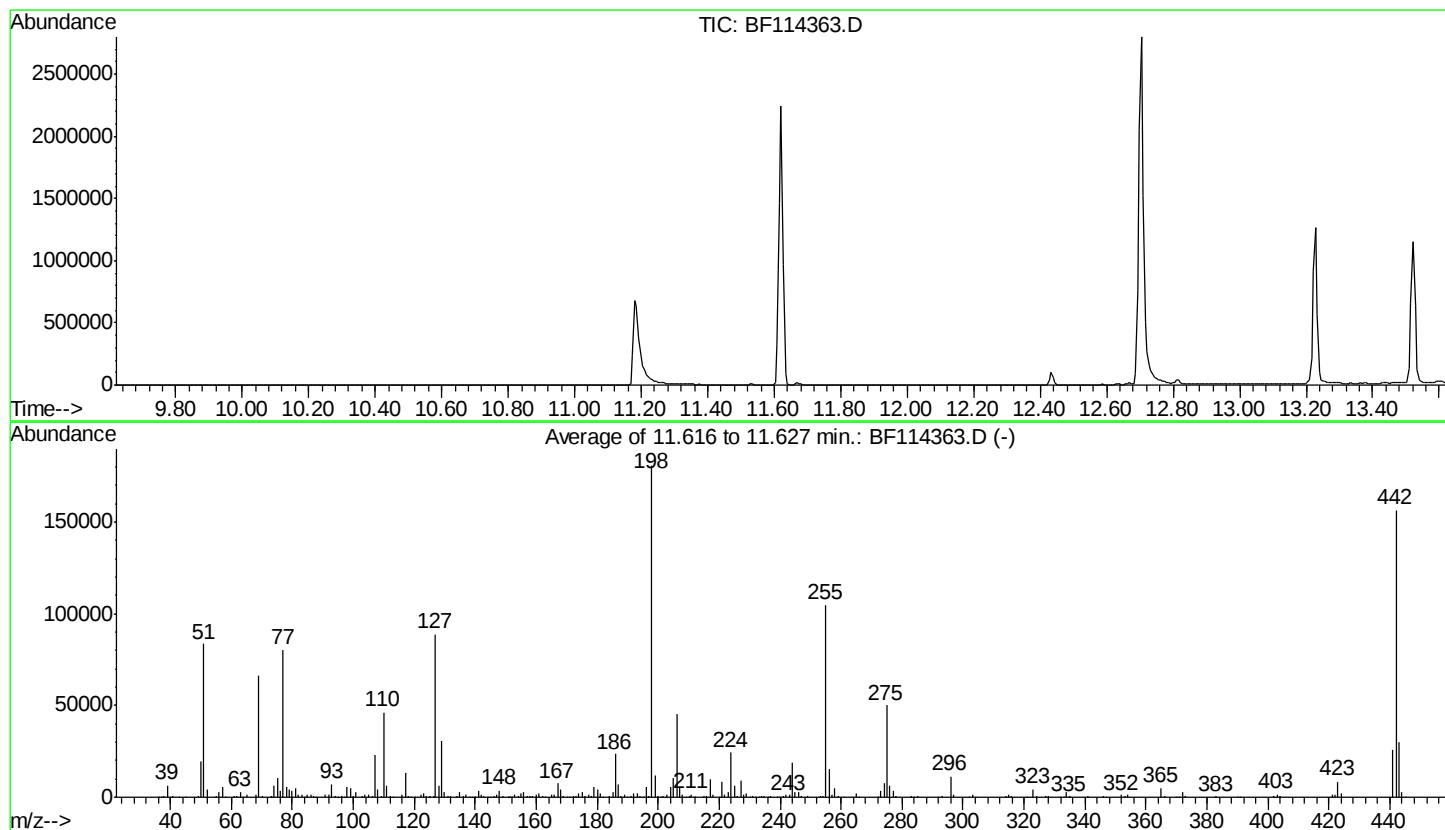

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	83720	PASS
68	69	0.00	2	1.7	1142	PASS
69	198	0.00	100	36.6	66109	PASS
70	69	0.00	2	0.6	378	PASS
127	198	10	80	49.1	88730	PASS
197	198	0.00	2	0.4	787	PASS
198	198	100	100	100.0	180805	PASS
199	198	5	9	6.6	11886	PASS
275	198	10	60	27.8	50200	PASS
365	198	1	100	2.8	5025	PASS
441	198	0.01	100	14.4	26118	PASS
442	198	50	100	86.6	156632	PASS
443	442	15	24	19.0	29720	PASS