
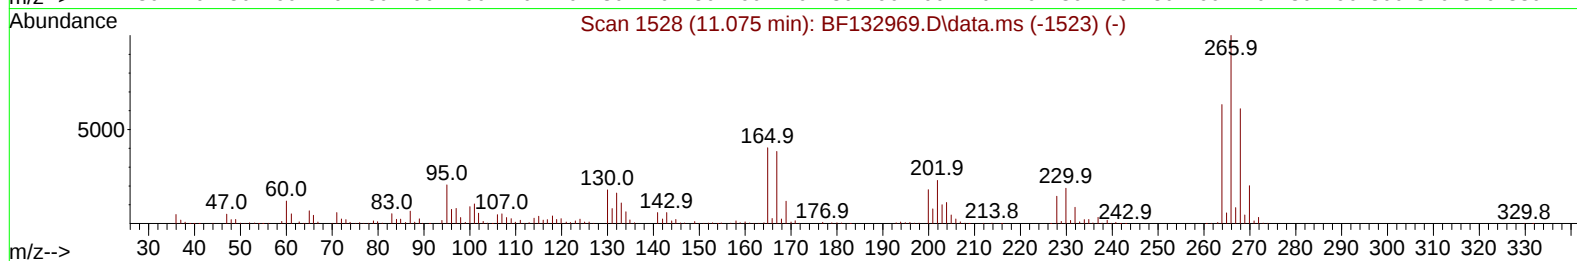
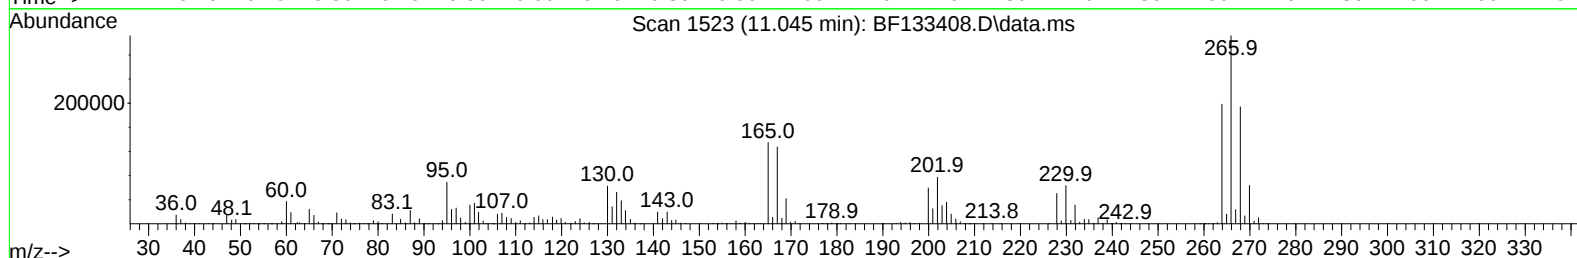


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051723\
 Data File : BF133408.D
 Acq On : 17 May 2023 11:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 18:24:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 16 14:39:29 2023
 Response via : Initial Calibration

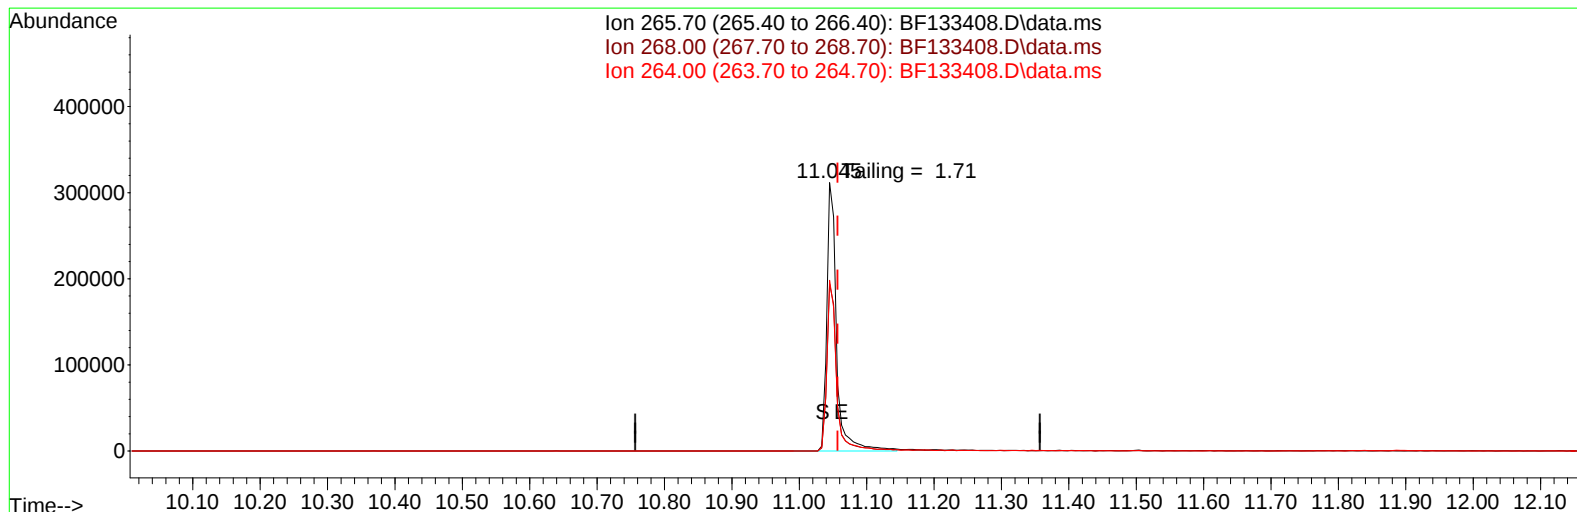

TIC: BF133408.D\data.ms

(70) Pentachlorophenol (C)




11.045min (-0.012) 26587.22 ng m

response 316282

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.26
264.00	63.30	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051723\
Data File : BF133408.D
Acq On : 17 May 2023 11:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 18:24:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 16 14:39:29 2023
Response via : Initial Calibration

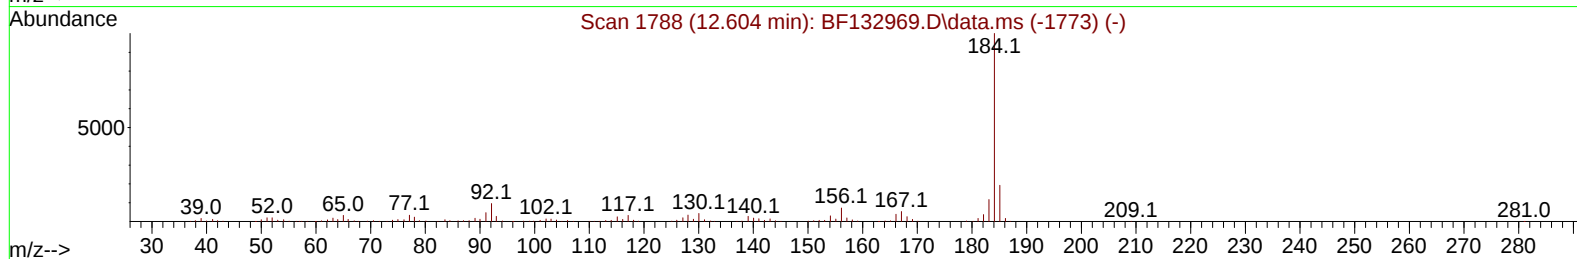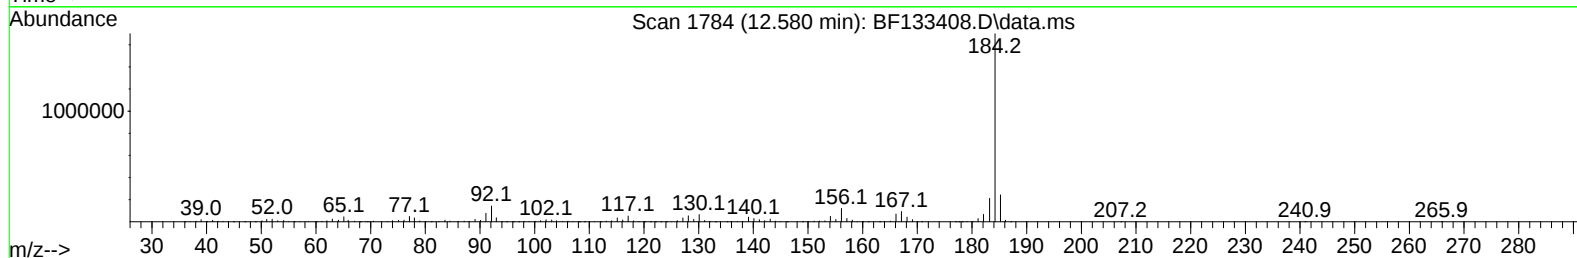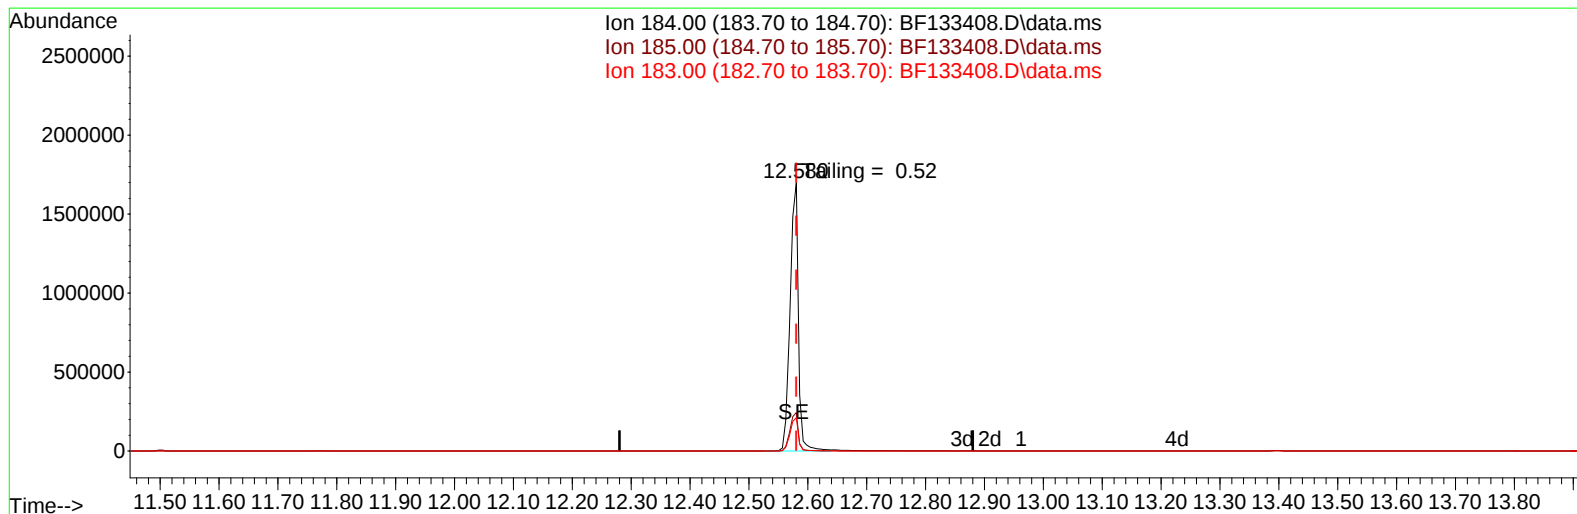

TIC: BF133408.D\data.ms

(77) Benzidine

12.580min (-0.000) 1076037.84 ng m

response 1692262

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.32#
183.00	11.70	12.42
0.00	0.00	0.00