
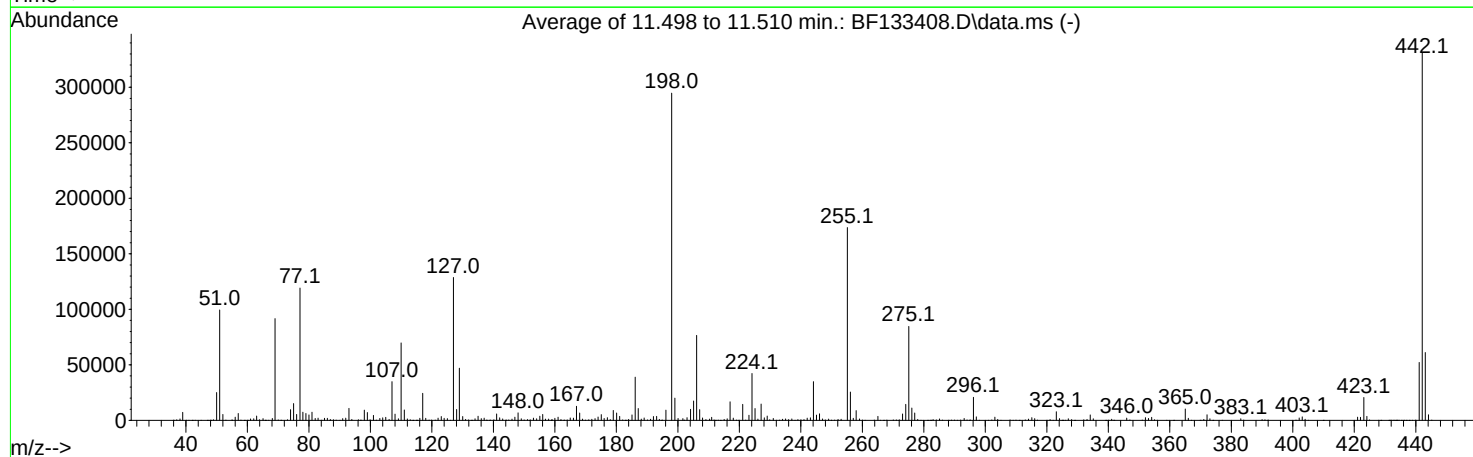


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051723\
 Data File : BF133408.D
 Acq On : 17 May 2023 11:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 16 14:39:29 2023

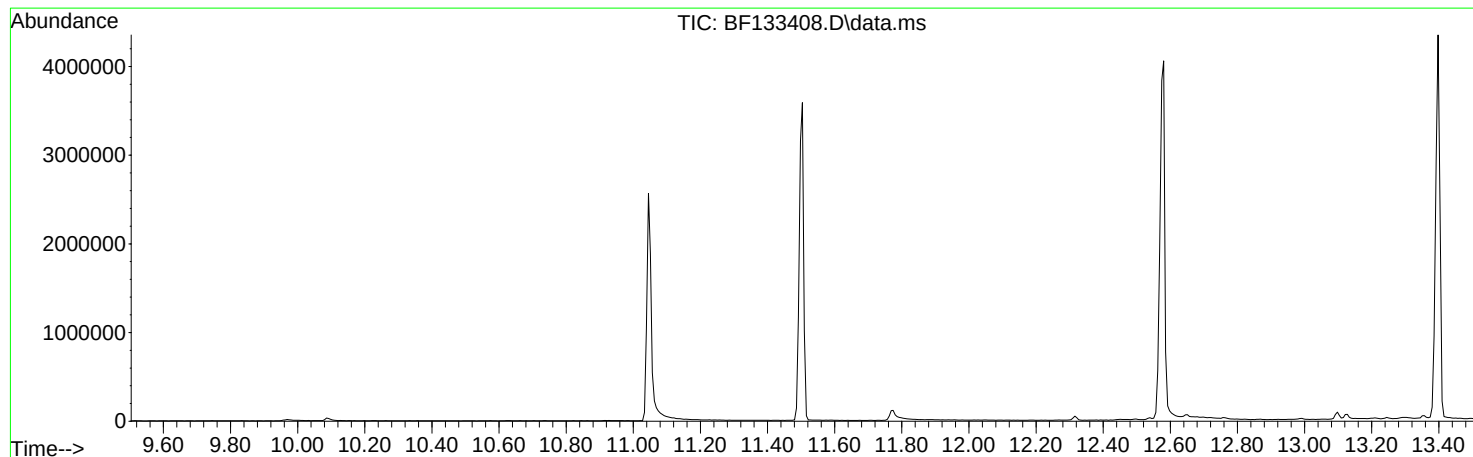




AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	99424	PASS
68	69	0.00	2	1.9	1736	PASS
69	198	0.00	100	31.1	91624	PASS
70	69	0.00	2	0.5	444	PASS
127	198	10	80	43.7	128656	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	294744	PASS
199	198	5	9	6.8	20082	PASS
275	198	10	60	28.7	84664	PASS
365	198	1	100	3.5	10228	PASS
441	198	0.01	100	17.7	52171	PASS
442	442	50	100	100.0	331307	PASS
443	442	15	24	18.4	61096	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051723\
 Data File : BF133408.D
 Acq On : 17 May 2023 11:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 17 18:24:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 16 14:39:29 2023
 Response via : Initial Calibration

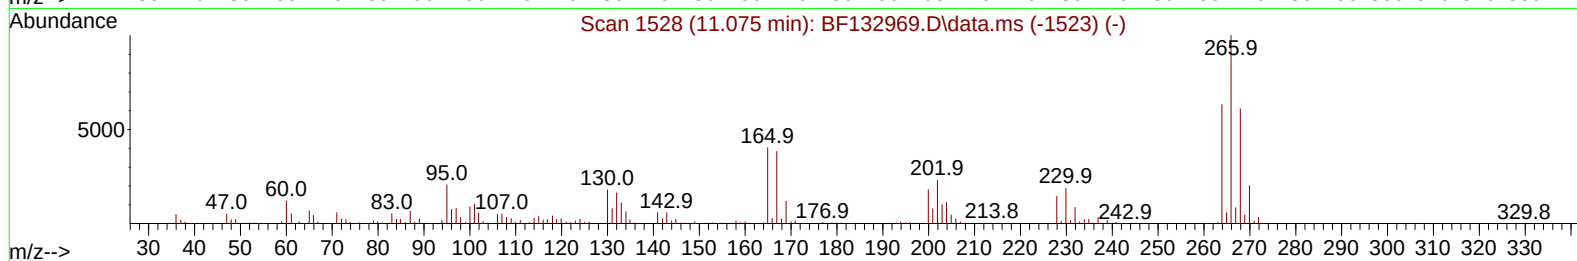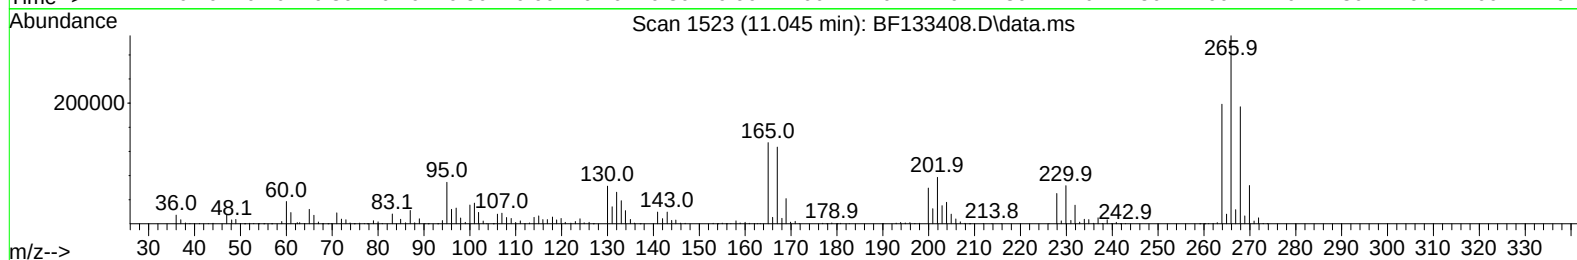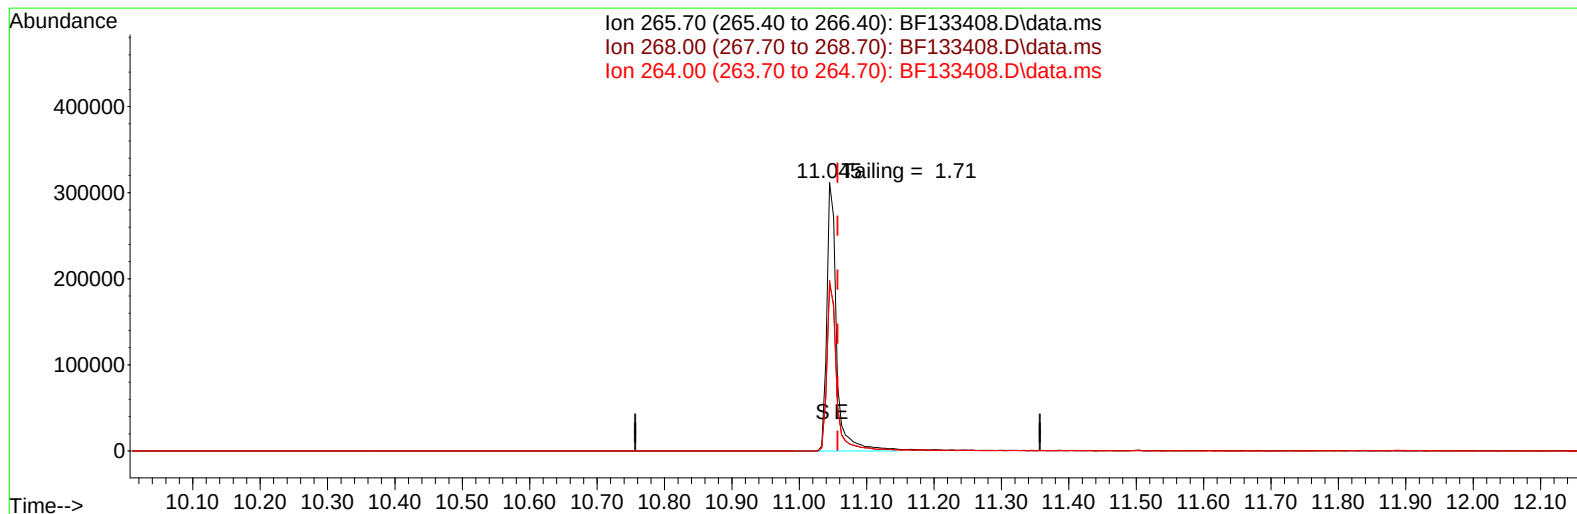

TIC: BF133408.D\data.ms

(70) Pentachlorophenol (C)

11.045min (-0.012) 26587.22 ng m




response 316282

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.26
264.00	63.30	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051723\
Data File : BF133408.D
Acq On : 17 May 2023 11:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 17 18:24:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 16 14:39:29 2023
Response via : Initial Calibration

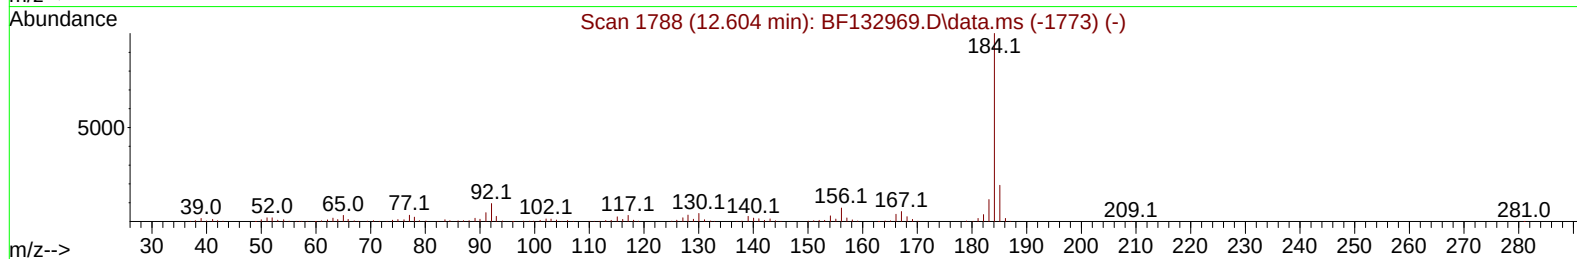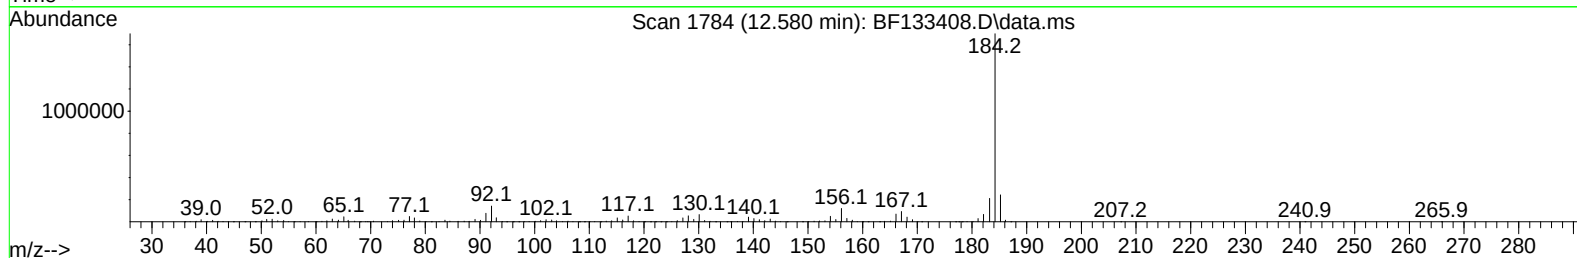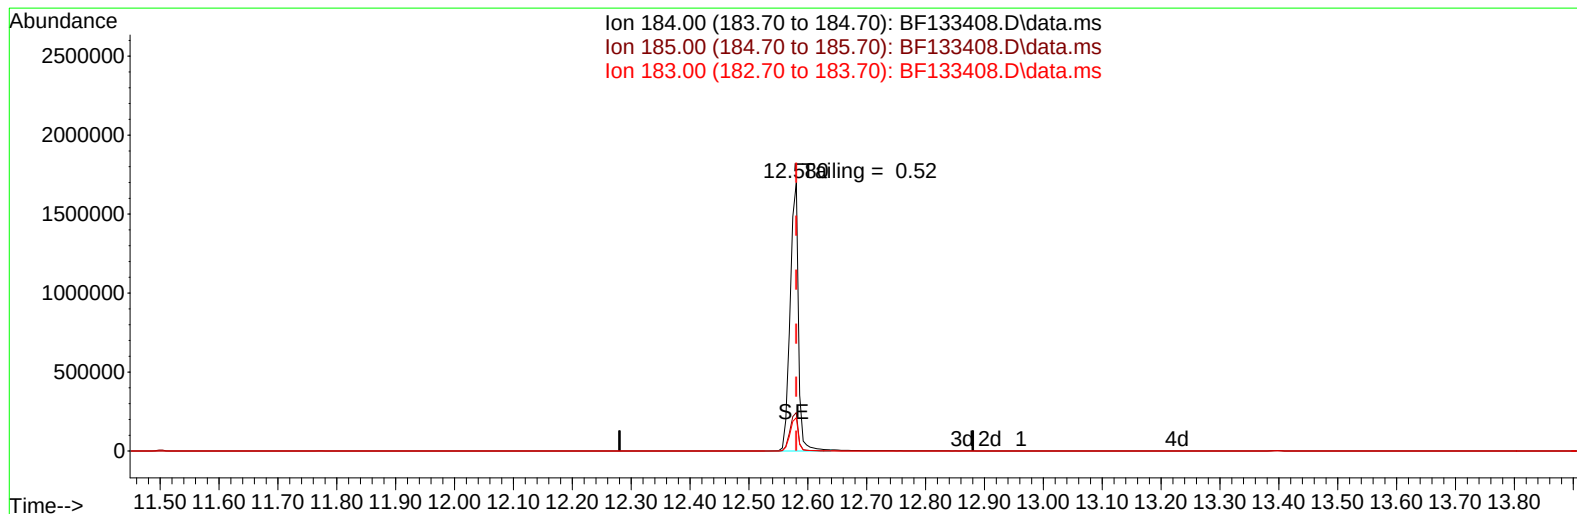

TIC: BF133408.D\data.ms

(77) Benzidine

12.580min (-0.000) 1076037.84 ng m

response 1692262

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.32#
183.00	11.70	12.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/17/2023	BNA_F	<u>BF133408.D</u>
Compound Name	Response	Retention Time
DDT	781597	13.398
DDD	24750	13.098
DDE	2642	12.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27392	808989	3.39

Instrument :
BNA_F
ClientSampleId :
DFTPP