
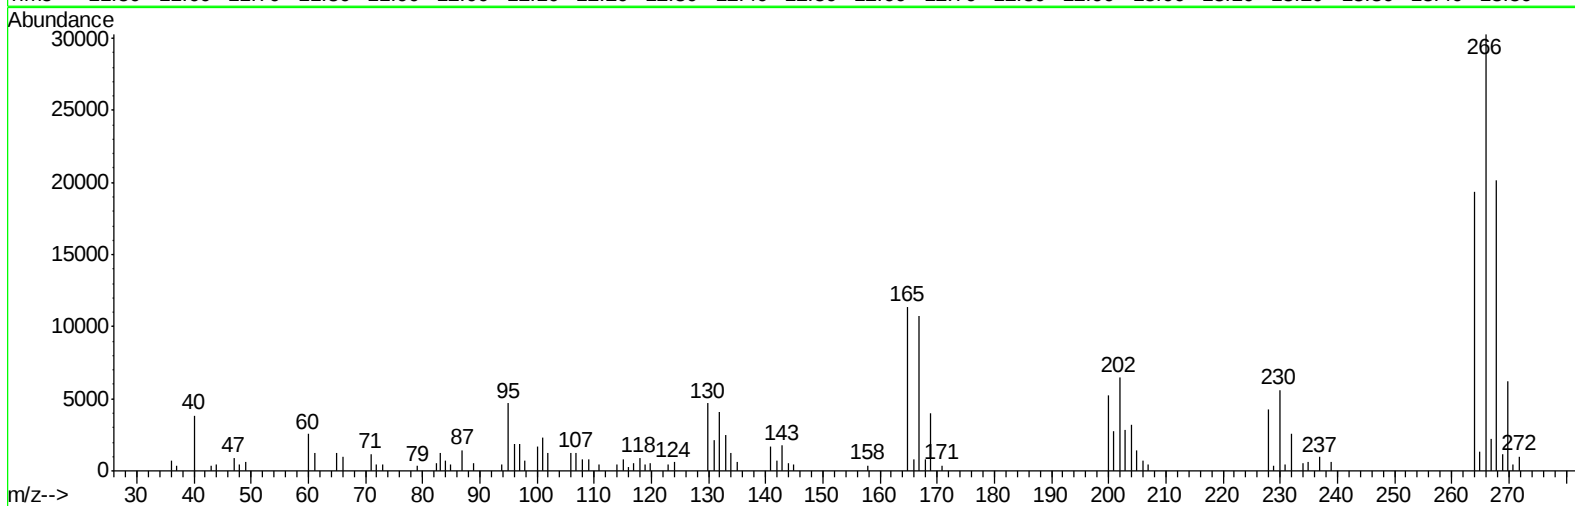


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF051815\  
Data File : BF079310.D  
Acq On : 18 May 2015 10:52  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 05:44:54 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF043015.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 19 05:25:25 2015  
Response via : Initial Calibration

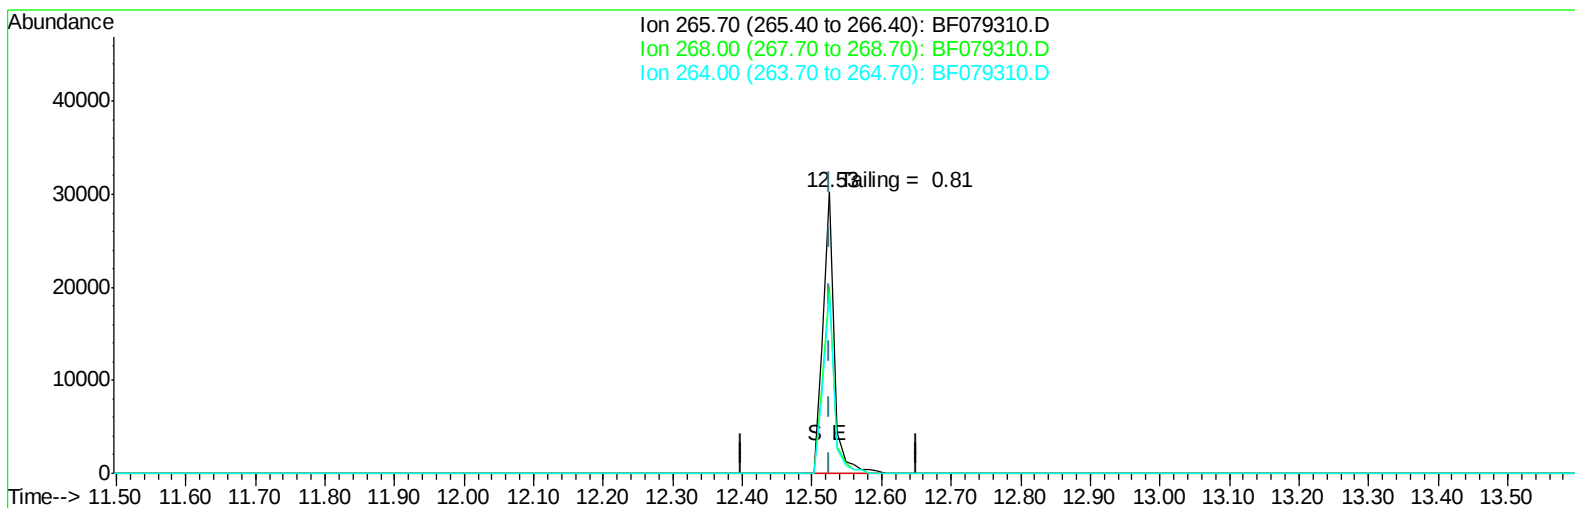

TIC: BF079310.D

(69) Pentachlorophenol (C)



12.525min (-0.000) 0.00ng

response 35119

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 68.80 | 66.44 |
| 264.00 | 63.60 | 64.01 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF051815\  
Data File : BF079310.D  
Acq On : 18 May 2015 10:52  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 05:44:54 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF043015.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 19 05:25:25 2015  
Response via : Initial Calibration

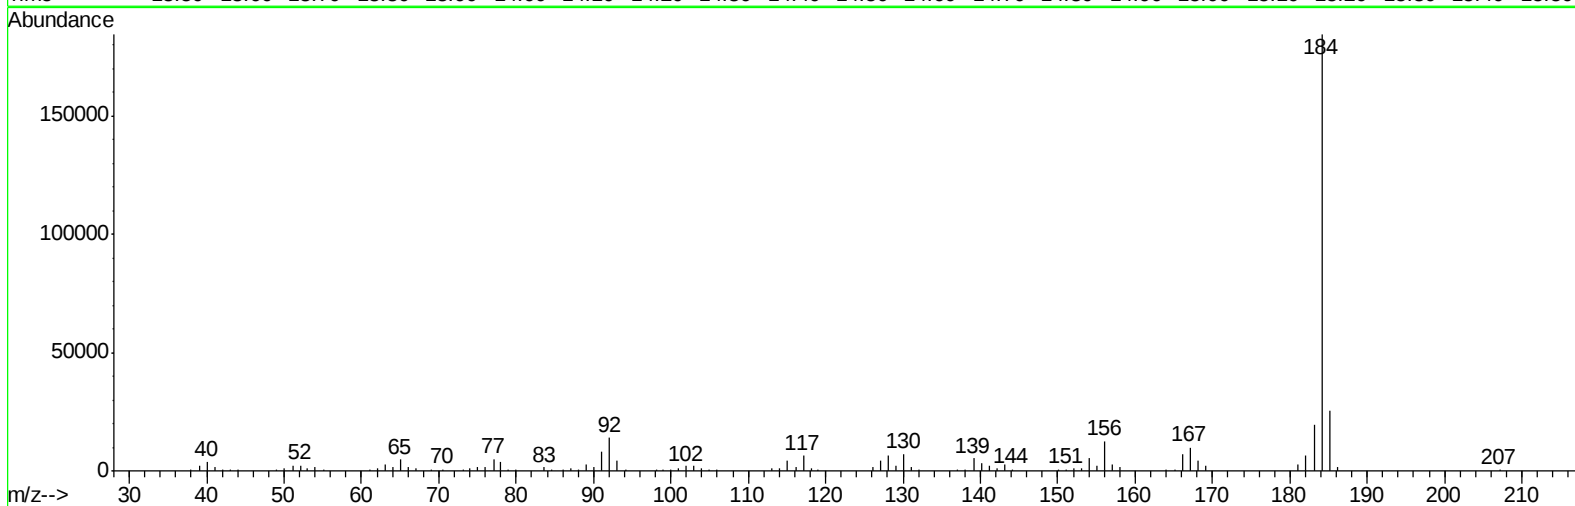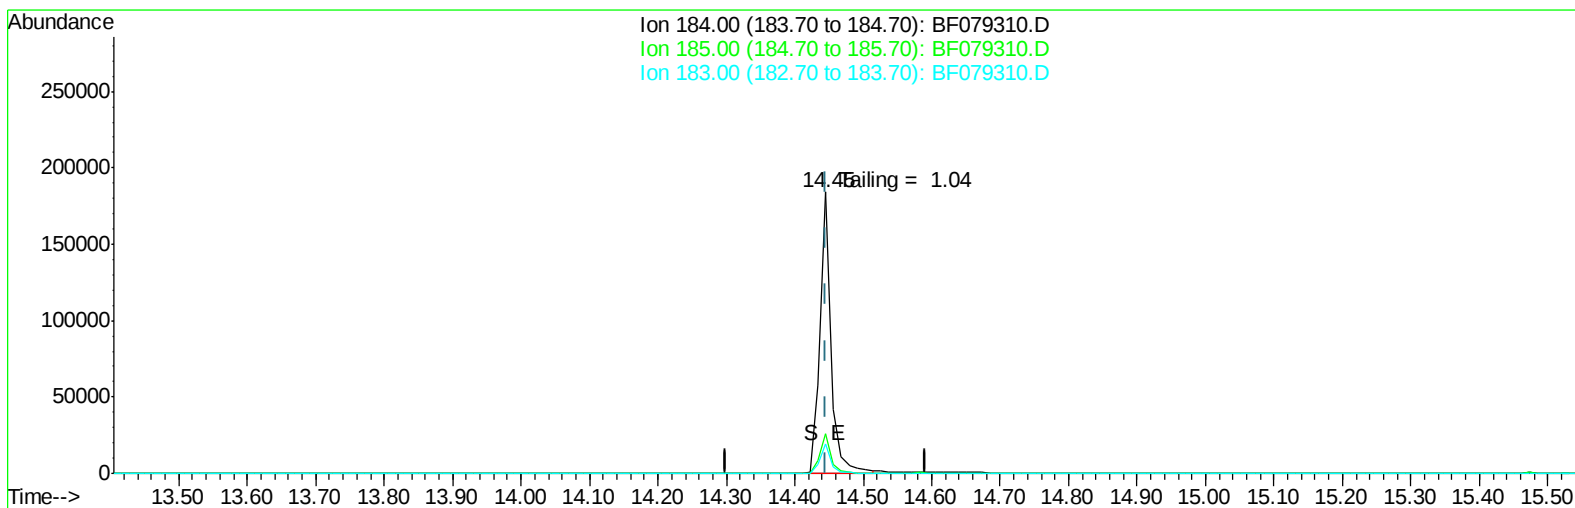

TIC: BF079310.D

(76) Benzidine

14.445min (-0.000) 0.00ng

response 213686

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.00 | 13.93 |
| 183.00 | 11.20 | 10.67 |
| 0.00   | 0.00  | 0.00  |