
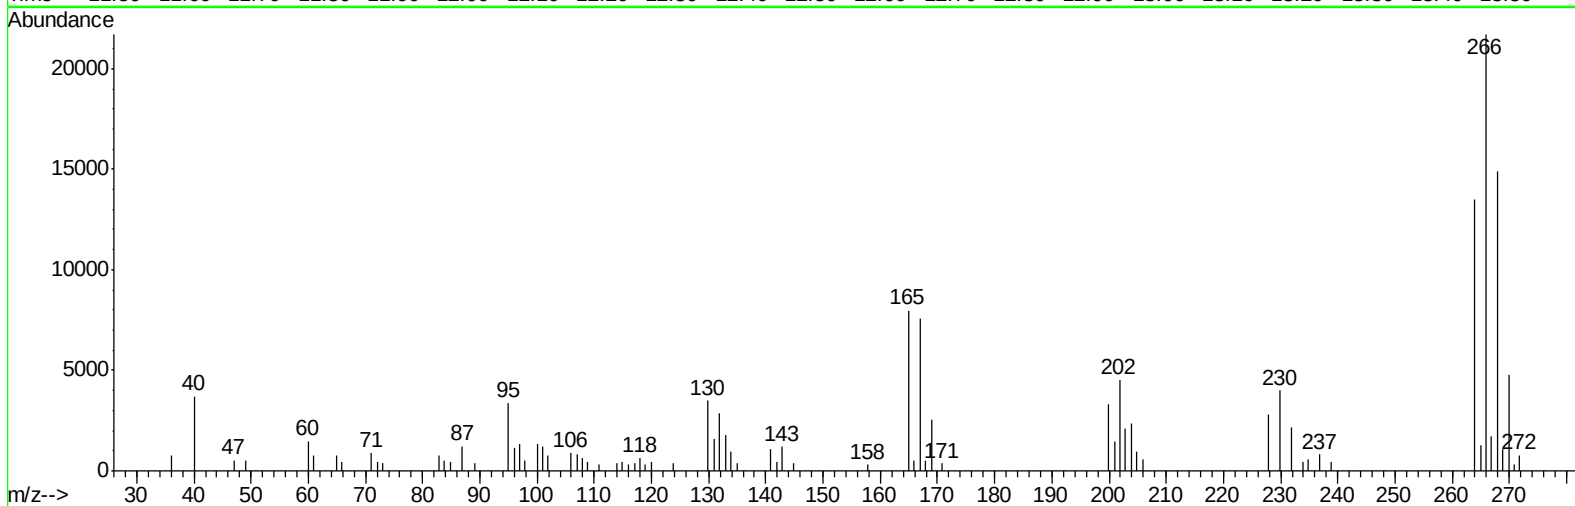


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051815\
Data File : BF079316.D
Acq On : 18 May 2015 20:24
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 05:45:42 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 19 05:25:25 2015
Response via : Initial Calibration

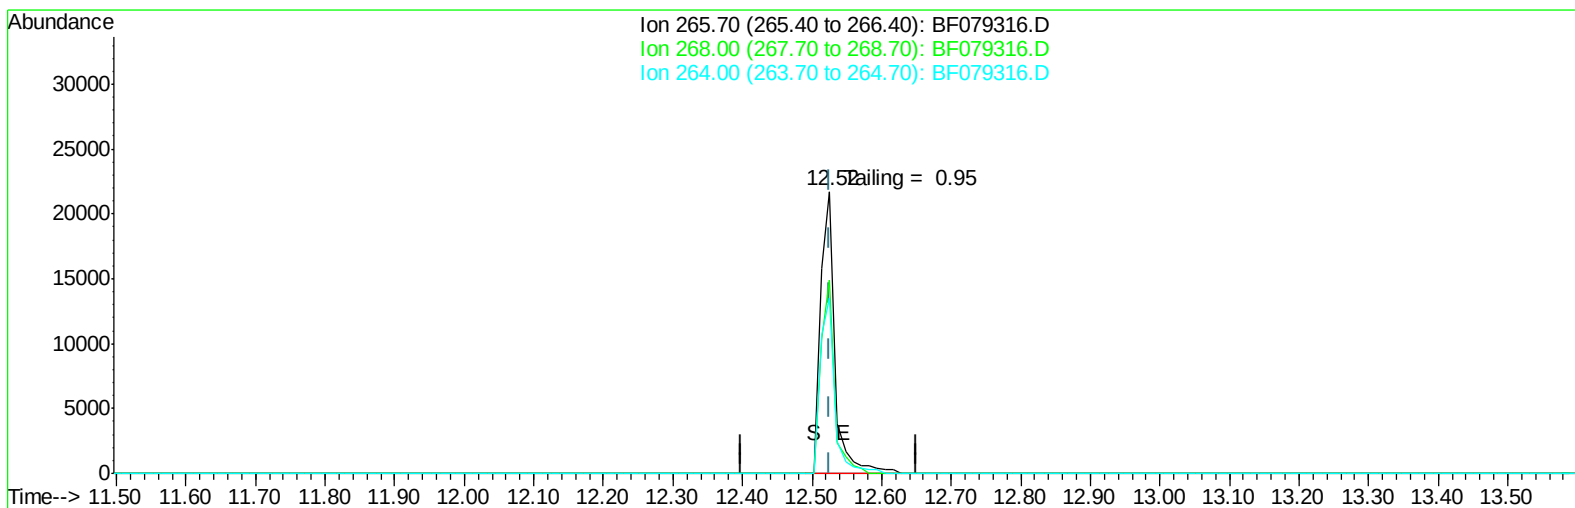

TIC: BF079316.D

(69) Pentachlorophenol (C)

12.525min (-0.000) 0.00ng

response 31426

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	68.56
264.00	63.60	62.07
0.00	0.00	0.00

