

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051816\
 Data File : BF087158.D
 Acq On : 18 May 2016 22:13
 Operator : UM/SJ
 Sample : H3143-29
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 3-AB-AC(0-2)

Quant Time: May 19 03:53:02 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 16:55:01 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.58	152	129088	20.00	ng	-0.02
21) Naphthalene-d8	7.86	136	533807	20.00	ng	-0.03
38) Acenaphthene-d10	9.61	164	259208	20.00	ng	-0.03
63) Phenanthrene-d10	11.08	188	472941	20.00	ng	-0.03
75) Chrysene-d12	13.71	240	357668	20.00	ng	-0.05
86) Perylene-d12	15.06	264	323643	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	681198	88.70	ng	-0.03
7) Phenol-d6	6.24	99	850107	82.53	ng	-0.05
23) Nitrobenzene-d5	7.15	82	621015	57.98	ng	-0.03
41) 2,4,6-Tribromophenol	10.40	330	201515	70.35	ng	-0.05
44) 2-Fluorobiphenyl	8.95	172	942152	60.20	ng	-0.03
78) Terphenyl-d14	12.67	244	765760	48.43	ng	-0.03
Target Compounds						Qvalue
9) Benzaldehyde	6.35	77	17921	2.32	ng	86
19) n-Nitroso-di-n-propylamine	7.15	70	85794	10.96	ng	# 76
25) Isophorone	7.15	82	494430	25.22	ng	# 68
49) Dimethylphthalate	9.35	163	125476	6.35	ng	100
50) 2,6-Dinitrotoluene	9.61	165	33001	7.69	ng	# 21
56) 2,4-Dinitrotoluene	9.61	165	33001	6.00	ng	# 16
66) 4-Bromophenyl-phenylether	10.40	248	12826	2.64	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051816\
Data File : BF087158.D
Acq On : 18 May 2016 22:13
Operator : UM/SJ
Sample : H3143-29
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
3-AB-AC(0-2)

Quant Time: May 19 03:53:02 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 16:55:01 2016
Response via : Initial Calibration

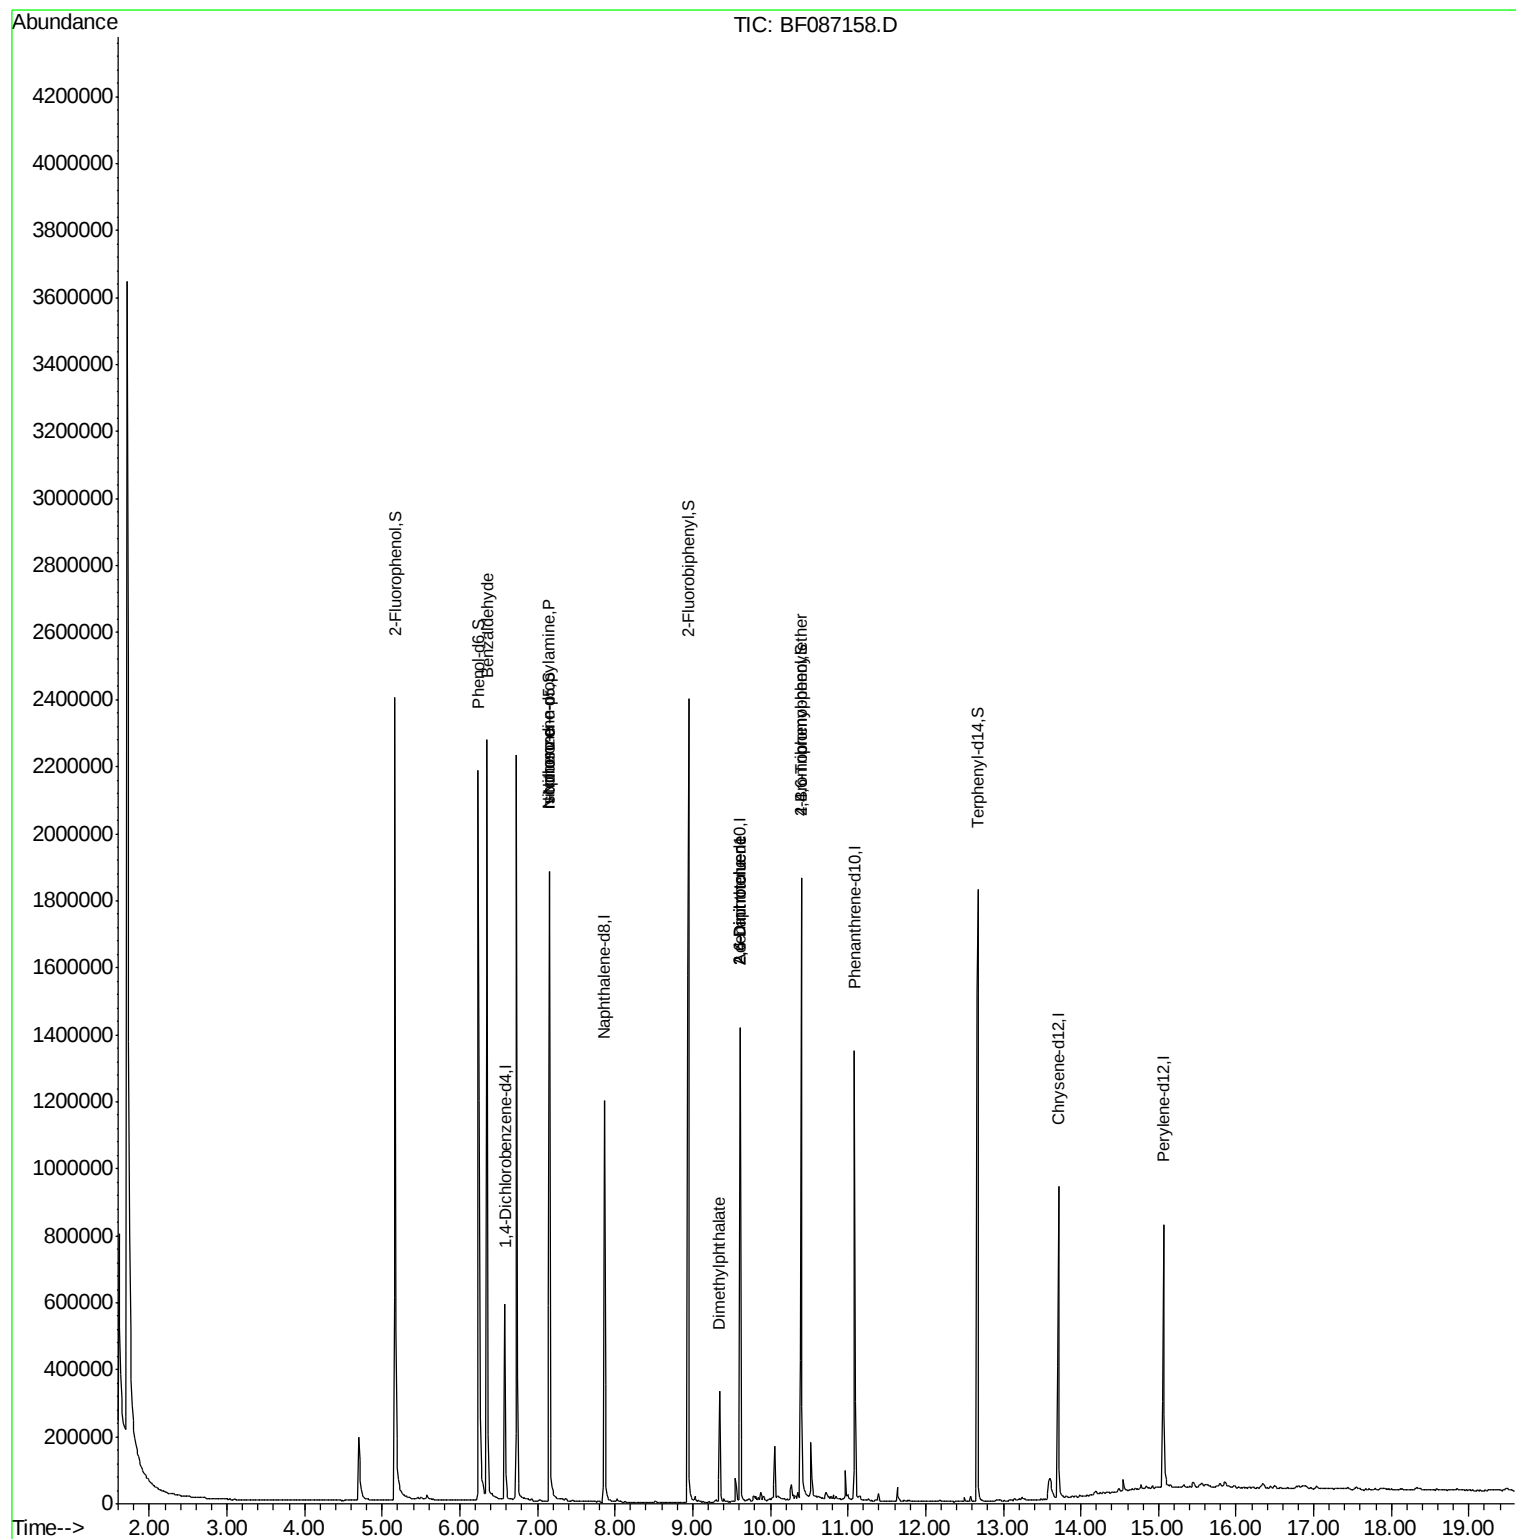



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.58 min Scan# 437

Delta R.T. -0.02 min

Lab File: BF087158.D

Acq: 18 May 2016 22:13

Instrument :

BNA_F

ClientSampleId :

3-AB-AC(0-2)


Tgt Ion:152 Resp: 129088

Ion Ratio Lower Upper

152 100

150 152.3 125.8 188.6




115 56.5 51.5 77.3

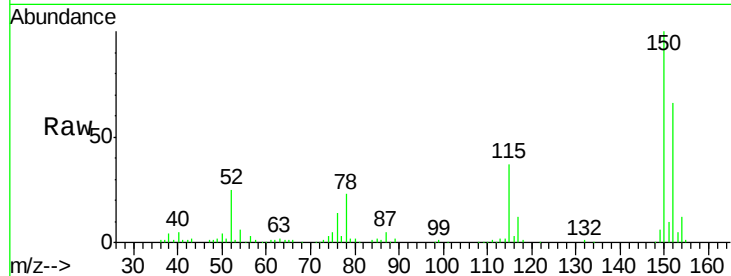

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

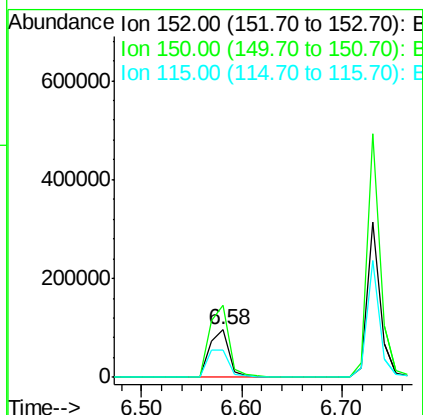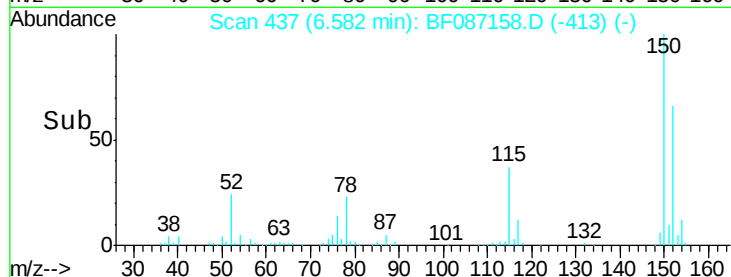

#5

2-Fluorophenol

Concen: 88.70 ng

RT: 5.16 min Scan# 313

Delta R.T. -0.03 min

Lab File: BF087158.D

Acq: 18 May 2016 22:13


Tgt Ion:112 Resp: 681198

Ion Ratio Lower Upper

112 100

64 69.2 52.1 78.1



63 37.5 25.7 38.5



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

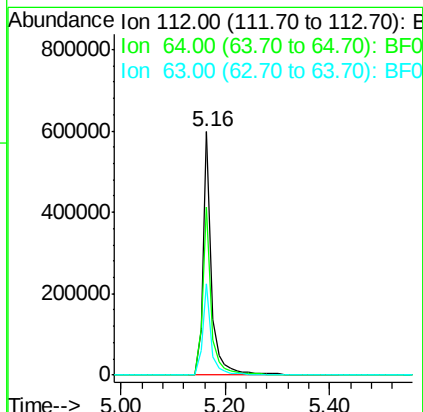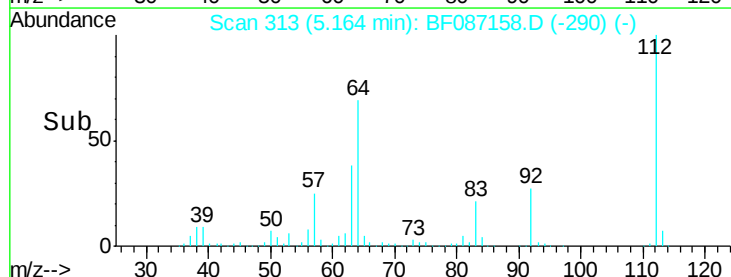



#7

Phenol-d6

Concen: 82.53 ng

RT: 6.24 min Scan# 407

Delta R.T. -0.05 min

Lab File: BF087158.D

Acq: 18 May 2016 22:13

Instrument :

BNA_F

ClientSampleId :

3-AB-AC(0-2)


Tgt Ion: 99 Resp: 850107

Ion Ratio Lower Upper

99 100

42 32.8 13.6 20.4#




71 40.2 24.6 36.8#

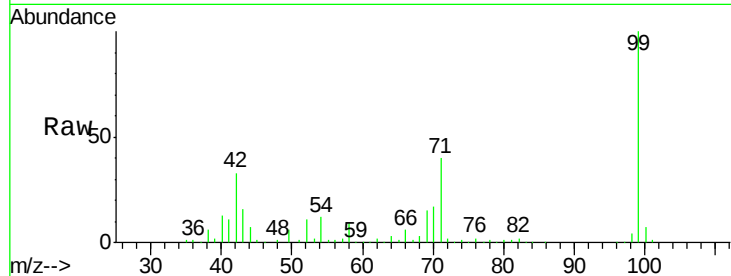

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

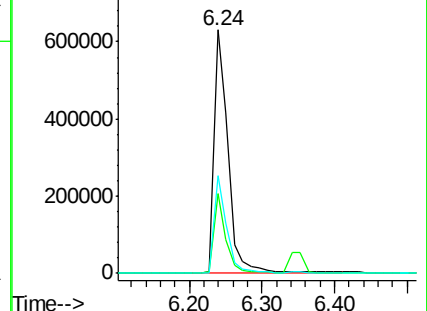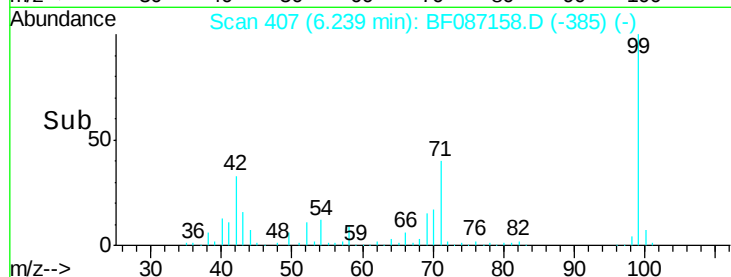

#9

Benzaldehyde

Concen: 2.32 ng

RT: 6.35 min Scan# 417

Delta R.T. 0.21 min

Lab File: BF087158.D

Acq: 18 May 2016 22:13


Tgt Ion: 77 Resp: 17921

Ion Ratio Lower Upper

77 100

105 84.2 72.7 112.7



106 72.3 70.8 110.8






Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): BF0

Ion 106.00 (105.70 to 106.70): BF0



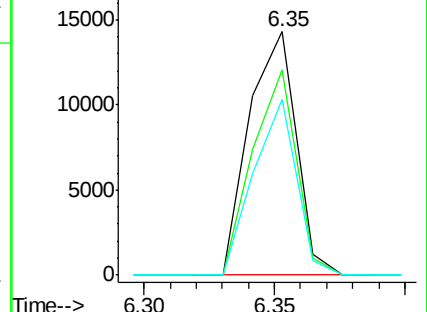
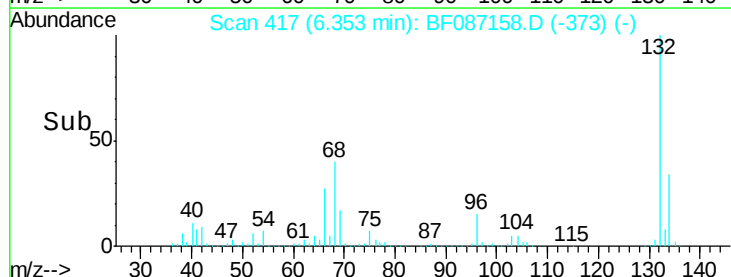


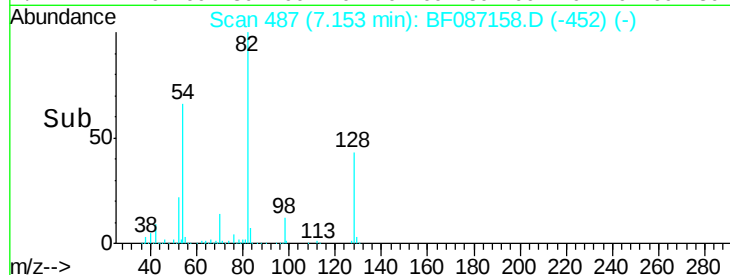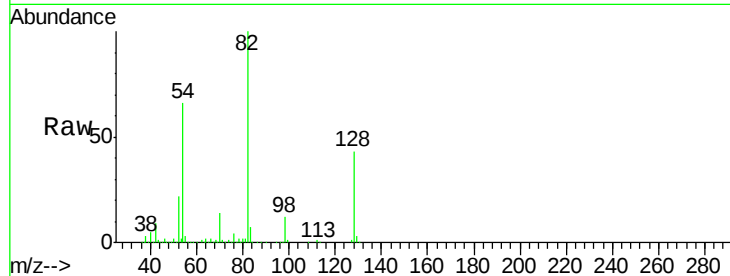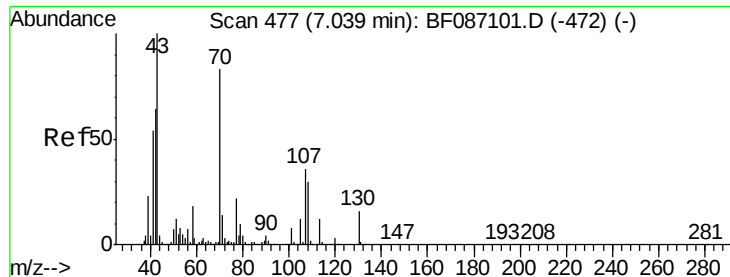

#19
n-Nitroso-di-n-propylamine
Concen: 10.96 ng
RT: 7.15 min Scan# 487
Delta R.T. 0.10 min
Lab File: BF087158.D
Acq: 18 May 2016 22:13


Instrument :
BNA_F
ClientSampleId :
3-AB-AC(0-2)


Tgt Ion: 70 Resp: 85794
Ion Ratio Lower Upper
70 100
42 64.1 43.1 64.7
101 0.0 8.1 12.1#
130 1.8 18.6 28.0#

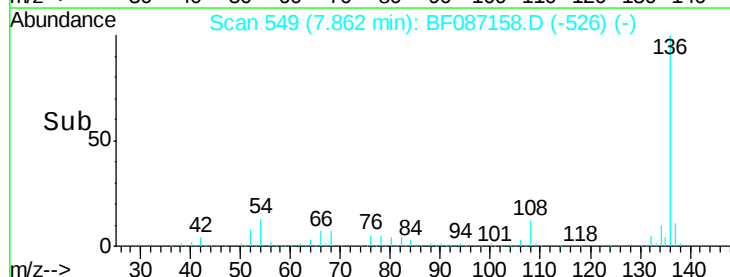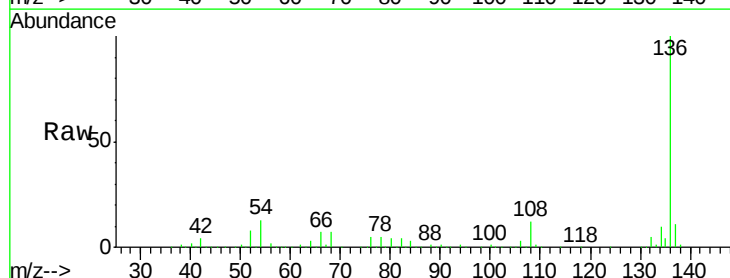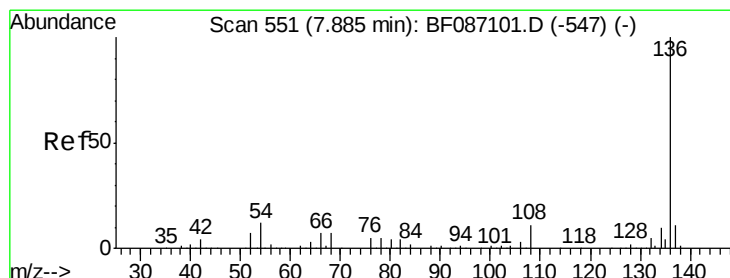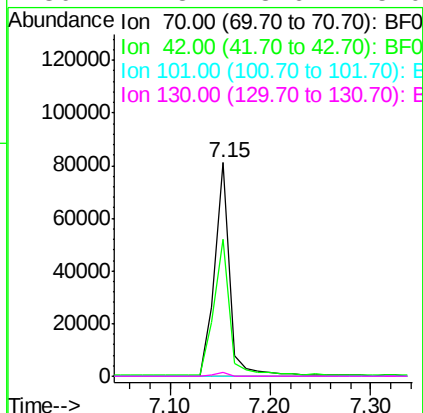

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.86 min Scan# 549
Delta R.T. -0.03 min
Lab File: BF087158.D
Acq: 18 May 2016 22:13

Tgt Ion: 136 Resp: 533807
Ion Ratio Lower Upper
136 100
137 11.2 8.8 13.2
54 13.5 5.0 7.4#
68 7.1 4.4 6.6#




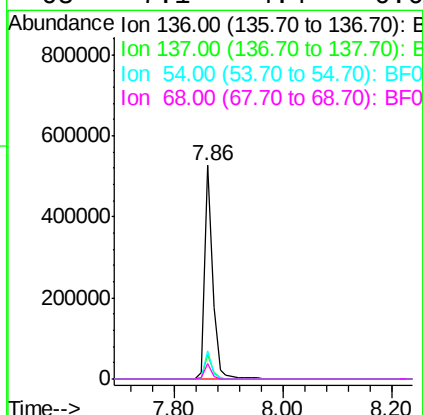


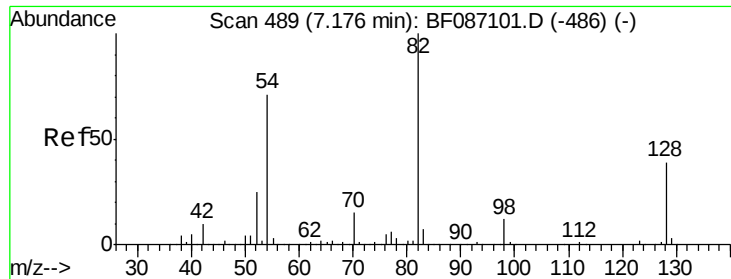

#23
Nitrobenzene-d5
Concen: 57.98 ng
RT: 7.15 min Scan# 487
Delta R.T. -0.03 min
Lab File: BF087158.D
Acq: 18 May 2016 22:13




Instrument :
BNA_F
ClientSampleId :
3-AB-AC(0-2)


Tgt Ion	Ratio	Lower	Upper
82	100		
128	42.6	40.6	61.0
54	65.8	38.1	57.1#

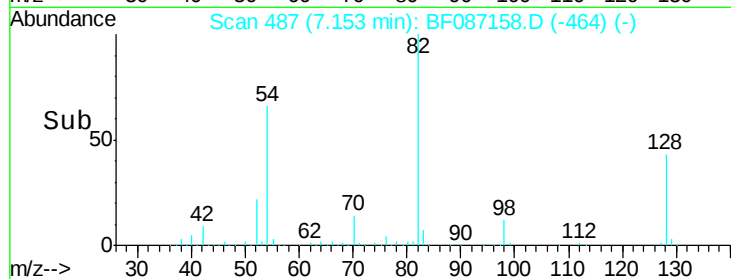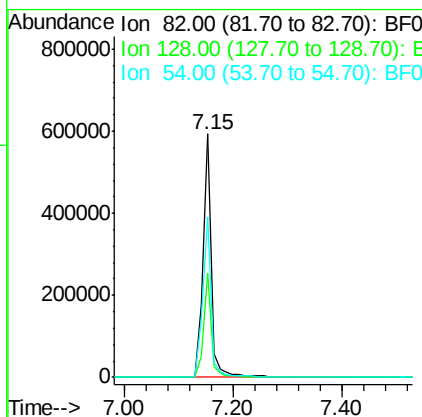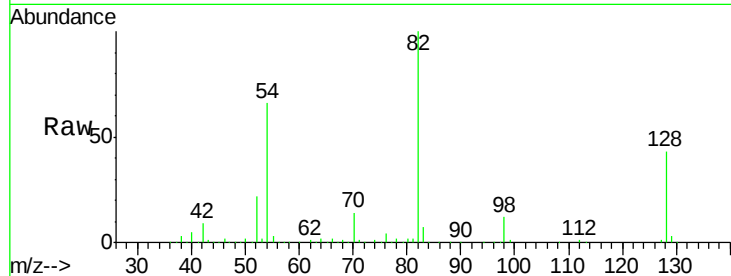

#25
Isophorone
Concen: 25.22 ng
RT: 7.15 min Scan# 487
Delta R.T. -0.30 min
Lab File: BF087158.D
Acq: 18 May 2016 22:13

Tgt Ion	Ratio	Lower	Upper
82	100		
95	0.0	5.1	7.7#
138	0.0	12.4	18.6#

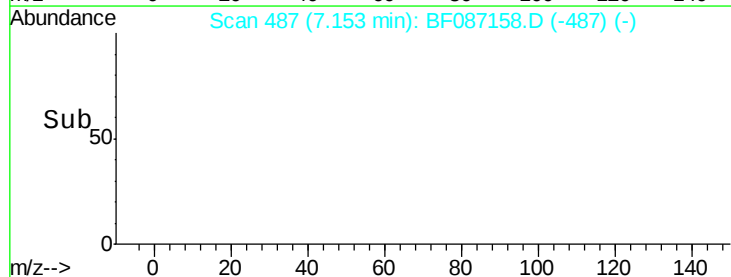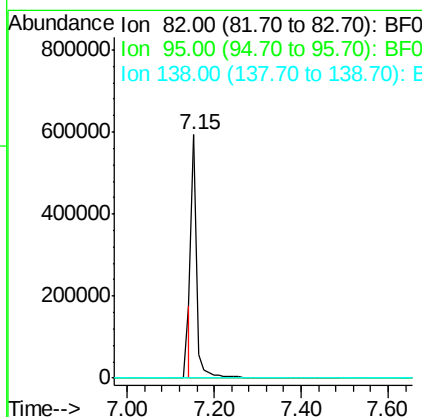

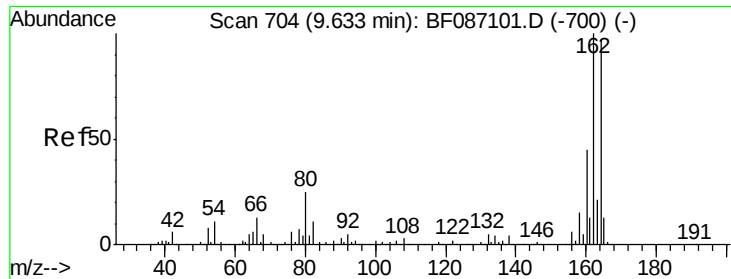

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.61 min Scan# 702

Delta R.T. -0.03 min

Lab File: BF087158.D

Acq: 18 May 2016 22:13

Instrument :

BNA_F

ClientSampleId :

3-AB-AC(0-2)


Tgt Ion:164 Resp: 259208

Ion Ratio Lower Upper

164 100

162 104.1 82.8 124.2




160 46.2 36.9 55.3

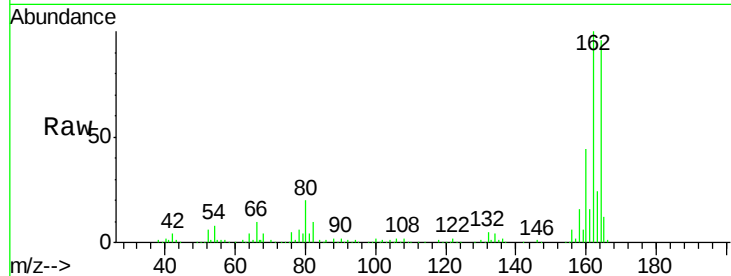

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

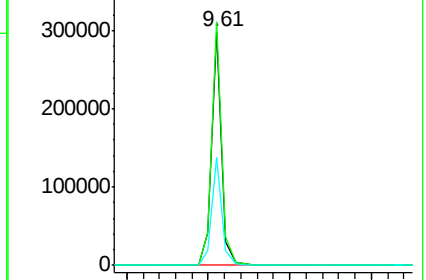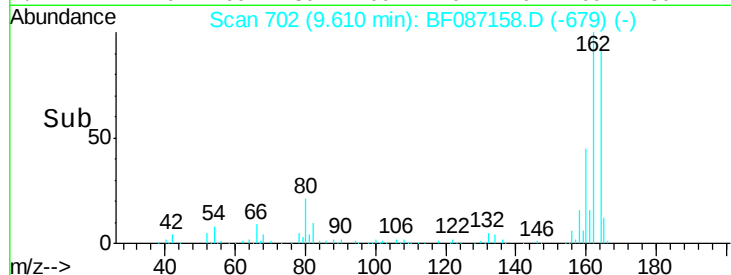

#41

2,4,6-Tribromophenol

Concen: 70.35 ng

RT: 10.40 min Scan# 771

Delta R.T. -0.05 min

Lab File: BF087158.D

Acq: 18 May 2016 22:13


Tgt Ion:330 Resp: 201515

Ion Ratio Lower Upper

330 100

332 96.6 79.0 118.4



141 39.8 31.2 46.8




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



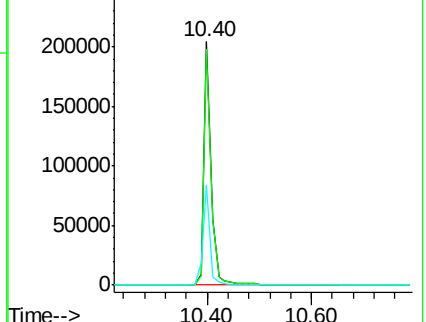
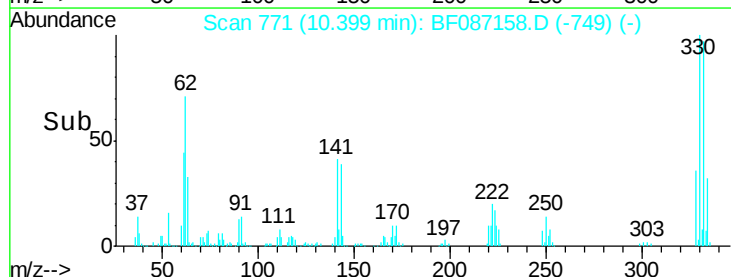


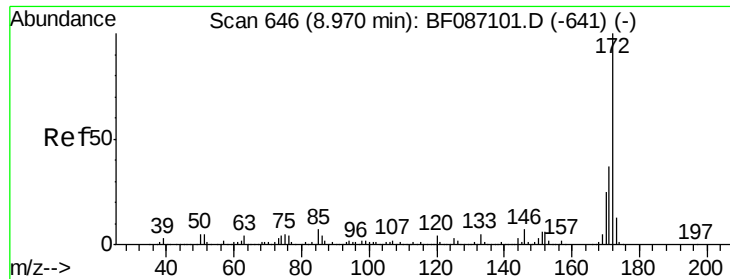

#44
 2-Fluorobiphenyl
 Concen: 60.20 ng
 RT: 8.95 min Scan# 644
 Delta R.T. -0.03 min
 Lab File: BF087158.D
 Acq: 18 May 2016 22:13




Instrument :
 BNA_F
 ClientSampleId :
 3-AB-AC(0-2)


Tgt Ion:172 Resp: 942152
 Ion Ratio Lower Upper
 172 100
 171 35.6 29.0 43.6
 170 24.0 19.8 29.8

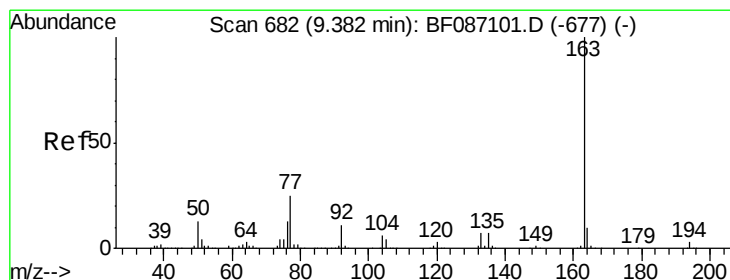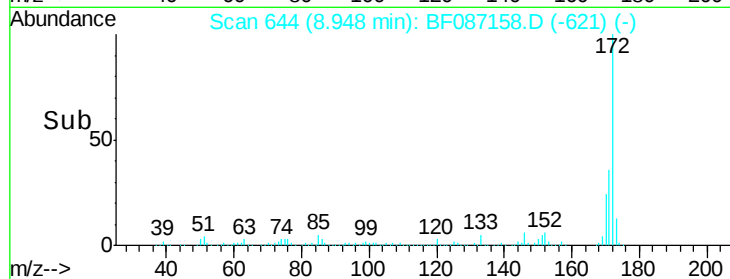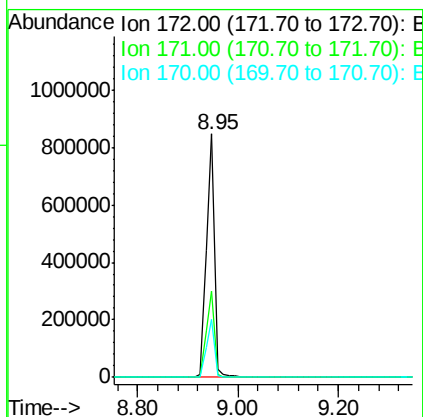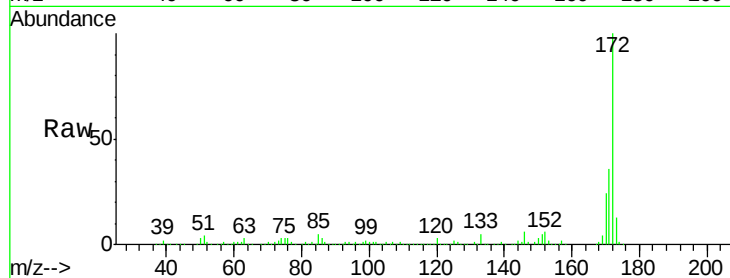

#49
 Dimethylphthalate
 Concen: 6.35 ng
 RT: 9.35 min Scan# 679
 Delta R.T. -0.05 min
 Lab File: BF087158.D
 Acq: 18 May 2016 22:13

Tgt Ion:163 Resp: 125476
 Ion Ratio Lower Upper
 163 100
 194 3.4 2.6 4.0
 164 10.2 8.2 12.4

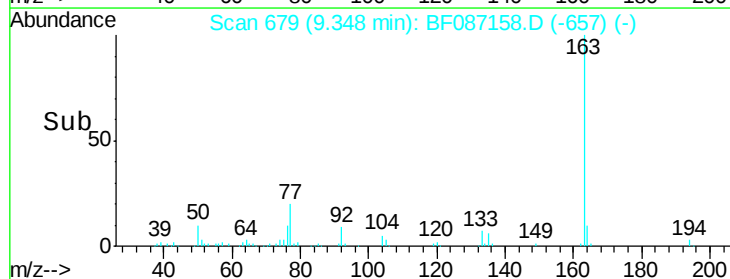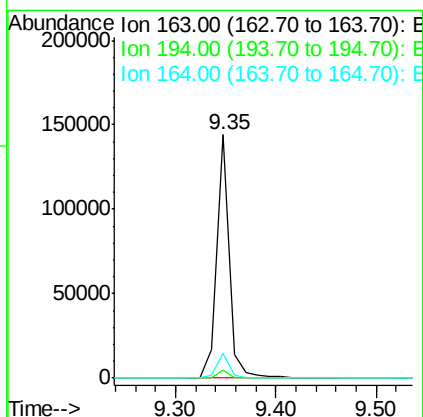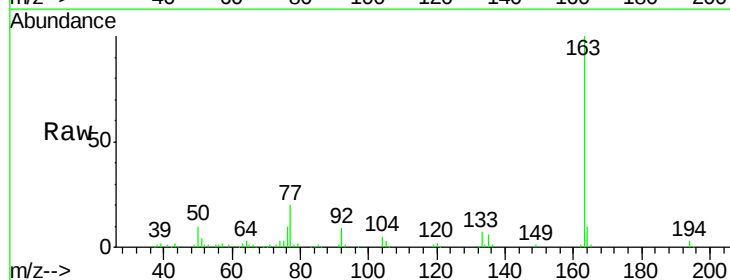

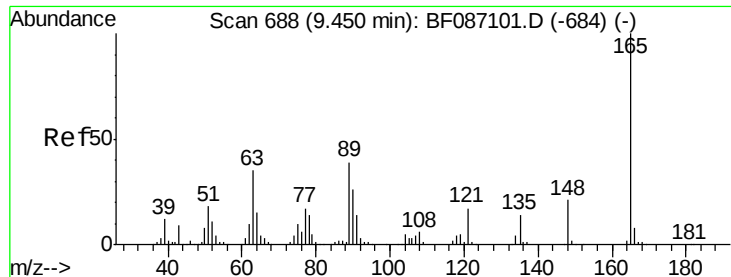

#50

2,6-Dinitrotoluene

Concen: 7.69 ng

RT: 9.61 min Scan# 702

Delta R.T. 0.15 min

Lab File: BF087158.D

Acq: 18 May 2016 22:13

Instrument :

BNA_F

ClientSampleId :

3-AB-AC(0-2)


Tgt Ion:165 Resp: 33001

Ion Ratio Lower Upper

165 100

63 2.0 51.8 77.8#




89 1.7 50.7 76.1#



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

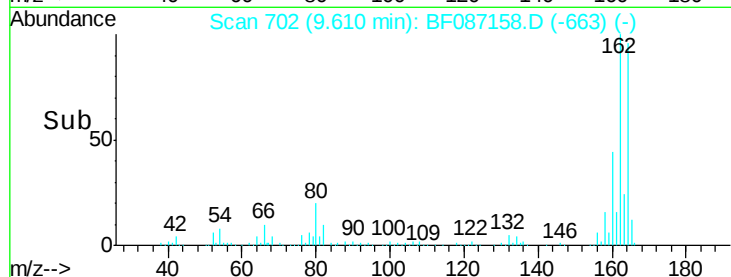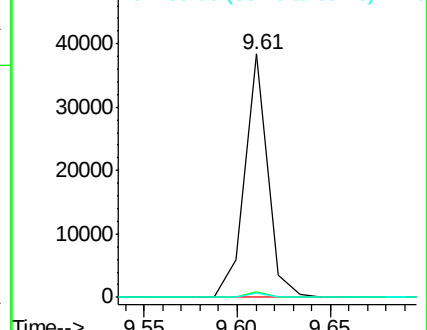

#56

2,4-Dinitrotoluene

Concen: 6.00 ng

RT: 9.61 min Scan# 702

Delta R.T. -0.25 min

Lab File: BF087158.D

Acq: 18 May 2016 22:13

Tgt Ion:165 Resp: 33001


Ion Ratio Lower Upper

165 100

63 2.0 44.3 66.5#

89 1.7 70.0 105.0#

182 0.0 1.8 2.6#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E



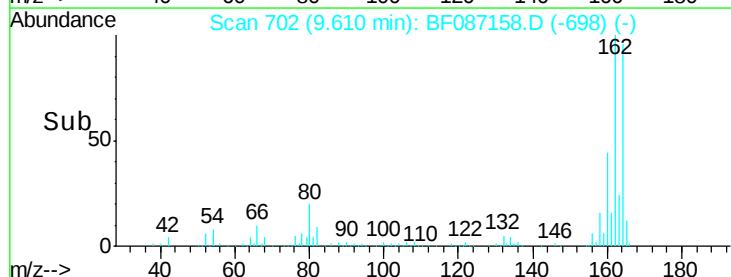
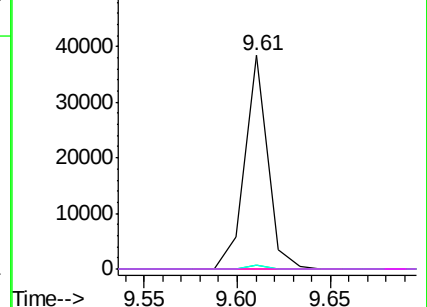


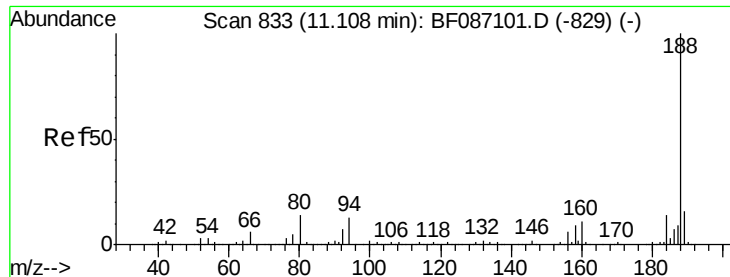

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.08 min Scan# 831
 Delta R.T. -0.03 min
 Lab File: BF087158.D
 Acq: 18 May 2016 22:13




Instrument :
 BNA_F
 ClientSampleId :
 3-AB-AC(0-2)


Tgt Ion:188 Resp: 472941
 Ion Ratio Lower Upper
 188 100
 94 11.1 6.8 10.2#
 80 12.7 7.1 10.7#

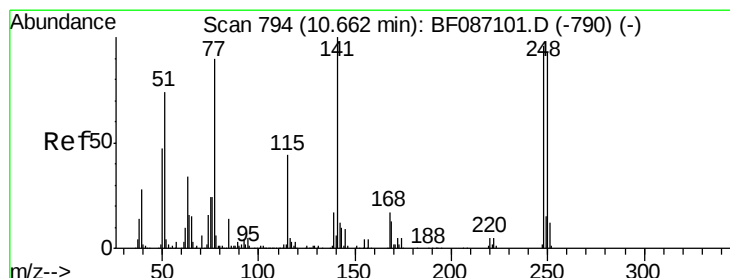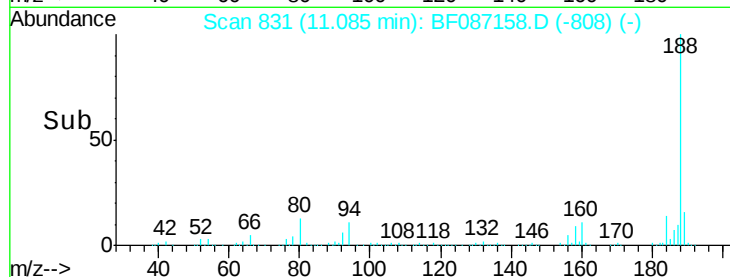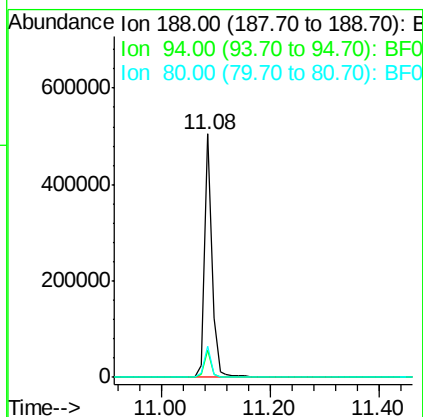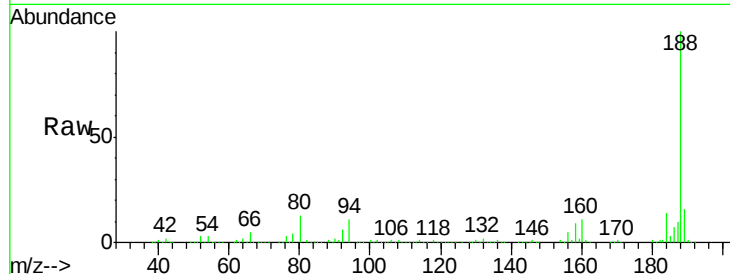

#66
 4-Bromophenyl-phenylether
 Concen: 2.64 ng
 RT: 10.40 min Scan# 771
 Delta R.T. -0.27 min
 Lab File: BF087158.D
 Acq: 18 May 2016 22:13

Tgt Ion:248 Resp: 12826
 Ion Ratio Lower Upper
 248 100
 250 194.1 78.6 117.8#
 141 563.3 76.0 114.0#

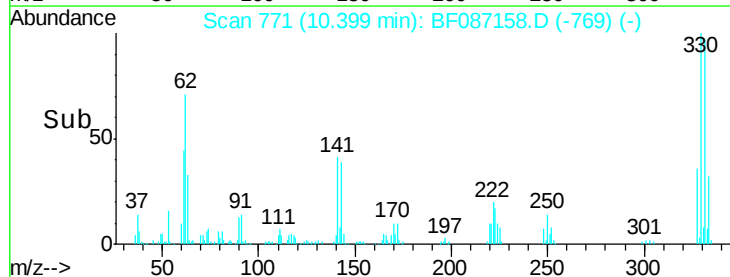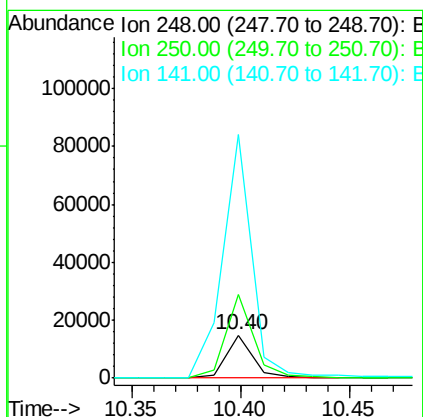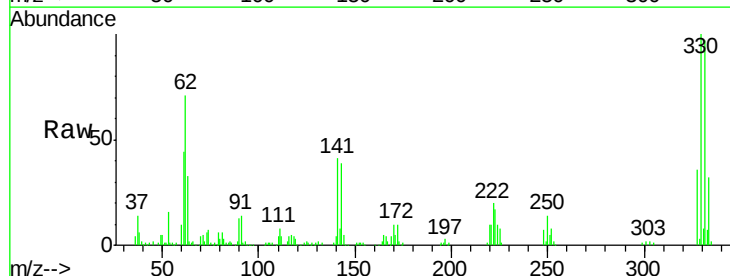

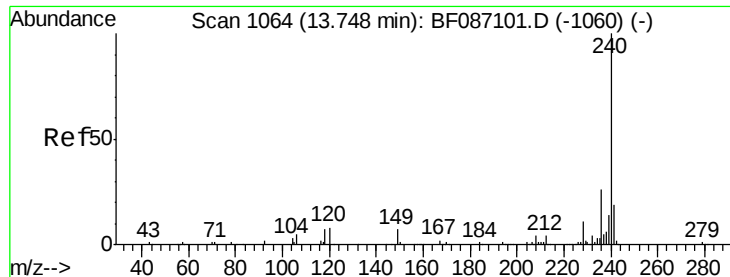

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.71 min Scan# 1061

Delta R.T. -0.05 min

Lab File: BF087158.D

Acq: 18 May 2016 22:13

Instrument :

BNA_F

ClientSampleId :

3-AB-AC(0-2)


Tgt Ion:240 Resp: 357668

Ion Ratio Lower Upper

240 100

120 8.9 11.2 16.8#




236 26.6 21.2 31.8

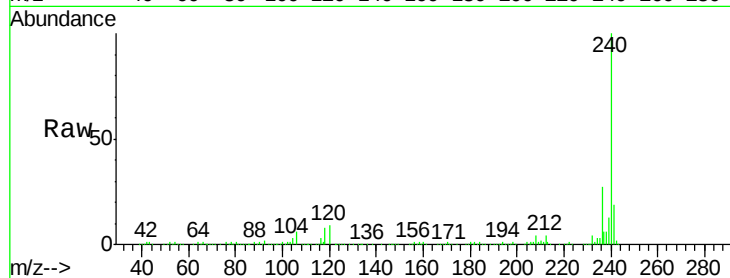

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

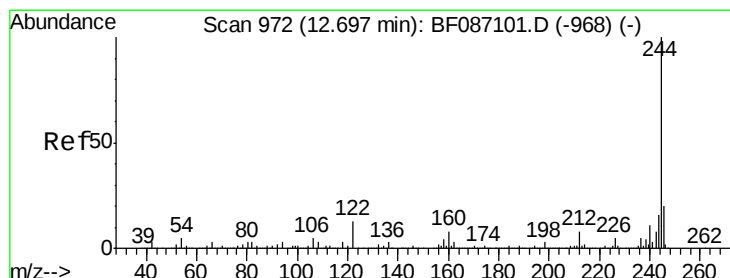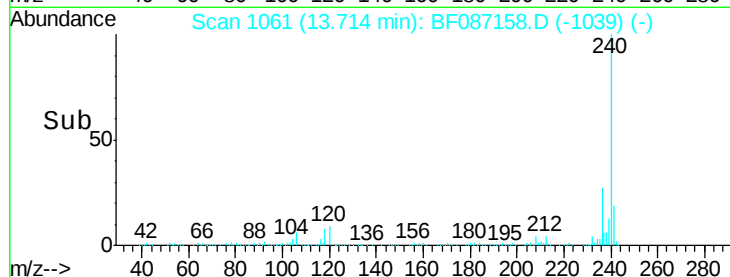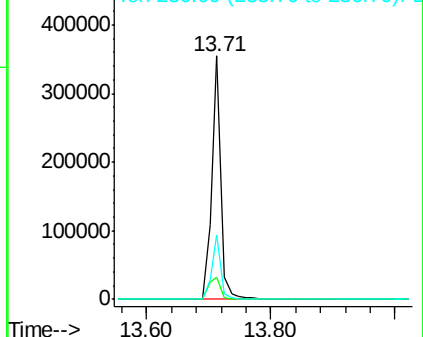

#78

Terphenyl-d14

Concen: 48.43 ng

RT: 12.67 min Scan# 970

Delta R.T. -0.03 min

Lab File: BF087158.D

Acq: 18 May 2016 22:13


Tgt Ion:244 Resp: 765760

Ion Ratio Lower Upper

244 100

212 7.0 6.2 9.2



122 7.9 12.0 18.0#

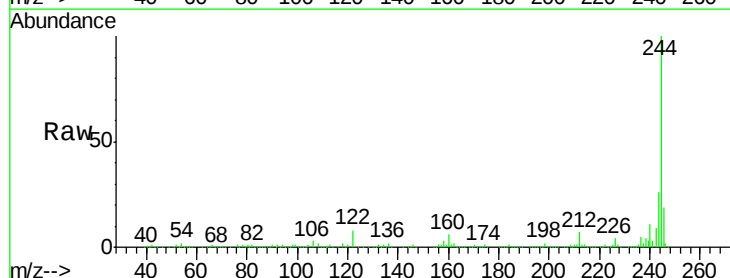


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

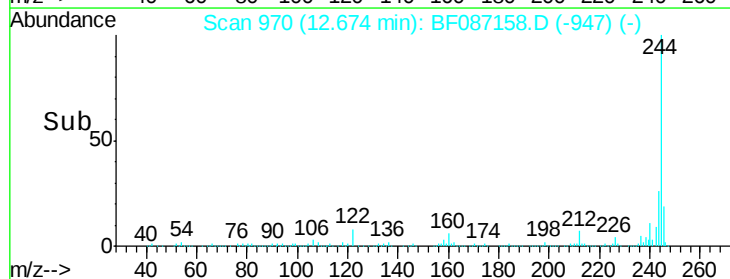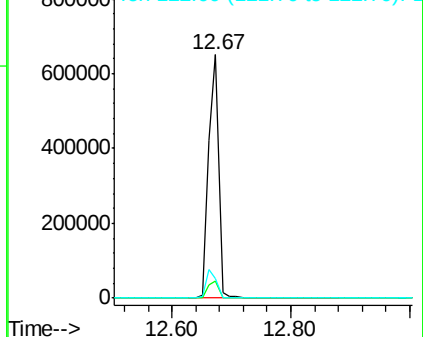


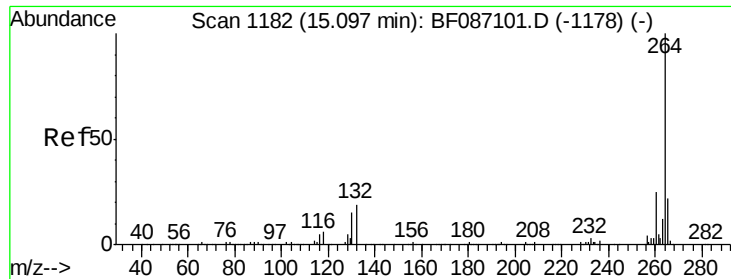

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.06 min Scan# 1179
Delta R.T. -0.05 min
Lab File: BF087158.D
Acq: 18 May 2016 22:13

Instrument :
BNA_F
ClientSampleId :
3-AB-AC(0-2)

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.1	19.5	29.3
265	21.5	17.3	25.9



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

