
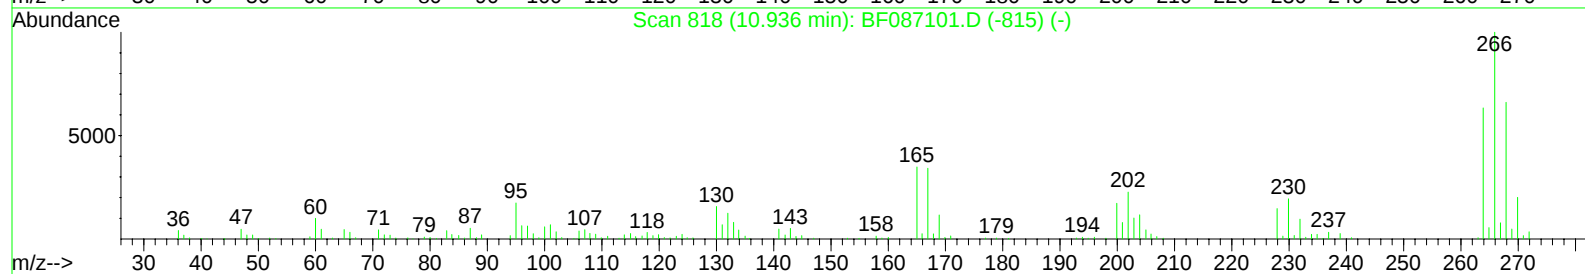
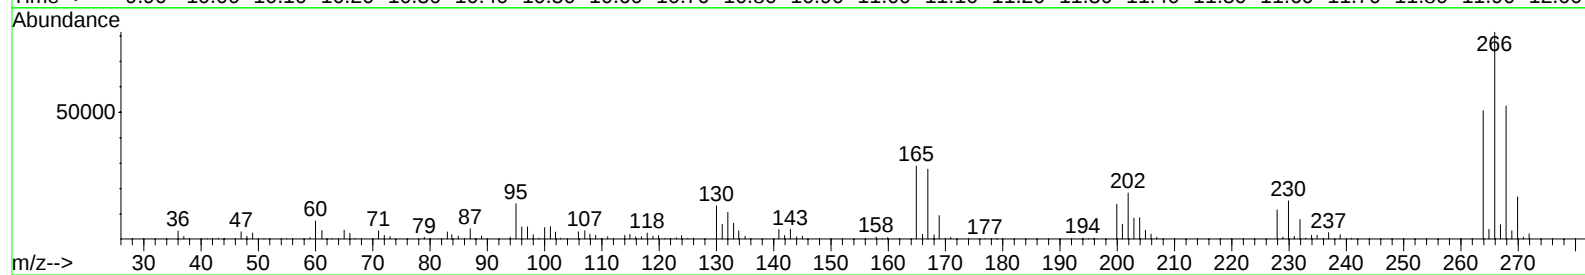


Data Path : Z:\HPCHEM1\BNA F\Data\BF051816\
Data File : BF087143.D
Acq On : 18 May 2016 13:21
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 18:39:13 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 18 17:13:00 2016
Response via : Initial Calibration

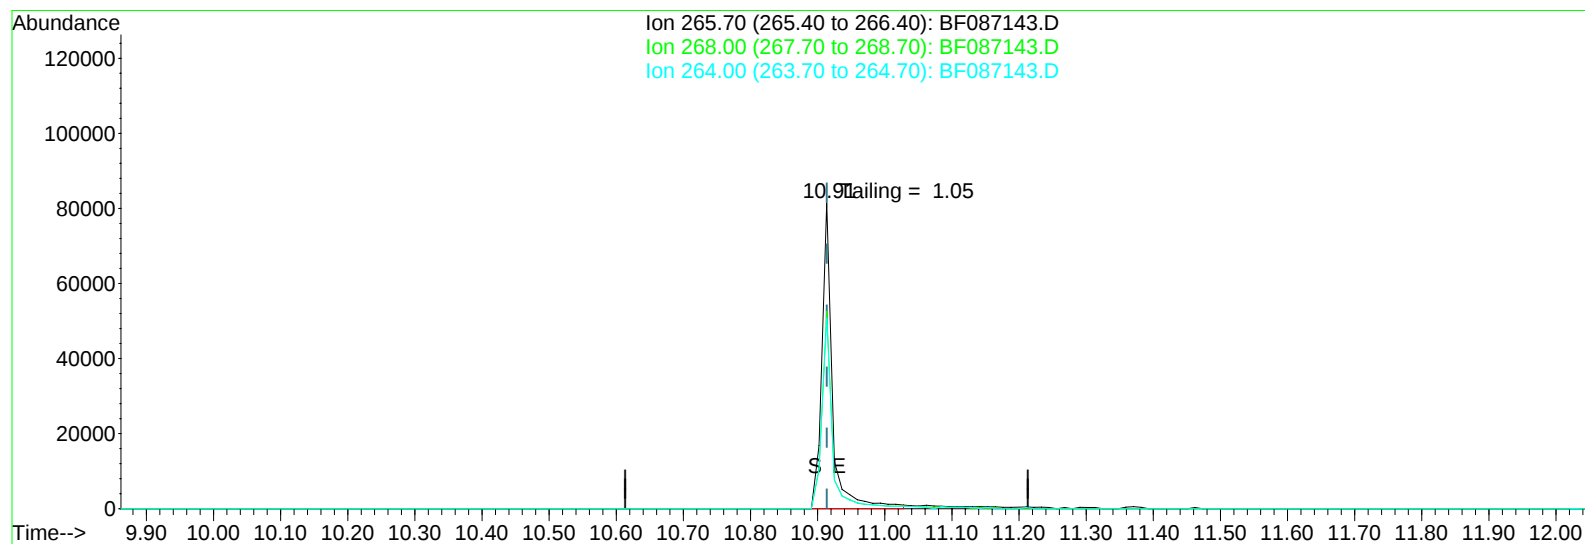

TIC: BF087143.D

(69) Pentachlorophenol (C)




10.914min (+0.000) 0.00ng

response 90342

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.45
264.00	66.10	62.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF051816\
Data File : BF087143.D
Acq On : 18 May 2016 13:21
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 18:39:13 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 18 17:13:00 2016
Response via : Initial Calibration

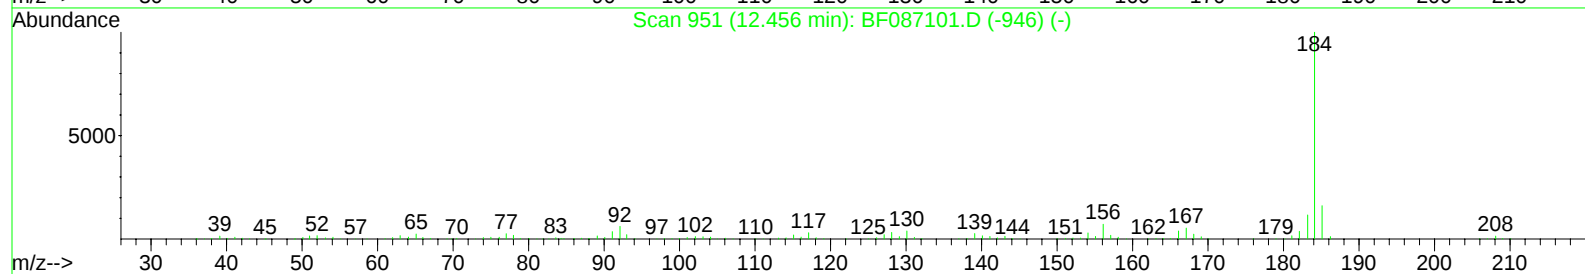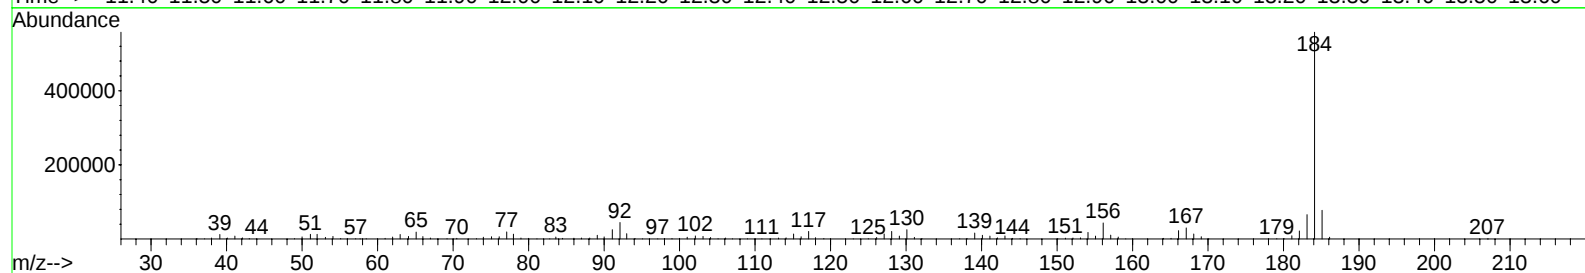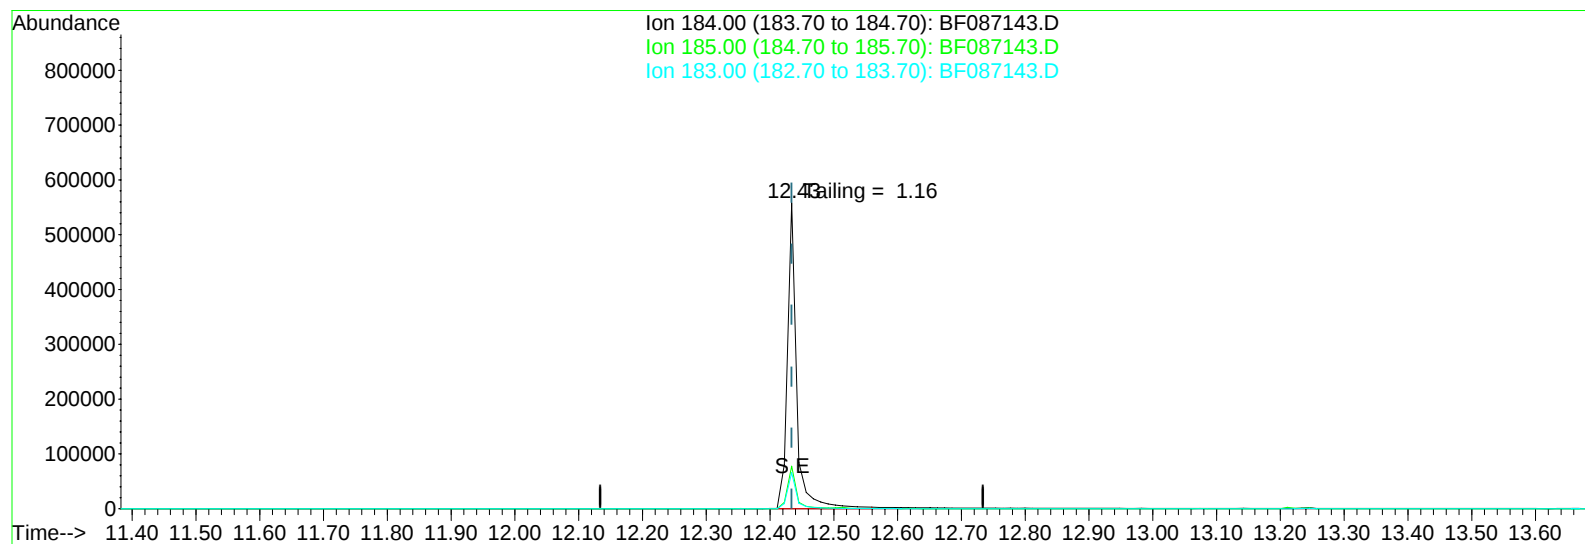

TIC: BF087143.D

(76) Benzidine

12.434min (+0.000) 0.00ng

response 573766

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	13.88
183.00	12.20	11.76
0.00	0.00	0.00