
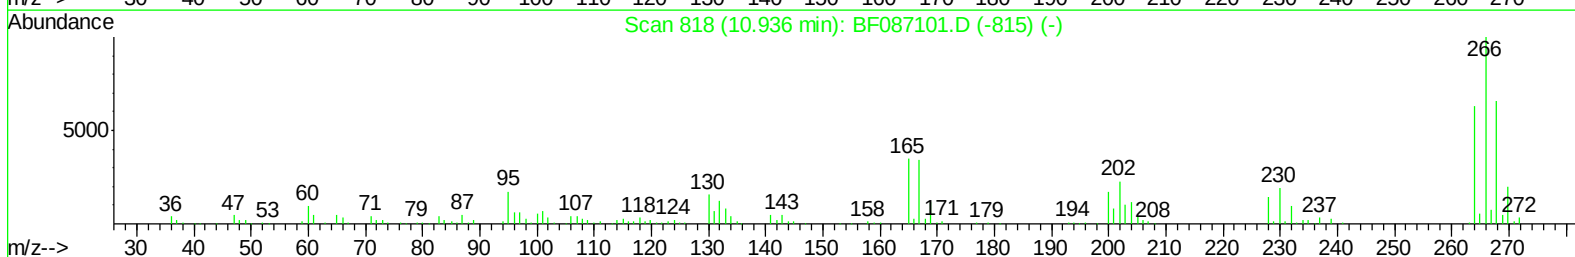
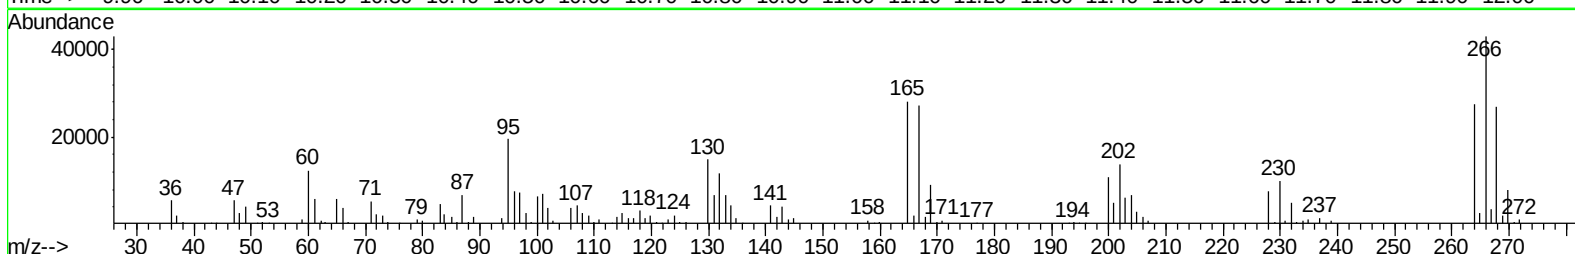


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051816\
Data File : BF087164.D
Acq On : 19 May 2016 1:54
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 08:04:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 16:55:01 2016
Response via : Initial Calibration

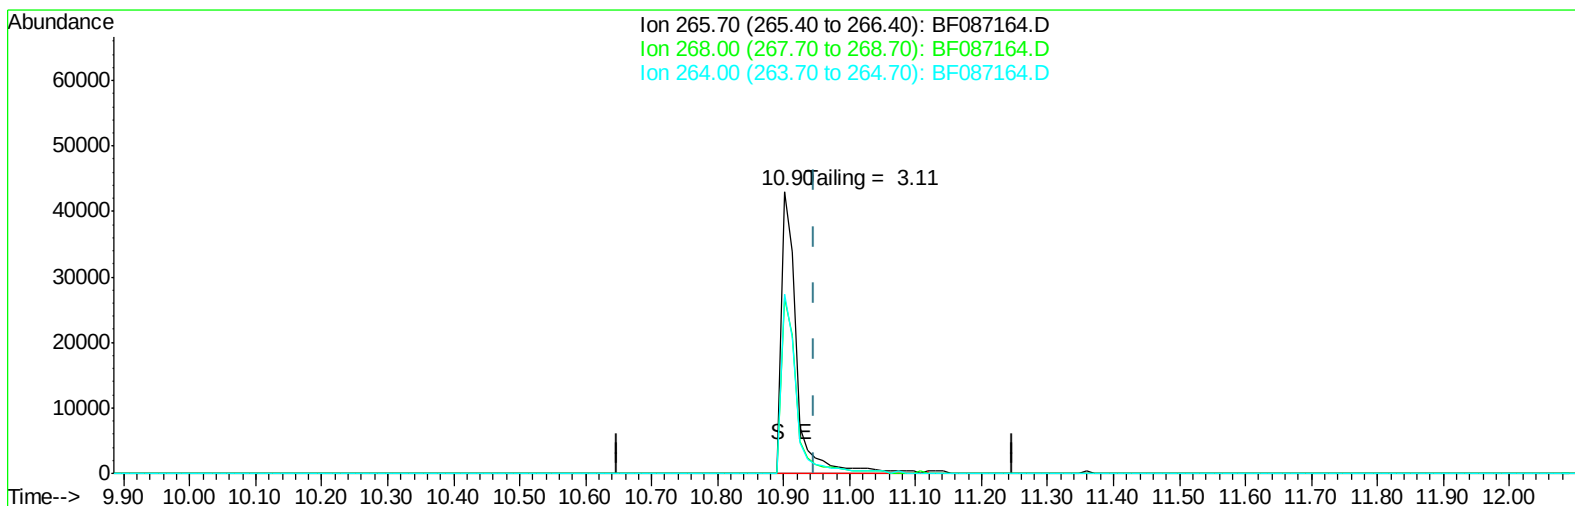

TIC: BF087164.D

(69) Pentachlorophenol (C)




10.902min (-0.046) 17959.72ng

response 68293

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.42
264.00	66.10	63.83
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051816\
Data File : BF087164.D
Acq On : 19 May 2016 1:54
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 08:04:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 16:55:01 2016
Response via : Initial Calibration

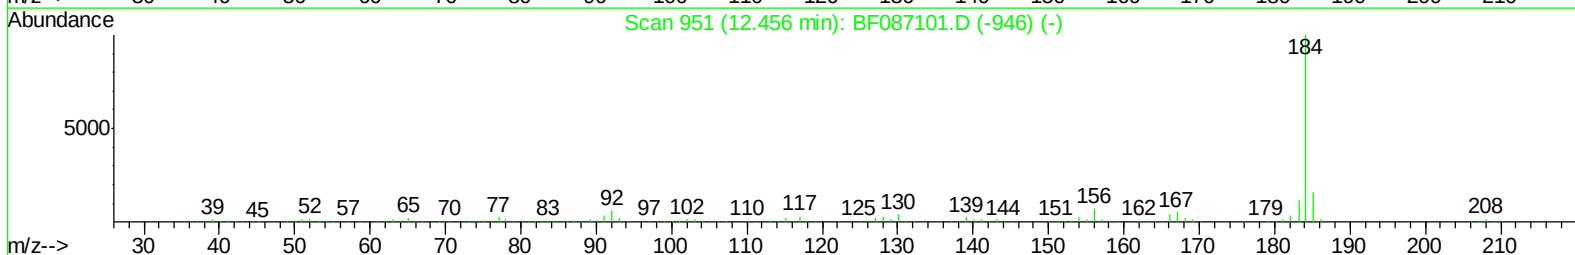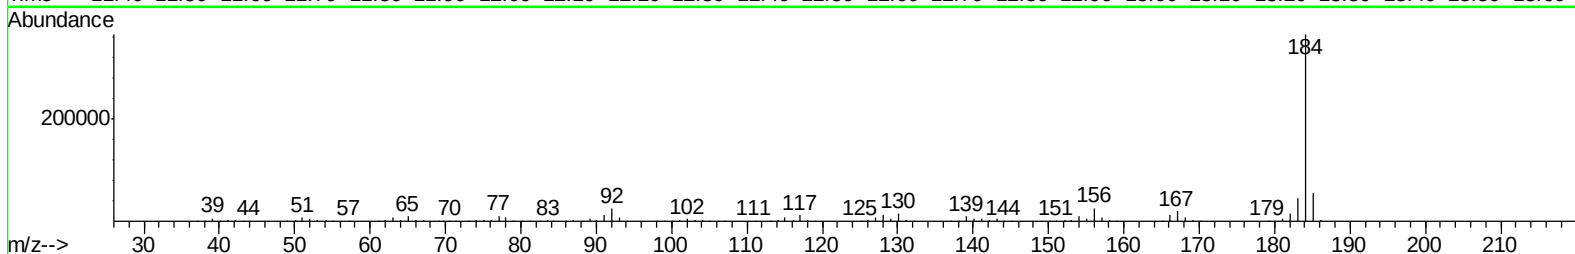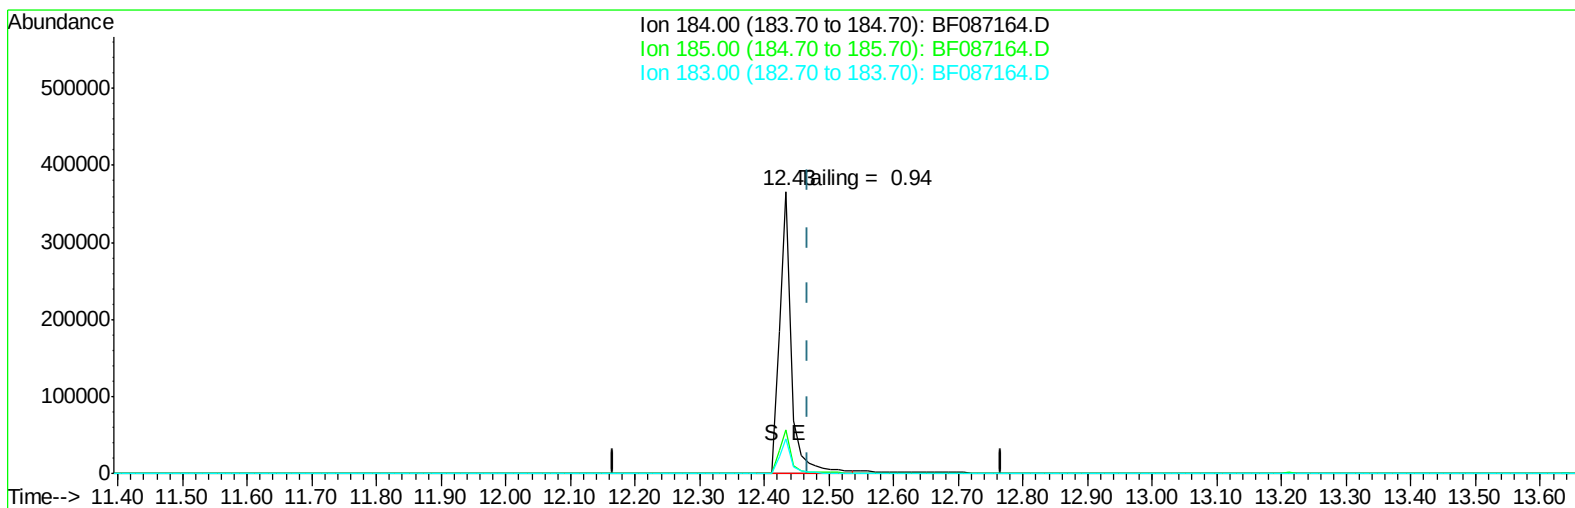

TIC: BF087164.D

(76) Benzidine

12.434min (-0.033) -20.00ng

response 486522

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	15.25
183.00	12.20	12.26
0.00	0.00	0.00