

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051816\
 Data File : BF087157.D
 Acq On : 18 May 2016 21:43
 Operator : UM/SJ
 Sample : H3143-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 5-RAMP-AC(0-2)

Quant Time: May 19 04:30:22 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 19 04:01:26 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.58	152	129962	20.00	ng	0.00
21) Naphthalene-d8	7.86	136	528642	20.00	ng	-0.01
38) Acenaphthene-d10	9.61	164	258219	20.00	ng	-0.01
63) Phenanthrene-d10	11.08	188	482098	20.00	ng	-0.01
75) Chrysene-d12	13.71	240	345305	20.00	ng	-0.01
86) Perylene-d12	15.06	264	315915	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	679673	87.90	ng	0.00
7) Phenol-d6	6.24	99	900260	86.81	ng	-0.01
23) Nitrobenzene-d5	7.15	82	636222	59.98	ng	0.00
41) 2,4,6-Tribromophenol	10.40	330	202234	70.87	ng	-0.01
44) 2-Fluorobiphenyl	8.95	172	968271	62.10	ng	0.00
78) Terphenyl-d14	12.67	244	761307	49.87	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.35	163	108993	5.53	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051816\
Data File : BF087157.D
Acq On : 18 May 2016 21:43
Operator : UM/SJ
Sample : H3143-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
5-RAMP-AC(0-2)

Quant Time: May 19 04:30:22 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 19 04:01:26 2016
Response via : Initial Calibration

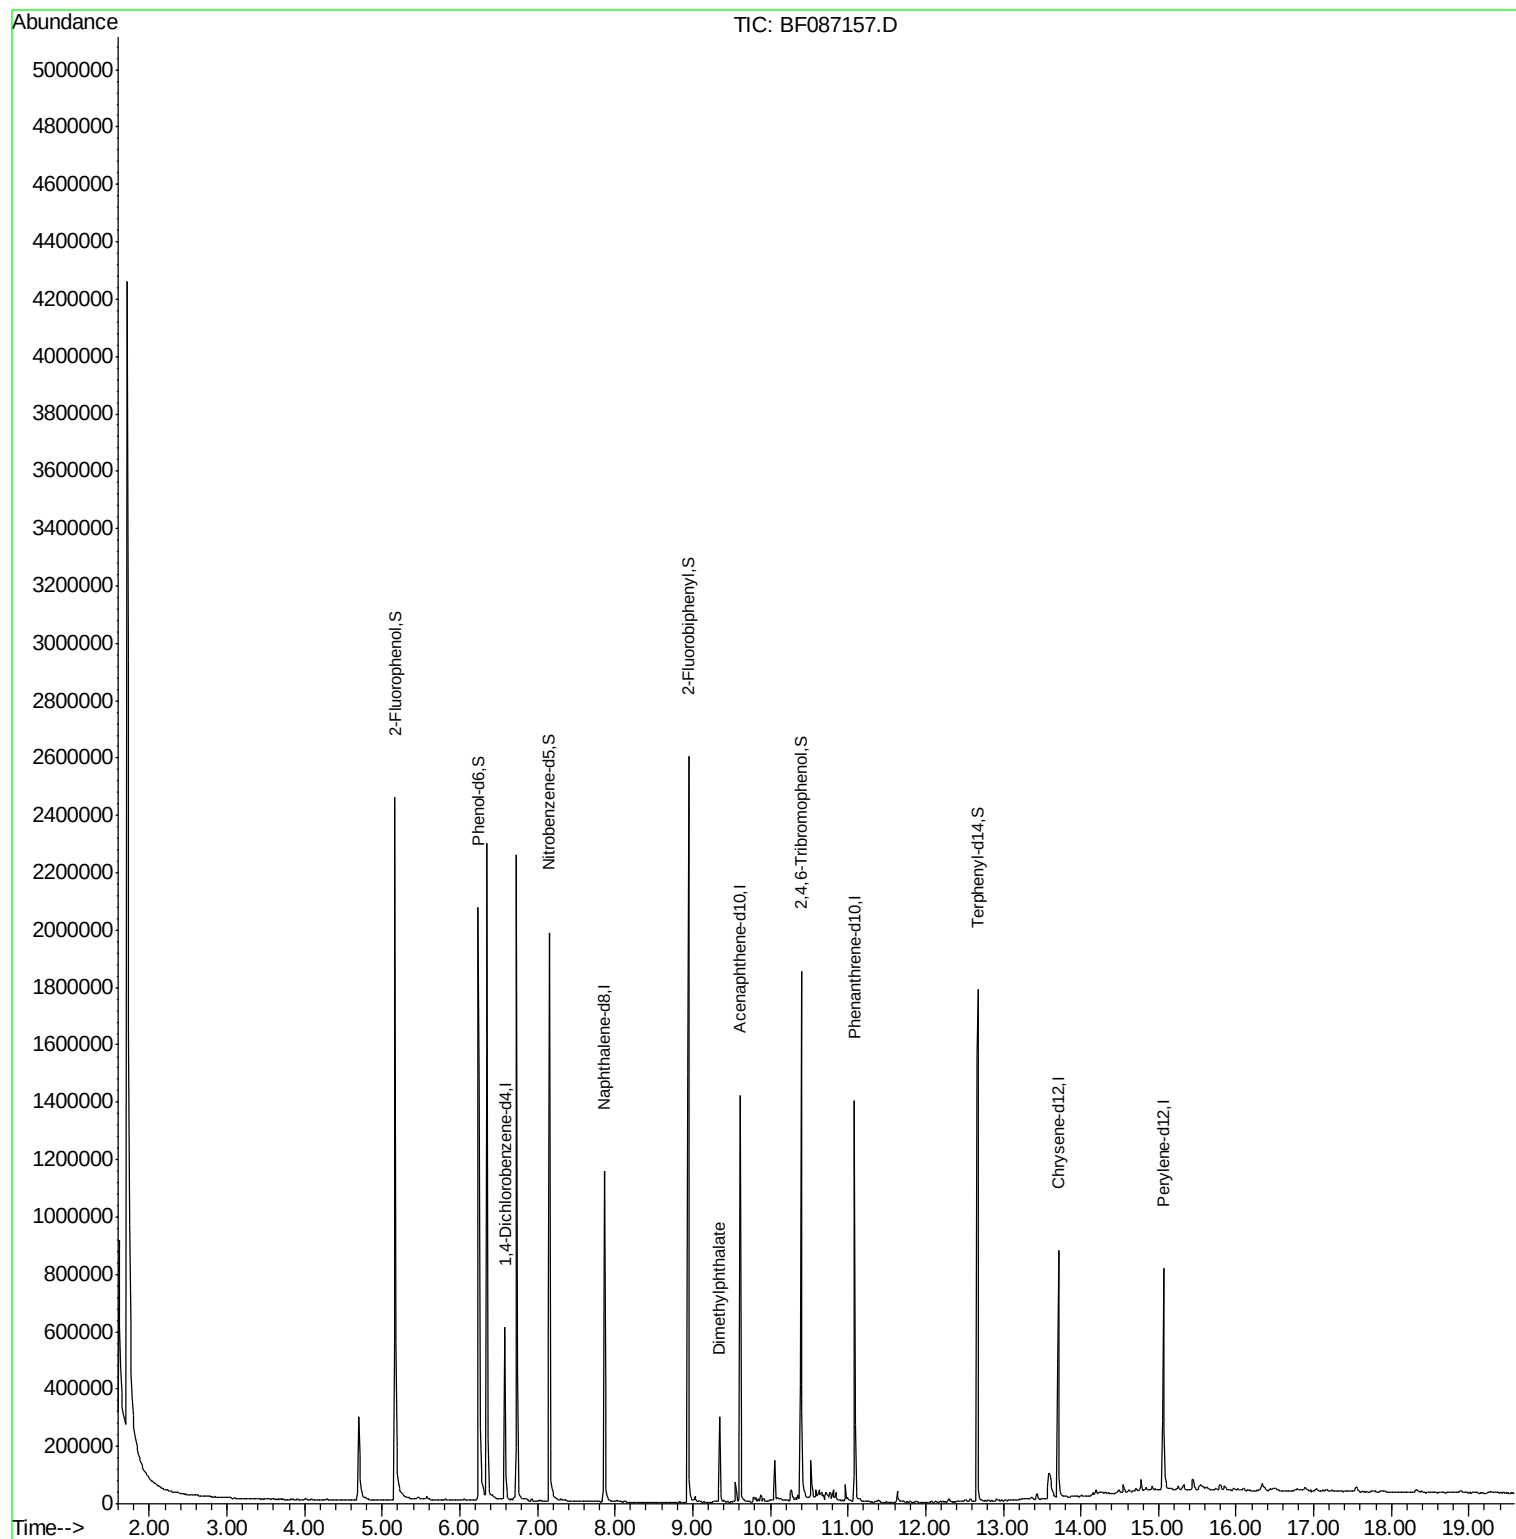

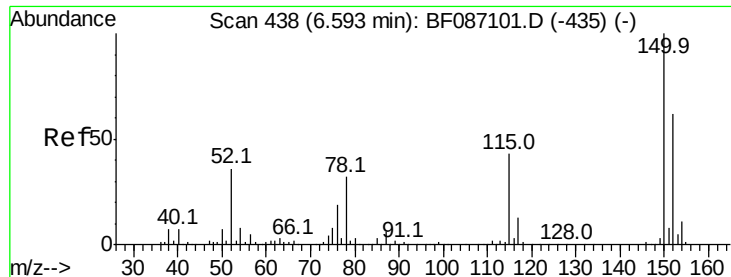

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.58 min Scan# 437

Delta R.T. -0.00 min

Lab File: BF087157.D

Acq: 18 May 2016 21:43

Instrument :

BNA_F

ClientSampleId :

5-RAMP-AC(0-2)


Tot Ion:152 Resp: 129962

Ion Ratio Lower Upper

152 100

150 149.8 125.8 188.6




115 54.6 51.5 77.3



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

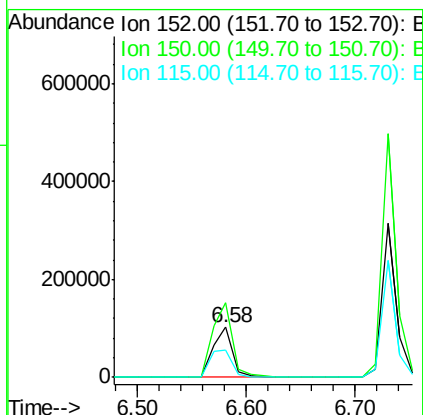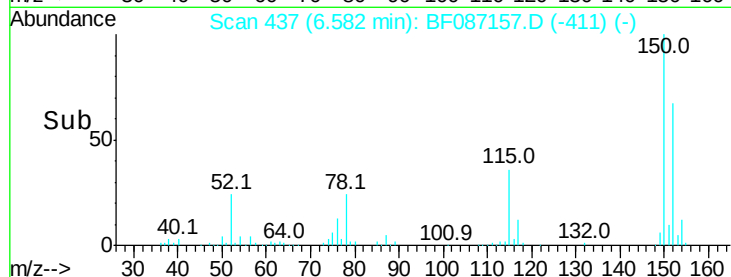

#5

2-Fluorophenol

Concen: 87.90 ng

RT: 5.16 min Scan# 313

Delta R.T. -0.00 min

Lab File: BF087157.D

Acq: 18 May 2016 21:43


Tgt Ion:112 Resp: 679673

Ion Ratio Lower Upper

112 100

64 71.1 52.1 78.1



63 38.3 25.7 38.5




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

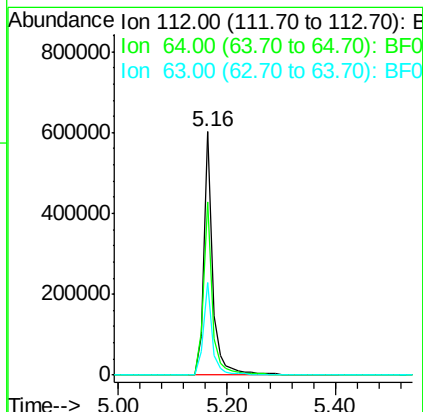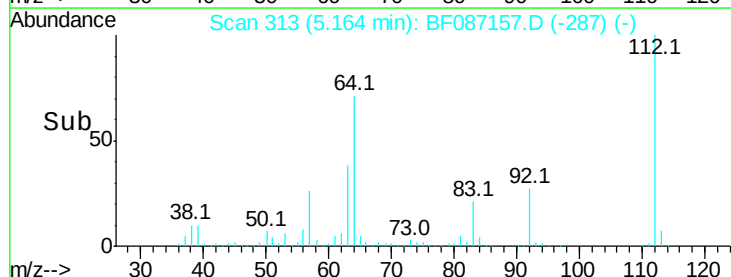

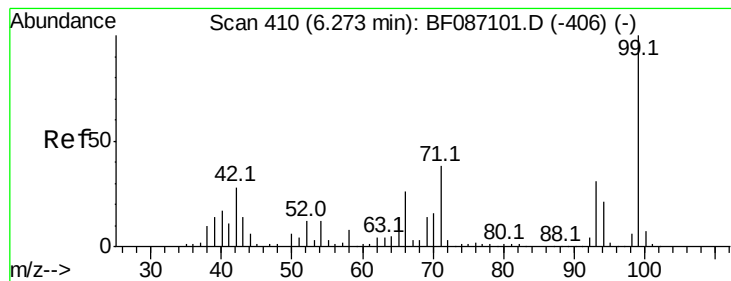

#7

Phenol-d6

Concen: 86.81 ng

RT: 6.24 min Scan# 407

Delta R.T. -0.01 min

Lab File: BF087157.D

Acq: 18 May 2016 21:43

Instrument :

BNA_F

ClientSampleId :

5-RAMP-AC(0-2)


Tot Ion: 99 Resp: 900260

Ion Ratio Lower Upper




99 100

42 32.9 13.6 20.4#

71 40.7 24.6 36.8#



Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

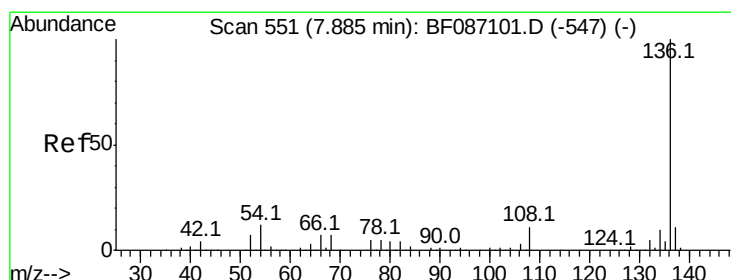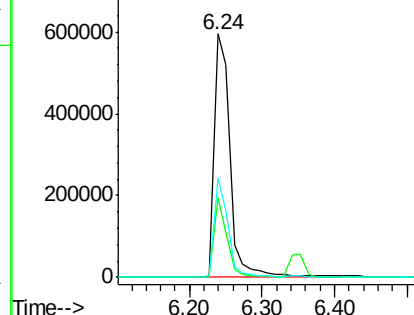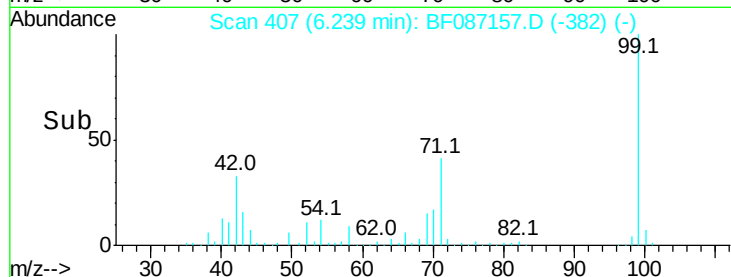

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.86 min Scan# 549

Delta R.T. -0.01 min

Lab File: BF087157.D

Acq: 18 May 2016 21:43

Tgt Ion: 136 Resp: 528642


Ion Ratio Lower Upper

136 100



137 11.2 8.8 13.2


54 14.1 5.0 7.4#

68 7.5 4.4 6.6#



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0



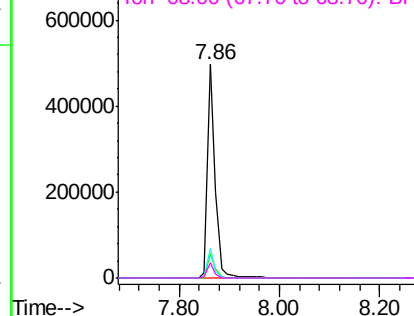
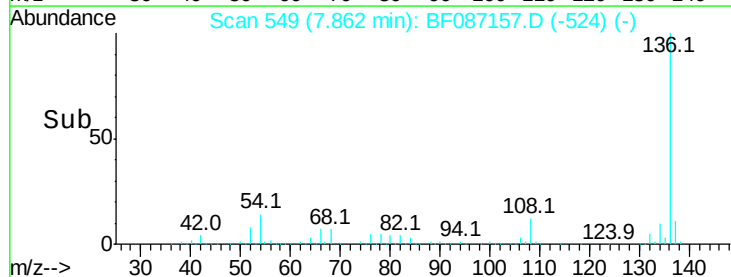


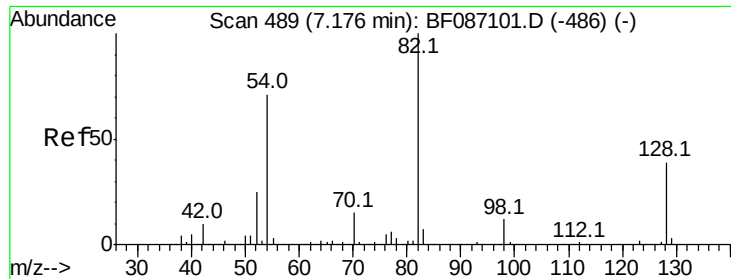

#23
 Nitrobenzene-d5
 Concen: 59.98 ng
 RT: 7.15 min Scan# 487
 Delta R.T. -0.00 min
 Lab File: BF087157.D
 Acq: 18 May 2016 21:43




Instrument :
 BNA_F
 ClientSampleId :
 5-RAMP-AC(0-2)


Tot Ion: 82 Resp: 636222
 Ion Ratio Lower Upper
 82 100
 128 41.5 40.6 61.0
 54 67.4 38.1 57.1#

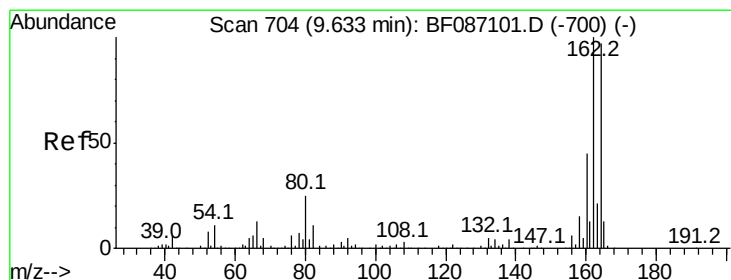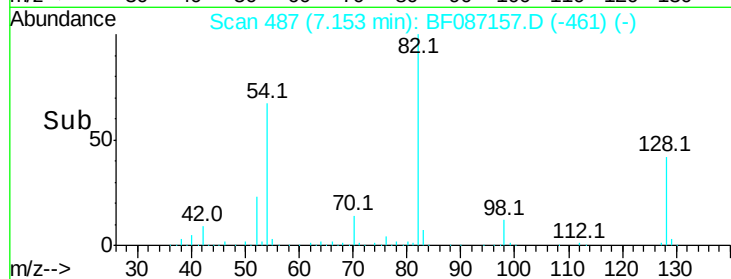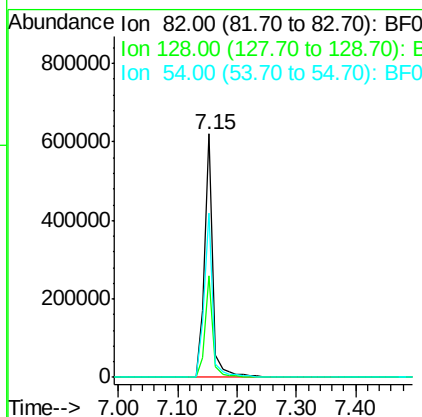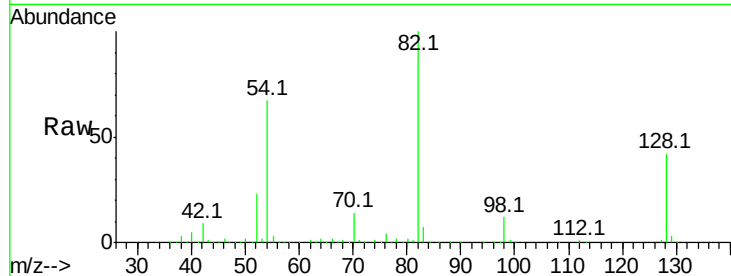

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.61 min Scan# 702
 Delta R.T. -0.01 min
 Lab File: BF087157.D
 Acq: 18 May 2016 21:43

Tgt Ion: 164 Resp: 258219
 Ion Ratio Lower Upper
 164 100
 162 102.2 82.8 124.2
 160 45.7 36.9 55.3

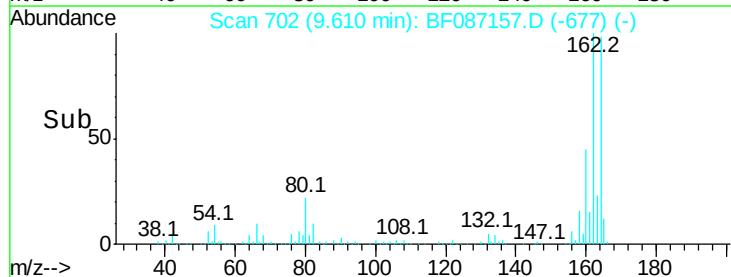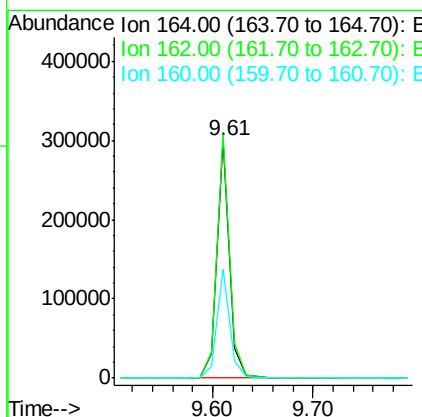

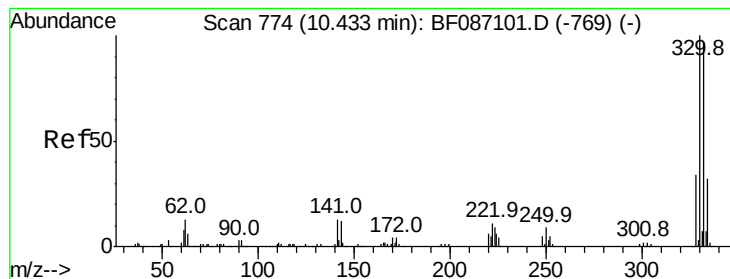

#41

2,4,6-Tribromophenol

Concen: 70.87 ng

RT: 10.40 min Scan# 771

Delta R.T. -0.01 min

Lab File: BF087157.D

Acq: 18 May 2016 21:43

Instrument :

BNA_F

ClientSampleId :

5-RAMP-AC(0-2)


Tot Ion:330 Resp: 202234

Ion Ratio Lower Upper

330 100

332 96.8 79.0 118.4




141 40.0 31.2 46.8

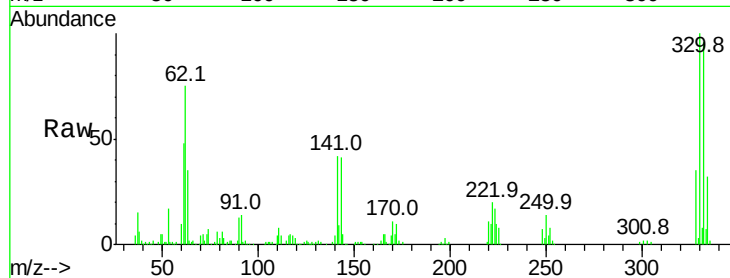

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

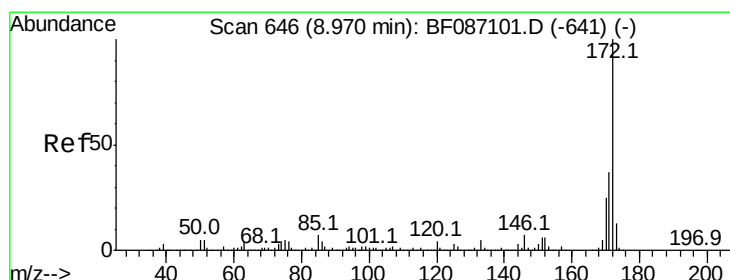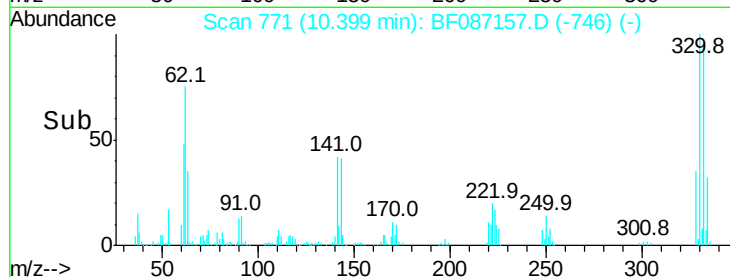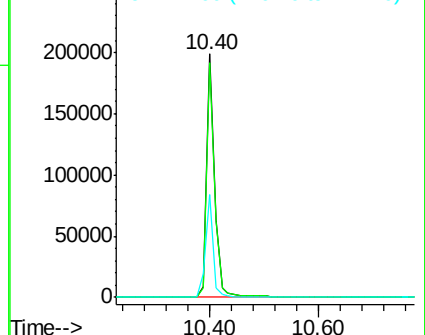

#44

2-Fluorobiphenyl

Concen: 62.10 ng

RT: 8.95 min Scan# 644

Delta R.T. -0.00 min

Lab File: BF087157.D

Acq: 18 May 2016 21:43


Tgt Ion:172 Resp: 968271

Ion Ratio Lower Upper

172 100

171 35.8 29.0 43.6



170 24.1 19.8 29.8

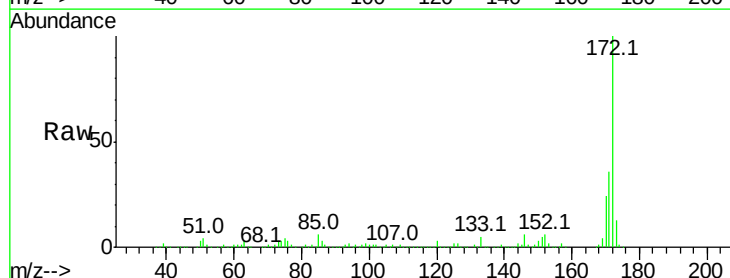


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

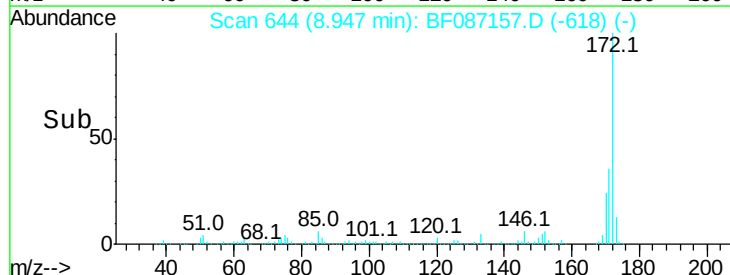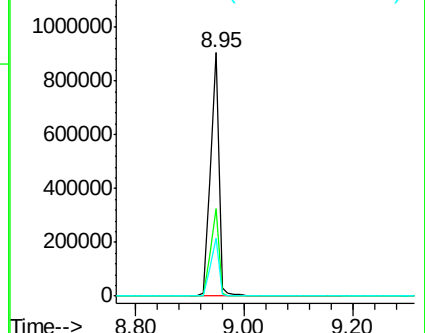

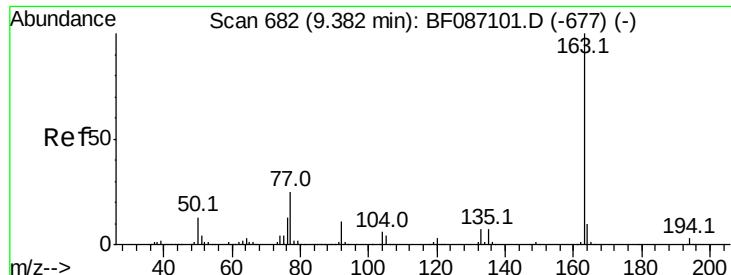

#49

Dimethylphthalate

Concen: 5.53 ng

RT: 9.35 min Scan# 679

Delta R.T. -0.01 min

Lab File: BF087157.D

Acq: 18 May 2016 21:43

Instrument :

BNA_F

ClientSampleId :

5-RAMP-AC(0-2)


Tot Ion:163 Resp: 108993

Ion Ratio Lower Upper

163 100

194 3.1 2.6 4.0




164 9.9 8.2 12.4



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

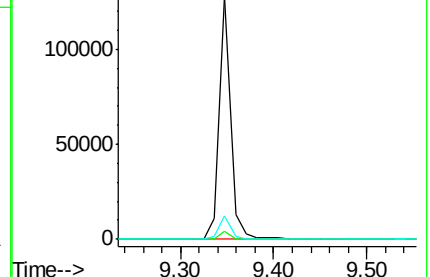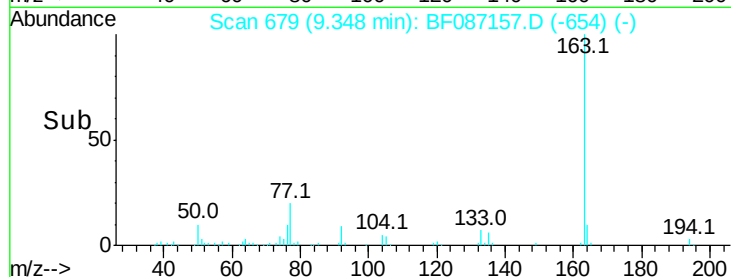

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.08 min Scan# 831

Delta R.T. -0.01 min

Lab File: BF087157.D

Acq: 18 May 2016 21:43


Tgt Ion:188 Resp: 482098

Ion Ratio Lower Upper

188 100

94 10.8 6.8 10.2#



80 12.4 7.1 10.7#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

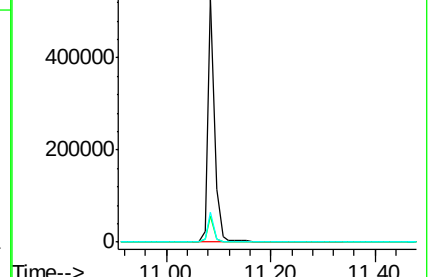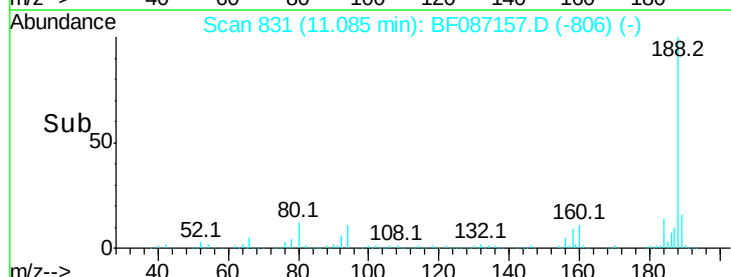

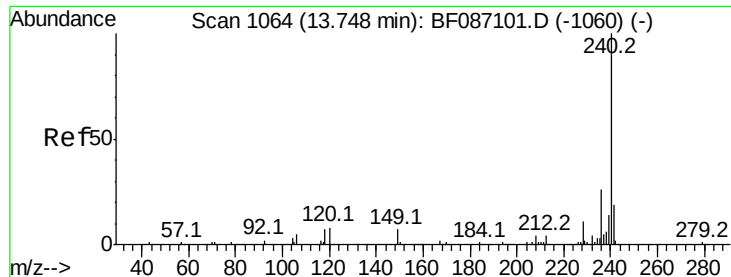

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.71 min Scan# 1061

Delta R.T. -0.01 min

Lab File: BF087157.D

Acq: 18 May 2016 21:43

Instrument :

BNA_F

ClientSampleId :

5-RAMP-AC(0-2)


Tot Ion:240 Resp: 345305

Ion Ratio Lower Upper

240 100

120 8.8 11.2 16.8#




236 26.4 21.2 31.8



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

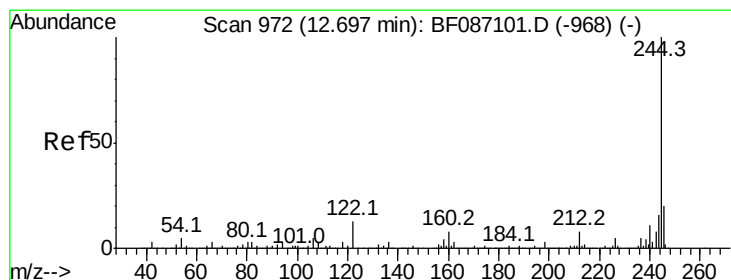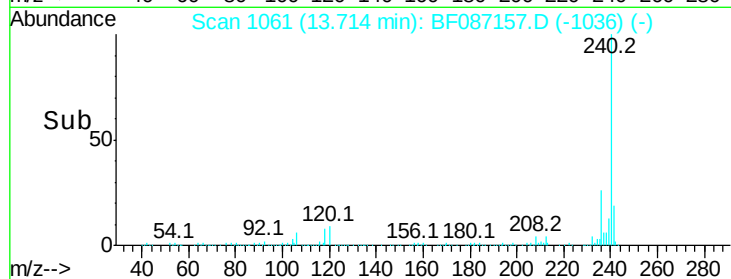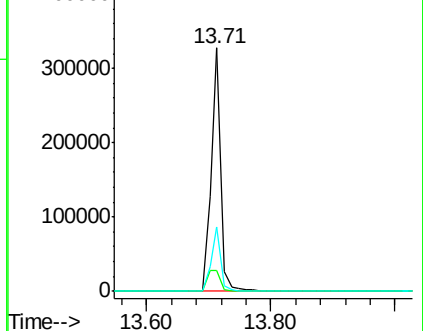

#78

Terphenyl-d14

Concen: 49.87 ng

RT: 12.67 min Scan# 970

Delta R.T. -0.00 min

Lab File: BF087157.D

Acq: 18 May 2016 21:43


Tgt Ion:244 Resp: 761307

Ion Ratio Lower Upper

244 100

212 6.9 6.2 9.2



122 7.1 12.0 18.0#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

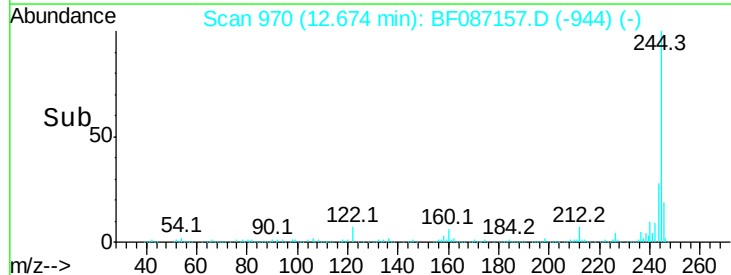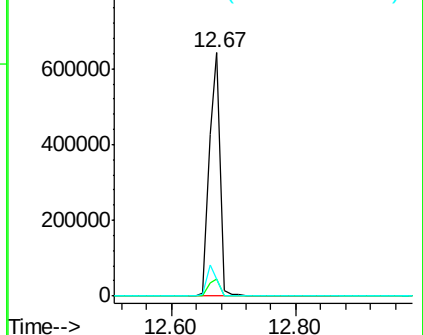


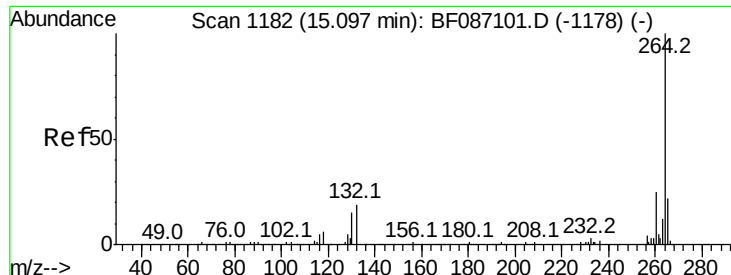

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.06 min Scan# 1179
 Delta R.T. -0.01 min
 Lab File: BF087157.D
 Acq: 18 May 2016 21:43

Instrument :
 BNA_F
 ClientSampleId :
 5-RAMP-AC(0-2)

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.8	19.5	29.3
265	21.8	17.3	25.9

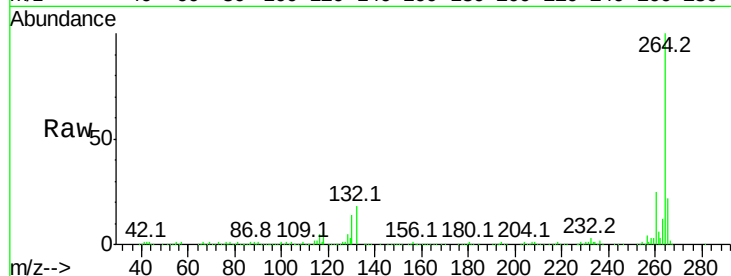

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

