

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051816\
 Data File : BF087173.D
 Acq On : 19 May 2016 6:16
 Operator : UM/SJ
 Sample : H3105-05
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 W-06RR

Quant Time: May 19 06:57:43 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 16:55:01 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.58	152	118236	20.00	ng	-0.02
21) Naphthalene-d8	7.86	136	474326	20.00	ng	-0.03
38) Acenaphthene-d10	9.61	164	227930	20.00	ng	-0.03
63) Phenanthrene-d10	11.08	188	371877	20.00	ng	-0.03
75) Chrysene-d12	13.71	240	275043	20.00	ng	-0.05
86) Perylene-d12	15.06	264	285118	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	540973	76.90	ng	-0.03
7) Phenol-d6	6.24	99	466967	49.50	ng	-0.05
23) Nitrobenzene-d5	7.15	82	916908	96.34	ng	-0.03
41) 2,4,6-Tribromophenol	10.40	330	312741	124.17	ng	-0.05
44) 2-Fluorobiphenyl	8.95	172	1500355	109.02	ng	-0.03
78) Terphenyl-d14	12.67	244	1226898	100.91	ng	-0.03
Target Compounds						
49) Dimethylphthalate	9.35	163	47046	2.71	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051816\
Data File : BF087173.D
Acq On : 19 May 2016 6:16
Operator : UM/SJ
Sample : H3105-05
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-06RR

Quant Time: May 19 06:57:43 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 16:55:01 2016
Response via : Initial Calibration

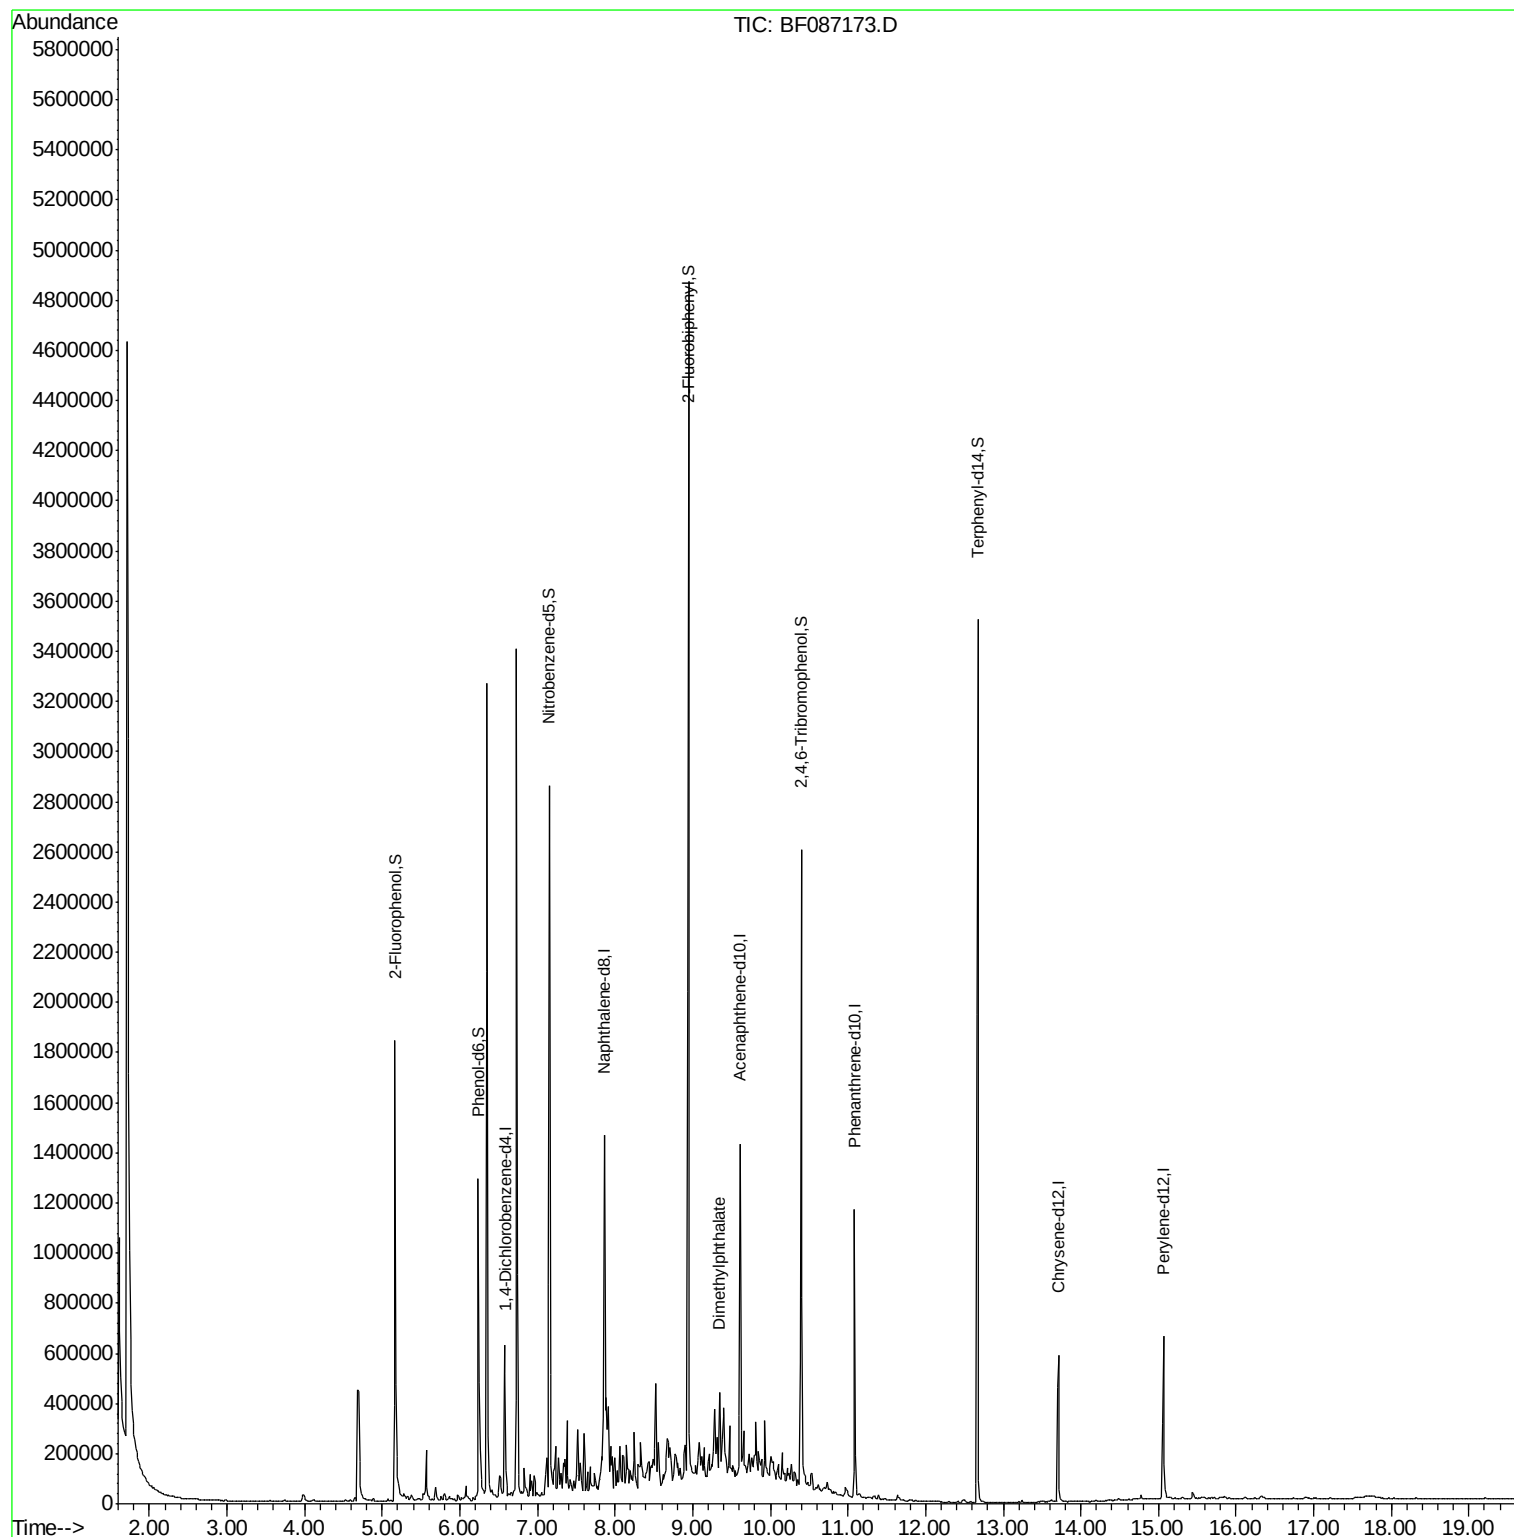

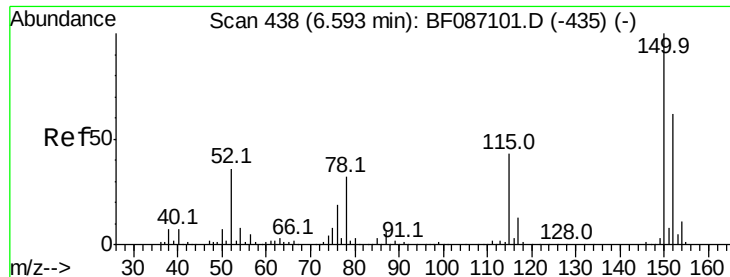

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.58 min Scan# 437

Delta R.T. -0.02 min

Lab File: BF087173.D

Acq: 19 May 2016 6:16

Instrument :

BNA_F

ClientSampleId :

W-06RR


Tot Ion:152 Resp: 118236

Ion Ratio Lower Upper

152 100

150 155.2 125.8 188.6




115 55.6 51.5 77.3

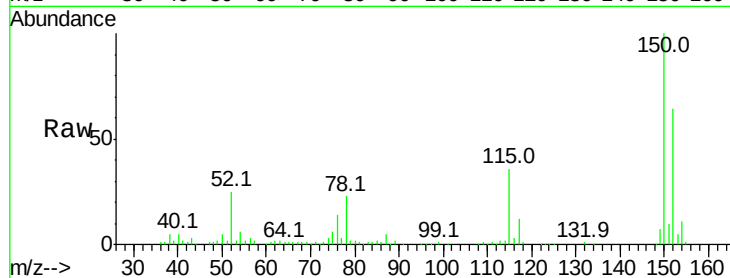

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

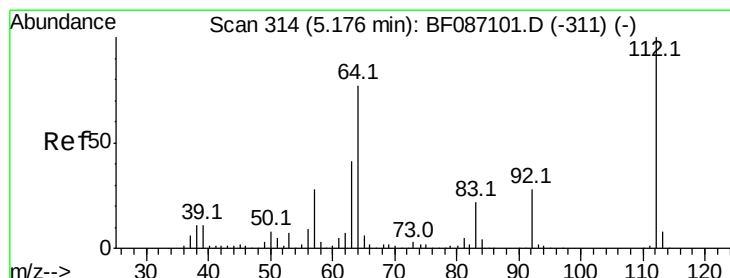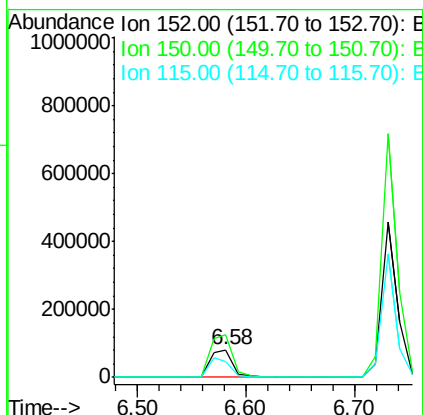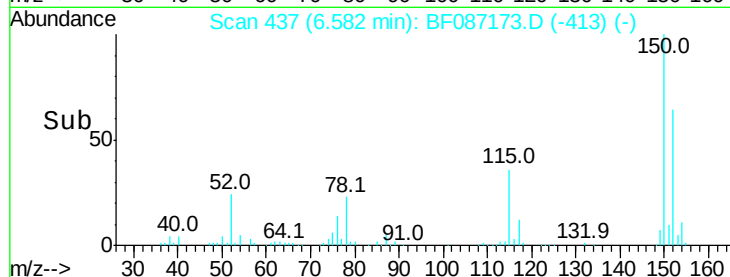

#5

2-Fluorophenol

Concen: 76.90 ng

RT: 5.16 min Scan# 313

Delta R.T. -0.03 min

Lab File: BF087173.D

Acq: 19 May 2016 6:16


Tgt Ion:112 Resp: 540973

Ion Ratio Lower Upper

112 100

64 68.1 52.1 78.1



63 36.9 25.7 38.5

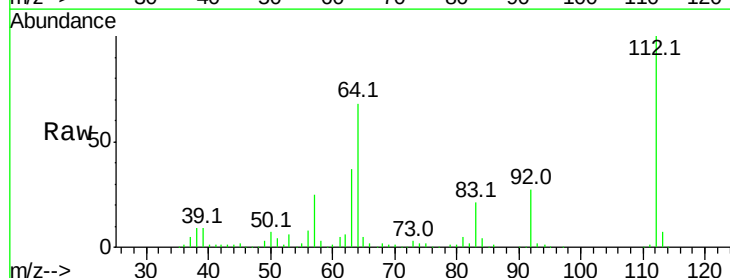


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

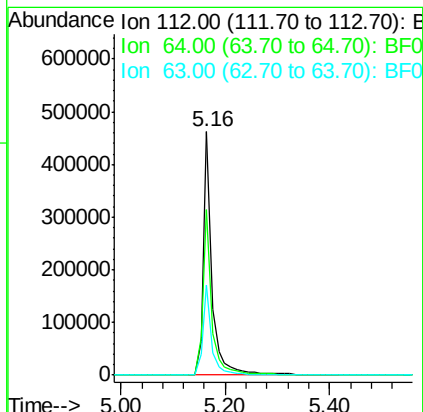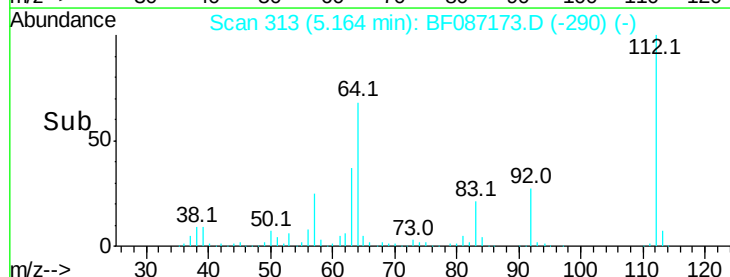



#7

Phenol-d6

Concen: 49.50 ng

RT: 6.24 min Scan# 407

Delta R.T. -0.05 min

Lab File: BF087173.D

Acq: 19 May 2016 6:16

Instrument :

BNA_F

ClientSampled :

W-06RR





Tot Ion: 99 Resp: 466967

Ion Ratio Lower Upper

99 100

42 31.2 13.6 20.4#

71 39.0 24.6 36.8#

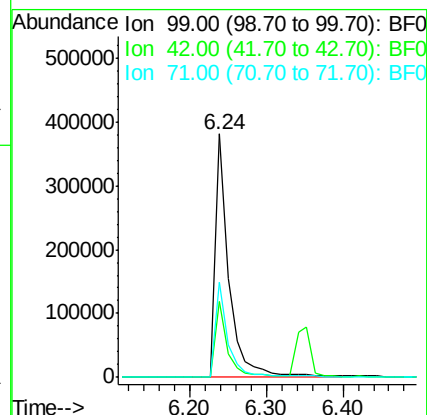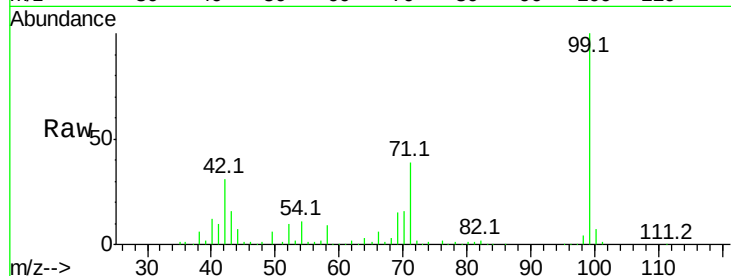

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.86 min Scan# 549

Delta R.T. -0.03 min

Lab File: BF087173.D

Acq: 19 May 2016 6:16

Tgt Ion: 136 Resp: 474326




Ion Ratio Lower Upper


136 100

137 11.2 8.8 13.2

54 13.8 5.0 7.4#

68 7.3 4.4 6.6#



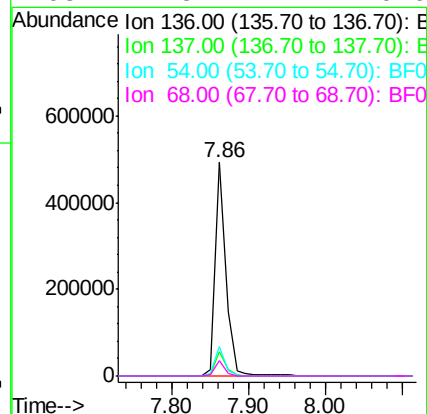





#23
 Nitrobenzene-d5
 Concen: 96.34 ng
 RT: 7.15 min Scan# 487
 Delta R.T. -0.03 min
 Lab File: BF087173.D
 Acq: 19 May 2016 6:16




Instrument :
 BNA_F
 ClientSampleId :
 W-06RR


Tot Ion	82	Resp	916908
Ion Ratio	100	Lower	Upper
128	39.0	40.6	61.0#
54	71.7	38.1	57.1#

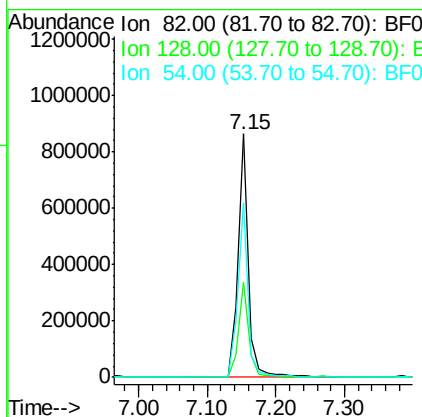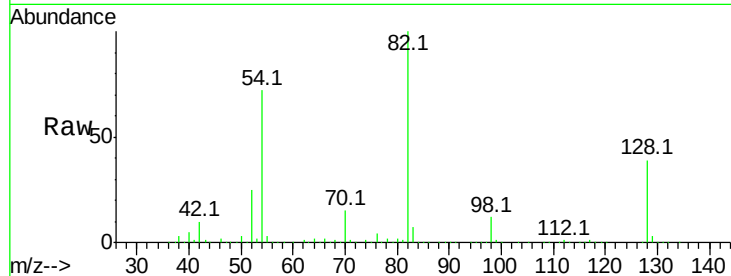

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.61 min Scan# 702
 Delta R.T. -0.03 min
 Lab File: BF087173.D
 Acq: 19 May 2016 6:16

Tgt Ion	164	Resp	227930
Ion Ratio	100	Lower	Upper
162	102.2	82.8	124.2
160	46.7	36.9	55.3

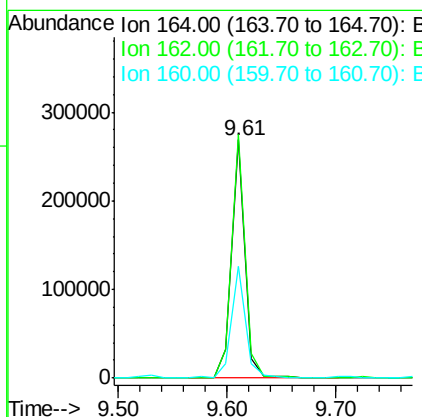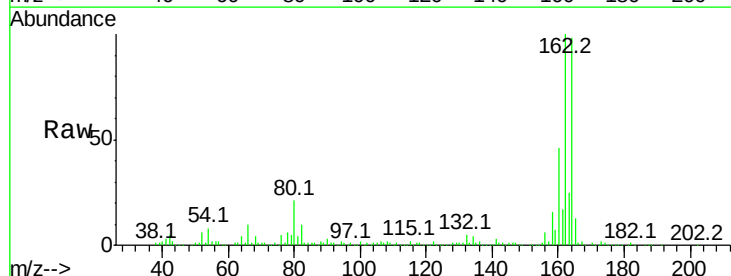







#41
 2,4,6-Tribromophenol
 Concen: 124.17 ng
 RT: 10.40 min Scan# 771
 Delta R.T. -0.05 min
 Lab File: BF087173.D
 Acq: 19 May 2016 6:16

Instrument :
 BNA_F
 ClientSampleId :
 W-06RR

Tot Ion:330 Resp: 312741
 Ion Ratio Lower Upper
 330 100
 332 97.8 79.0 118.4
 141 36.9 31.2 46.8

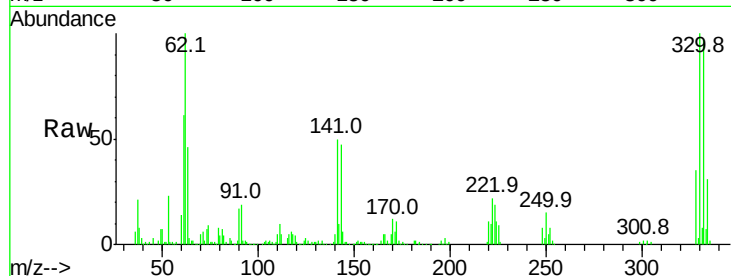


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


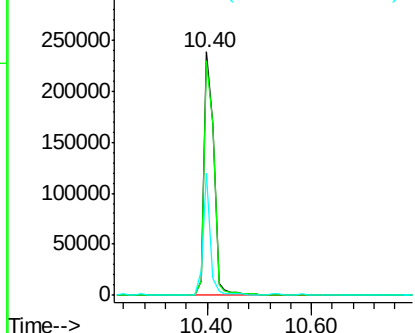



#44
 2-Fluorobiphenyl
 Concen: 109.02 ng
 RT: 8.95 min Scan# 644
 Delta R.T. -0.03 min
 Lab File: BF087173.D
 Acq: 19 May 2016 6:16

Tgt Ion:172 Resp: 1500355
 Ion Ratio Lower Upper
 172 100
 171 37.0 29.0 43.6
 170 24.9 19.8 29.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

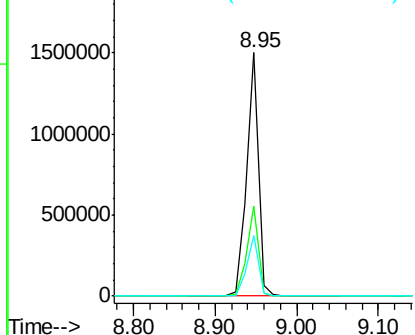


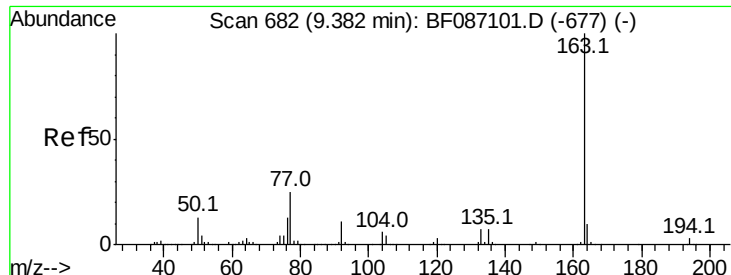




#49
Dimethylphthalate
Concen: 2.71 ng
RT: 9.35 min Scan# 679
Delta R.T. -0.05 min
Lab File: BF087173.D
Acq: 19 May 2016 6:16

Instrument :
BNA_F
ClientSampleId :
W-06RR

Tot Ion:163 Resp: 47046
Ion Ratio Lower Upper
163 100
194 3.5 2.6 4.0
164 10.0 8.2 12.4

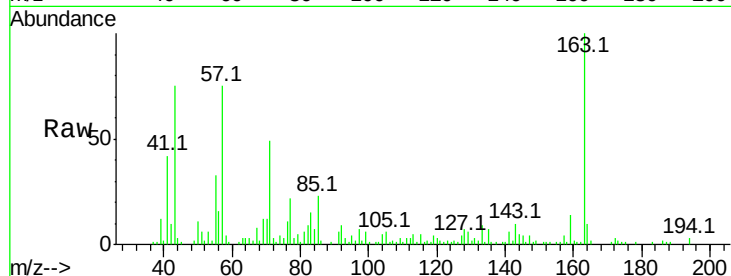


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E


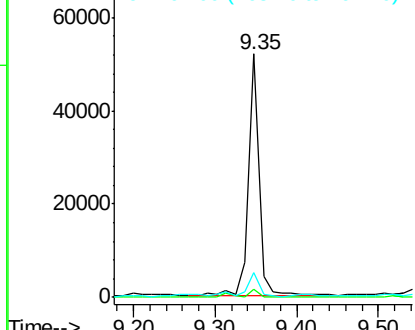



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.08 min Scan# 831
Delta R.T. -0.03 min
Lab File: BF087173.D
Acq: 19 May 2016 6:16

Tgt Ion:188 Resp: 371877
Ion Ratio Lower Upper
188 100
94 10.5 6.8 10.2#
80 11.4 7.1 10.7#



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

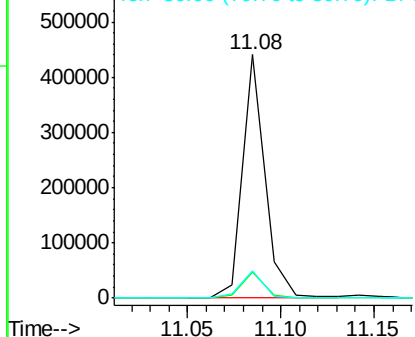



#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.71 min Scan# 1061

Delta R.T. -0.05 min

Lab File: BF087173.D

Acq: 19 May 2016 6:16

Instrument :

BNA_F

ClientSampleId :

W-06RR


Tot Ion:240 Resp: 275043

Ion Ratio Lower Upper

240 100

120 8.1 11.2 16.8#




236 25.7 21.2 31.8



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

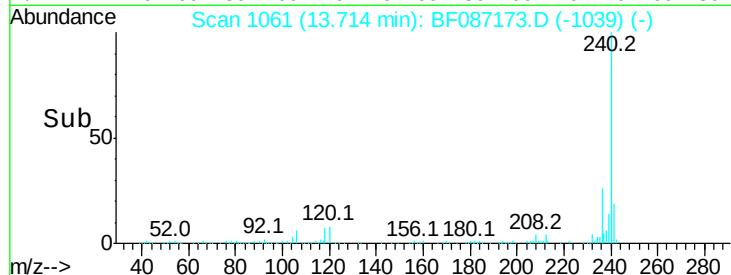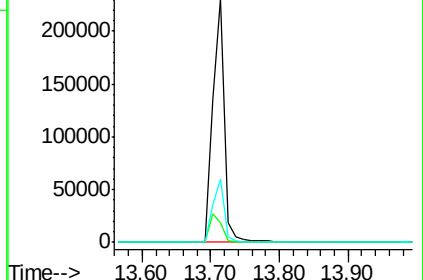

#78

Terphenyl-d14

Concen: 100.91 ng

RT: 12.67 min Scan# 970

Delta R.T. -0.03 min

Lab File: BF087173.D

Acq: 19 May 2016 6:16


Tgt Ion:244 Resp: 1226898

Ion Ratio Lower Upper

244 100

212 7.6 6.2 9.2



122 10.2 12.0 18.0#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

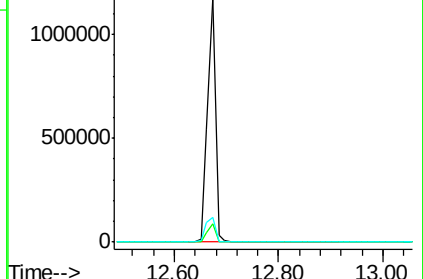


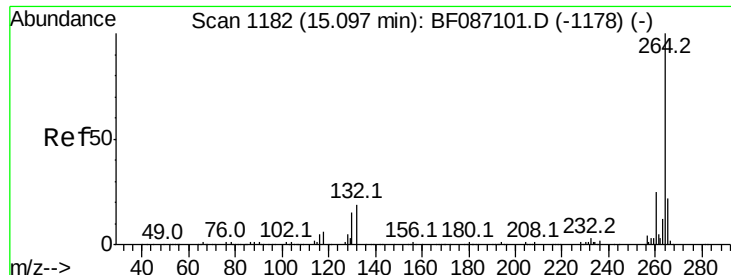

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.06 min Scan# 1179
Delta R.T. -0.05 min
Lab File: BF087173.D
Acq: 19 May 2016 6:16

Instrument :
BNA_F
ClientSampleId :
W-06RR

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.3	19.5	29.3
265	21.8	17.3	25.9

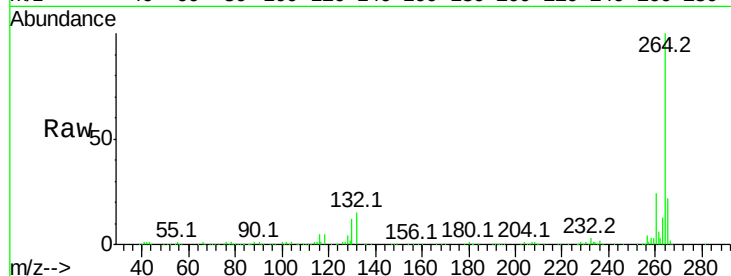

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

