


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051816\
 Data File : BF087164.D
 Acq On : 19 May 2016 1:54
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 17 16:55:01 2016

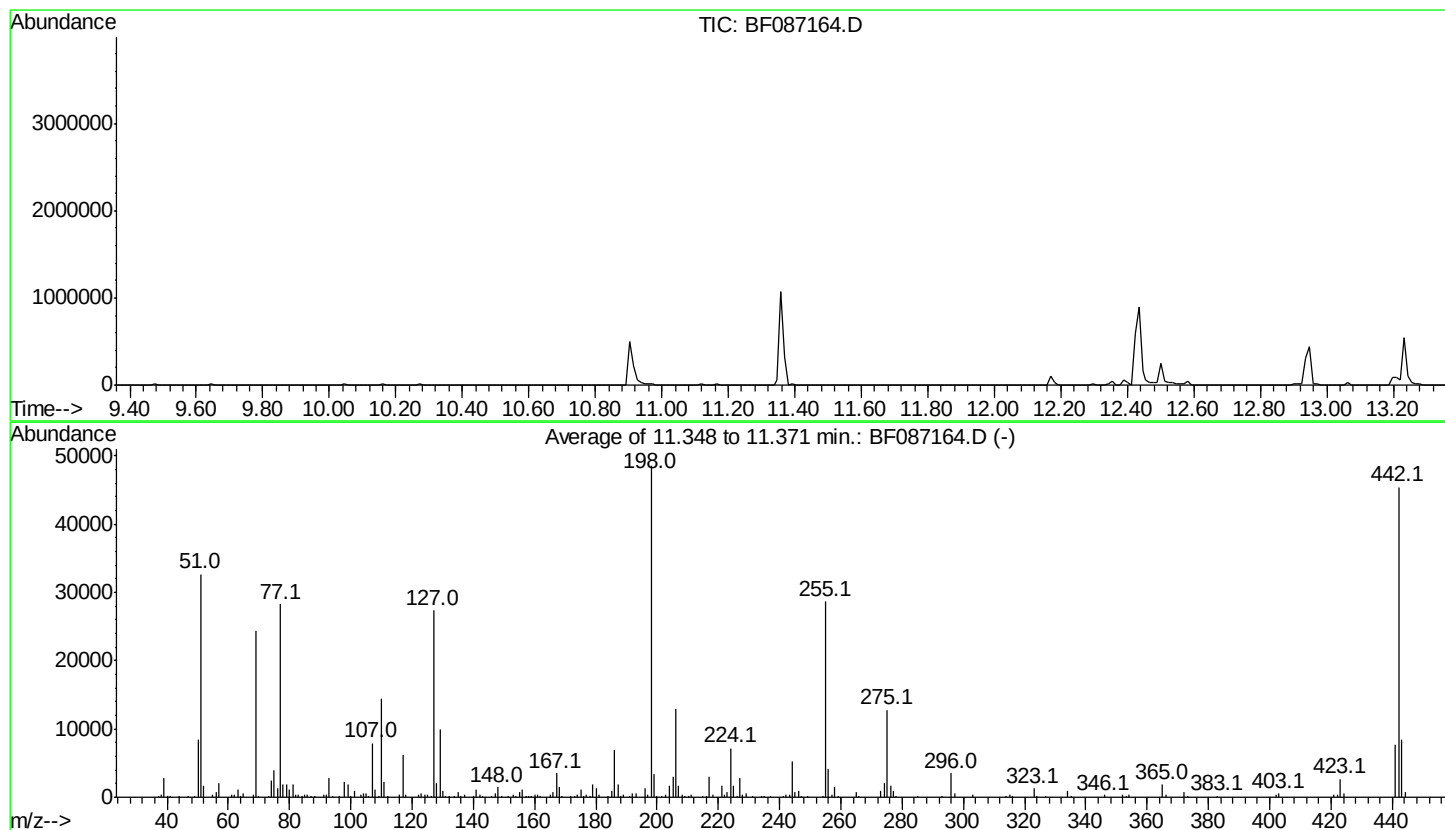

AutoFind: Scans 854, 855, 856; Background Corrected with Scan 851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.3	32715	PASS
68	69	0.00	2	1.7	411	PASS
69	198	0.00	100	50.3	24414	PASS
70	69	0.00	2	0.4	104	PASS
127	198	10	80	56.2	27305	PASS
197	198	0.00	2	0.6	304	PASS
198	198	100	100	100.0	48585	PASS
199	198	5	9	6.8	3311	PASS
275	198	10	60	26.3	12755	PASS
365	198	1	100	3.7	1811	PASS
441	442	0.01	24	16.9	7660	PASS
442	198	50	100	93.5	45405	PASS
443	442	15	24	18.6	8423	PASS