
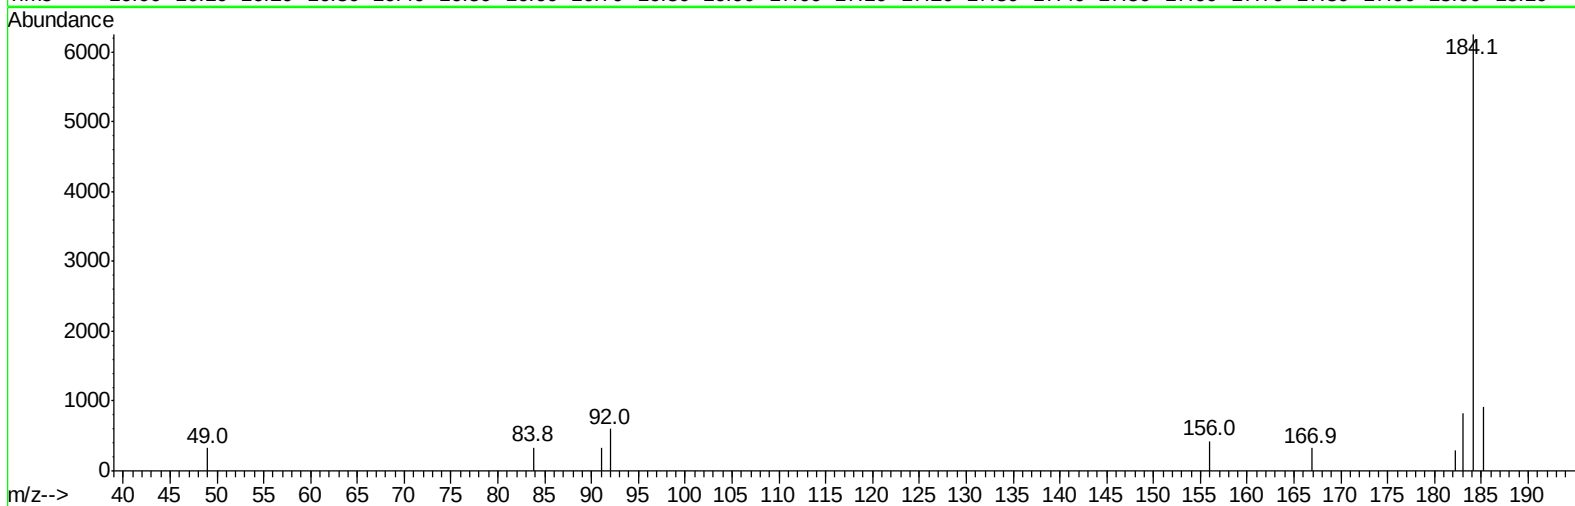


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051817\
Data File : BF095245.D
Acq On : 19 May 2017 3:27
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 07:23:30 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 17:07:53 2017
Response via : Initial Calibration

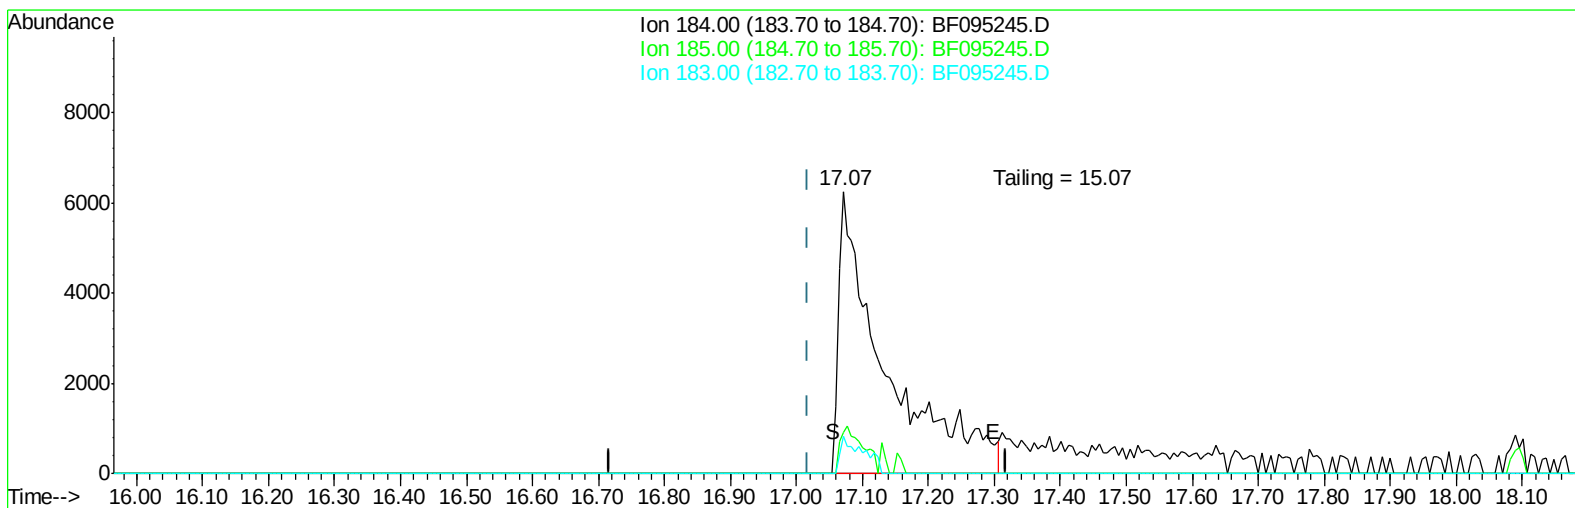

TIC: BF095245.D

(76) Benzidine



17.071min (+0.053) 0.00ng

response 22839

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.68#
183.00	12.20	13.27
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051817\
Data File : BF095245.D
Acq On : 19 May 2017 3:27
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 07:23:30 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 17:07:53 2017
Response via : Initial Calibration

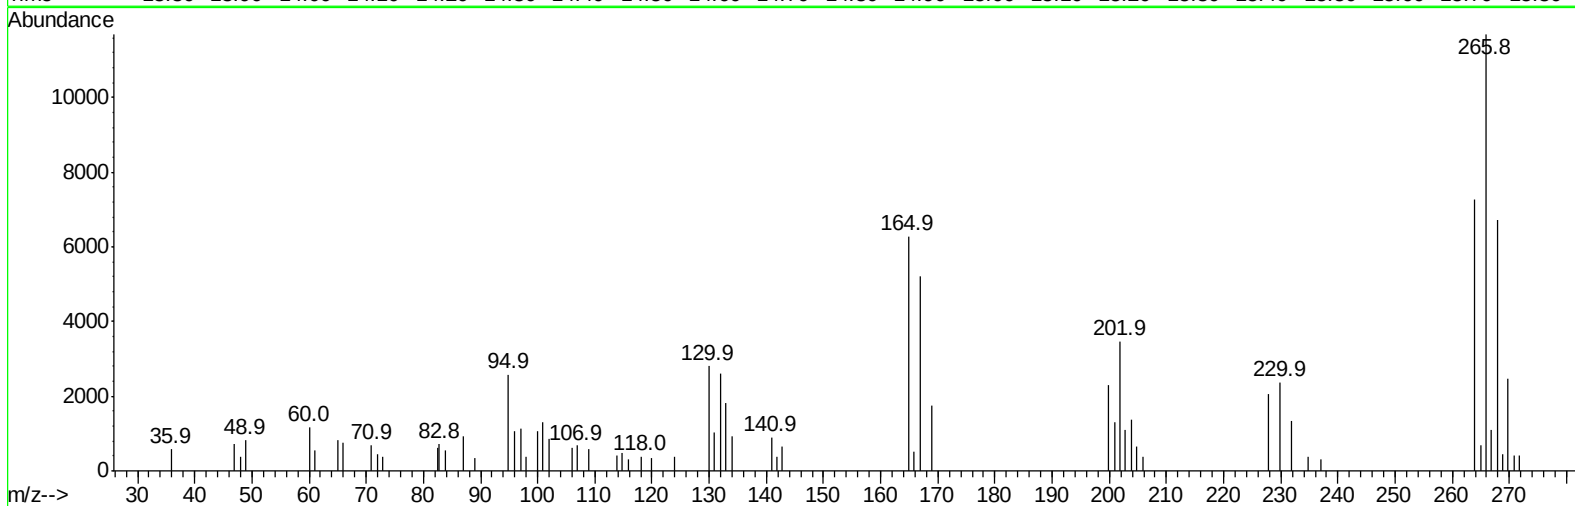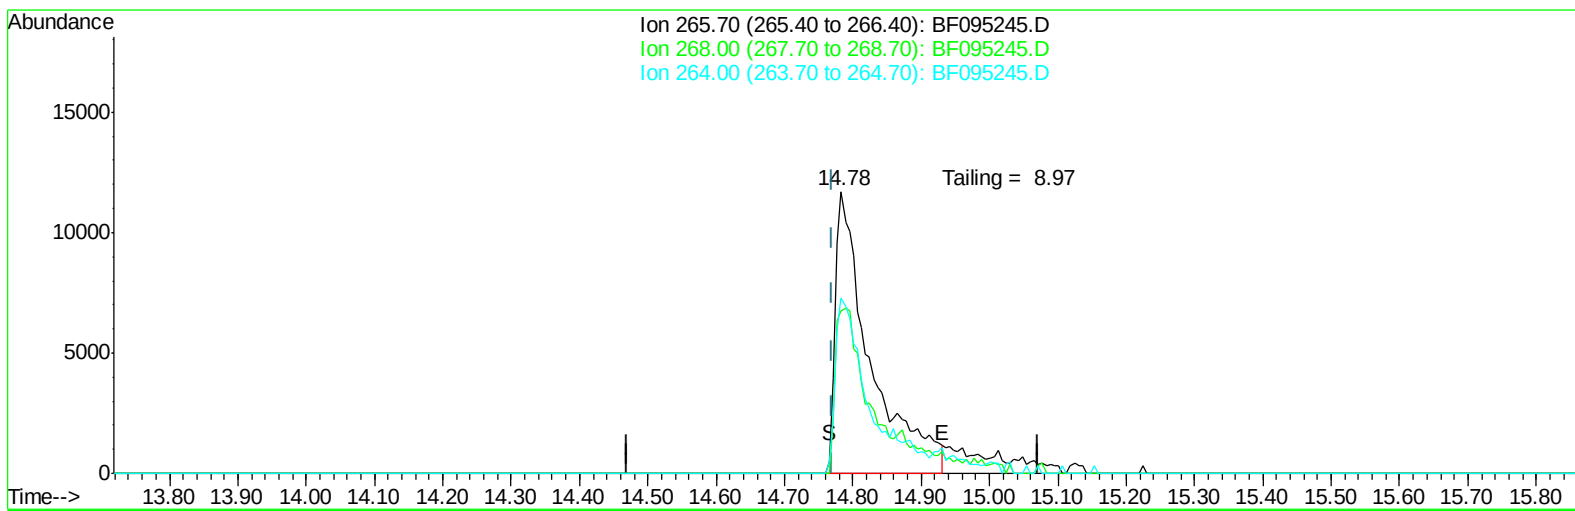

TIC: BF095245.D

(69) Pentachlorophenol (C)

14.783min (+0.012) 0.00ng m

response 41070

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.62
264.00	64.60	62.25
0.00	0.00	0.00