


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051817\
 Data File : BF095221.D
 Acq On : 18 May 2017 14:23
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 18 17:07:53 2017

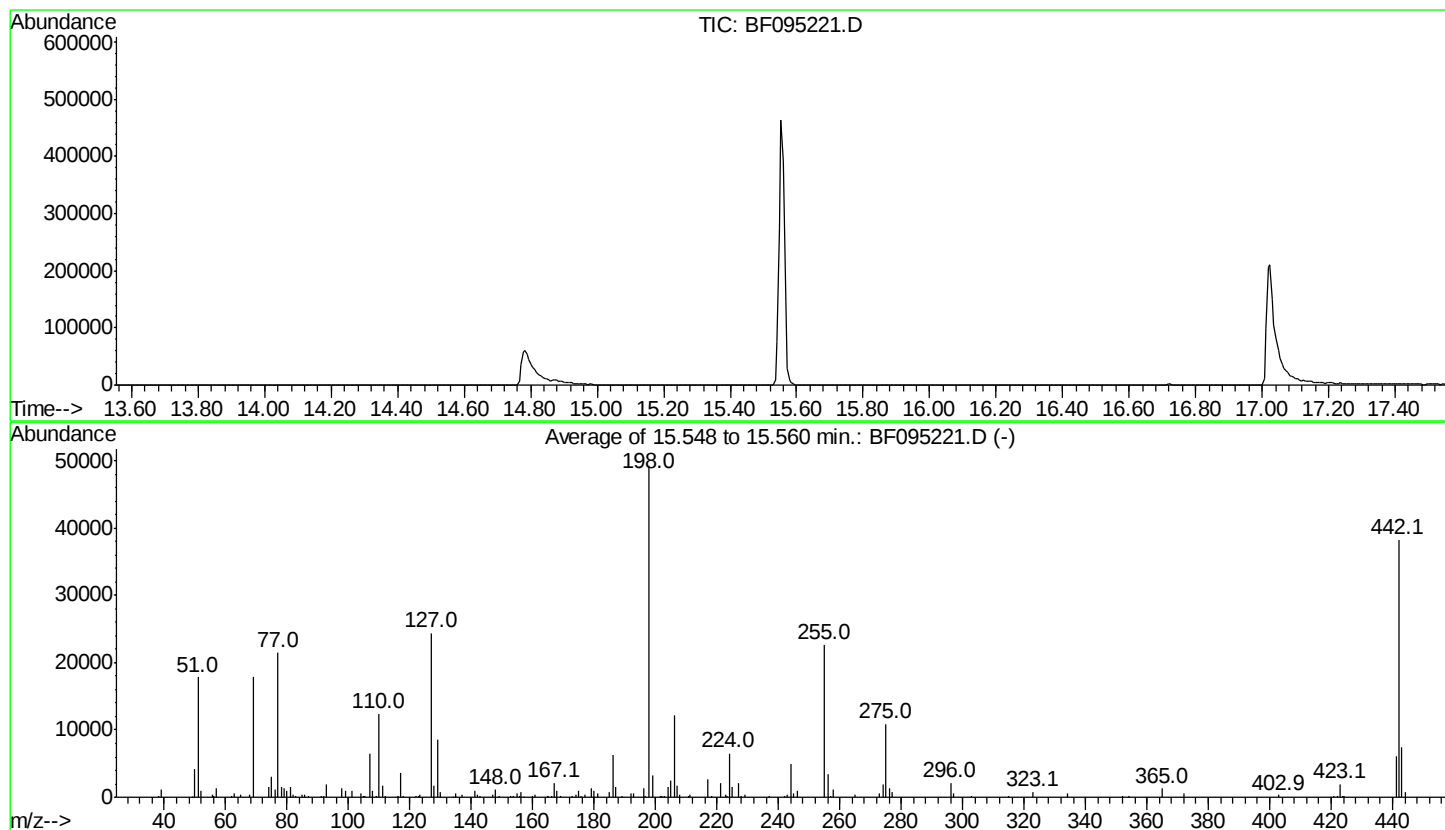

AutoFind: Scans 2314, 2315, 2316; Background Corrected with Scan 2309

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	17839	PASS
68	69	0.00	2	2.3	407	FAIL*
69	198	0.00	100	36.3	17890	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.5	24416	PASS
197	198	0.00	2	0.4	197	PASS
198	198	100	100	100.0	49296	PASS
199	198	5	9	6.5	3213	PASS
275	198	10	60	22.2	10920	PASS
365	198	1	100	2.5	1256	PASS
441	442	0.01	24	16.1	6143	PASS
442	198	50	100	77.6	38266	PASS
443	442	15	24	19.2	7339	PASS