

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF051819\
 Data File : BF114419.D
 Acq On : 19 May 2019 4:57
 Operator : JU/SJ
 Sample : K2880-03
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: May 20 04:15:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 10 15:56:46 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	222715	20.00	ng	-0.02
21) Naphthalene-d8	8.12	136	836573	20.00	ng	-0.02
39) Acenaphthene-d10	9.87	164	368498	20.00	ng	-0.02
64) Phenanthrene-d10	11.35	188	649052	20.00	ng	-0.02
76) Chrysene-d12	13.99	240	442086	20.00	ng	-0.03
87) Perylene-d12	15.46	264	488117	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	1380988	99.79	ng	0.00
7) Phenol-d6	6.49	99	1677826	102.50	ng	0.00
23) Nitrobenzene-d5	7.40	82	1183441	79.39	ng	-0.02
42) 2,4,6-Tribromophenol	10.66	330	438060	114.99	ng	-0.02
45) 2-Fluorobiphenyl	9.19	172	1930667	79.25	ng	-0.02
79) Terphenyl-d14	12.93	244	1818268	84.79	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.40	70	153117	14.758	ng	# 76
25) Isophorone	7.40	82	1183433	42.806	ng	# 64
32) Benzoic acid	8.02	122	614	7.084	ng	92
51) 2,6-Dinitrotoluene	9.87	165	47088	7.848	ng	# 22
57) 2,4-Dinitrotoluene	9.87	165	47089	5.782	ng	# 25
67) 4-Bromophenyl-phenylether	10.66	248	28447	3.981	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF051819\
Data File : BF114419.D
Acq On : 19 May 2019 4:57
Operator : JU/SJ
Sample : K2880-03
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: May 20 04:15:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 10 15:56:46 2019
Response via : Initial Calibration

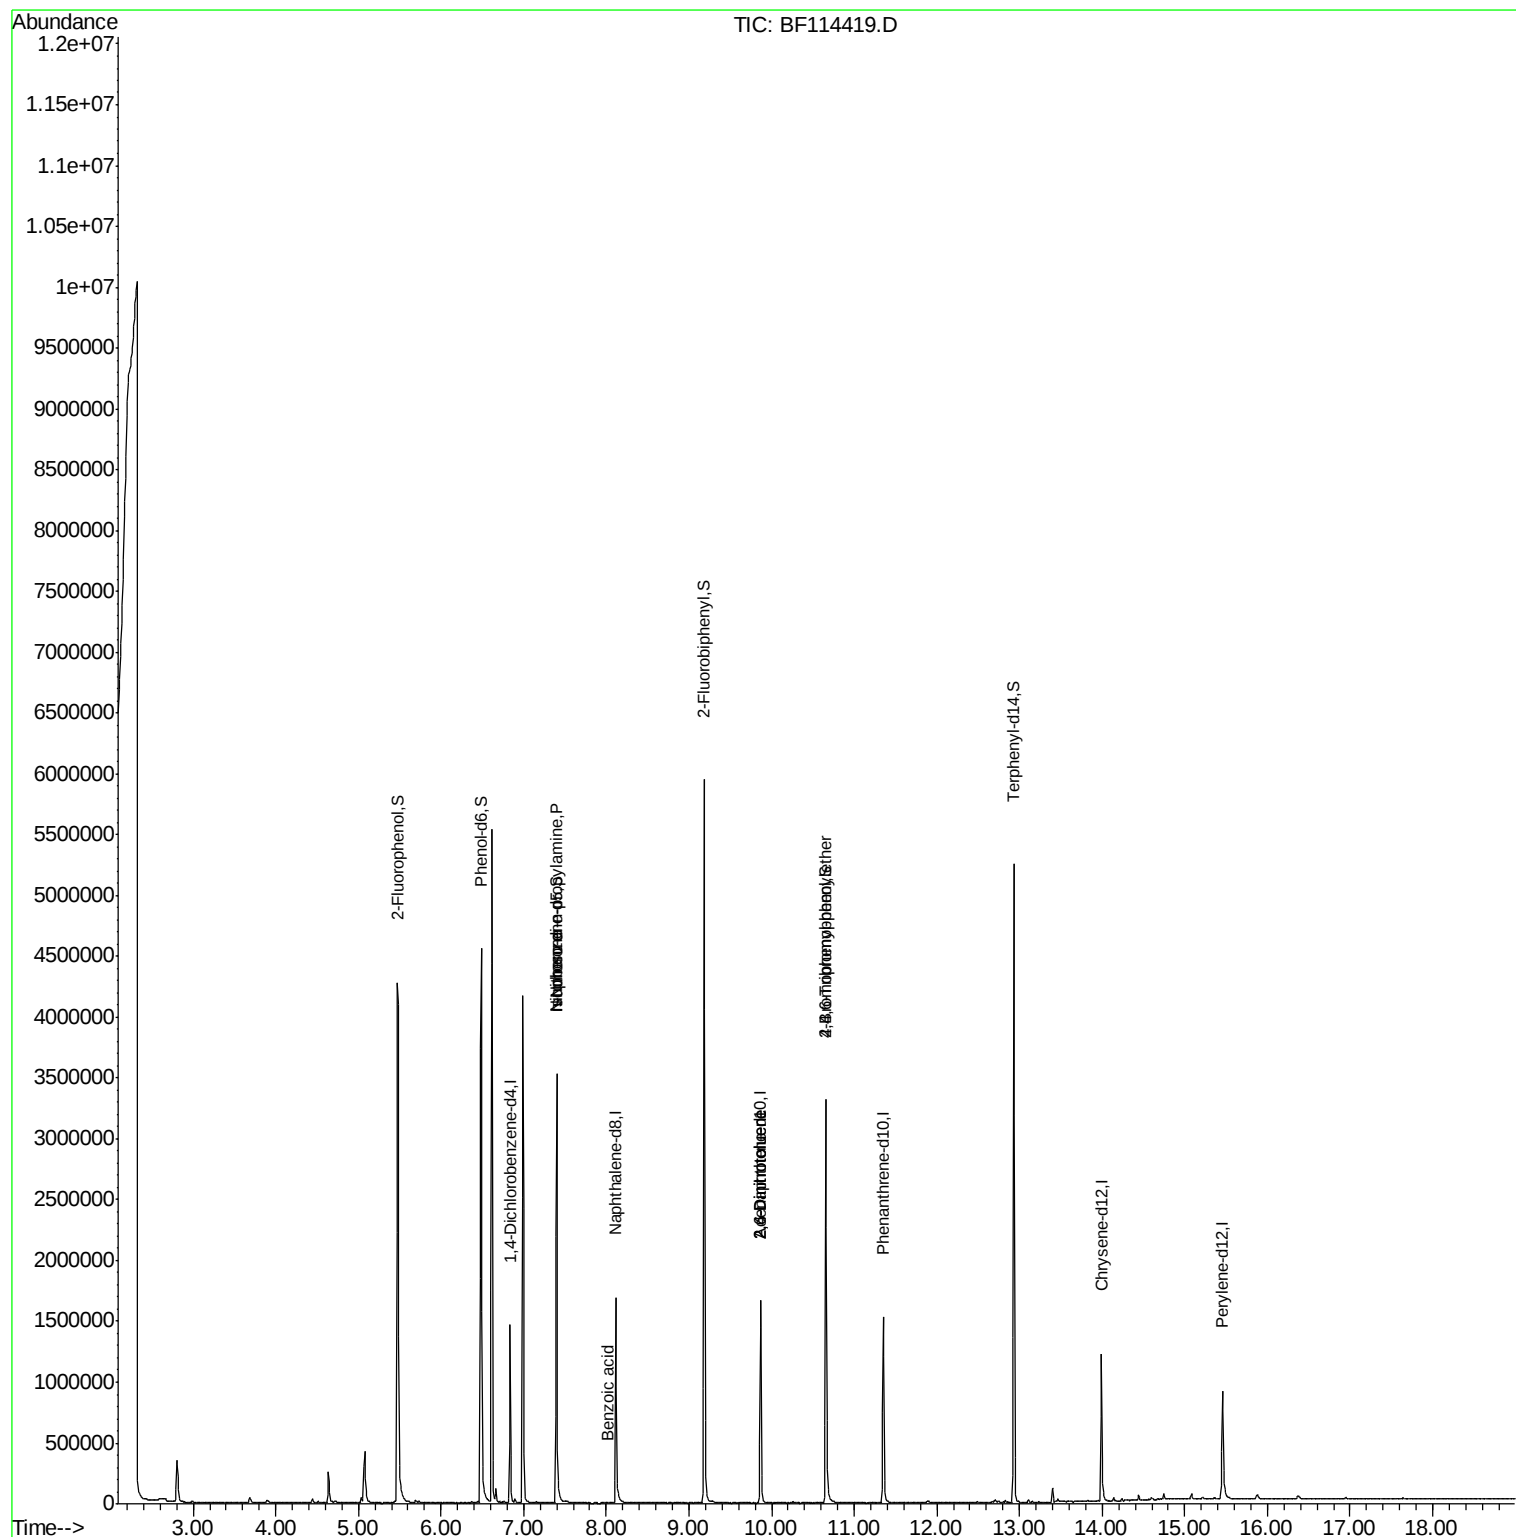

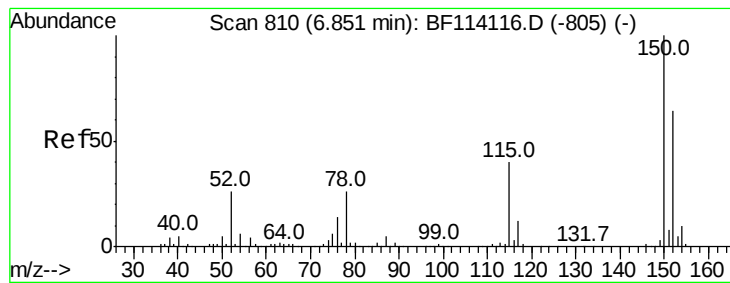


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.83 min Scan# 807
Delta R.T. -0.02 min
Lab File: BF114419.D
Acq: 19 May 2019 4:57

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 222715
Ion Ratio Lower Upper
152 100
150 155.6 124.3 186.5
115 60.8 49.1 73.7

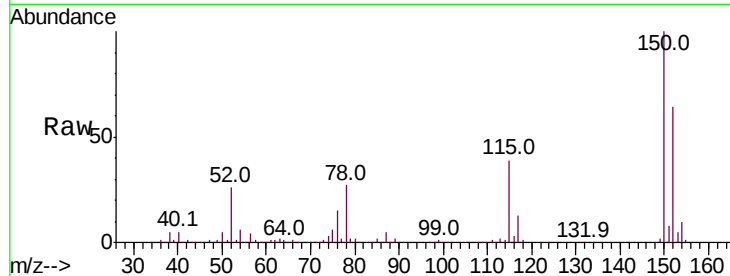


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

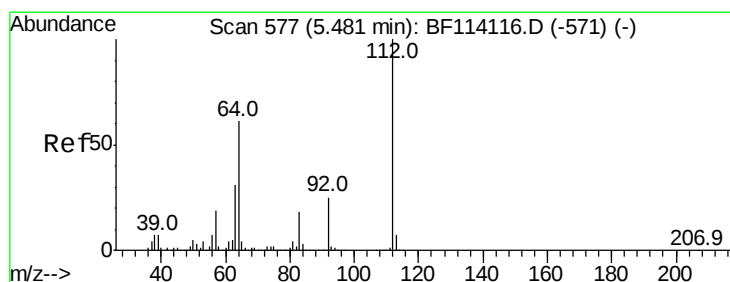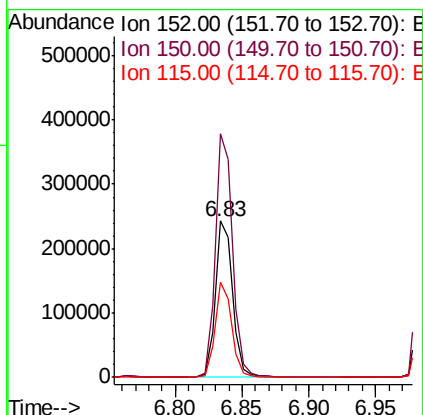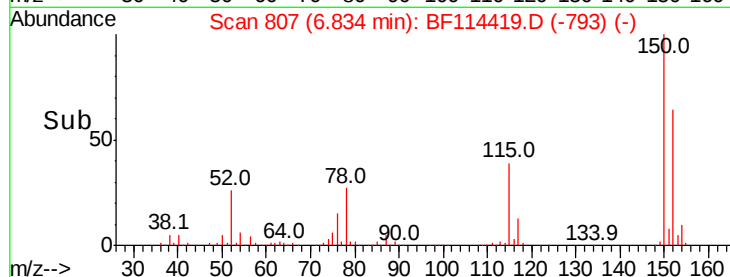



#5

2-Fluorophenol
Concen: 99.785 ng
RT: 5.48 min Scan# 577
Delta R.T. 0.00 min
Lab File: BF114419.D
Acq: 19 May 2019 4:57

Tgt Ion:112 Resp: 1380988
Ion Ratio Lower Upper
112 100
64 61.6 49.0 73.6
63 31.0 24.6 37.0

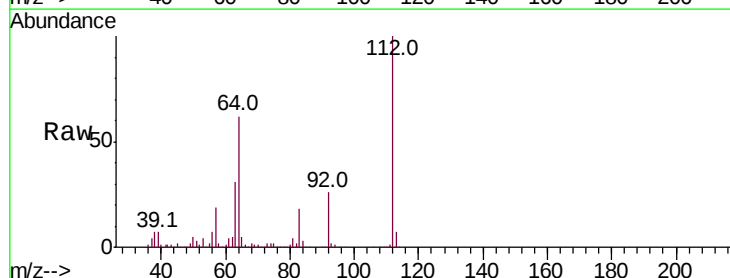

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

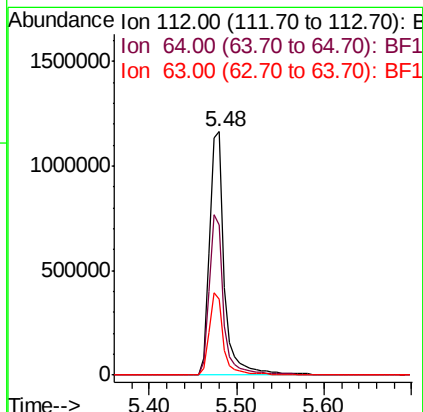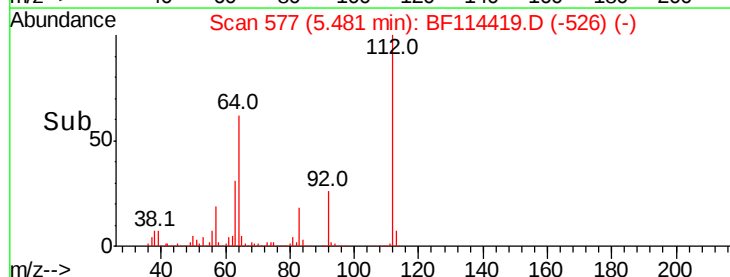



#7

Phenol-d6

Concen: 102.503 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF114419.D

Acq: 19 May 2019 4:57





Instrument :

BNA_F

ClientSampleId :

Tot Ion: 99 Resp: 1677826

Ion	Ratio	Lower	Upper
99	100		
42	22.0	17.9	26.9
71	33.0	26.2	39.2

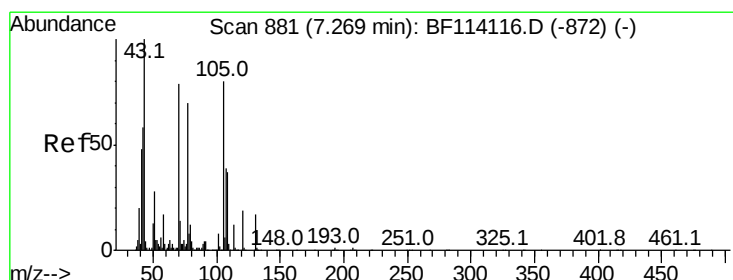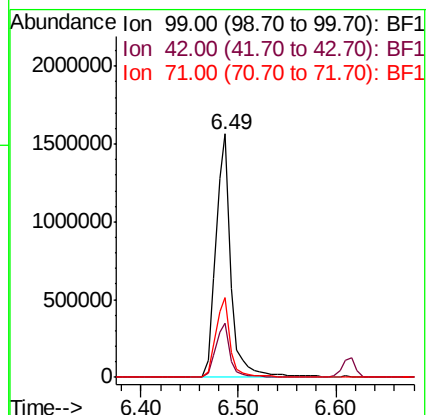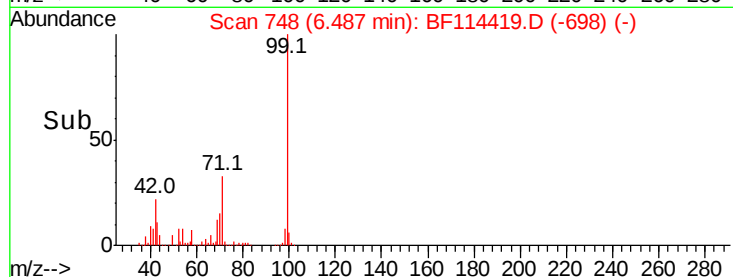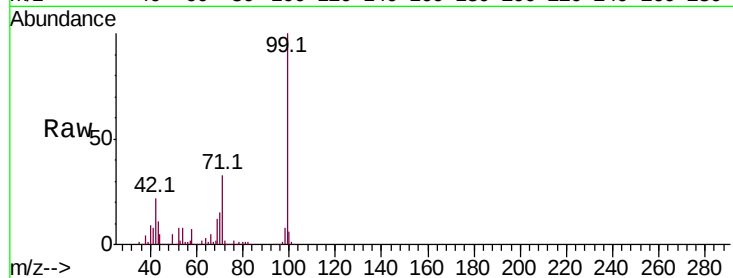

#19

n-Nitroso-di-n-propylamine

Concen: 14.758 ng

RT: 7.40 min Scan# 903




Delta R.T. 0.13 min


Lab File: BF114419.D

Acq: 19 May 2019 4:57

Tgt Ion: 70 Resp: 153117

Ion	Ratio	Lower	Upper
70	100		
42	57.1	58.6	87.8#
101	0.0	7.8	11.8#
130	2.4	17.1	25.7#

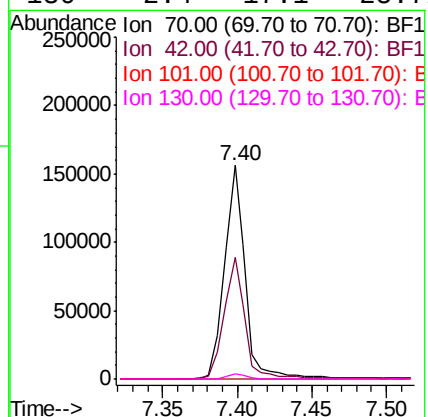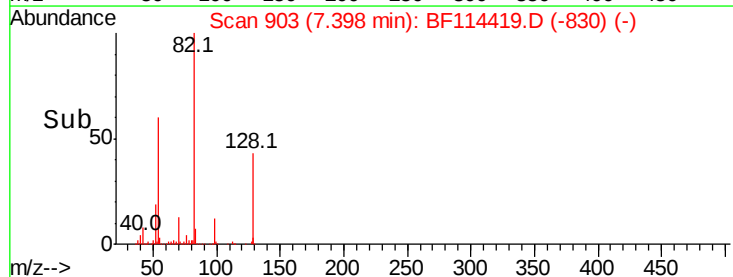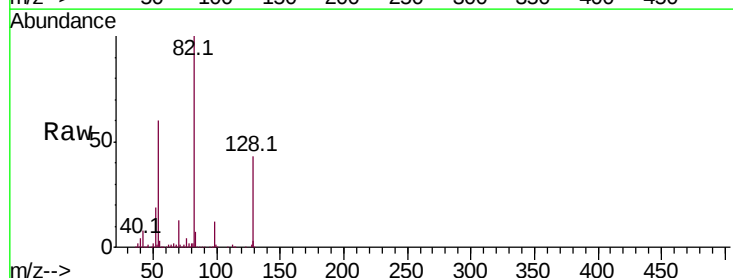


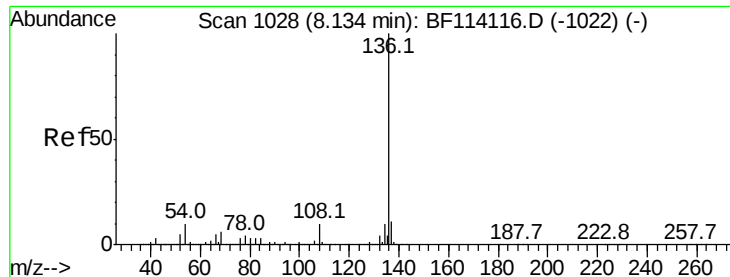




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.12 min Scan# 1025
Delta R.T. -0.02 min
Lab File: BF114419.D
Acq: 19 May 2019 4:57

Instrument :
BNA_F
ClientSampleId :

Tot Ion:136	Resp:	836573
Ion	Ratio	Lower Upper
136	100	
137	10.9	8.8 13.2
54	9.1	7.8 11.8
68	5.8	5.1 7.7

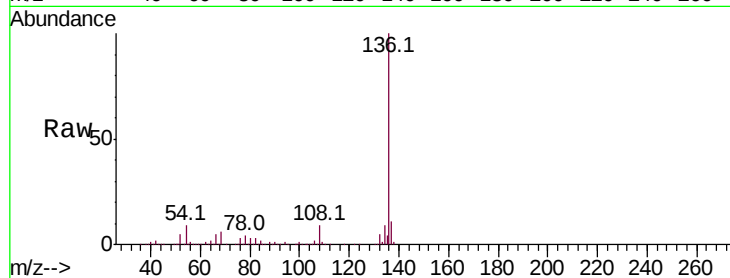


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

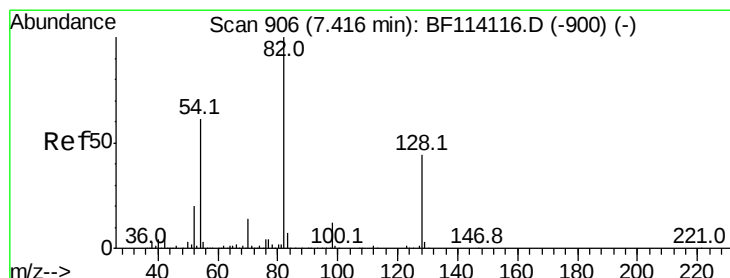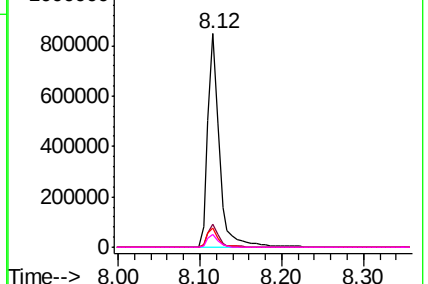
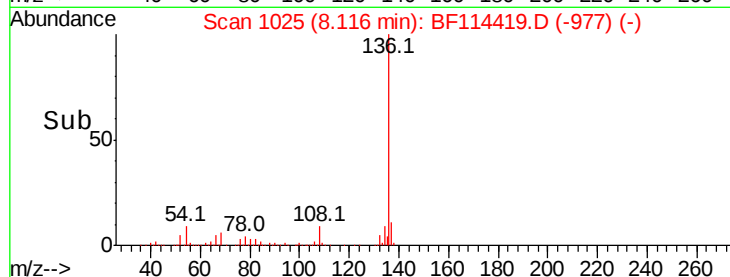


#23
Nitrobenzene-d5
Concen: 79.389 ng
RT: 7.40 min Scan# 903
Delta R.T. -0.02 min
Lab File: BF114419.D
Acq: 19 May 2019 4:57

Tgt Ion: 82	Resp: 1183441
Ion Ratio	Lower Upper
82 100	
128 43.4	35.5 53.3
54 59.8	48.5 72.7

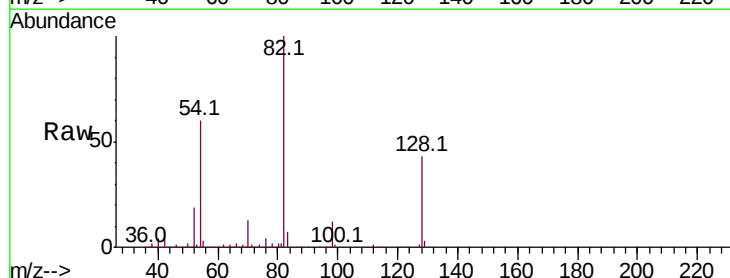

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

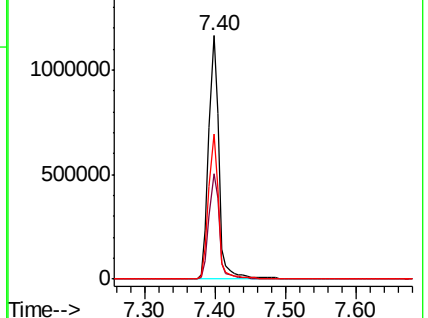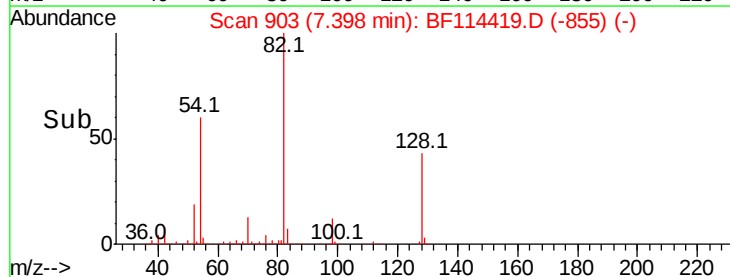



#25

Isophorone

Concen: 42.806 ng

RT: 7.40 min Scan# 903

Delta R.T. -0.28 min

Lab File: BF114419.D

Acq: 19 May 2019 4:57

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 1183433

Ion Ratio Lower Upper

82 100

95 0.0 5.6 8.4#




138 0.0 14.8 22.2#

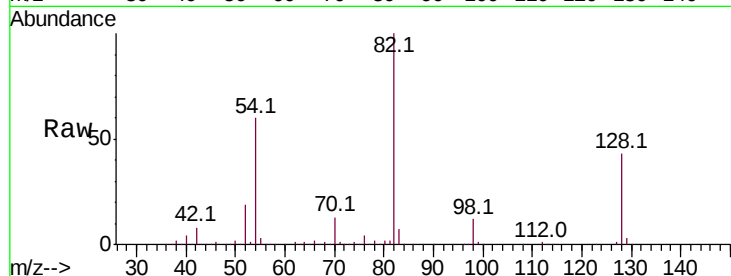

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

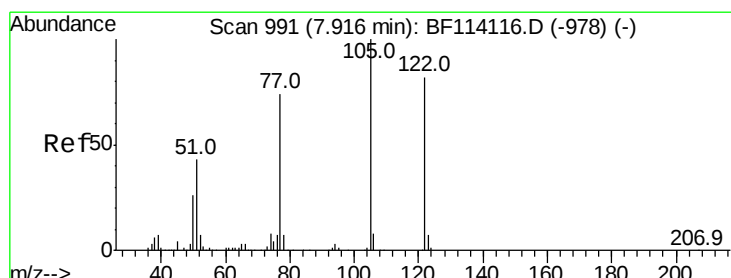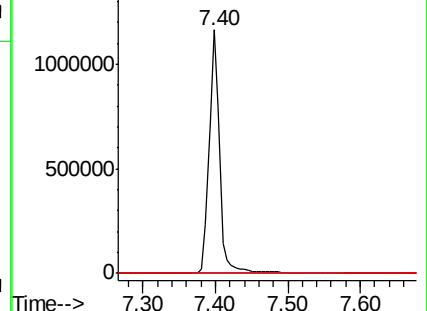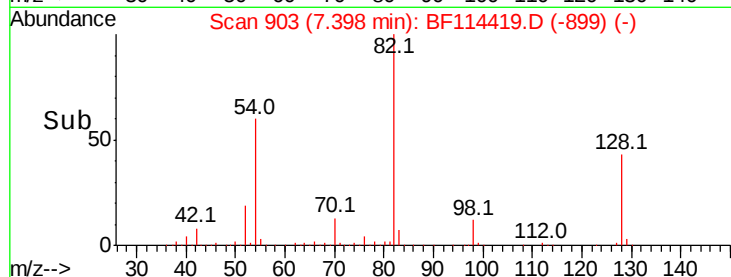

#32

Benzoic acid

Concen: 7.084 ng

RT: 8.02 min Scan# 1008

Delta R.T. 0.10 min

Lab File: BF114419.D

Acq: 19 May 2019 4:57


Tgt Ion:122 Resp: 614

Ion Ratio Lower Upper

122 100

105 108.4 99.9 139.9



77 94.5 69.4 109.4

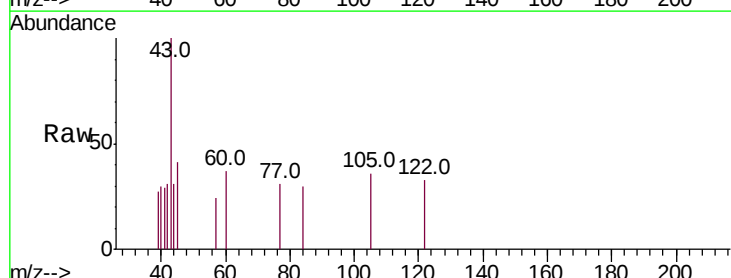


Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BF1

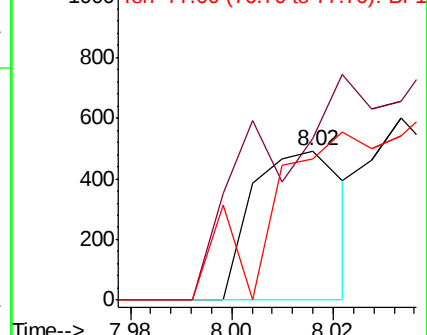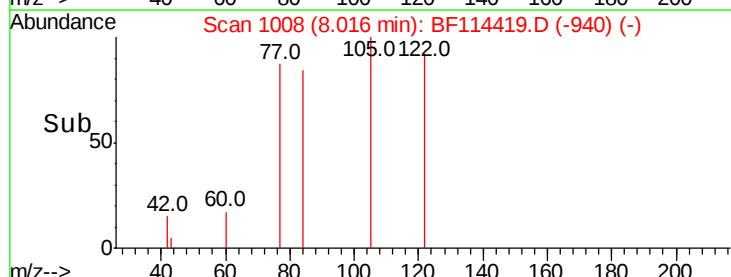


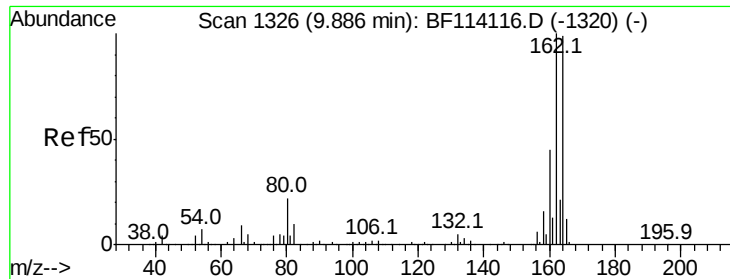




#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. -0.02 min
 Lab File: BF114419.D
 Acq: 19 May 2019 4:57

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
164	100		
162	102.0	80.6	120.8
160	46.1	36.5	54.7

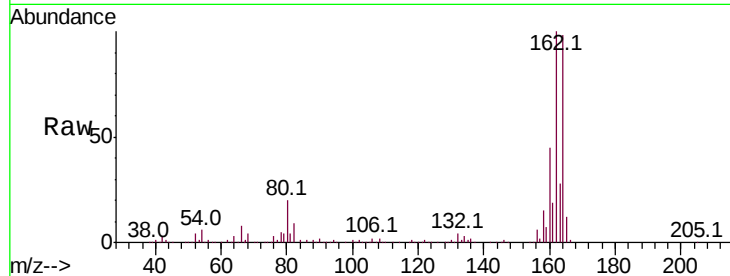


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

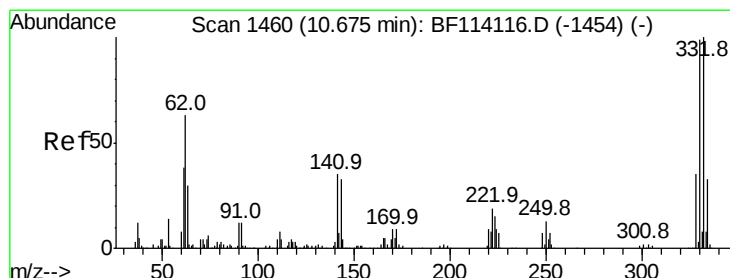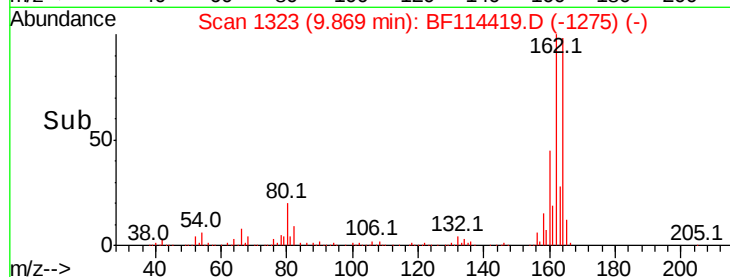
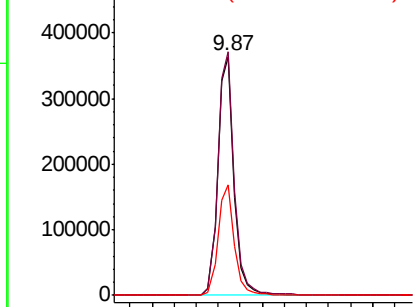



#42
 2,4,6-Tribromophenol
 Concen: 114.987 ng
 RT: 10.66 min Scan# 1457
 Delta R.T. -0.02 min
 Lab File: BF114419.D
 Acq: 19 May 2019 4:57

Tgt Ion	Ratio	Lower	Upper
330	100		
332	104.2	81.4	122.2
141	34.0	26.6	40.0

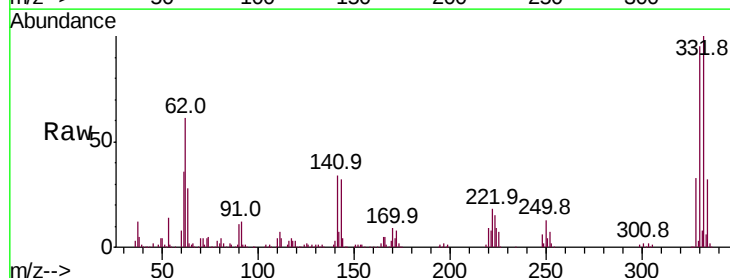

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

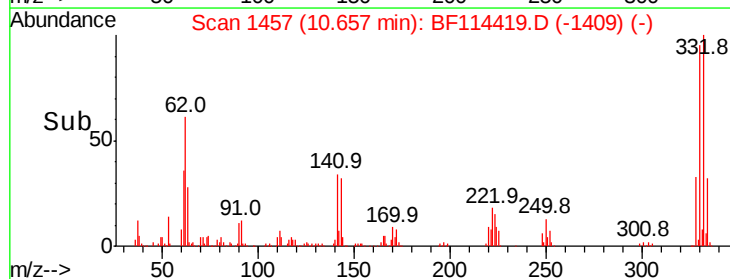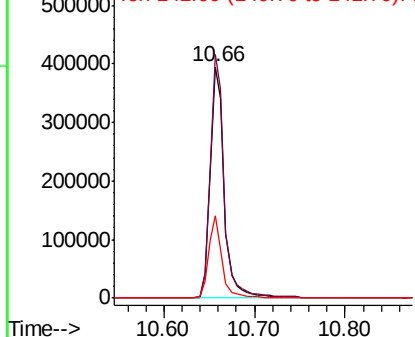




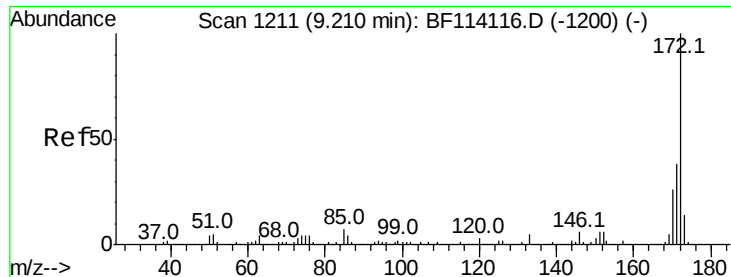


#45
 2-Fluorobiphenyl
 Concen: 79.253 ng
 RT: 9.19 min Scan# 1207
 Delta R.T. -0.02 min
 Lab File: BF114419.D
 Acq: 19 May 2019 4:57

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:172 Resp: 1930667




Ion	Ratio	Lower	Upper
172	100		
171	36.2	30.7	46.1
170	24.4	20.5	30.7

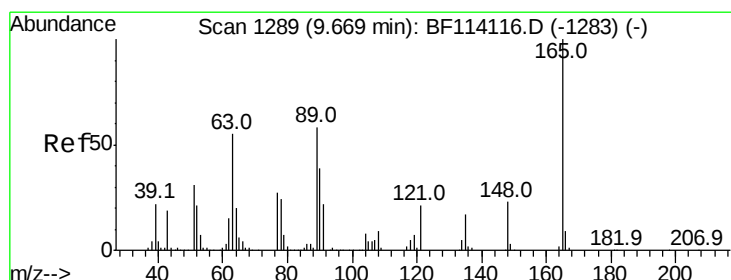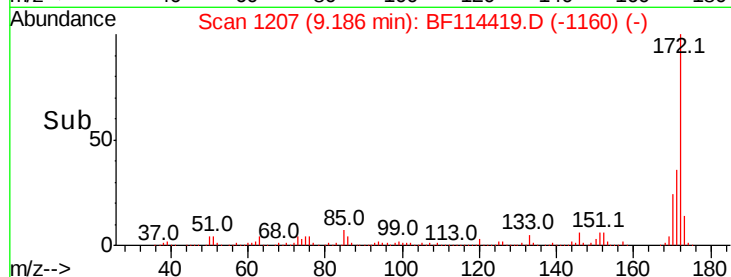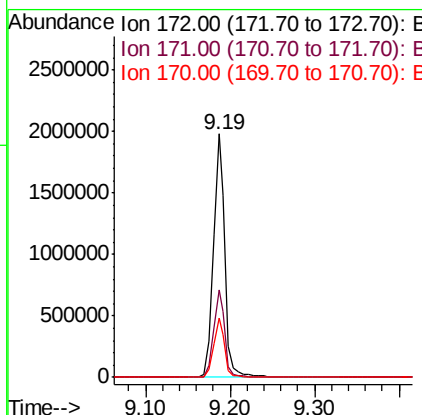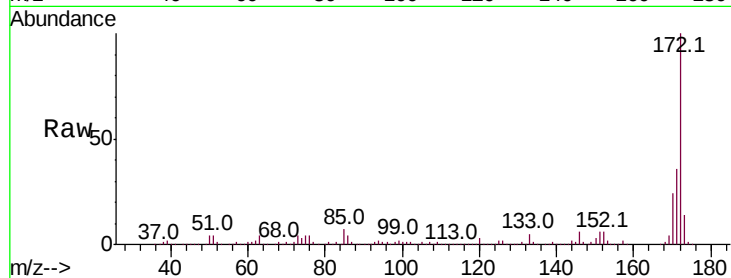


#51
 2,6-Dinitrotoluene
 Concen: 7.848 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. 0.20 min
 Lab File: BF114419.D
 Acq: 19 May 2019 4:57

Tgt Ion:165 Resp: 47088

Ion	Ratio	Lower	Upper
165	100		
63	1.2	50.2	75.4#
89	1.4	46.6	69.8#

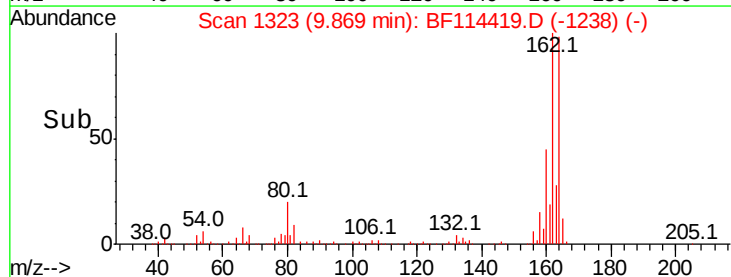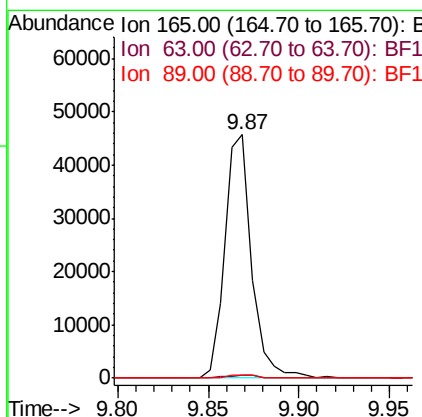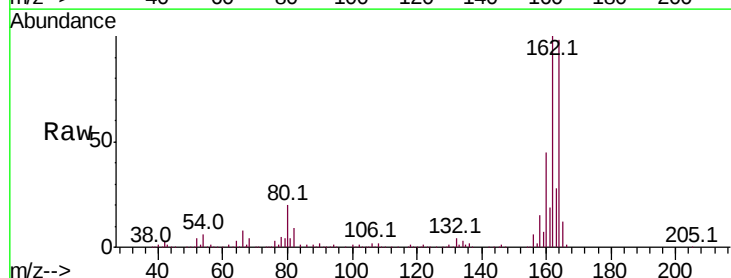


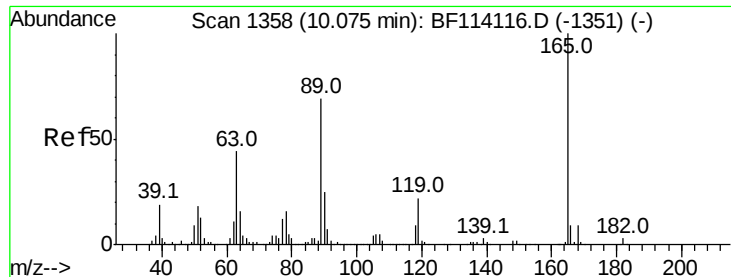

#57
 2,4-Dinitrotoluene
 Concen: 5.782 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. -0.21 min
 Lab File: BF114419.D
 Acq: 19 May 2019 4:57

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.2	35.5	53.3#
89	1.4	55.2	82.8#
182	0.0	2.2	3.2#



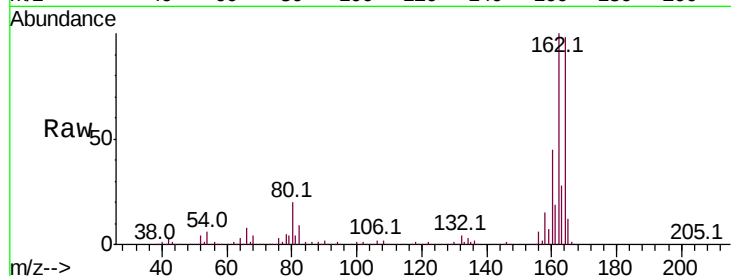


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1


Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

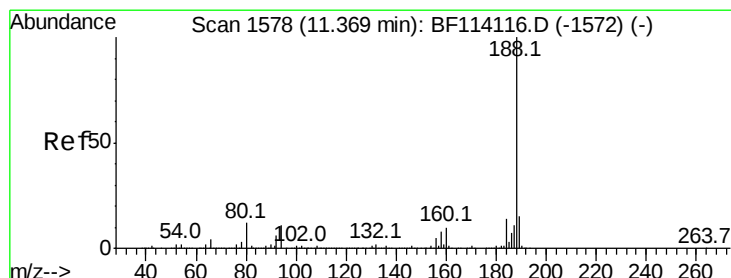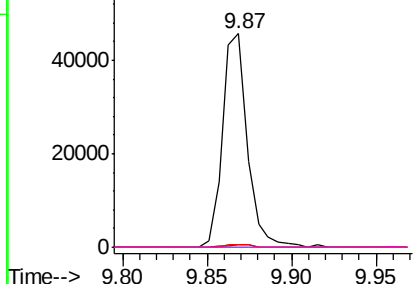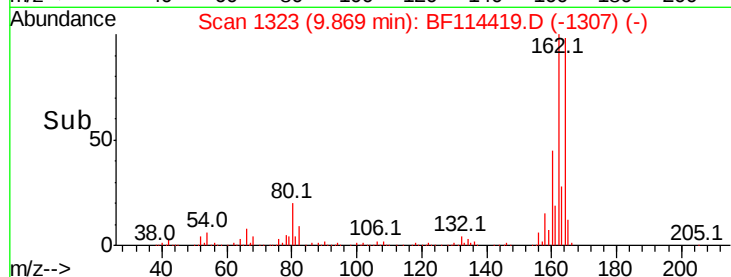

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.35 min Scan# 1575
 Delta R.T. -0.02 min
 Lab File: BF114419.D
 Acq: 19 May 2019 4:57



Tgt Ion	Ratio	Lower	Upper
188	100		
94	10.6	8.4	12.6
80	11.2	9.2	13.8

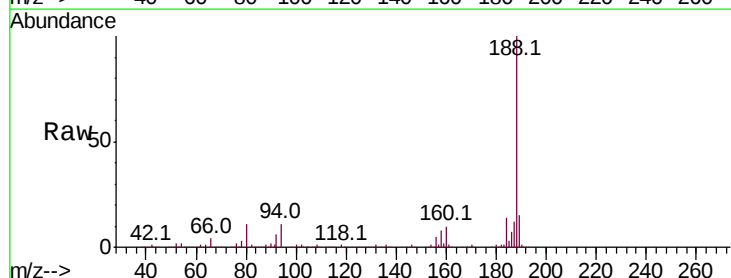


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

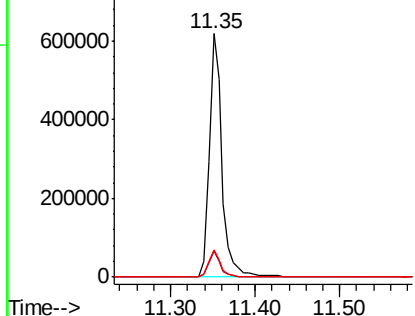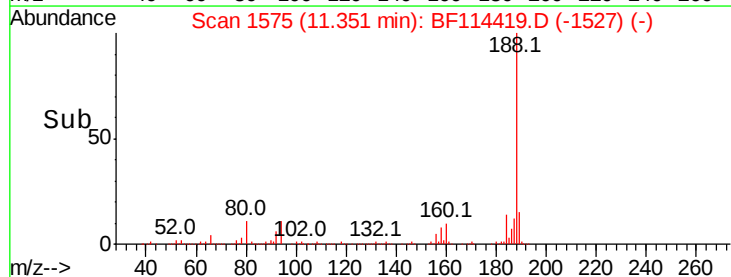

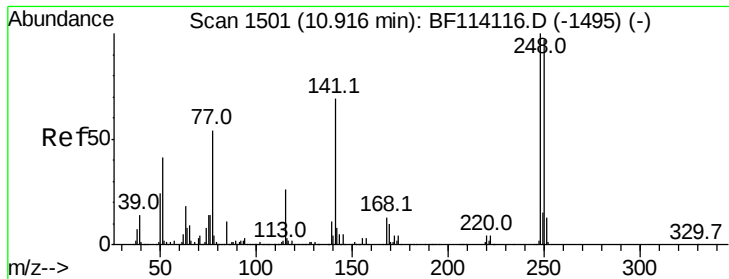

#67

4-Bromophenyl-phenylether

Concen: 3.981 ng

RT: 10.66 min Scan# 1457

Delta R.T. -0.26 min

Lab File: BF114419.D

Acq: 19 May 2019 4:57

Instrument :

BNA_F

ClientSampleId :


Tot Ion:248 Resp: 28447

Ion Ratio Lower Upper

248 100

250 210.8 77.4 116.2#




141 539.7 55.6 83.4#

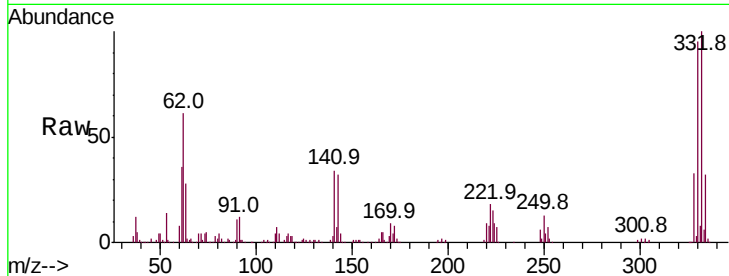

Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

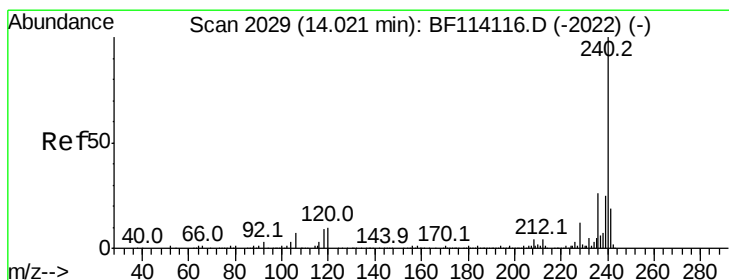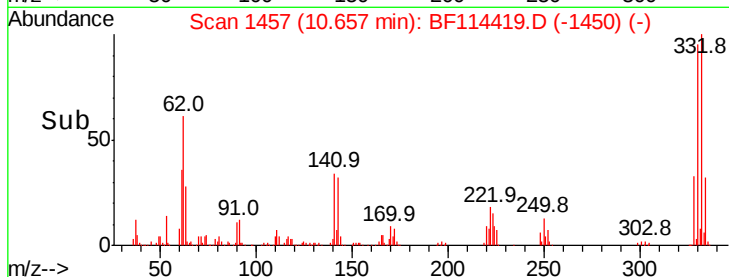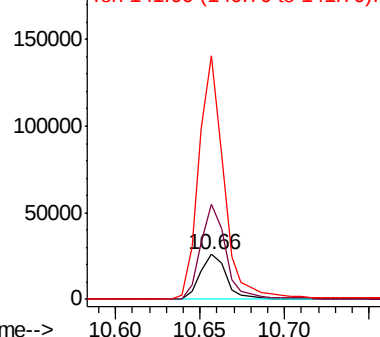

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.99 min Scan# 2024

Delta R.T. -0.03 min

Lab File: BF114419.D

Acq: 19 May 2019 4:57


Tgt Ion:240 Resp: 442086

Ion Ratio Lower Upper

240 100

120 12.9 8.3 12.5#



236 26.4 20.8 31.2

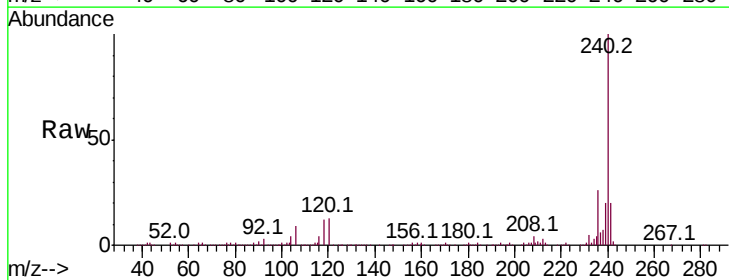


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

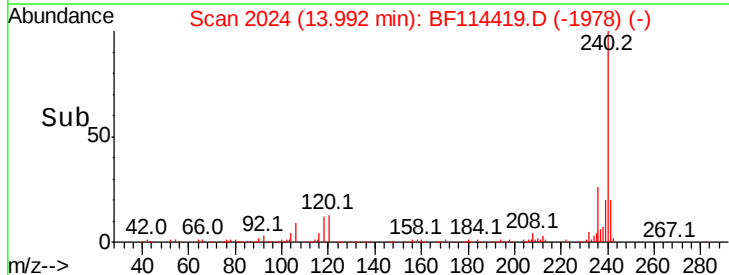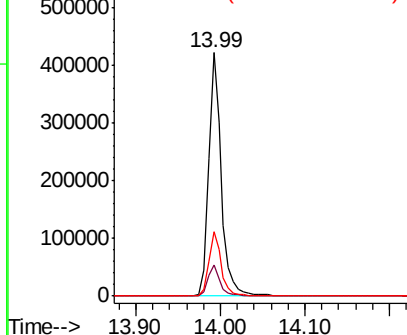

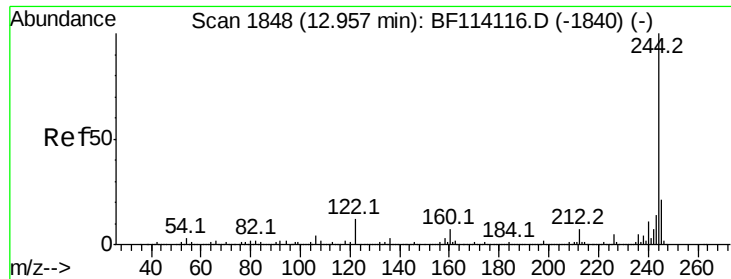

#79

Terphenyl-d14

Concen: 84.785 ng

RT: 12.93 min Scan# 1844

Delta R.T. -0.02 min

Lab File: BF114419.D

Acq: 19 May 2019 4:57

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 1818268

Ion Ratio Lower Upper

244 100

212 6.9 5.8 8.6




122 13.0 9.4 14.2

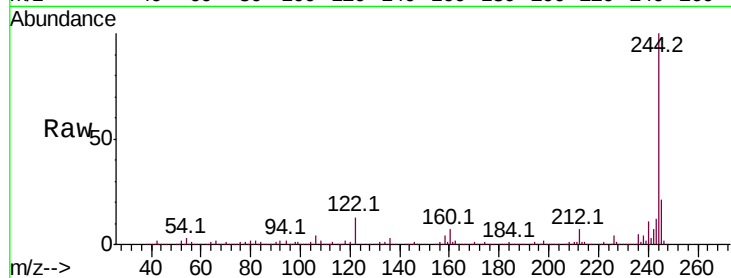

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

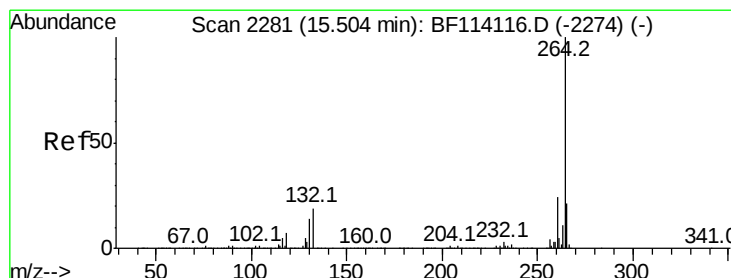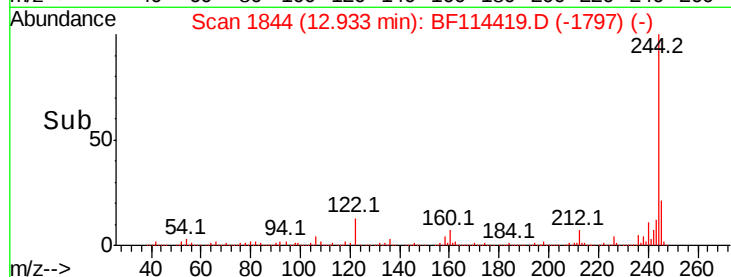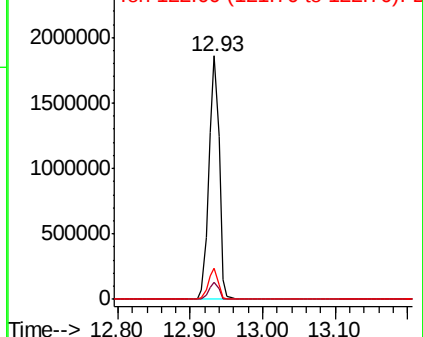

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.46 min Scan# 2273

Delta R.T. -0.05 min

Lab File: BF114419.D

Acq: 19 May 2019 4:57


Tgt Ion:264 Resp: 488117

Ion Ratio Lower Upper

264 100

260 24.5 19.4 29.0

265 22.5 16.9 25.3

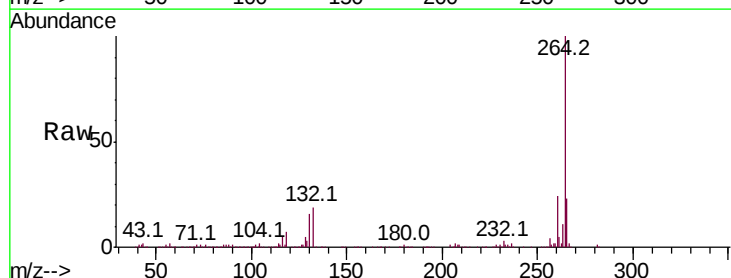

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

