

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
 Data File : BF114410.D
 Acq On : 19 May 2019 00:59
 Operator : JU/SJ
 Sample : K2896-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-20-S

Quant Time: May 20 08:09:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 10 15:56:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.84	152	223700	20.00	ng	-0.01
21) Naphthalene-d8	8.12	136	858576	20.00	ng	-0.02
39) Acenaphthene-d10	9.87	164	397675	20.00	ng	-0.02
64) Phenanthrene-d10	11.35	188	760166	20.00	ng	-0.02
76) Chrysene-d12	13.99	240	451287	20.00	ng	-0.03
87) Perylene-d12	15.46	264	499543	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	1516906	109.12	ng	0.00
7) Phenol-d6	6.49	99	1840856	111.97	ng	0.00
23) Nitrobenzene-d5	7.40	82	1325100	86.61	ng	-0.02
42) 2,4,6-Tribromophenol	10.66	330	505108	122.86	ng	-0.02
45) 2-Fluorobiphenyl	9.19	172	2265835	86.19	ng	-0.02
79) Terphenyl-d14	12.93	244	2050339	93.66	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
Data File : BF114410.D
Acq On : 19 May 2019 00:59
Operator : JU/SJ
Sample : K2896-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-20-S

Quant Time: May 20 08:09:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 10 15:56:46 2019
Response via : Initial Calibration

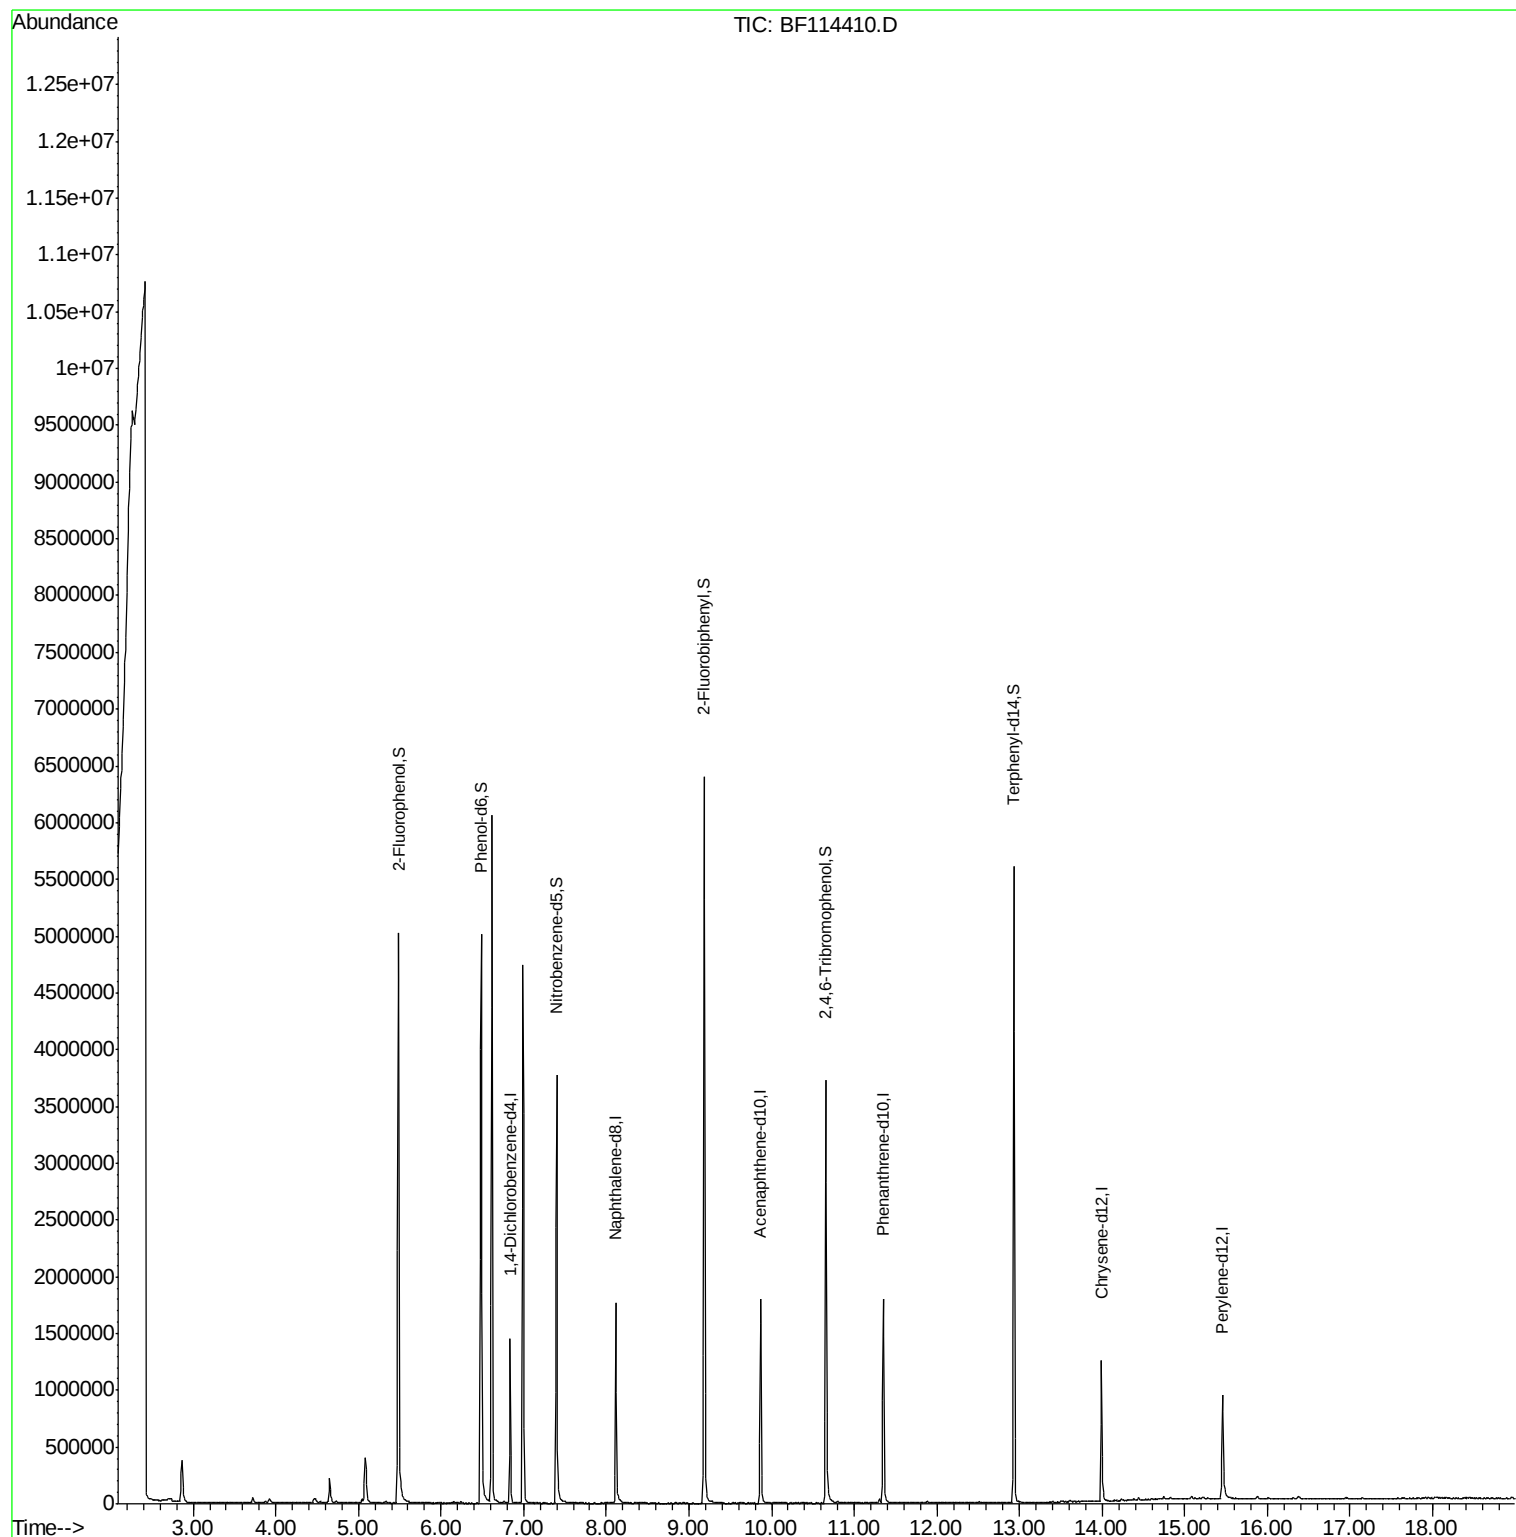

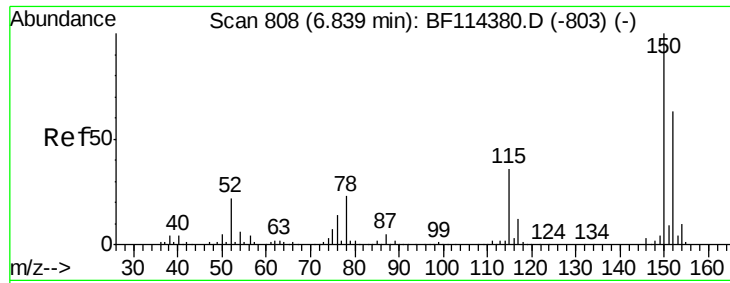


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.84 min Scan# 808
Delta R.T. -0.01 min
Lab File: BF114410.D
Acq: 19 May 2019 00:59

Instrument :
BNA_F
ClientSampleId :
TP-20-S

Tgt Ion:152 Resp: 223700
Ion Ratio Lower Upper
152 100
150 157.0 124.3 186.5
115 59.2 49.1 73.7

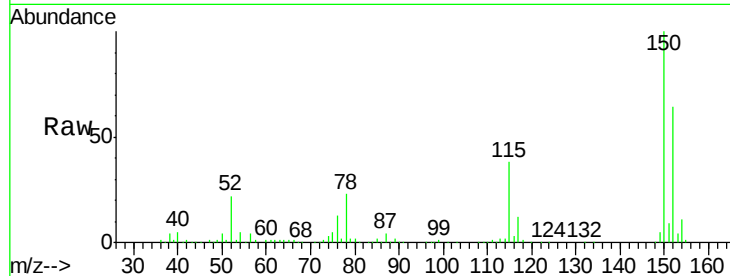


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

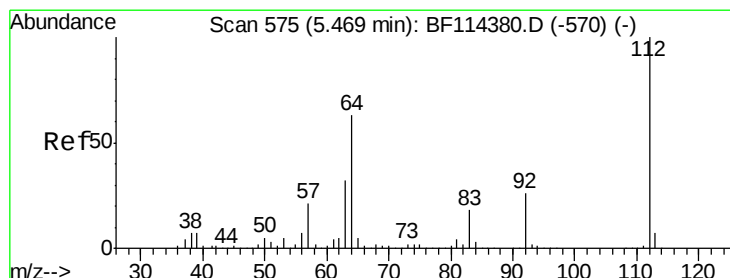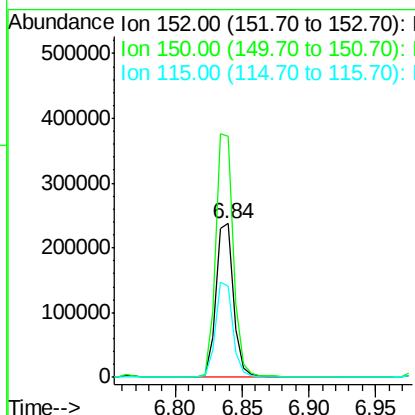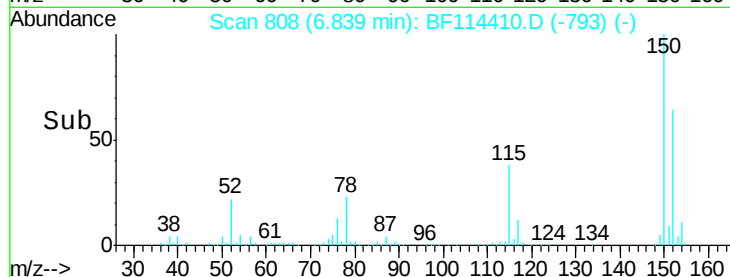



#5


2-Fluorophenol
Concen: 109.124 ng
RT: 5.49 min Scan# 578
Delta R.T. 0.01 min
Lab File: BF114410.D
Acq: 19 May 2019 00:59

Tgt Ion:112 Resp: 1516906
Ion Ratio Lower Upper
112 100
64 63.5 49.0 73.6
63 32.8 24.6 37.0

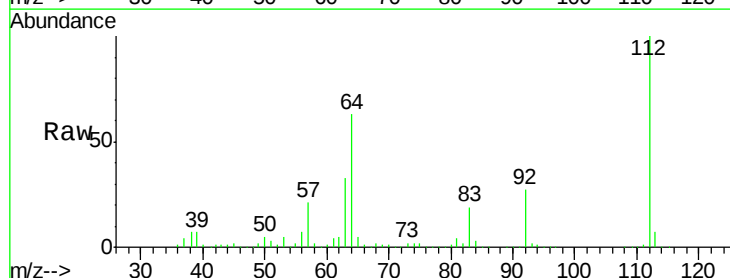

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

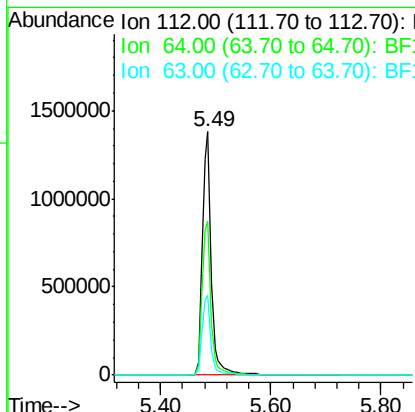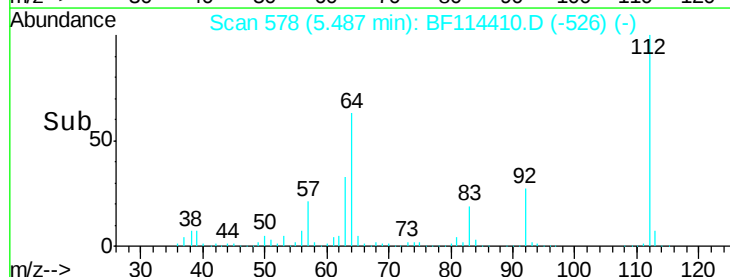

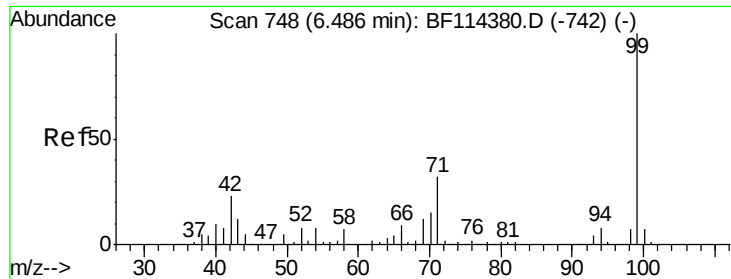

#7

Phenol-d6

Concen: 111.968 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF114410.D

Acq: 19 May 2019 00:59

Instrument :

BNA_F

ClientSampleId :

TP-20-S


Tgt Ion: 99 Resp: 1840856

Ion Ratio Lower Upper

99 100

42 22.0 17.9 26.9




71 32.9 26.2 39.2

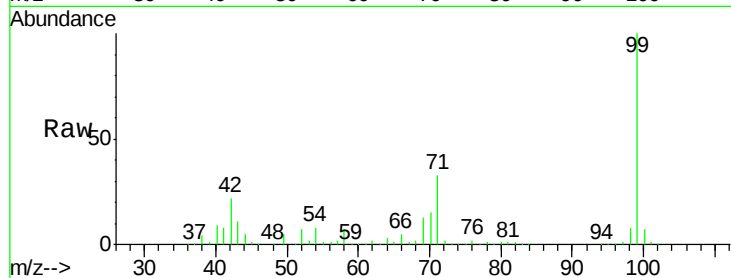

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

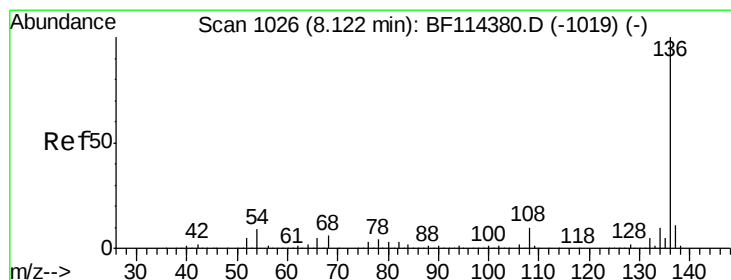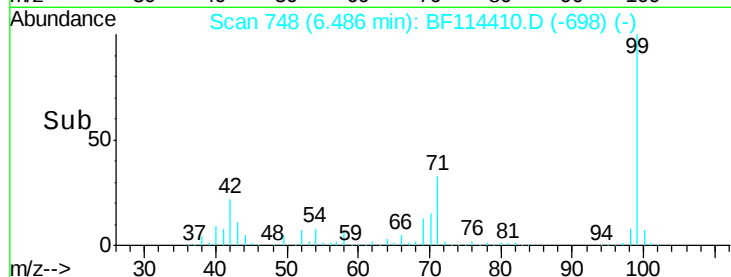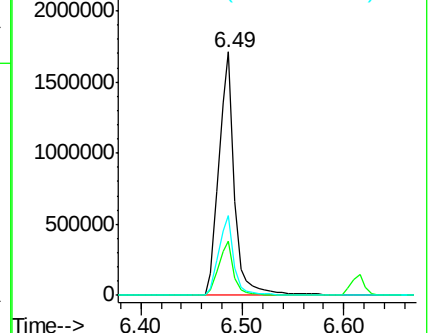

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.02 min

Lab File: BF114410.D

Acq: 19 May 2019 00:59

Tgt Ion: 136 Resp: 858576


Ion Ratio Lower Upper

136 100

137 11.0 8.8 13.2

54 9.6 7.8 11.8

68 6.1 5.1 7.7


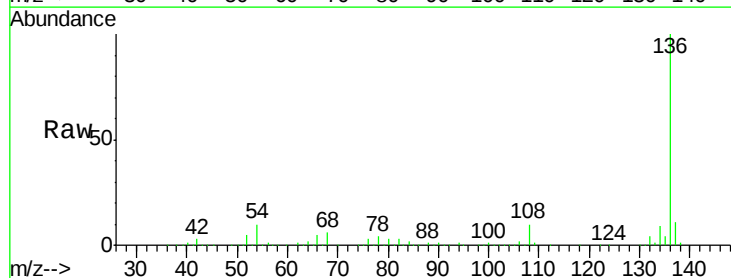


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



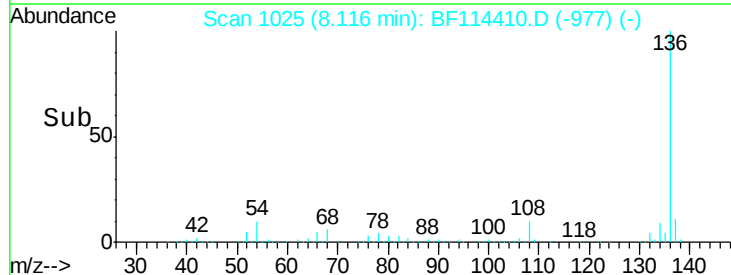
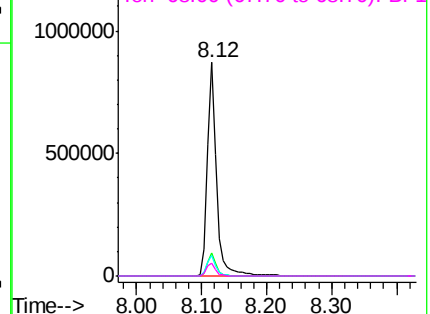




#23
 Nitrobenzene-d5
 Concen: 86.614 ng
 RT: 7.40 min Scan# 903
 Delta R.T. -0.02 min
 Lab File: BF114410.D
 Acq: 19 May 2019 00:59




Instrument :
 BNA_F
 ClientSampleId :
 TP-20-S

Tgt Ion: 82 Resp: 1325100
 Ion Ratio Lower Upper
 82 100
 128 44.1 35.5 53.3
 54 59.6 48.5 72.7

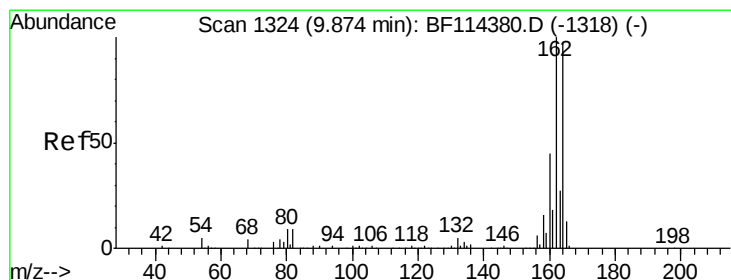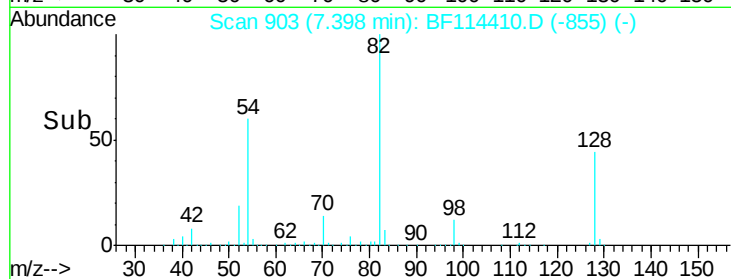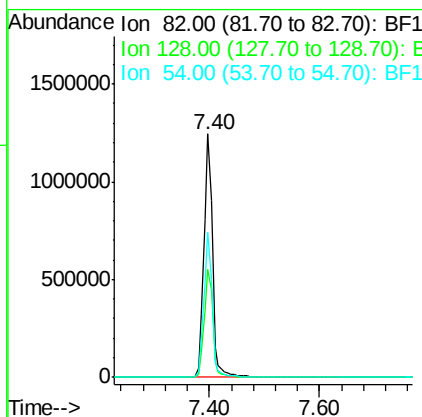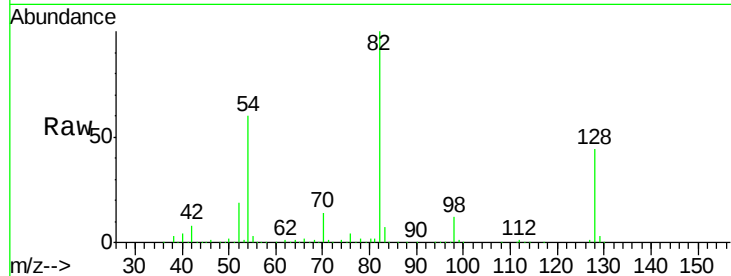

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. -0.02 min
 Lab File: BF114410.D
 Acq: 19 May 2019 00:59

Tgt Ion: 164 Resp: 397675
 Ion Ratio Lower Upper
 164 100
 162 101.6 80.6 120.8
 160 46.2 36.5 54.7

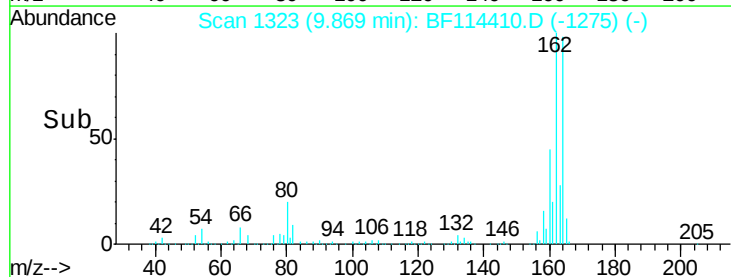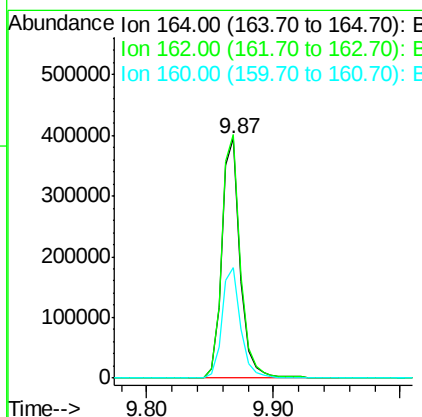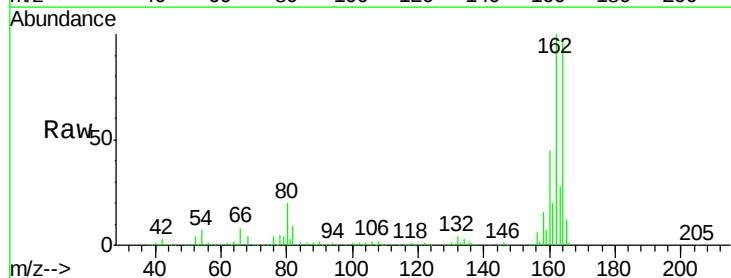



#42

2,4,6-Tribromophenol

Concen: 122.859 ng

RT: 10.66 min Scan# 1457

Delta R.T. -0.02 min

Lab File: BF114410.D

Acq: 19 May 2019 00:59

Instrument :

BNA_F

ClientSampleId :

TP-20-S


Tgt Ion:330 Resp: 505108

Ion Ratio Lower Upper

330 100

332 102.6 81.4 122.2




141 33.2 26.6 40.0

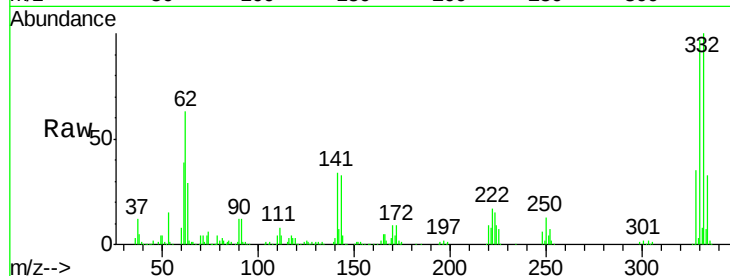

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

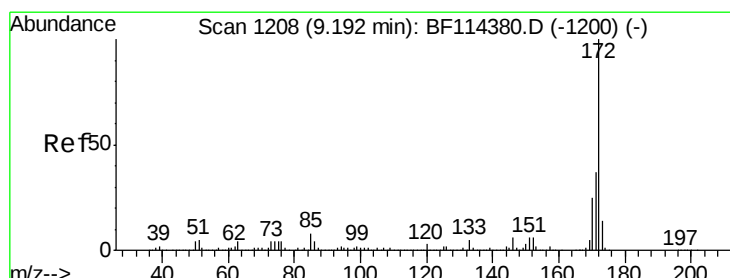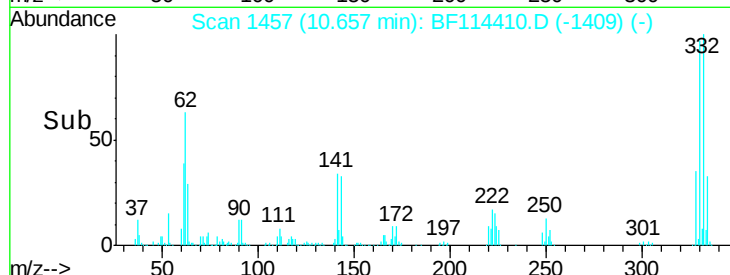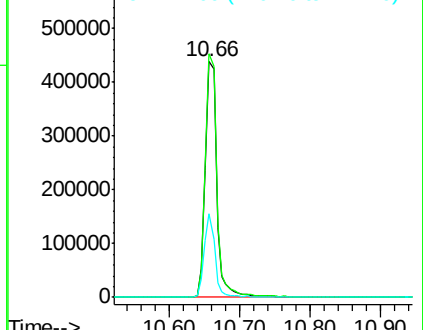

#45

2-Fluorobiphenyl

Concen: 86.187 ng

RT: 9.19 min Scan# 1207

Delta R.T. -0.02 min

Lab File: BF114410.D

Acq: 19 May 2019 00:59


Tgt Ion:172 Resp: 2265835

Ion Ratio Lower Upper

172 100

171 36.8 30.7 46.1



170 24.8 20.5 30.7

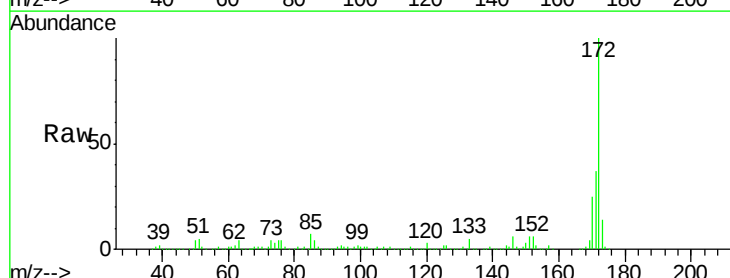


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



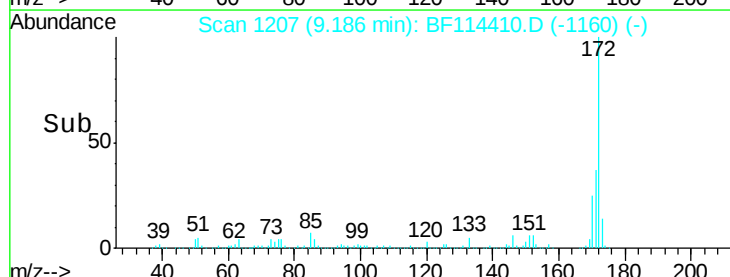
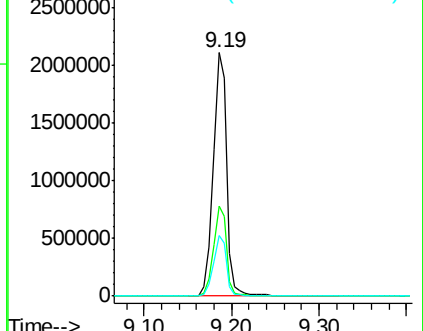


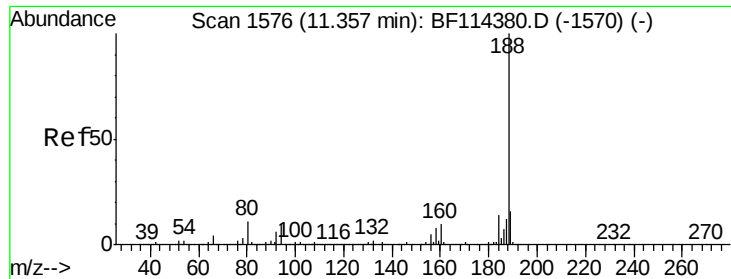

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.35 min Scan# 1575
Delta R.T. -0.02 min
Lab File: BF114410.D
Acq: 19 May 2019 00:59




Instrument :
BNA_F
ClientSampleId :
TP-20-S


Tgt Ion:188 Resp: 760166
Ion Ratio Lower Upper
188 100
94 10.3 8.4 12.6
80 10.7 9.2 13.8

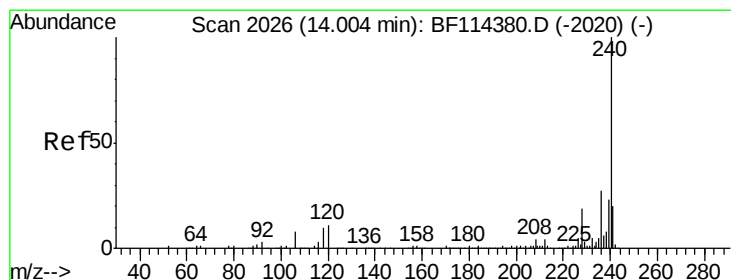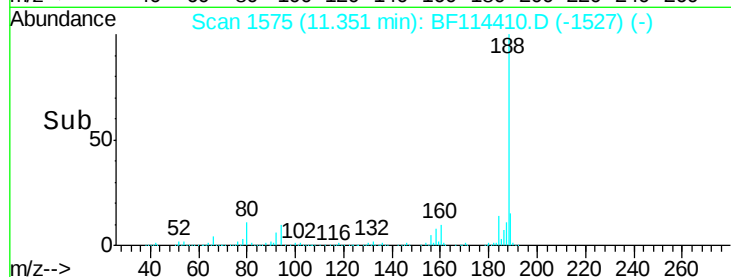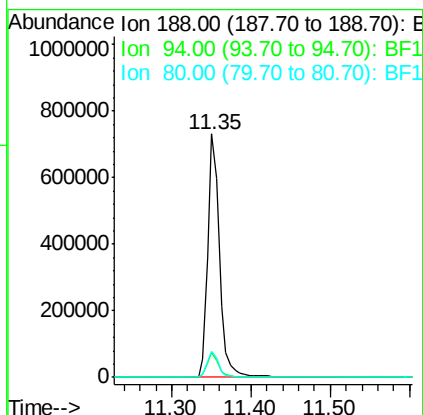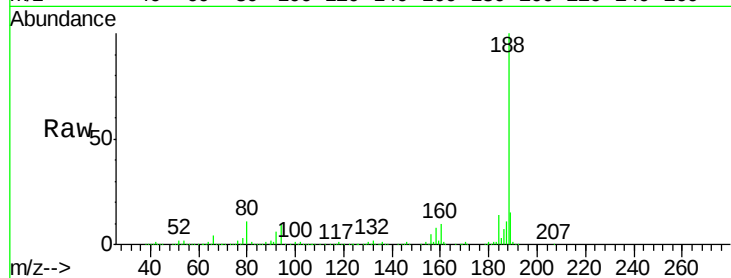

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.99 min Scan# 2024
Delta R.T. -0.03 min
Lab File: BF114410.D
Acq: 19 May 2019 00:59

Tgt Ion:240 Resp: 451287
Ion Ratio Lower Upper
240 100
120 12.7 8.3 12.5#
236 26.6 20.8 31.2

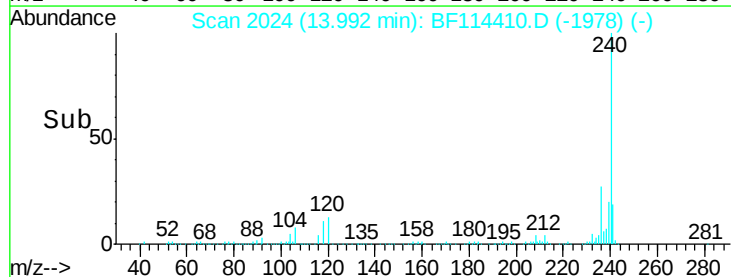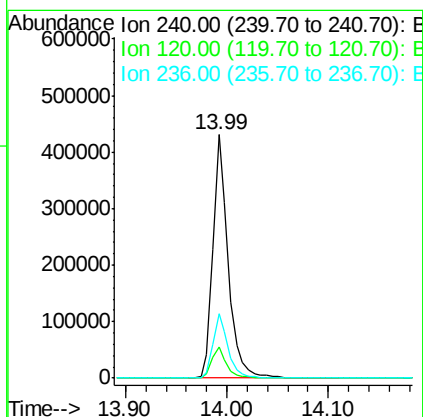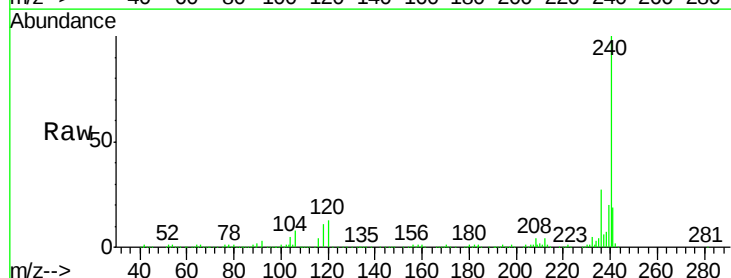

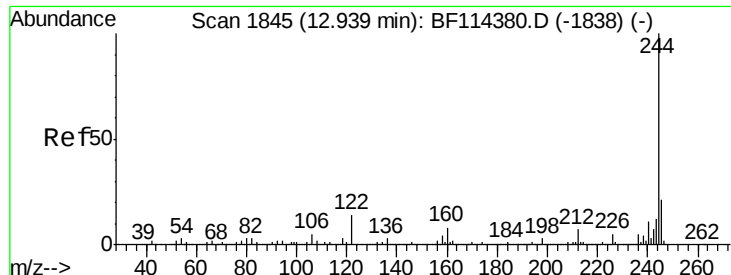

#79

Terphenyl-d14

Concen: 93.657 ng

RT: 12.93 min Scan# 1844

Delta R.T. -0.02 min

Lab File: BF114410.D

Acq: 19 May 2019 00:59

Instrument :

BNA_F

ClientSampleId :

TP-20-S


Tgt Ion:244 Resp: 2050339

Ion Ratio Lower Upper

244 100

212 7.0 5.8 8.6




122 13.2 9.4 14.2

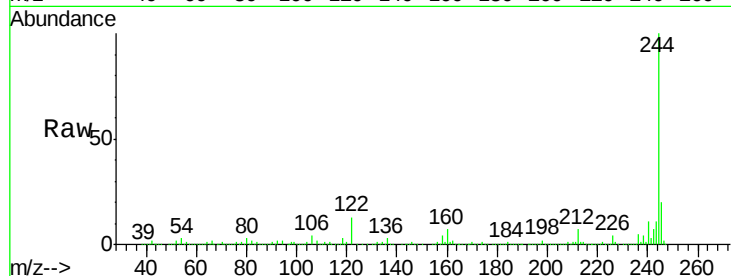

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

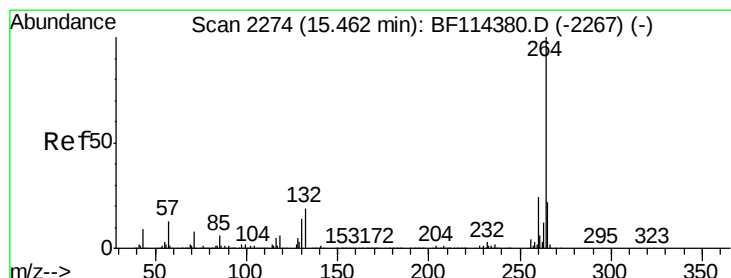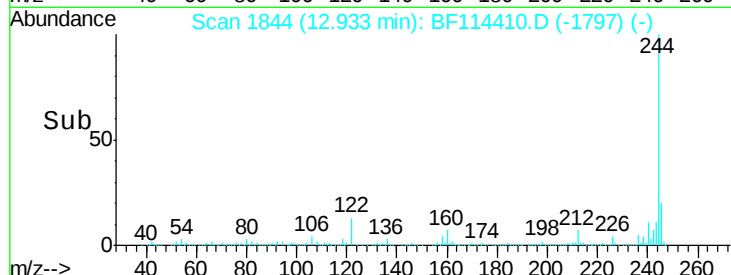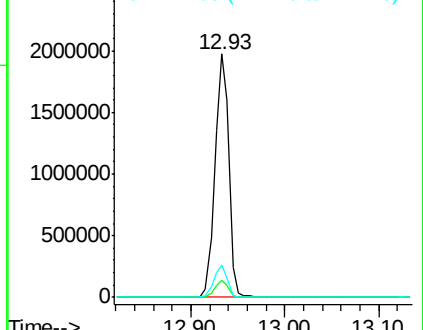

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.46 min Scan# 2273

Delta R.T. -0.05 min

Lab File: BF114410.D

Acq: 19 May 2019 00:59


Tgt Ion:264 Resp: 499543

Ion Ratio Lower Upper

264 100

260 22.8 19.4 29.0

265 21.6 16.9 25.3

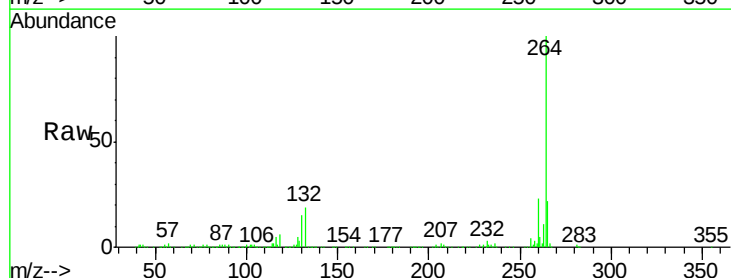

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

