

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
 Data File : BF114421.D
 Acq On : 19 May 2019 5:50
 Operator : JU/SJ
 Sample : PB119833TB
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB119833TB

Quant Time: May 20 08:58:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 10 15:56:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	235784	20.00	ng	-0.02
21) Naphthalene-d8	8.12	136	873766	20.00	ng	-0.02
39) Acenaphthene-d10	9.87	164	394842	20.00	ng	-0.02
64) Phenanthrene-d10	11.35	188	717500	20.00	ng	-0.02
76) Chrysene-d12	13.99	240	444717	20.00	ng	-0.03
87) Perylene-d12	15.46	264	472573	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	1555931	106.19	ng	0.00
7) Phenol-d6	6.49	99	2023515	116.77	ng	0.00
23) Nitrobenzene-d5	7.40	82	1269014	81.51	ng	-0.02
42) 2,4,6-Tribromophenol	10.66	330	400040	98.00	ng	-0.02
45) 2-Fluorobiphenyl	9.19	172	2187715	83.81	ng	-0.02
79) Terphenyl-d14	12.93	244	1843282	85.44	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
Data File : BF114421.D
Acq On : 19 May 2019 5:50
Operator : JU/SJ
Sample : PB119833TB
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119833TB

Quant Time: May 20 08:58:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 10 15:56:46 2019
Response via : Initial Calibration

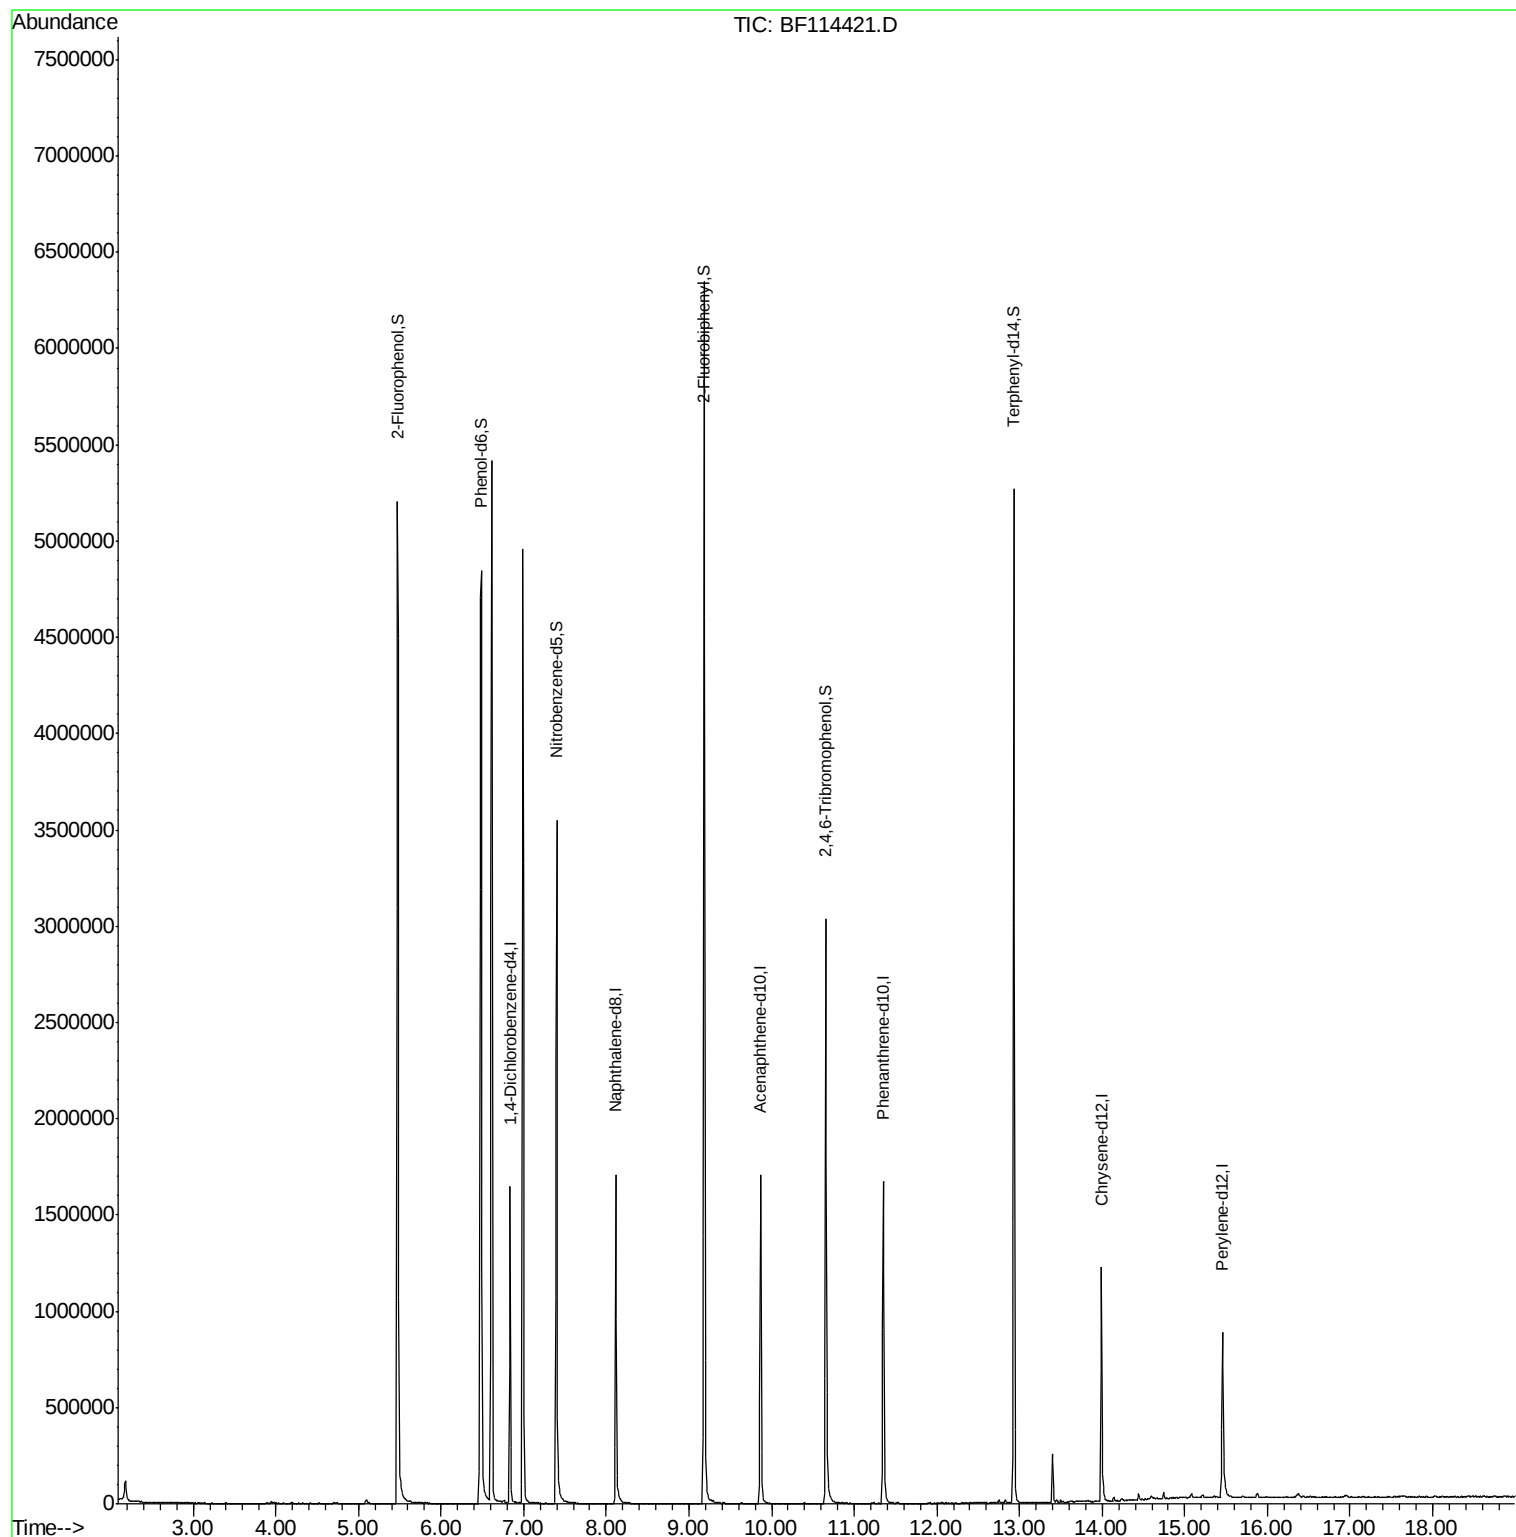

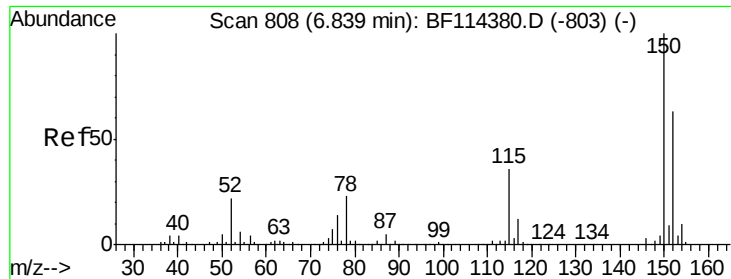


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.83 min Scan# 807
Delta R.T. -0.02 min
Lab File: BF114421.D
Acq: 19 May 2019 5:50

Instrument :
BNA_F
ClientSampleId :
PB119833TB

Tgt Ion:152 Resp: 235784
Ion Ratio Lower Upper
152 100
150 157.8 124.3 186.5
115 60.1 49.1 73.7

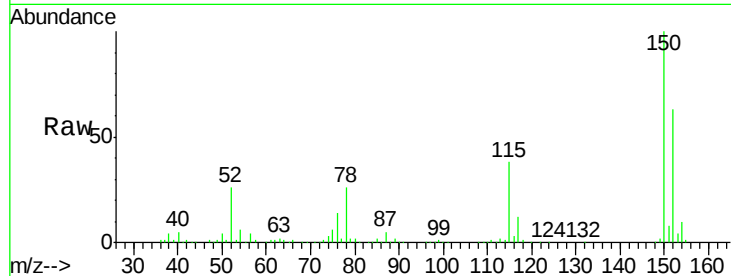


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

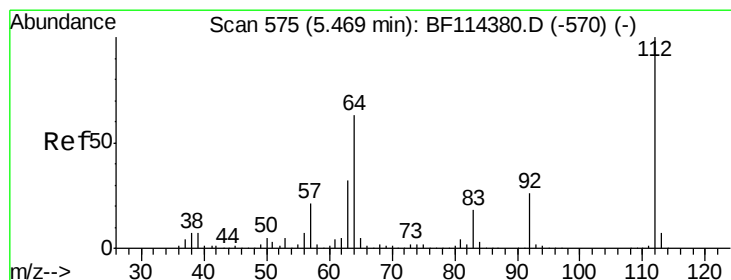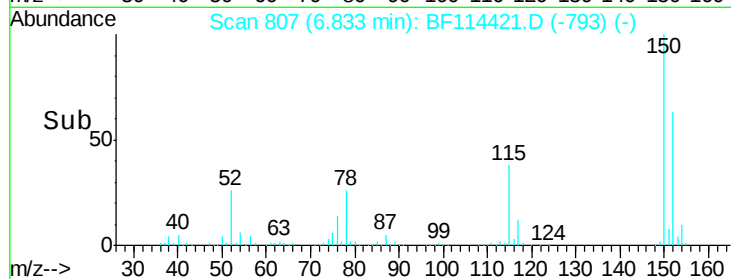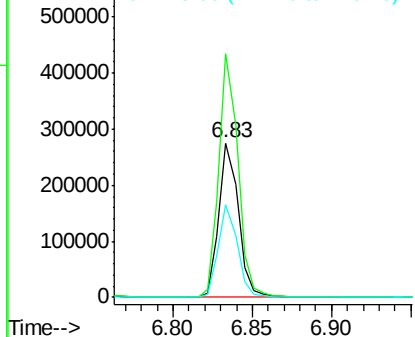



#5

2-Fluorophenol
Concen: 106.195 ng
RT: 5.47 min Scan# 576
Delta R.T. -0.01 min
Lab File: BF114421.D
Acq: 19 May 2019 5:50

Tgt Ion:112 Resp: 1555931
Ion Ratio Lower Upper
112 100
64 68.0 49.0 73.6
63 34.6 24.6 37.0

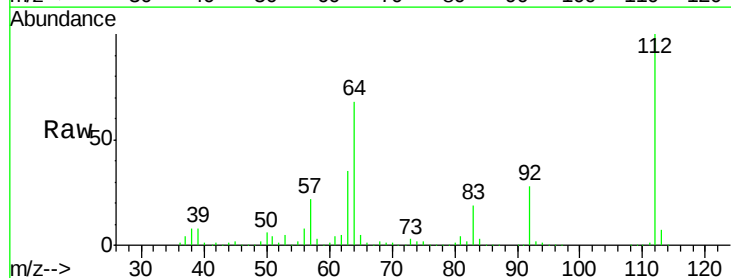

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

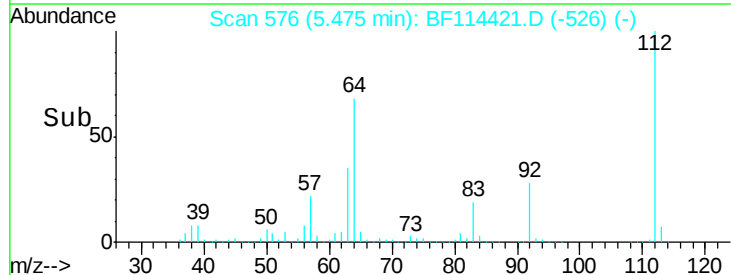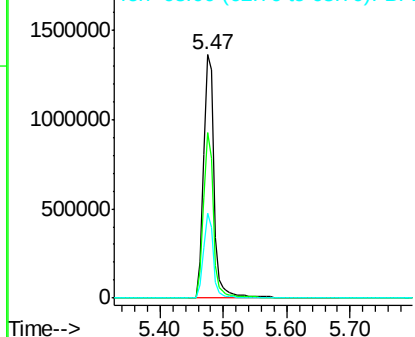



#7

Phenol-d6

Concen: 116.770 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF114421.D

Acq: 19 May 2019 5:50

Instrument :

BNA_F

ClientSampleId :

PB119833TB


Tgt Ion: 99 Resp: 2023515

Ion Ratio Lower Upper

99 100

42 21.4 17.9 26.9




71 33.2 26.2 39.2

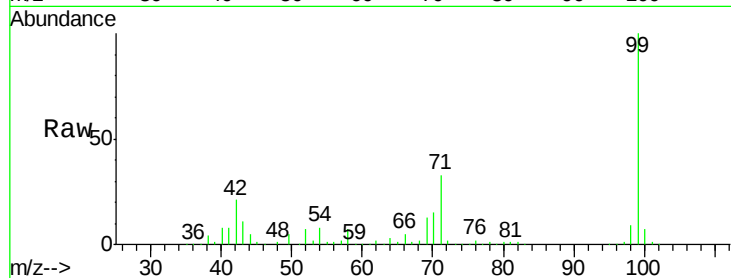

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

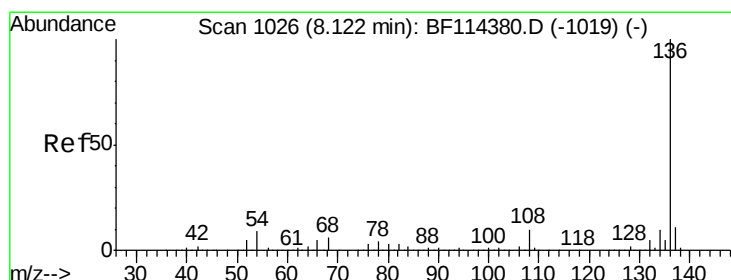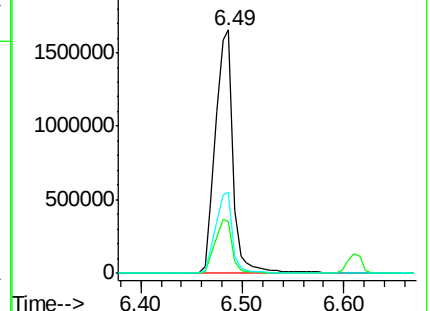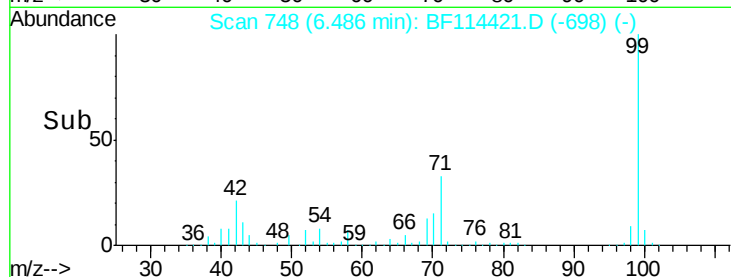

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.02 min

Lab File: BF114421.D

Acq: 19 May 2019 5:50

Tgt Ion: 136 Resp: 873766


Ion Ratio Lower Upper

136 100

137 11.3 8.8 13.2

54 9.2 7.8 11.8

68 6.2 5.1 7.7


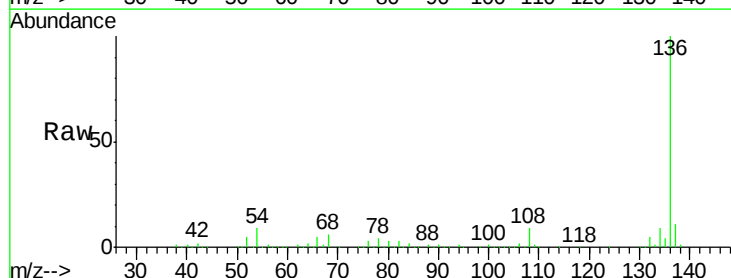


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



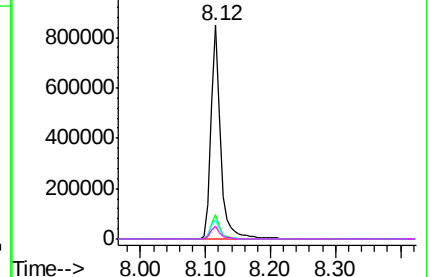
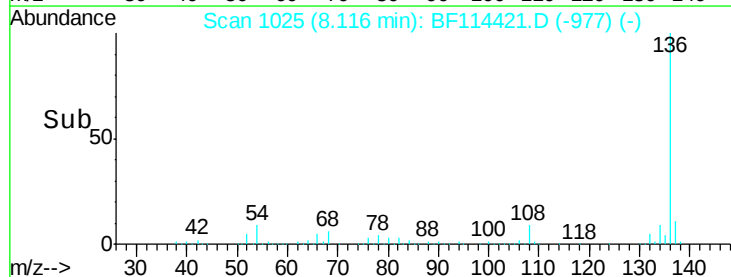




#23
Nitrobenzene-d5
Concen: 81.506 ng
RT: 7.40 min Scan# 903
Delta R.T. -0.02 min
Lab File: BF114421.D
Acq: 19 May 2019 5:50




Instrument :
BNA_F
ClientSampleId :
PB119833TB

Tgt Ion: 82 Resp: 1269014
Ion Ratio Lower Upper
82 100
128 45.1 35.5 53.3
54 59.0 48.5 72.7

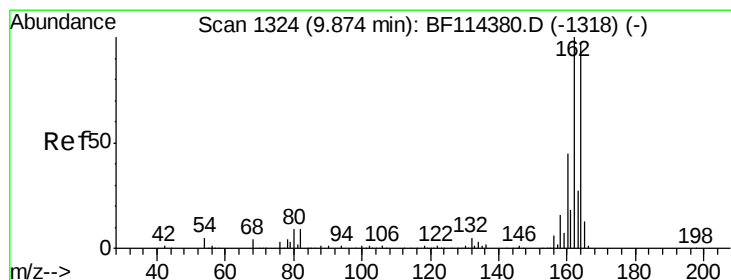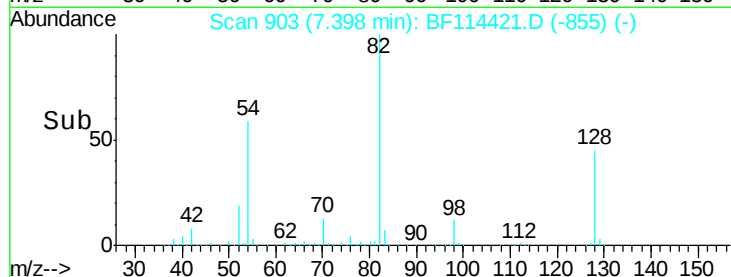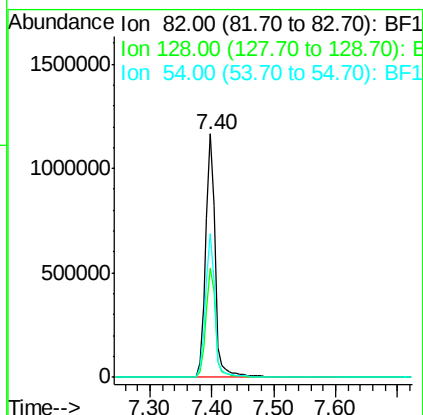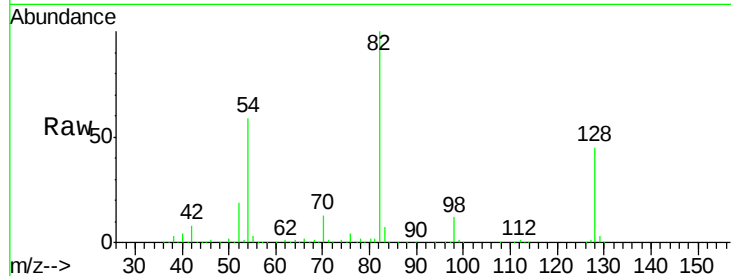

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.87 min Scan# 1323
Delta R.T. -0.02 min
Lab File: BF114421.D
Acq: 19 May 2019 5:50

Tgt Ion: 164 Resp: 394842
Ion Ratio Lower Upper
164 100
162 103.0 80.6 120.8
160 47.2 36.5 54.7

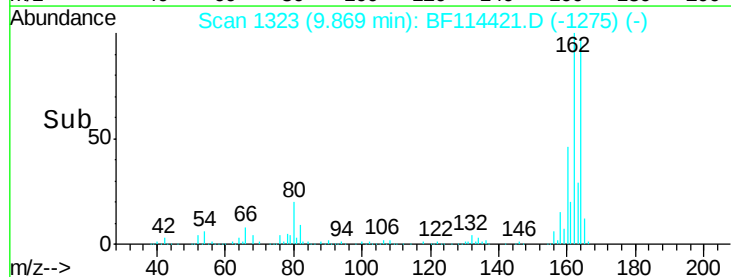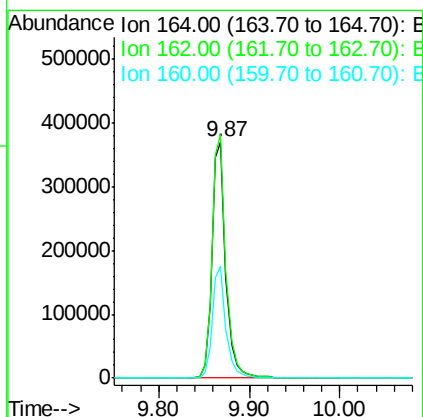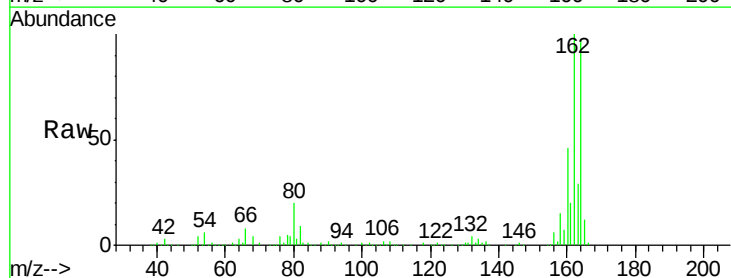



#42

2,4,6-Tribromophenol

Concen: 98.001 ng

RT: 10.66 min Scan# 1457

Delta R.T. -0.02 min

Lab File: BF114421.D

Acq: 19 May 2019 5:50

Instrument :

BNA_F

ClientSampleId :

PB119833TB


Tgt Ion:330 Resp: 400040

Ion Ratio Lower Upper

330 100

332 102.4 81.4 122.2




141 32.9 26.6 40.0

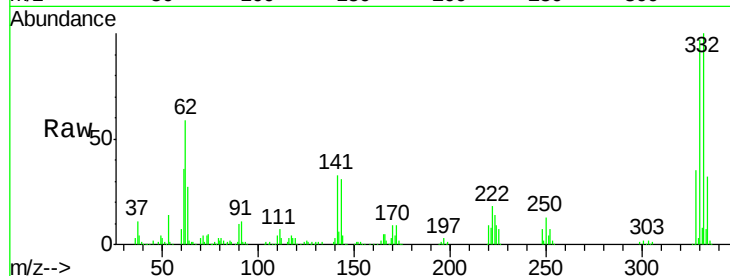

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

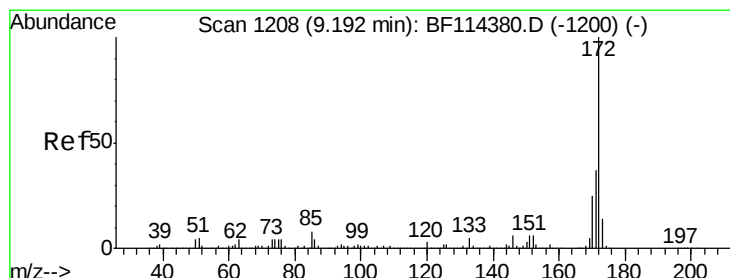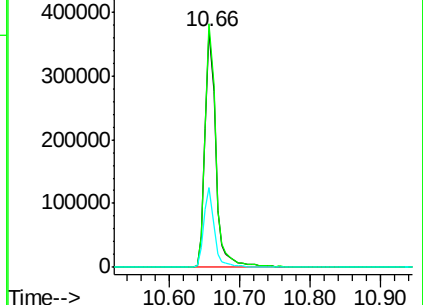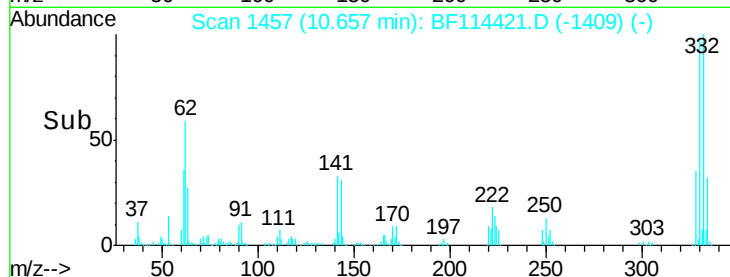

#45

2-Fluorobiphenyl

Concen: 83.813 ng

RT: 9.19 min Scan# 1207

Delta R.T. -0.02 min

Lab File: BF114421.D

Acq: 19 May 2019 5:50


Tgt Ion:172 Resp: 2187715

Ion Ratio Lower Upper

172 100

171 36.9 30.7 46.1



170 24.9 20.5 30.7

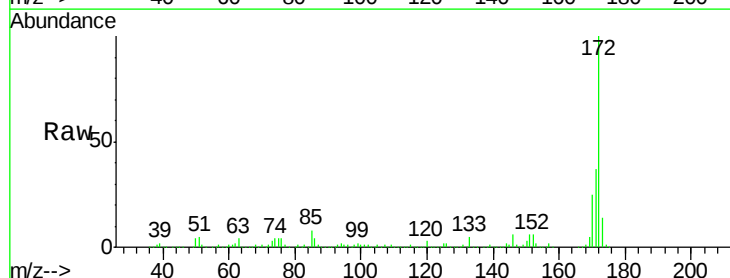


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



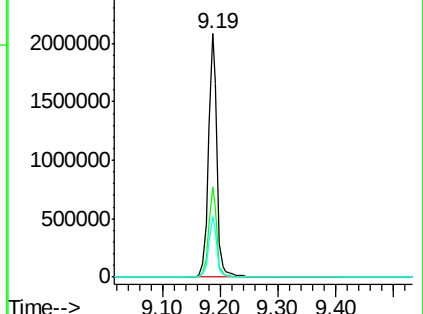
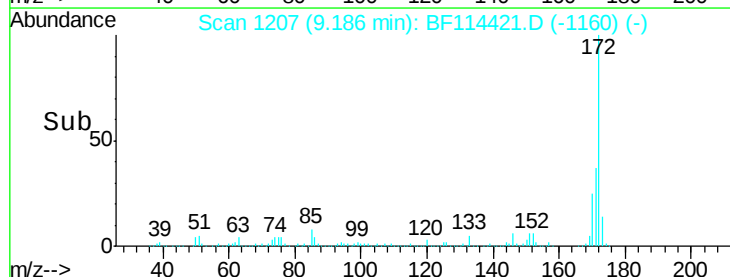


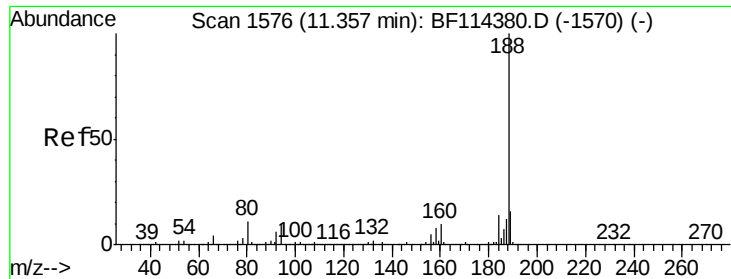

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.35 min Scan# 1575
Delta R.T. -0.02 min
Lab File: BF114421.D
Acq: 19 May 2019 5:50




Instrument :
BNA_F
ClientSampleId :
PB119833TB


Tgt Ion:188 Resp: 717500
Ion Ratio Lower Upper
188 100
94 10.4 8.4 12.6
80 10.6 9.2 13.8

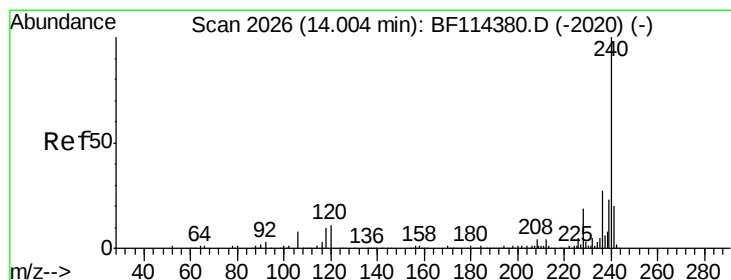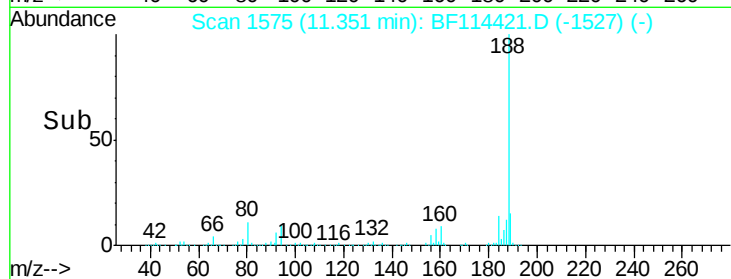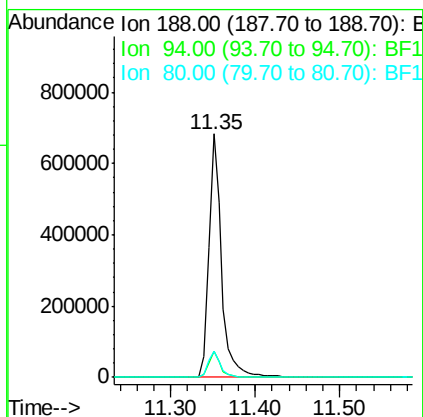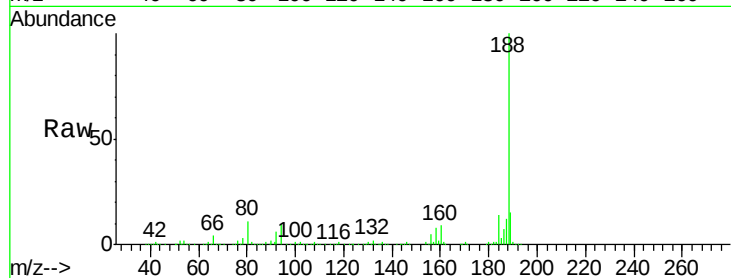

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.99 min Scan# 2024
Delta R.T. -0.03 min
Lab File: BF114421.D
Acq: 19 May 2019 5:50

Tgt Ion:240 Resp: 444717
Ion Ratio Lower Upper
240 100
120 12.8 8.3 12.5#
236 26.5 20.8 31.2

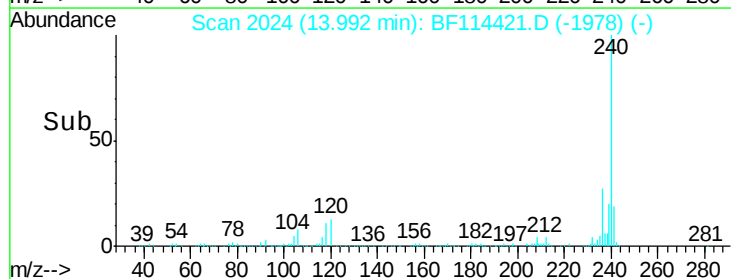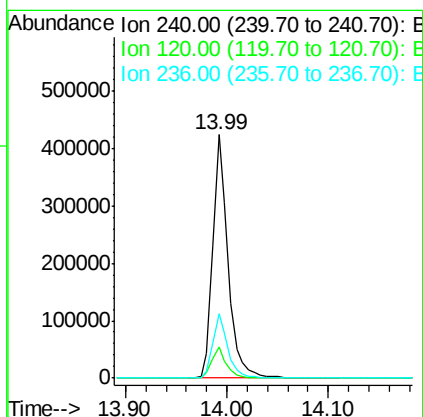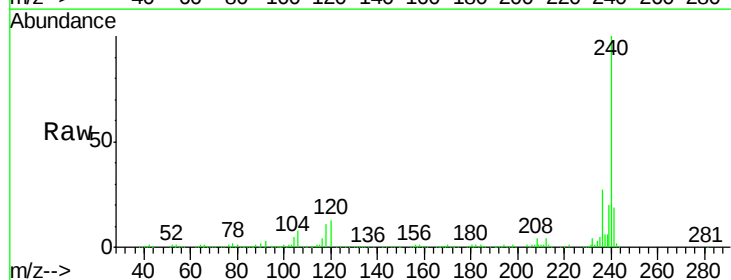

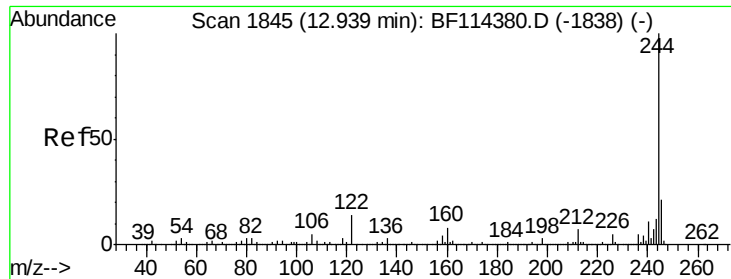

#79

Terphenyl-d14

Concen: 85.443 ng

RT: 12.93 min Scan# 1844

Delta R.T. -0.02 min

Lab File: BF114421.D

Acq: 19 May 2019 5:50

Instrument :

BNA_F

ClientSampleId :

PB119833TB


Tgt Ion:244 Resp: 1843282

Ion Ratio Lower Upper

244 100

212 6.8 5.8 8.6




122 12.7 9.4 14.2

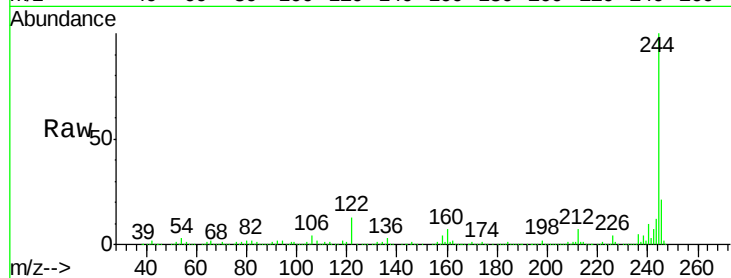

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

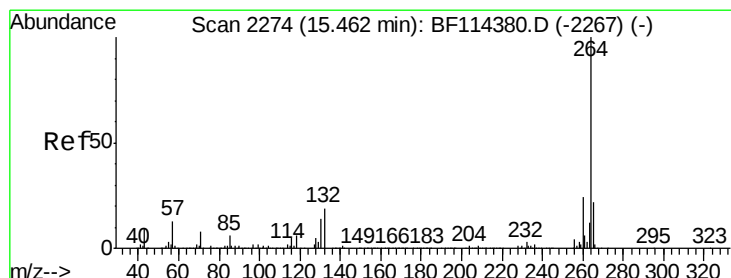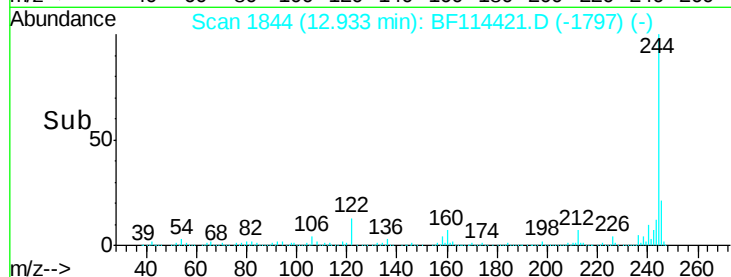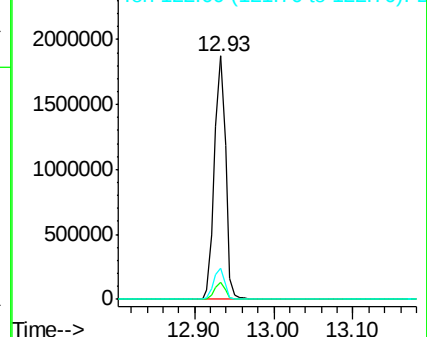

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.46 min Scan# 2273

Delta R.T. -0.05 min

Lab File: BF114421.D

Acq: 19 May 2019 5:50


Tgt Ion:264 Resp: 472573

Ion Ratio Lower Upper

264 100

260 23.1 19.4 29.0

265 20.6 16.9 25.3

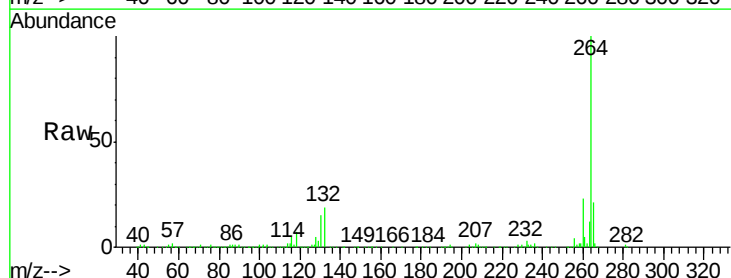

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

