

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
 Data File : BF114398.D
 Acq On : 18 May 2019 18:23
 Operator : JU/SJ
 Sample : K2643-07 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-02-051619-B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	571	574	595	rBV	719357	935466	48.46%	5.002%
2	6.475	743	746	760	rBV	765194	1026356	53.17%	5.488%
3	6.610	766	769	777	rBV	1098268	1002504	51.94%	5.361%
4	6.834	804	807	815	rBV	1551221	1363564	70.64%	7.292%
5	6.992	830	834	844	rBV	772003	776588	40.23%	4.153%
6	7.398	900	903	913	rBV	477594	610997	31.65%	3.267%
7	8.116	1019	1025	1032	rBV	1903160	1778360	92.13%	9.510%
8	8.175	1033	1035	1038	rVB	37869	36016	1.87%	0.193%
9	8.404	1067	1074	1080	rBV7	18467	37376	1.94%	0.200%
10	8.533	1093	1096	1098	rBV	41729	37425	1.94%	0.200%
11	8.657	1113	1117	1120	rBV6	15698	25257	1.31%	0.135%
12	8.704	1122	1125	1129	rVB	38210	36079	1.87%	0.193%
13	9.133	1195	1198	1203	rVB	43003	38583	2.00%	0.206%
14	9.186	1203	1207	1217	rBV	1114763	1074938	55.69%	5.748%
15	9.269	1217	1221	1224	rBV	42740	44893	2.33%	0.240%
16	9.528	1262	1265	1267	rBV3	17255	20986	1.09%	0.112%
17	9.580	1271	1274	1282	rVB	129628	158701	8.22%	0.849%
18	9.728	1297	1299	1302	rBV	28450	29893	1.55%	0.160%
19	9.792	1308	1310	1315	rVB	25394	24762	1.28%	0.132%
20	9.869	1319	1323	1332	rVB	1971995	1930263	100.00%	10.322%
21	10.416	1414	1416	1420	rVB	35212	34848	1.81%	0.186%
22	10.657	1453	1457	1468	rVB	545841	575907	29.84%	3.080%
23	10.769	1473	1476	1477	rBV3	19435	22307	1.16%	0.119%
24	11.251	1553	1558	1563	rVB3	22651	37354	1.94%	0.200%
25	11.351	1571	1575	1578	rBV	2093072	1907284	98.81%	10.199%
26	11.374	1578	1579	1586	rVV	292739	226633	11.74%	1.212%
27	11.433	1586	1589	1593	rVB	53686	53747	2.78%	0.287%
28	11.592	1613	1616	1621	rBV4	13087	22811	1.18%	0.122%
29	11.886	1658	1666	1672	rBV4	60543	141685	7.34%	0.758%
30	11.969	1677	1680	1683	rBV	51099	54475	2.82%	0.291%
31	12.045	1690	1693	1695	rBV3	22363	21214	1.10%	0.113%
32	12.404	1751	1754	1756	rBV	22903	21401	1.11%	0.114%
33	12.427	1756	1758	1763	rVB4	18199	22977	1.19%	0.123%
34	12.569	1778	1782	1785	rBV	235207	228077	11.82%	1.220%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
Data File : BF114398.D
Acq On : 18 May 2019 18:23
Operator : JU/SJ
Sample : K2643-07 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-051619-B

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.663	1796	1798	1805	rBV3	22788	31292	1.62%	0.167%
36	12.798	1815	1821	1827	rBV	213031	269756	13.98%	1.443%
37	12.927	1839	1843	1853	rVB	951576	866470	44.89%	4.633%
38	13.127	1874	1877	1879	rVB	27882	25297	1.31%	0.135%
39	13.192	1885	1888	1890	rBV	31069	28824	1.49%	0.154%
40	13.227	1892	1894	1899	rVB4	23553	32279	1.67%	0.173%
41	13.992	2019	2024	2027	rBV	1429494	1433969	74.29%	7.668%
42	14.745	2150	2152	2155	rBV	68005	58036	3.01%	0.310%
43	15.457	2268	2273	2287	rBV	1190830	1594791	82.62%	8.528%


Sum of corrected areas: 18700441

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
Data File : BF114398.D
Acq On : 18 May 2019 18:23
Operator : JU/SJ
Sample : K2643-07 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
OR-02-051619-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

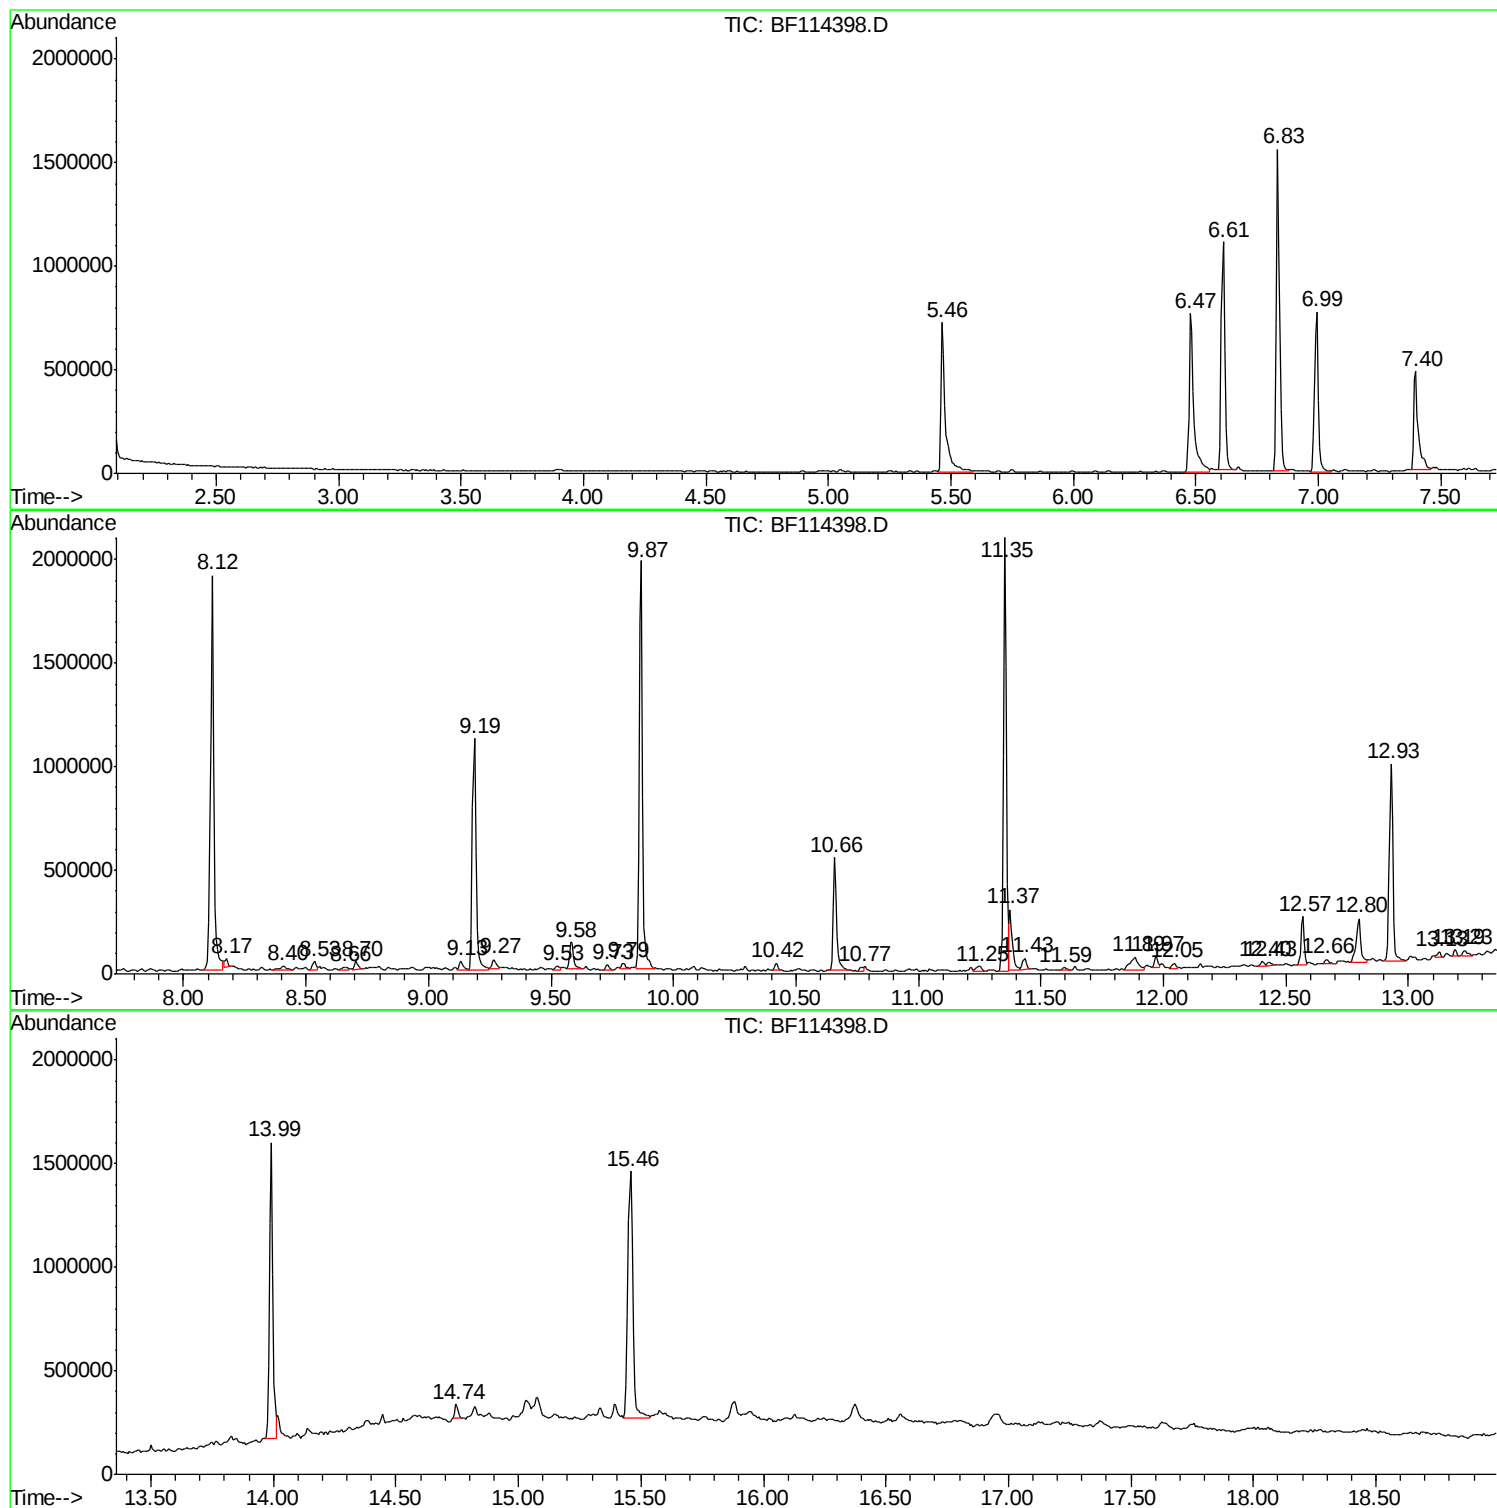

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
Data File : BF114398.D
Acq On : 18 May 2019 18:23
Operator : JU/SJ
Sample : K2643-07 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-051619-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.61 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.61	14.70 ng	1002500	1,4-Dichlorobenzene-d4	6.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	10

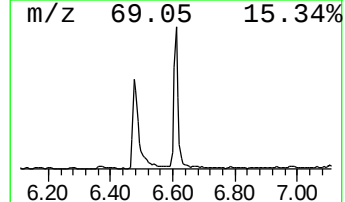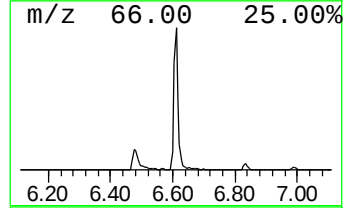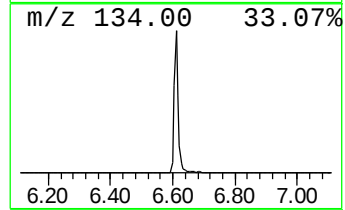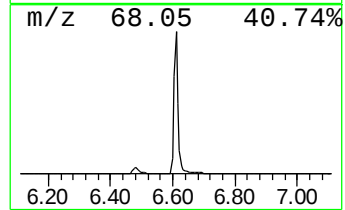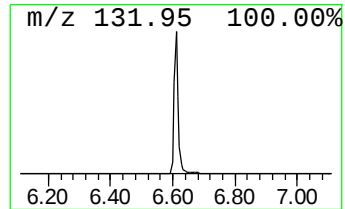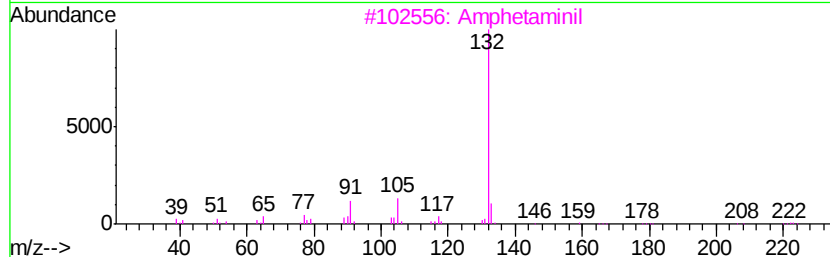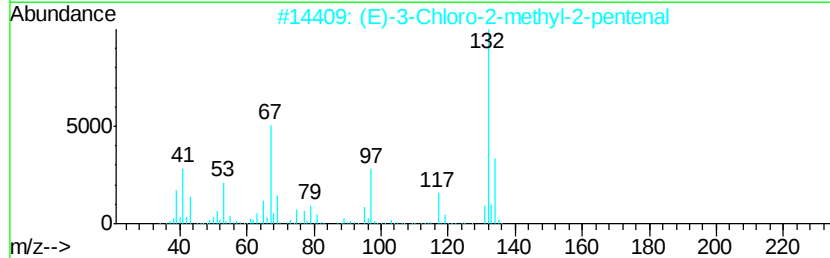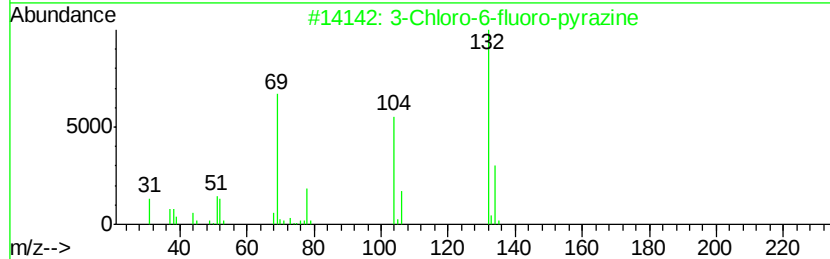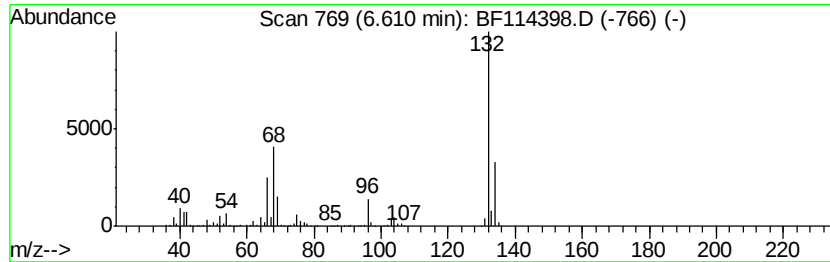

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
Data File : BF114398.D
Acq On : 18 May 2019 18:23
Operator : JU/SJ
Sample : K2643-07 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-051619-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.61	6.61	14.7	ng	1002500	1	6.83	1363560	20.0