

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
 Data File : BF114422.D
 Acq On : 19 May 2019 6:16
 Operator : JU/SJ
 Sample : PB119833BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB119833BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.187	13	17	28	rVB	59215	92918	1.41%	0.182%
2	5.475	572	576	597	rBV	5185292	5826276	88.55%	11.423%
3	6.481	742	747	765	rBV	4948796	6079894	92.40%	11.920%
4	6.610	765	769	773	rBV	5554090	5759690	87.53%	11.293%
5	6.834	804	807	815	rBV	1685038	1427469	21.69%	2.799%
6	6.992	830	834	848	rVB	5088854	4701338	71.45%	9.218%
7	7.398	898	903	922	rBV	3637761	3948382	60.01%	7.741%
8	8.116	1021	1025	1048	rBV	1751356	1789545	27.20%	3.509%
9	9.186	1201	1207	1223	rBV	6509963	6579875	100.00%	12.901%
10	9.869	1317	1323	1337	rBV	1708751	1880684	28.58%	3.687%
11	10.657	1453	1457	1479	rBV	3148632	3288813	49.98%	6.448%
12	11.351	1571	1575	1591	rBV	1734583	1797336	27.32%	3.524%
13	12.933	1839	1844	1847	rBV	5329139	5165555	78.51%	10.128%
14	13.992	2020	2024	2038	rBV	1227714	1360594	20.68%	2.668%
15	15.457	2268	2273	2287	rBV	860053	1305437	19.84%	2.559%


Sum of corrected areas: 51003806

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
Data File : BF114422.D
Acq On : 19 May 2019 6:16
Operator : JU/SJ
Sample : PB119833BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119833BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

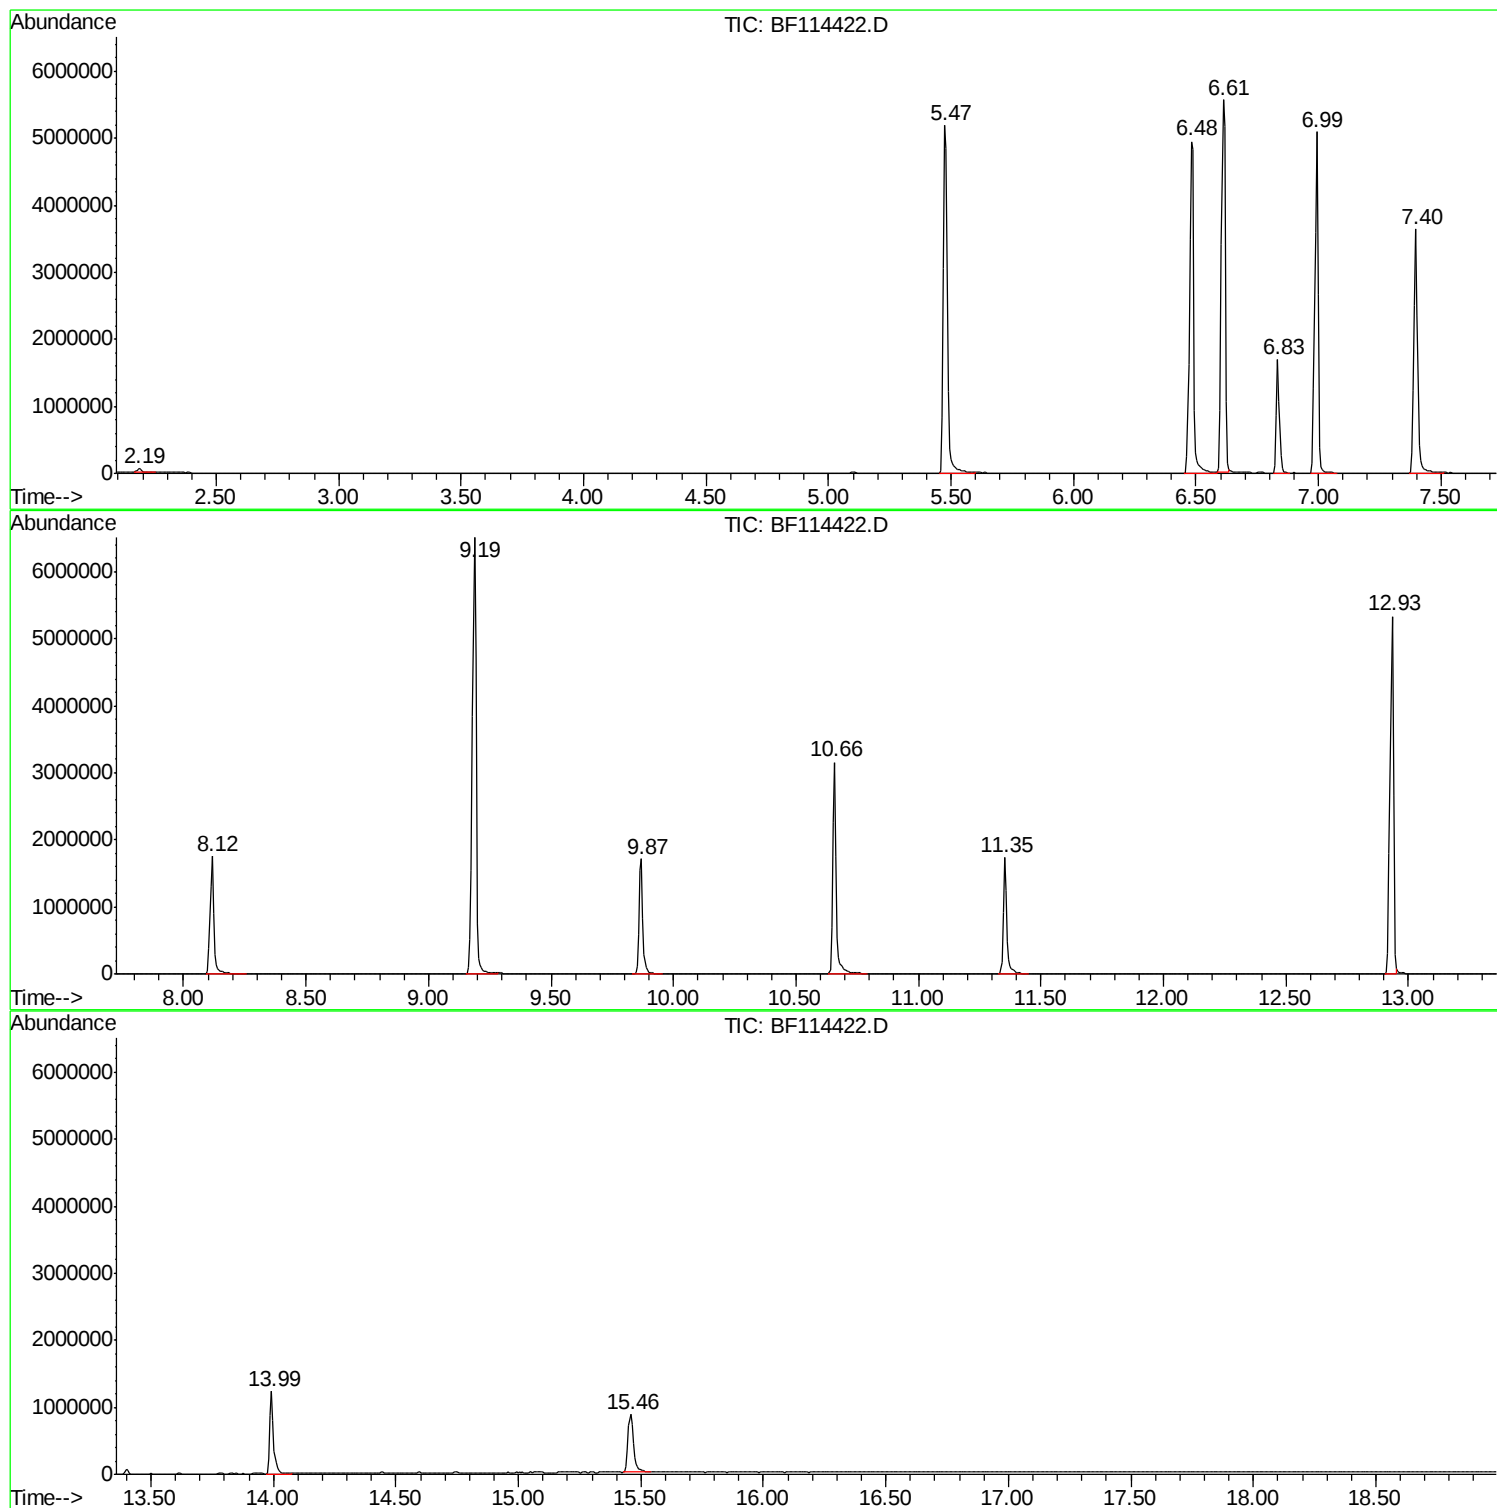

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
Data File : BF114422.D
Acq On : 19 May 2019 6:16
Operator : JU/SJ
Sample : PB119833BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119833BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.61 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.61	80.70 ng	5759690	1,4-Dichlorobenzene-d4	6.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

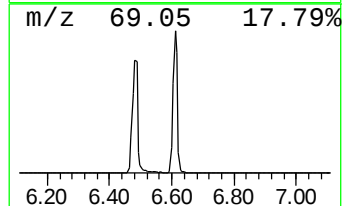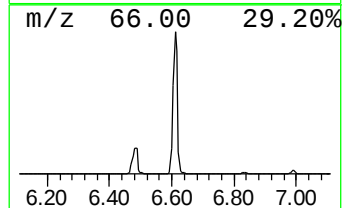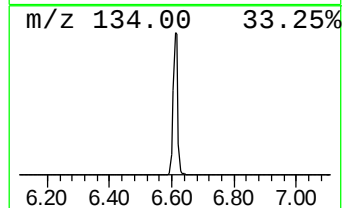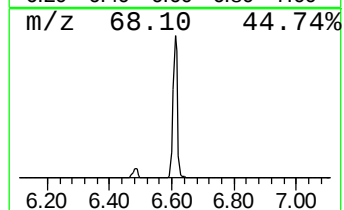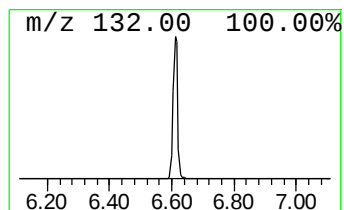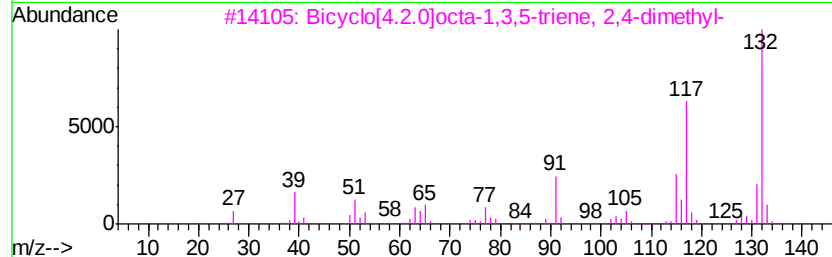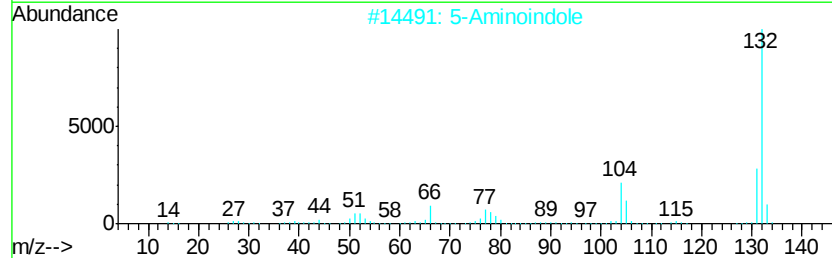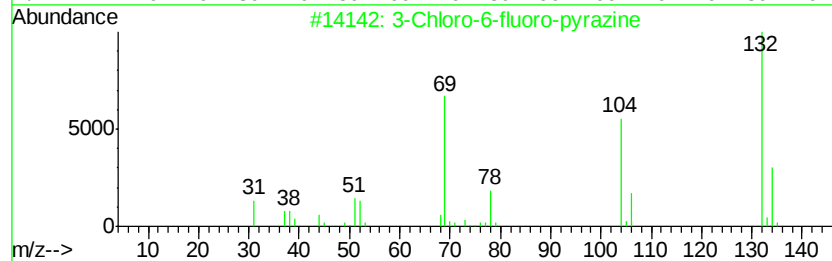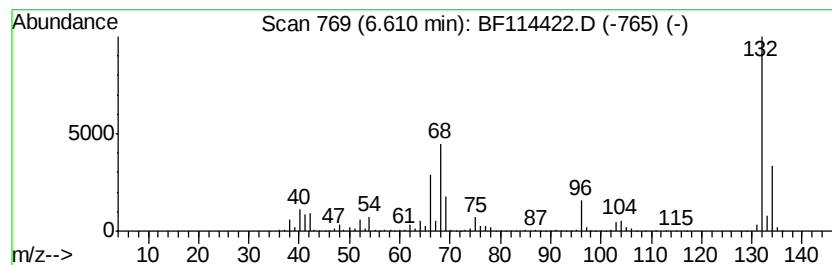

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
Data File : BF114422.D
Acq On : 19 May 2019 6:16
Operator : JU/SJ
Sample : PB119833BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119833BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.61	6.61	80.7	ng	5759690	1	6.83	1427470	20.0