


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051819\
 Data File : BF114379.D
 Acq On : 18 May 2019 9:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 20 04:47:40 2019

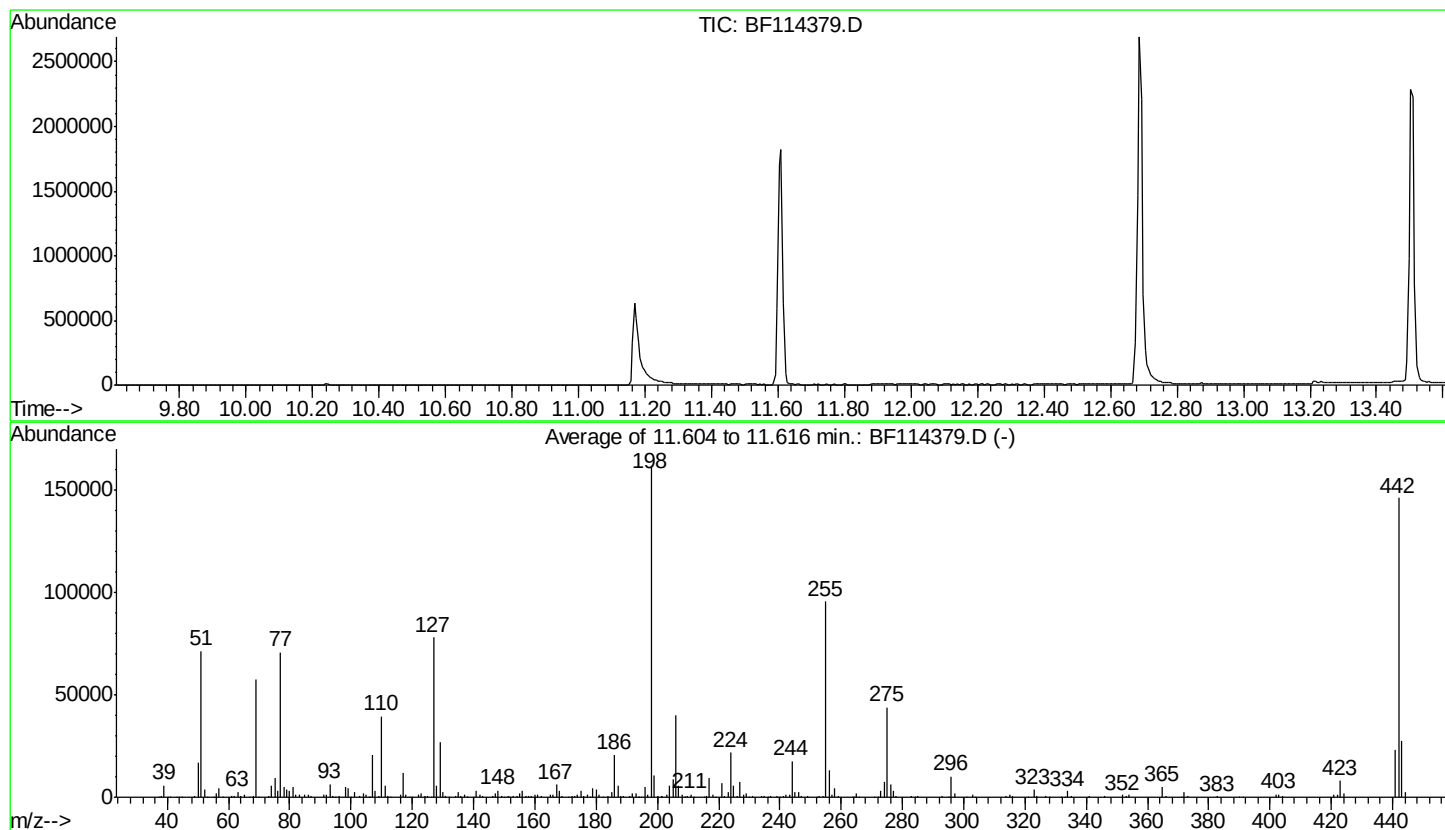

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	71429	PASS
68	69	0.00	2	1.5	862	PASS
69	198	0.00	100	35.4	57248	PASS
70	69	0.00	2	0.3	162	PASS
127	198	10	80	48.1	77834	PASS
197	198	0.00	2	0.7	1137	PASS
198	198	100	100	100.0	161666	PASS
199	198	5	9	6.6	10716	PASS
275	198	10	60	27.2	43922	PASS
365	198	1	100	3.2	5217	PASS
441	198	0.01	100	14.3	23104	PASS
442	198	50	100	90.2	145864	PASS
443	442	15	24	19.0	27648	PASS