

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051820\
 Data File : BF120340.D
 Acq On : 18 May 2020 14:35
 Operator : MA/SJ
 Sample : PB128931BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128931BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.210	527	531	561	rBV	6847646	8009915	87.26%	12.178%
2	6.257	704	709	744	rBV	6021898	8027272	87.44%	12.204%
3	6.598	763	767	789	rBV	1379316	1775068	19.34%	2.699%
4	6.757	789	794	818	rBV	5900638	6570966	71.58%	9.990%
5	7.175	859	865	882	rBV	4012198	5319601	57.95%	8.088%
6	7.886	981	986	1007	rBV	2031909	2392138	26.06%	3.637%
7	8.969	1164	1170	1184	rBV	8262590	9179850	100.00%	13.957%
8	9.639	1278	1284	1300	rBV	2453413	2567957	27.97%	3.904%
9	10.427	1413	1418	1435	rBV	4361583	5365192	58.45%	8.157%
10	11.116	1531	1535	1556	rBV	2395956	2683574	29.23%	4.080%
11	12.716	1799	1807	1821	rBV	7285954	8942012	97.41%	13.595%
12	13.751	1979	1983	1996	rBV	2473917	2604399	28.37%	3.960%
13	15.139	2214	2219	2232	rBV	1774441	2220490	24.19%	3.376%
14	15.756	2319	2324	2333	rVB5	38138	115960	1.26%	0.176%


Sum of corrected areas: 65774394

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF051820\
Data File : BF120340.D
Acq On : 18 May 2020 14:35
Operator : MA/SJ
Sample : PB128931BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128931BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

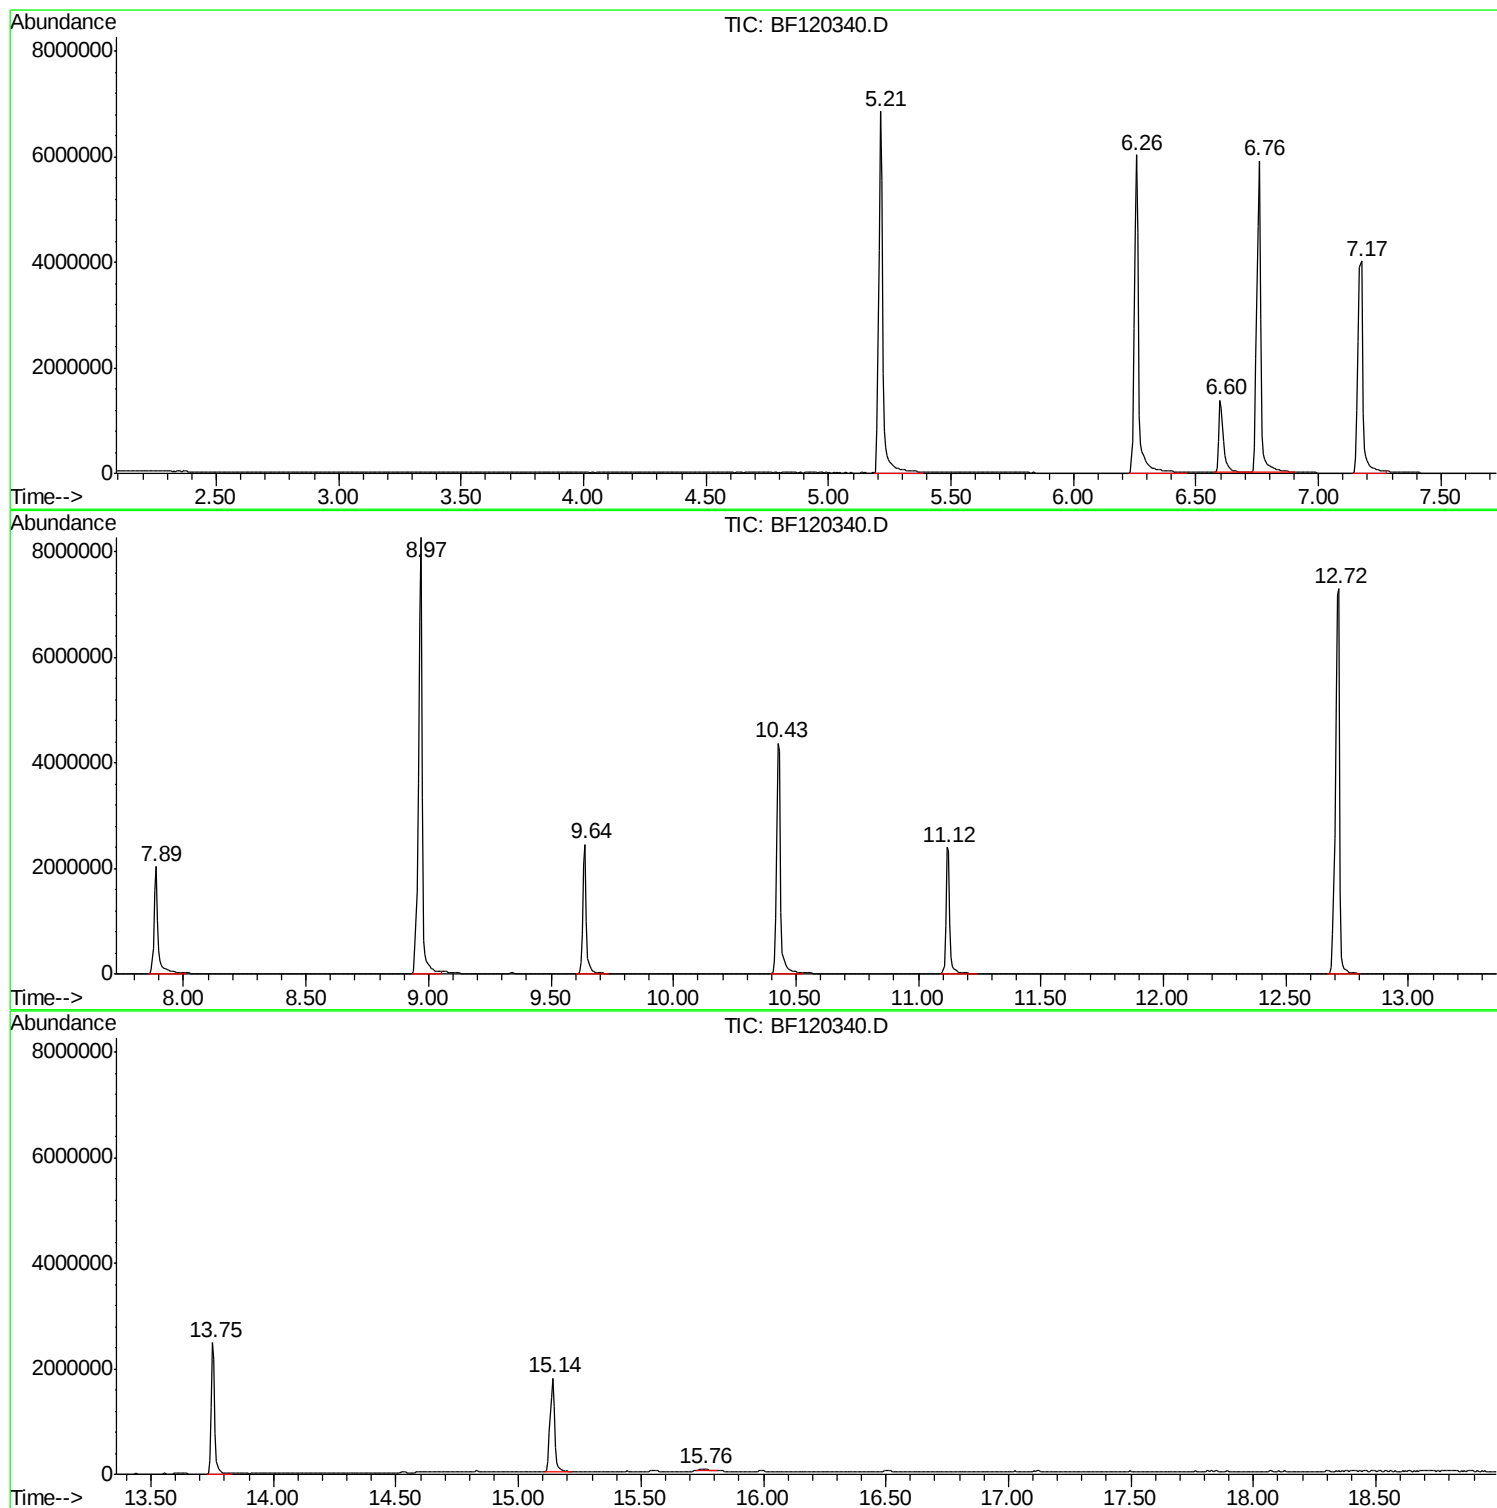

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051820\
Data_File : BF120340.D
Acq_On : 18_May, 2020 14:355
Operator : MA/SJJ
Sample : PB128931BLL
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB128931BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
