

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051820\
Data File : BF120342.D
Acq On : 18 May 2020 15:29
Operator : MA/SJ
Sample : PB128942BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128942BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.222	529	533	560	rBV	5793028	6493869	57.03%	9.378%
2	6.257	704	709	738	rBV	4989677	6348790	55.75%	9.168%
3	6.598	763	767	789	rBV	1717530	2011044	17.66%	2.904%
4	6.757	789	794	821	rVV	6491417	7525278	66.09%	10.867%
5	7.169	859	864	889	rBV	4632853	6330179	55.59%	9.141%
6	7.881	981	985	1010	rBV	2005226	2702475	23.73%	3.903%
7	8.969	1163	1170	1184	rBV	8373419	11387022	100.00%	16.444%
8	9.633	1277	1283	1305	rBV	2887776	3312067	29.09%	4.783%
9	10.428	1412	1418	1432	rBV	4106535	4479214	39.34%	6.468%
10	11.122	1530	1536	1544	rBV	2907416	2981176	26.18%	4.305%
11	12.716	1797	1807	1810	rBV	8440195	10104326	88.74%	14.592%
12	13.751	1979	1983	1992	rBV	2714529	2834029	24.89%	4.093%
13	15.139	2213	2219	2228	rBV	2135905	2737996	24.04%	3.954%


Sum of corrected areas: 69247465

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF051820\
Data File : BF120342.D
Acq On : 18 May 2020 15:29
Operator : MA/SJ
Sample : PB128942BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128942BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

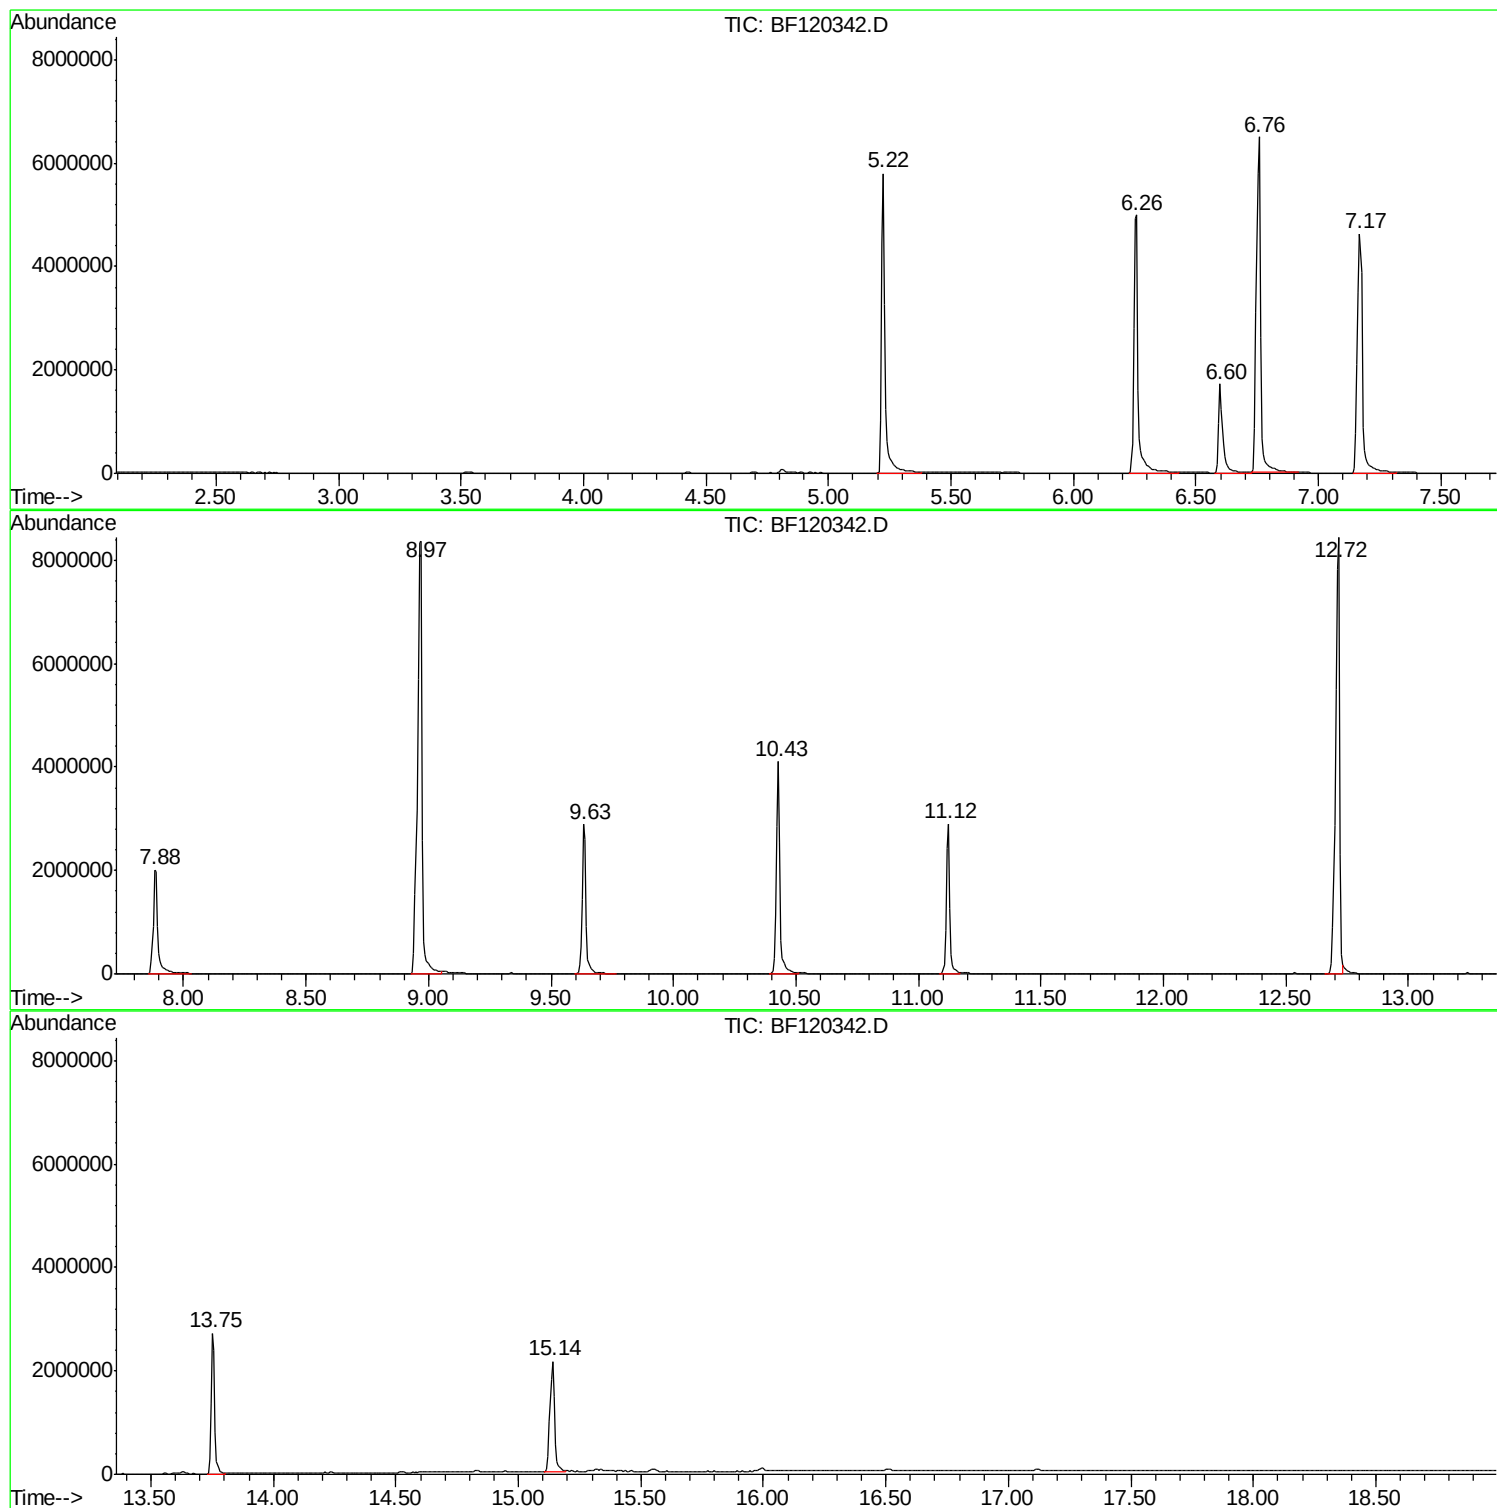

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051820\
Data_File : BF120342.D
Acq_On : 18_May, 2020 15:299
Operator : MA/SJJ
Sample : PB128942BLL
Misc :
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB128942BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
