

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051820\
 Data File : BF120345.D
 Acq On : 18 May 2020 16:50
 Operator : MA/SJ
 Sample : PB128946BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128946BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.210	527	531	560	rBV	6649344	7526012	91.87%	12.216%
2	6.257	704	709	742	rBV	5765809	7329589	89.47%	11.897%
3	6.598	763	767	789	rBV	1479663	1892983	23.11%	3.073%
4	6.757	789	794	830	rVB	5306537	6125078	74.77%	9.942%
5	7.169	859	864	890	rBV	3784381	4950600	60.43%	8.035%
6	7.886	981	986	1012	rBV	2327316	2861094	34.92%	4.644%
7	8.969	1164	1170	1185	rBV	7001849	8008362	97.76%	12.999%
8	9.639	1278	1284	1302	rBV	2416971	2591723	31.64%	4.207%
9	10.427	1413	1418	1442	rBV	4131871	4685558	57.20%	7.605%
10	11.122	1531	1536	1554	rBV	2514273	2630548	32.11%	4.270%
11	12.710	1800	1806	1820	rBV	7146453	8192159	100.00%	13.297%
12	13.757	1979	1984	1994	rBV	2282097	2515075	30.70%	4.082%
13	15.139	2214	2219	2229	rBV	1735098	2300966	28.09%	3.735%


Sum of corrected areas: 61609747

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF051820\
Data File : BF120345.D
Acq On : 18 May 2020 16:50
Operator : MA/SJ
Sample : PB128946BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128946BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

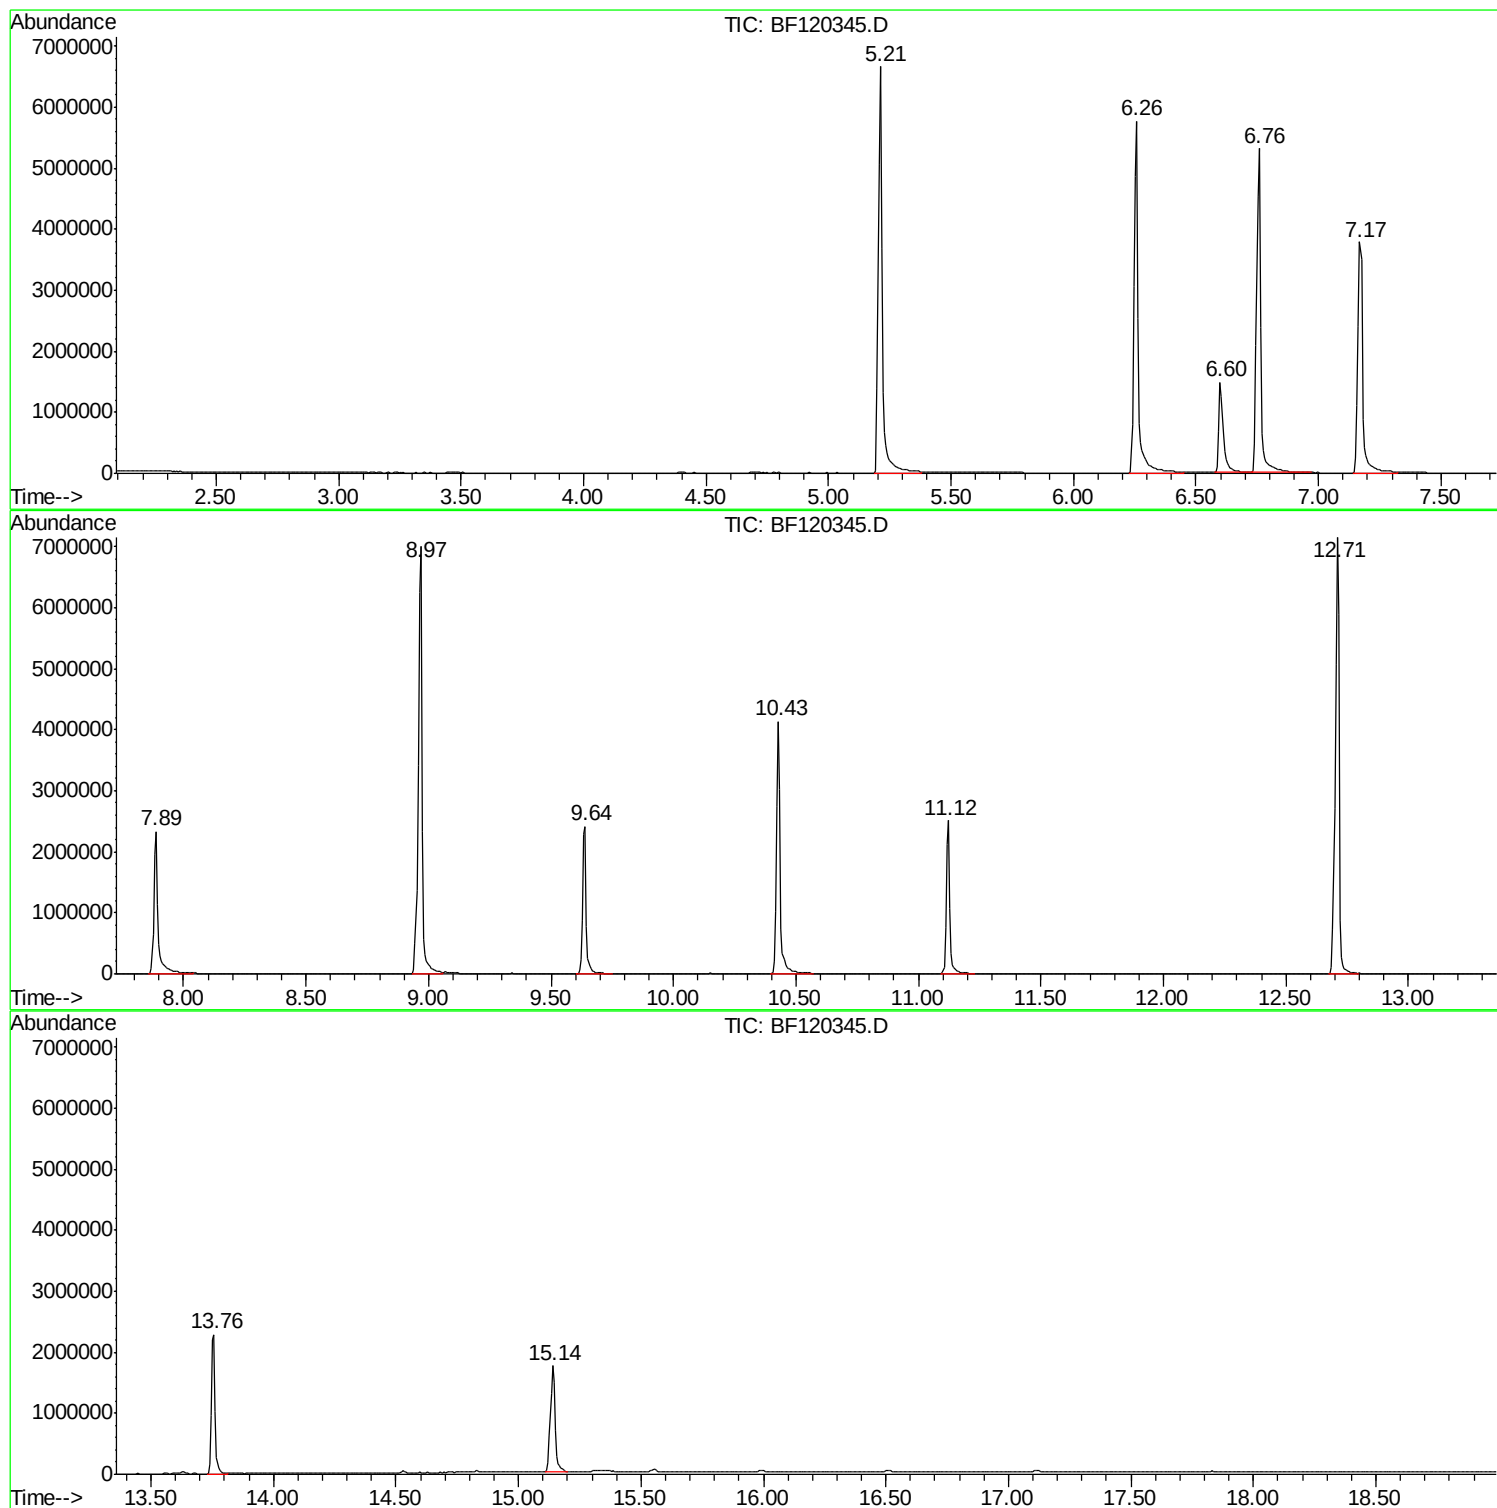

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051820\
Data_File : BF120345.D
Acq_On : 18_May, 2020 16:500
Operator : MA/SJJ
Sample : PB128946BLL
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB128946BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
