


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051820\
 Data File : BF120338.D
 Acq On : 18 May 2020 13:14
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 18 15:23:07 2020

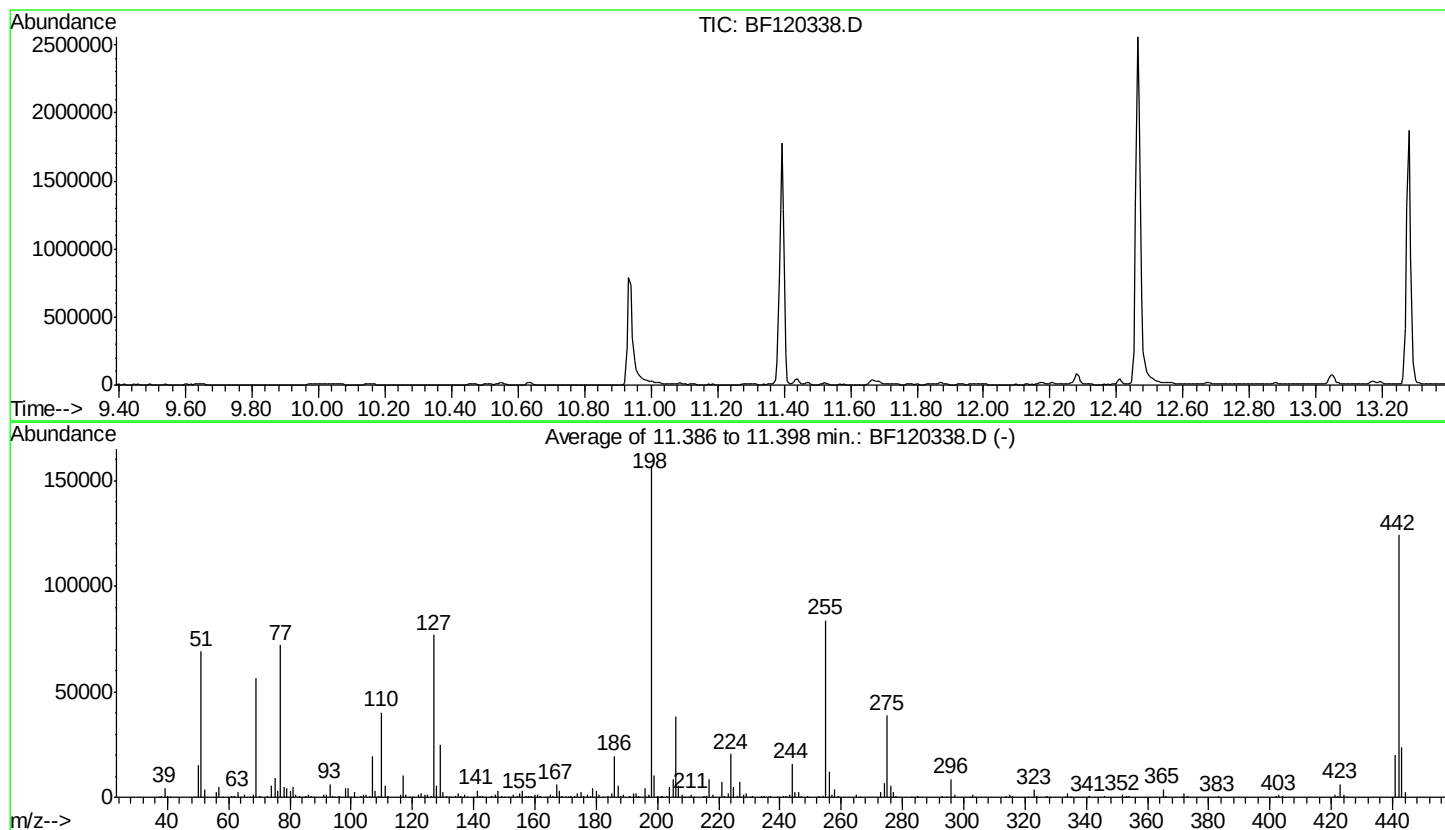

AutoFind: Scans 1581, 1582, 1583; Background Corrected with Scan 1575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	69066	PASS
68	69	0.00	2	1.9	1047	PASS
69	198	0.00	100	35.8	56321	PASS
70	69	0.00	2	0.6	366	PASS
127	198	10	80	49.0	77026	PASS
197	198	0.00	2	0.7	1115	PASS
198	198	100	100	100.0	157218	PASS
199	198	5	9	6.7	10564	PASS
275	198	10	60	24.6	38744	PASS
365	198	1	100	2.5	3957	PASS
441	198	0.01	100	12.9	20233	PASS
442	198	50	100	79.1	124400	PASS
443	442	15	24	19.1	23785	PASS