
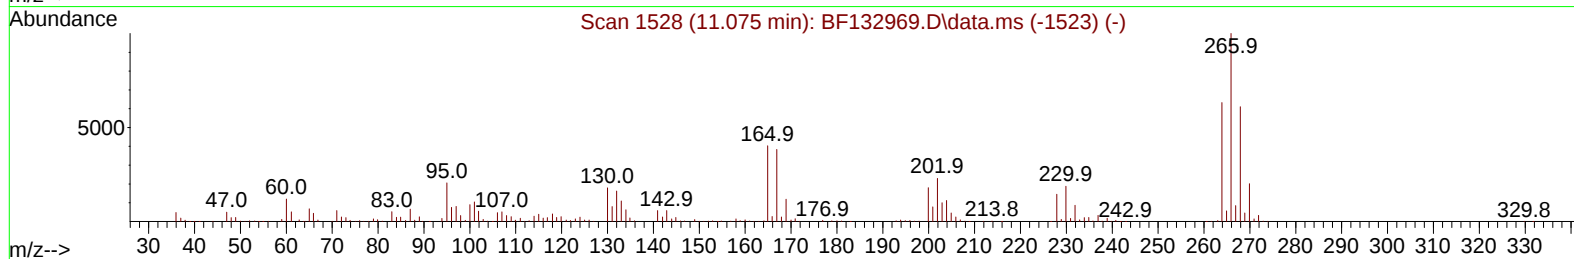
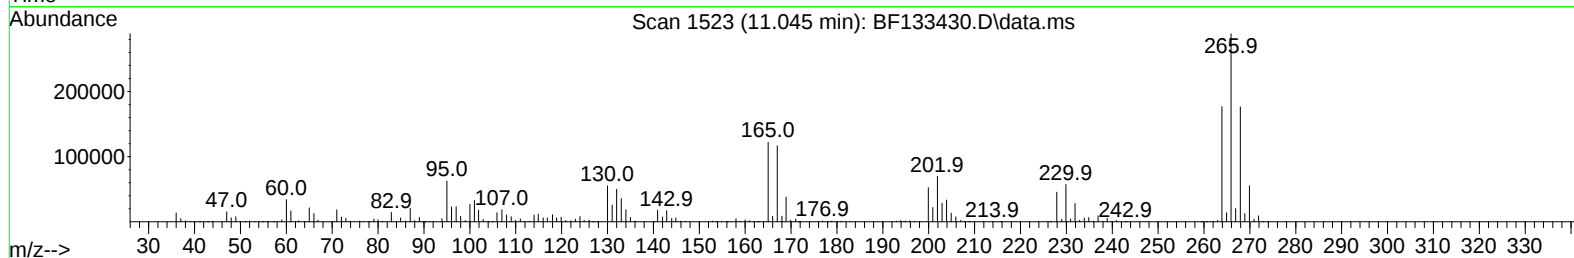


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051823\
Data File : BF133430.D
Acq On : 18 May 2023 09:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 14:31:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 16 14:39:29 2023
Response via : Initial Calibration

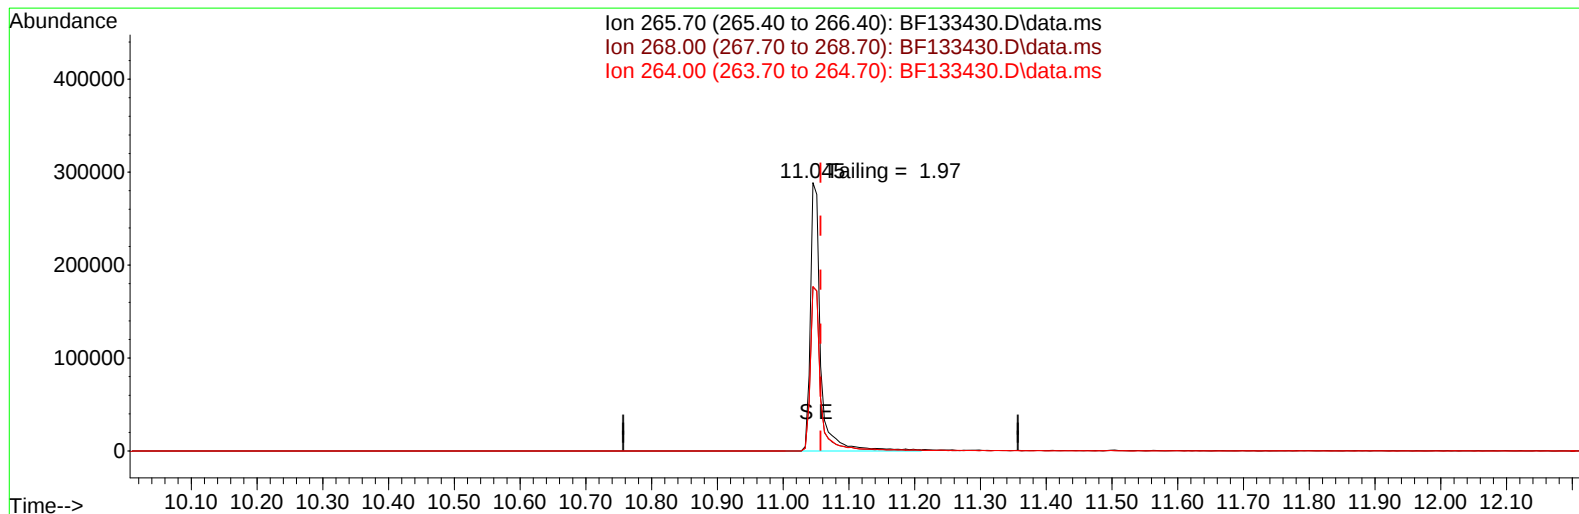

TIC: BF133430.D\data.ms




(70) Pentachlorophenol (C)

11.045min (-0.012) 24910.20 ng

response 315851

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	61.10
264.00	63.30	61.29
0.00	0.00	0.00

Quant Time: May 18 14:31:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 16 14:39:29 2023
Response via : Initial Calibration

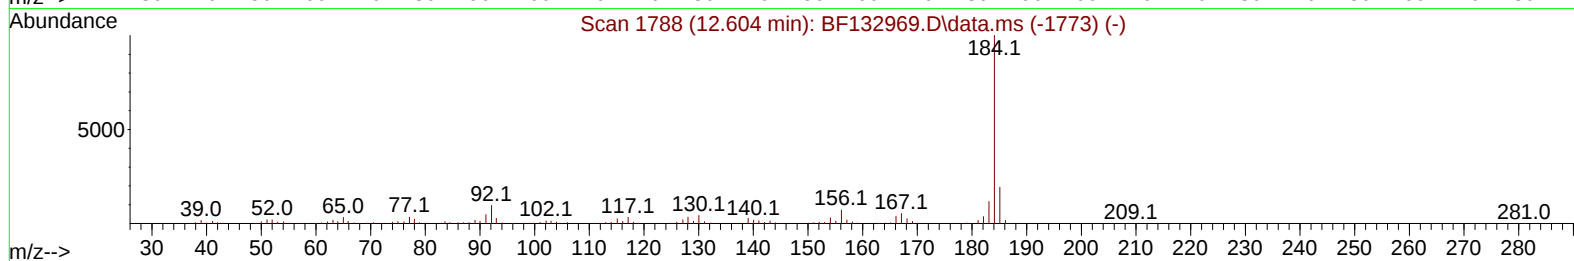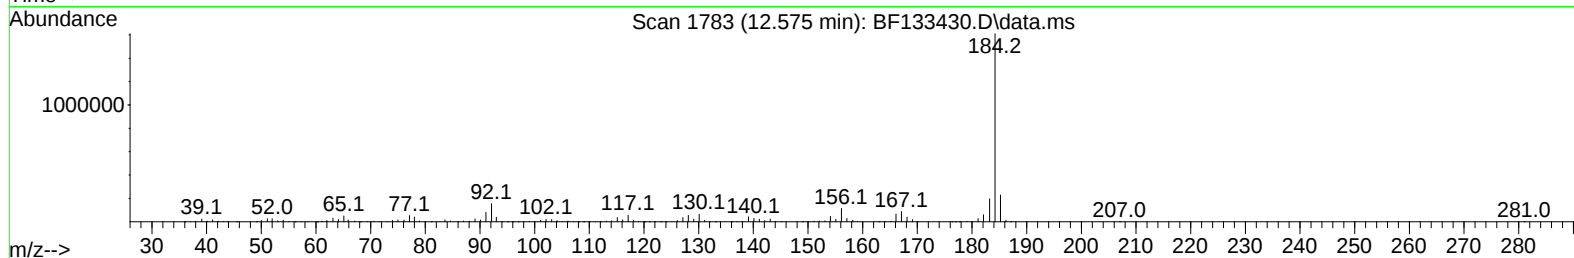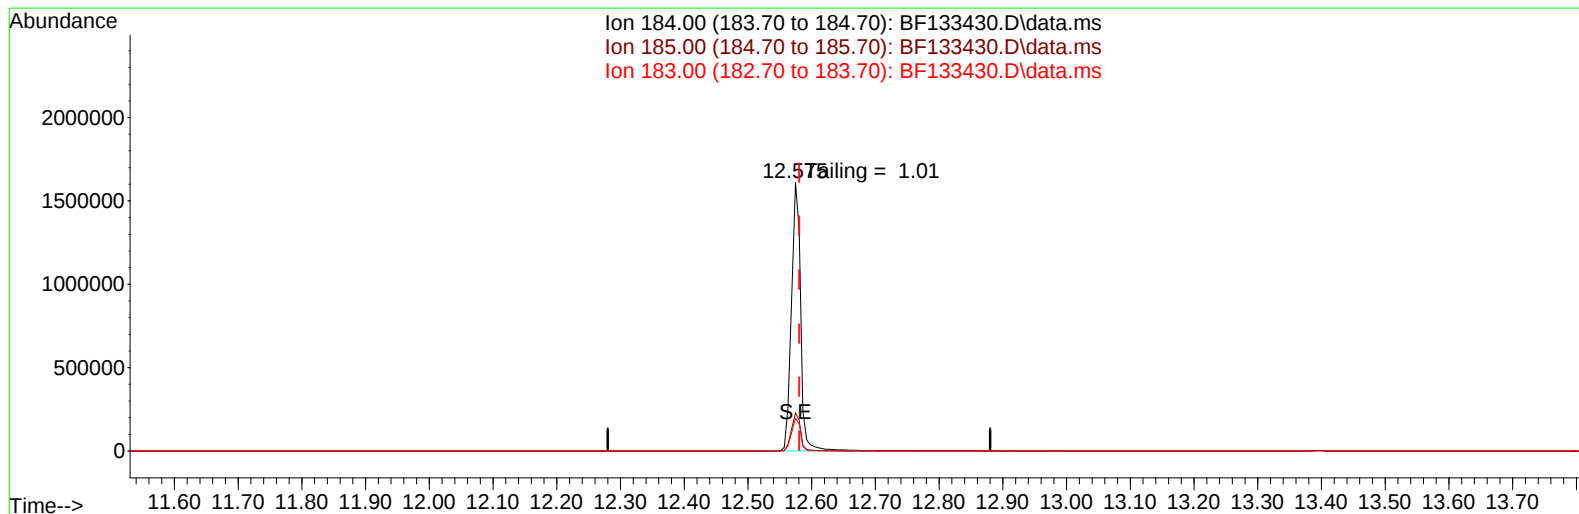

TIC: BF133430.D\data.ms

(77) Benzidine

12.575min (-0.006) 1277988.25 ng

response **1620859**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.27#
183.00	11.70	12.22
0.00	0.00	0.00