
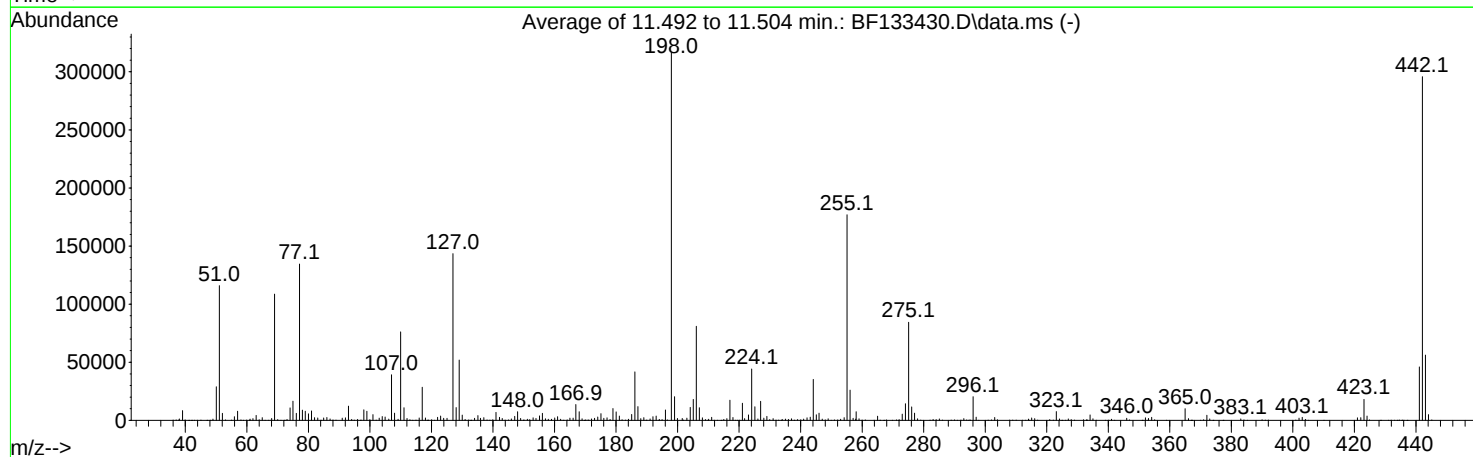


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051823\
Data File : BF133430.D
Acq On : 18 May 2023 09:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 18 18:12:00 2023

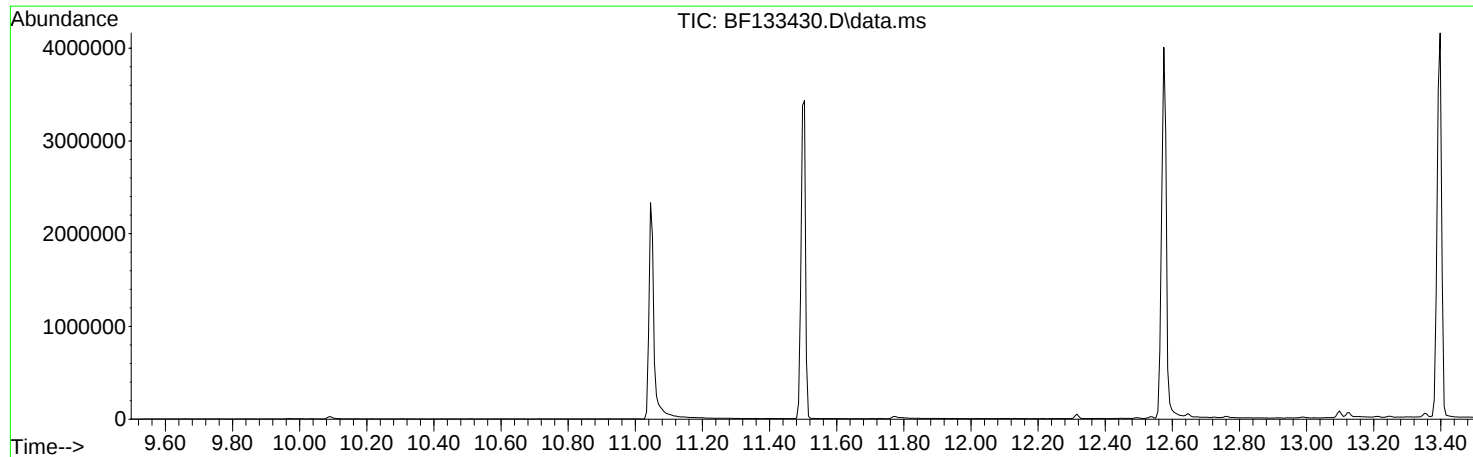

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	115928	PASS
68	69	0.00	2	1.5	1641	PASS
69	198	0.00	100	34.3	108680	PASS
70	69	0.00	2	0.6	640	PASS
127	198	10	80	45.3	143549	PASS
197	198	0.00	2	0.1	459	PASS
198	198	100	100	100.0	316587	PASS
199	198	5	9	6.5	20452	PASS
275	198	10	60	26.7	84427	PASS
365	198	1	100	3.2	10083	PASS
441	198	0.01	100	14.5	46057	PASS
442	442	50	100	100.0	295789	PASS
443	442	15	24	19.0	56133	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
5/18/2023	BNA_F	<u>BF133430.D</u>
Compound Name	Response	Retention Time
DDT	775986	13.398
DDD	22671	13.098
DDE	2545	12.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25216	801202	3.15

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051823\
 Data File : BF133430.D
 Acq On : 18 May 2023 09:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 18 14:31:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 16 14:39:29 2023
 Response via : Initial Calibration

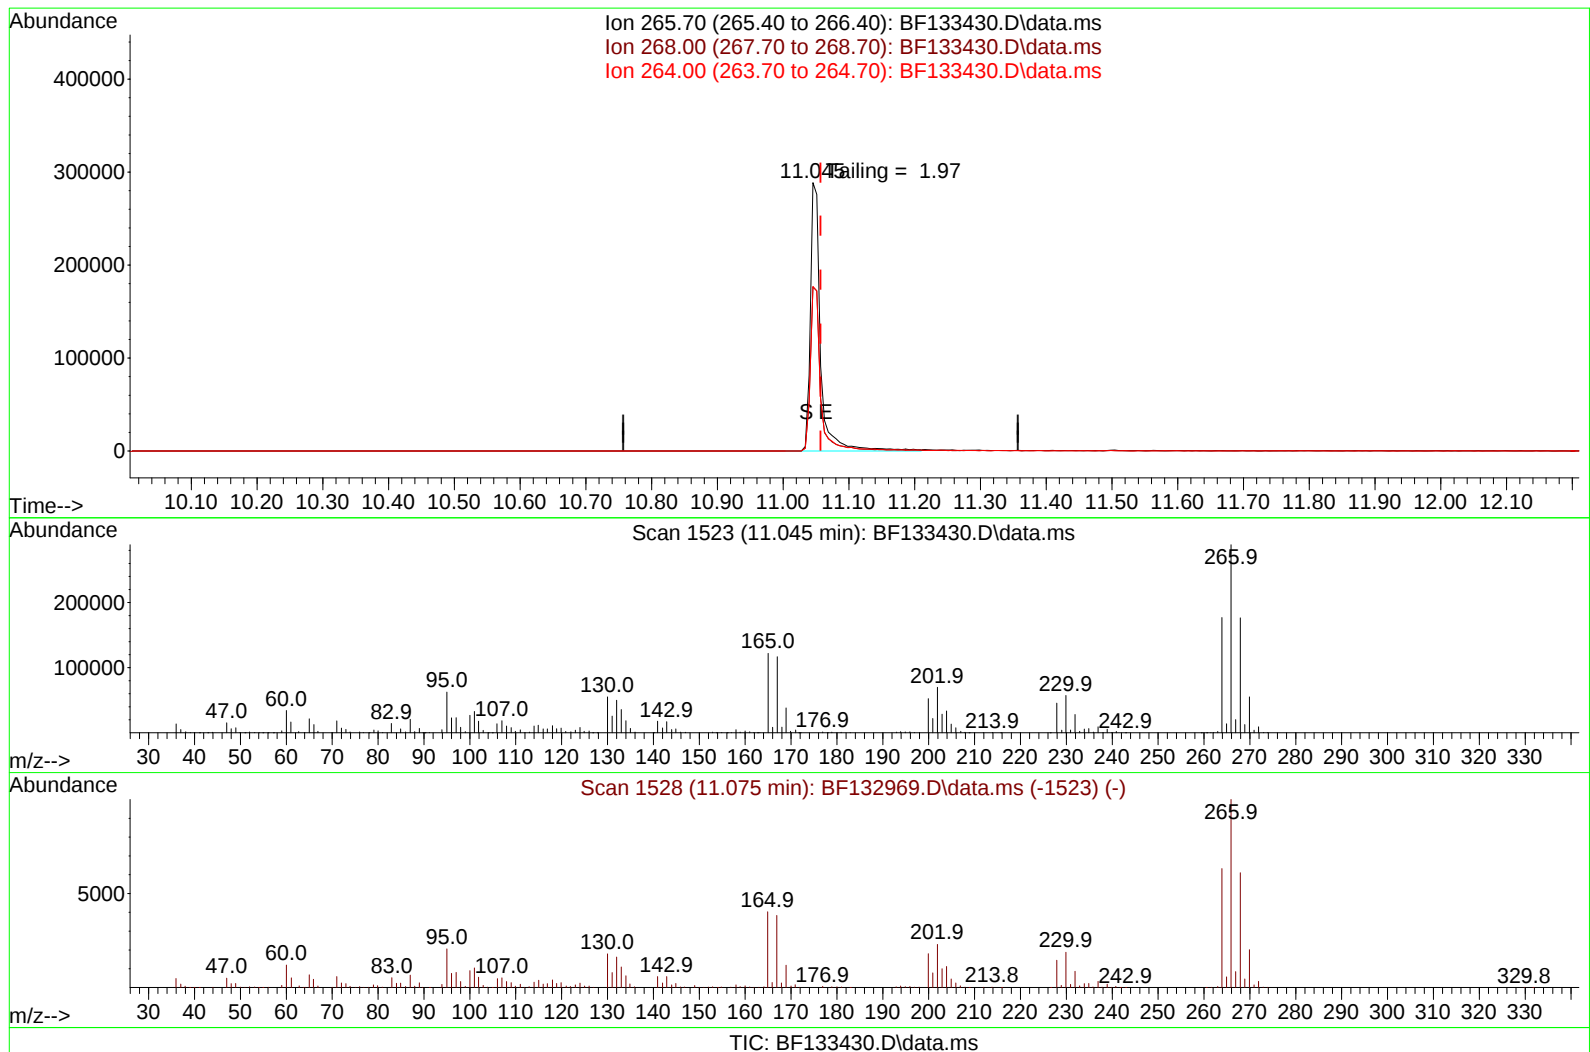

TIC: BF133430.D\data.ms

(70) Pentachlorophenol (C)

11.045min (-0.012) 24910.20 ng




response 315851

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	61.10
264.00	63.30	61.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051823\
 Data File : BF133430.D
 Acq On : 18 May 2023 09:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 18 14:31:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 16 14:39:29 2023
 Response via : Initial Calibration

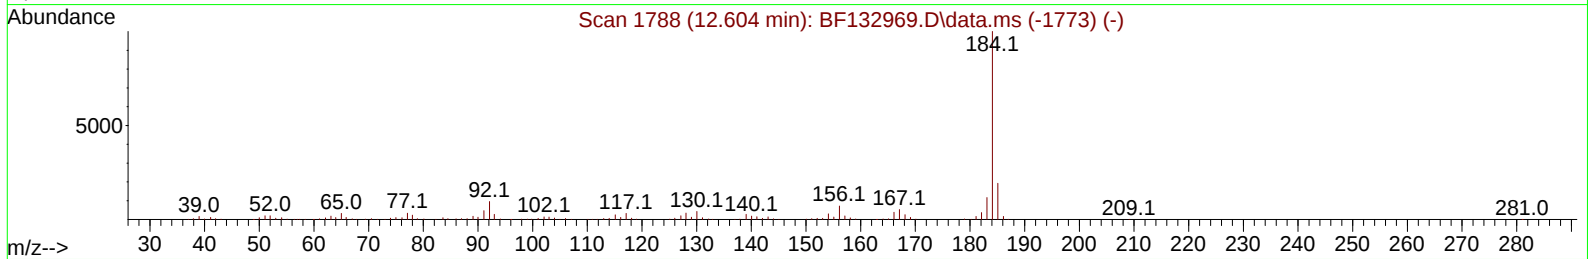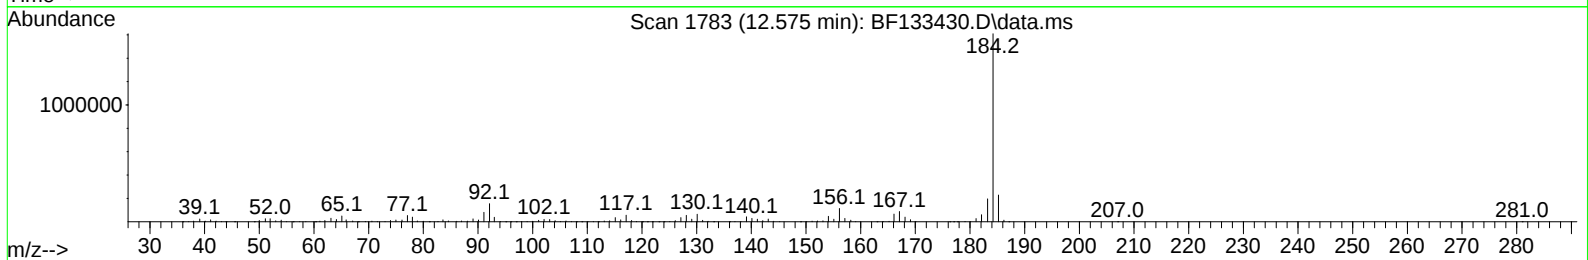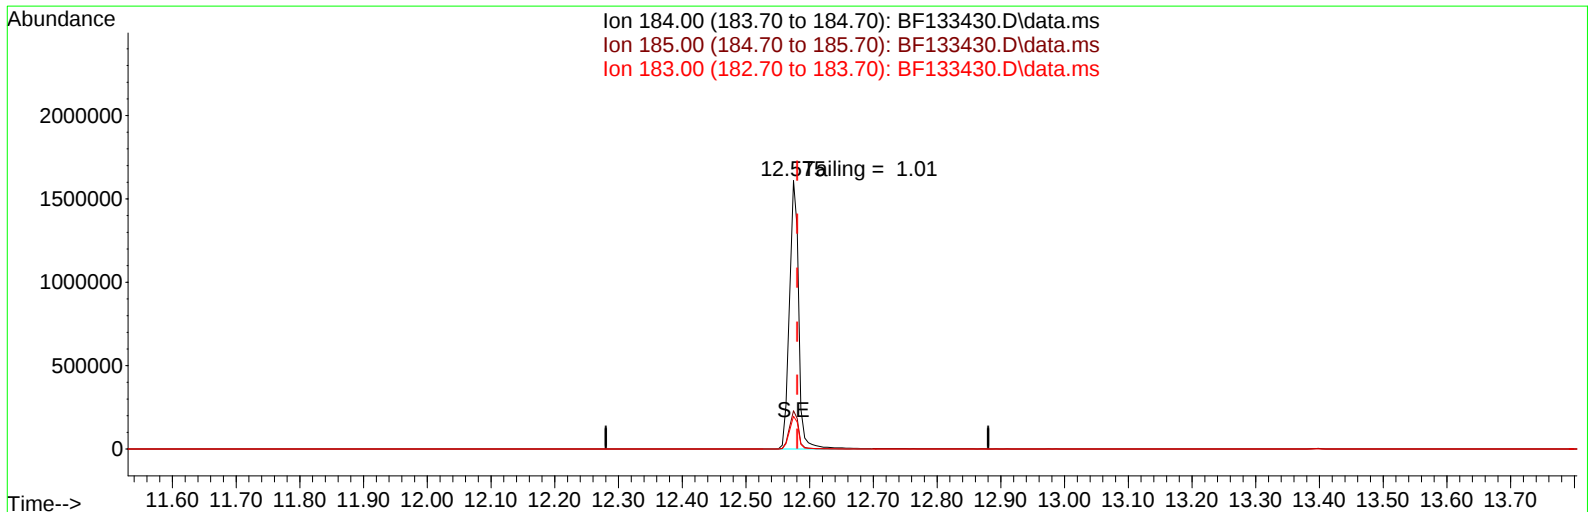

TIC: BF133430.D\data.ms

(77) Benzidine

12.575min (-0.006) 1277988.25 ng

response 1620859

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.27#
183.00	11.70	12.22
0.00	0.00	0.00