


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051915\
 Data File : BF079355.D
 Acq On : 19 May 2015 22:51
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 19 13:22:43 2015

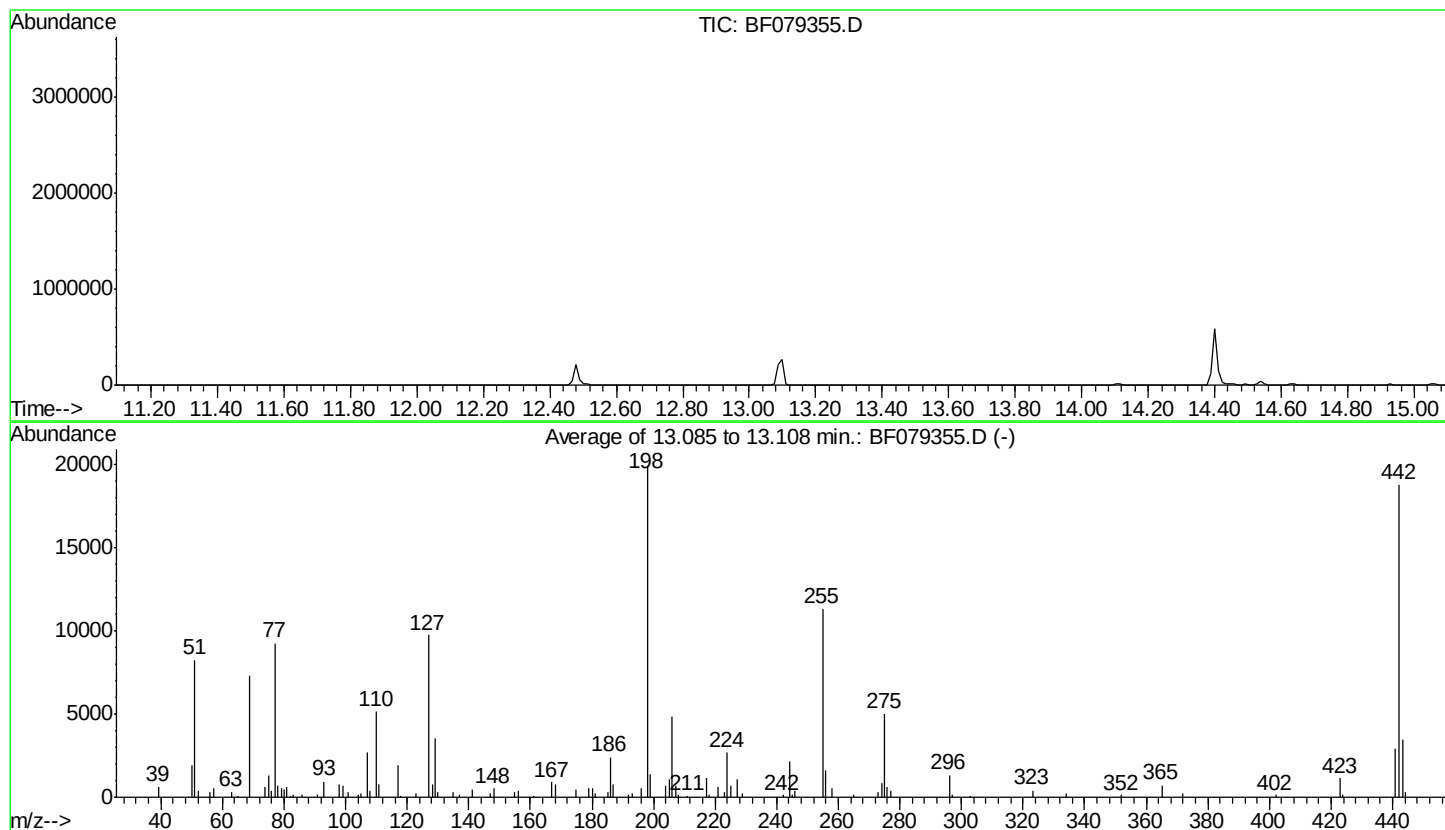

AutoFind: Scans 1041, 1042, 1043; Background Corrected with Scan 1037

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	8251	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.6	7277	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	9750	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19889	PASS
199	198	5	9	6.9	1373	PASS
275	198	10	60	25.3	5023	PASS
365	198	1	100	3.5	702	PASS
441	442	0.01	24	15.5	2911	PASS
442	198	50	100	94.3	18759	PASS
443	442	15	24	18.5	3462	PASS