
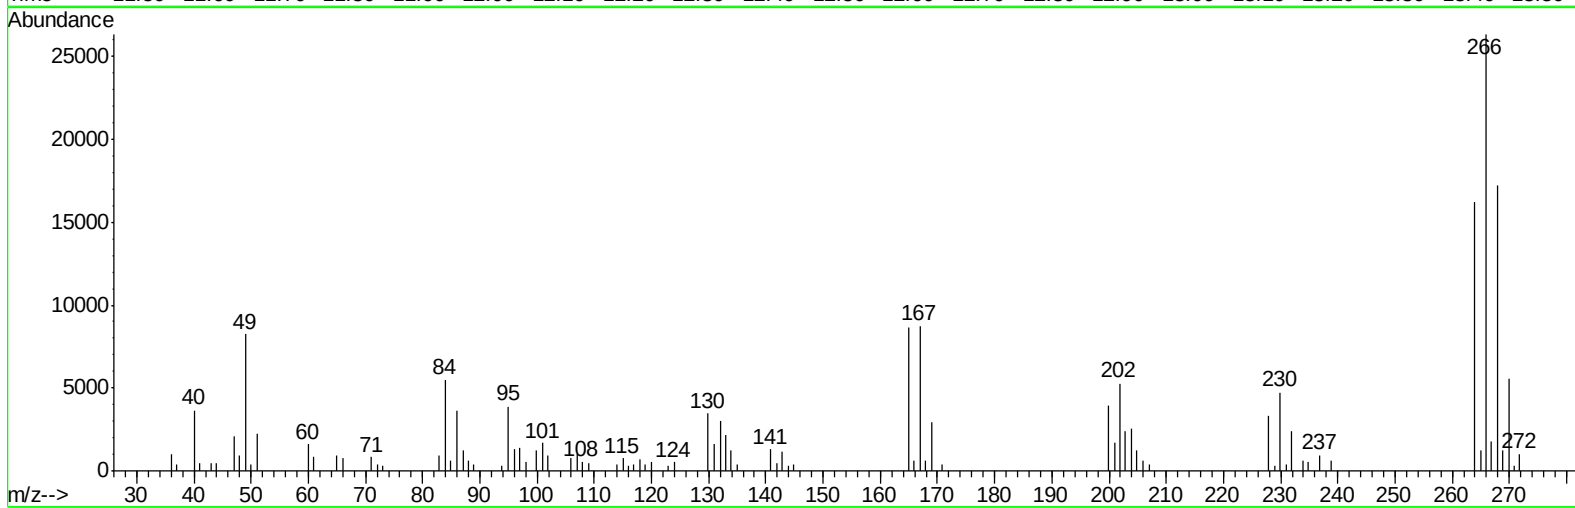


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051915\
Data File : BF079339.D
Acq On : 19 May 2015 11:48
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 07:09:28 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 20 05:08:22 2015
Response via : Initial Calibration

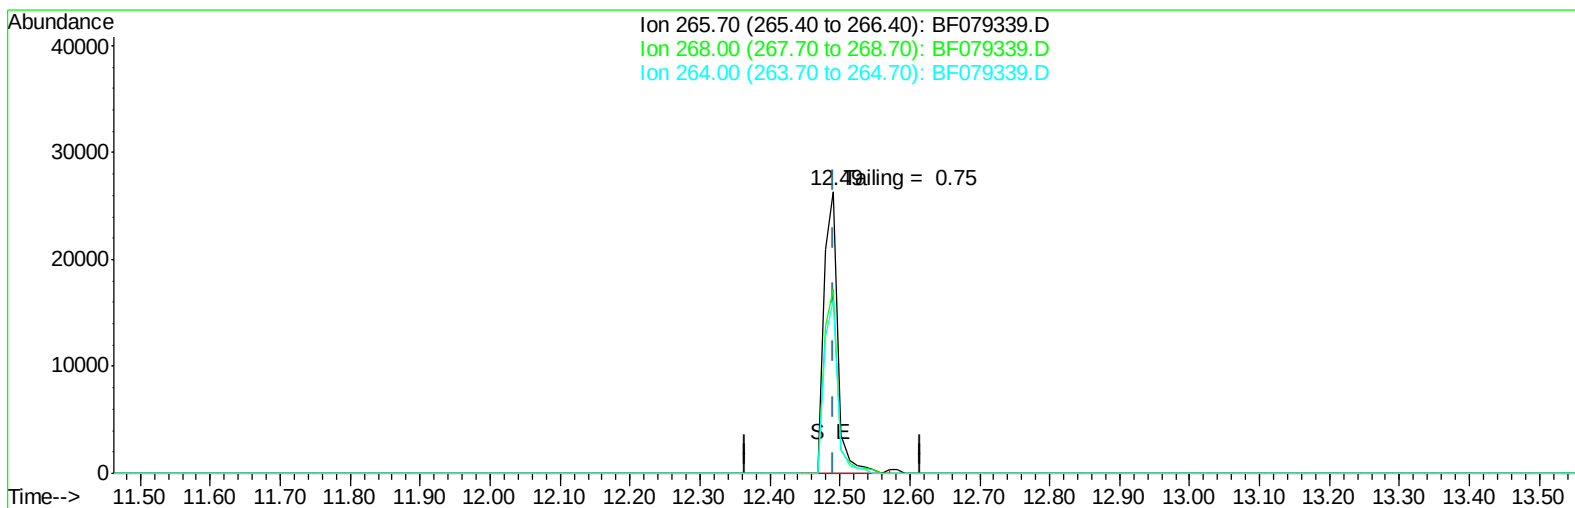

TIC: BF079339.D

(69) Pentachlorophenol (C)



12.491min (-0.000) 0.00ng

response 36913

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	65.31
264.00	63.60	61.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051915\
Data File : BF079339.D
Acq On : 19 May 2015 11:48
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 07:09:28 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 20 05:08:22 2015
Response via : Initial Calibration

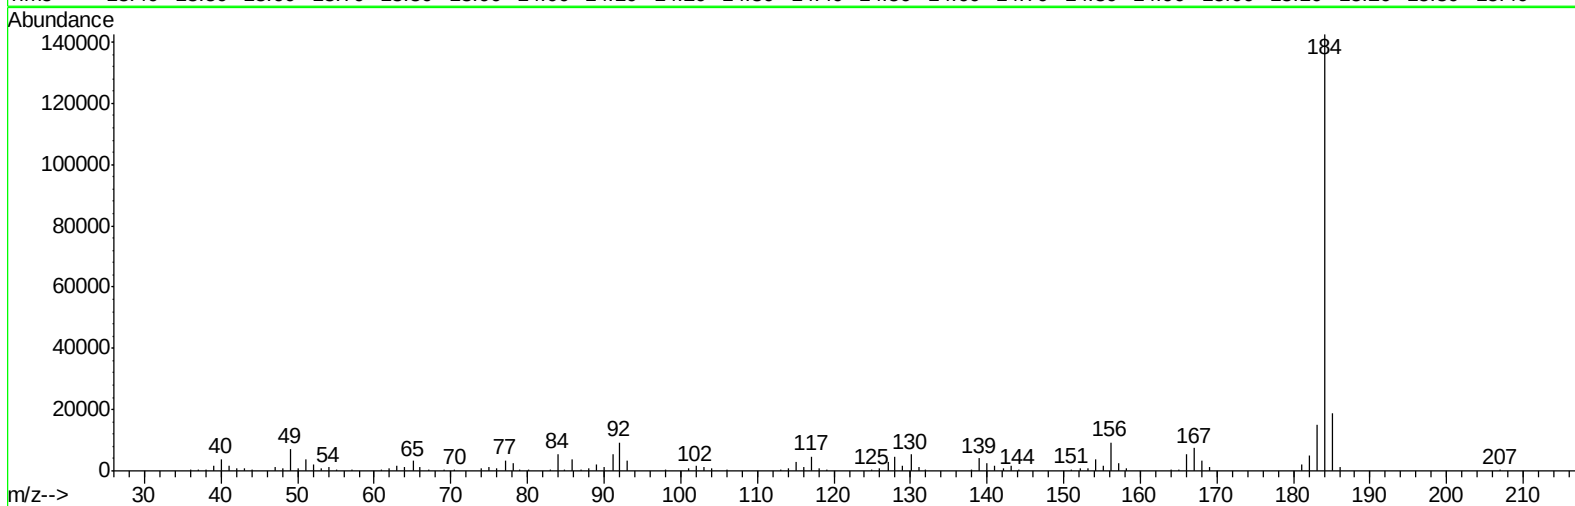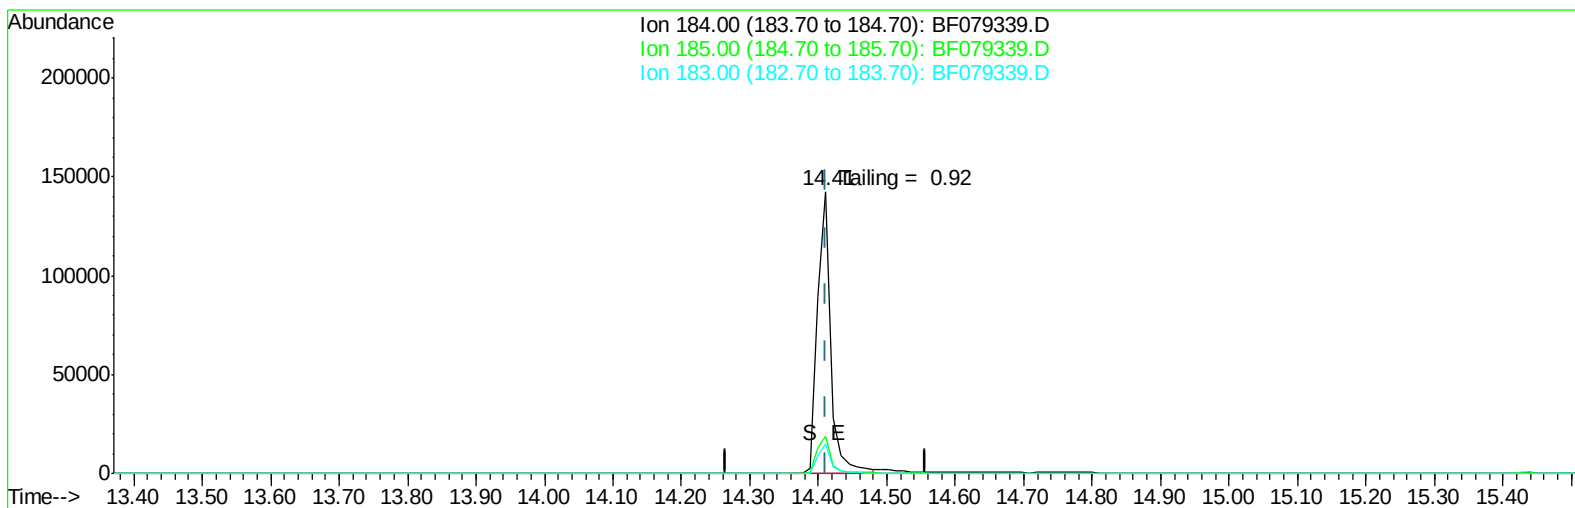

TIC: BF079339.D

(76) Benzidine

14.411min (-0.000) 0.00ng

response 197090

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	13.08
183.00	11.20	10.69
0.00	0.00	0.00