

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051915\
 Data File : BF079347.D
 Acq On : 19 May 2015 17:43
 Operator : TP/IZ
 Sample : G2265-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HW-12-5-14-15

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.393	15	18	29	rVB	170851	405959	4.82%	2.072%
2	1.553	29	32	39	rVV	324873	546620	6.49%	2.789%
3	1.644	39	40	48	rVV	310359	501732	5.96%	2.560%
4	1.758	48	50	91	rVB	3675390	8418669	100.00%	42.961%
5	5.404	367	369	372	rBV	315462	411492	4.89%	2.100%
6	6.696	480	482	485	rBV	285641	260766	3.10%	1.331%
7	6.833	492	494	497	rBV	832772	858709	10.20%	4.382%
8	7.130	517	520	522	rBV	215819	242762	2.88%	1.239%
9	7.313	533	536	538	rBV	919094	842930	10.01%	4.302%
10	7.816	578	580	583	rBV	548592	660572	7.85%	3.371%
11	8.708	655	658	660	rBV	254236	328413	3.90%	1.676%
12	10.045	773	775	778	rBV	1152778	1479956	17.58%	7.552%
13	10.868	845	847	850	rVB	297019	379610	4.51%	1.937%
14	11.851	931	933	936	rBV	1002792	1035009	12.29%	5.282%
15	12.708	1006	1008	1011	rBV	331915	408334	4.85%	2.084%
16	14.708	1180	1183	1186	rBV	1953720	1896079	22.52%	9.676%
17	16.000	1293	1296	1298	rBV	397189	447482	5.32%	2.284%
18	17.737	1445	1448	1451	rBV	346522	471051	5.60%	2.404%


Sum of corrected areas: 19596145

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051915\
Data File : BF079347.D
Acq On : 19 May 2015 17:43
Operator : TP/IZ
Sample : G2265-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HW-12-5-14-15

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

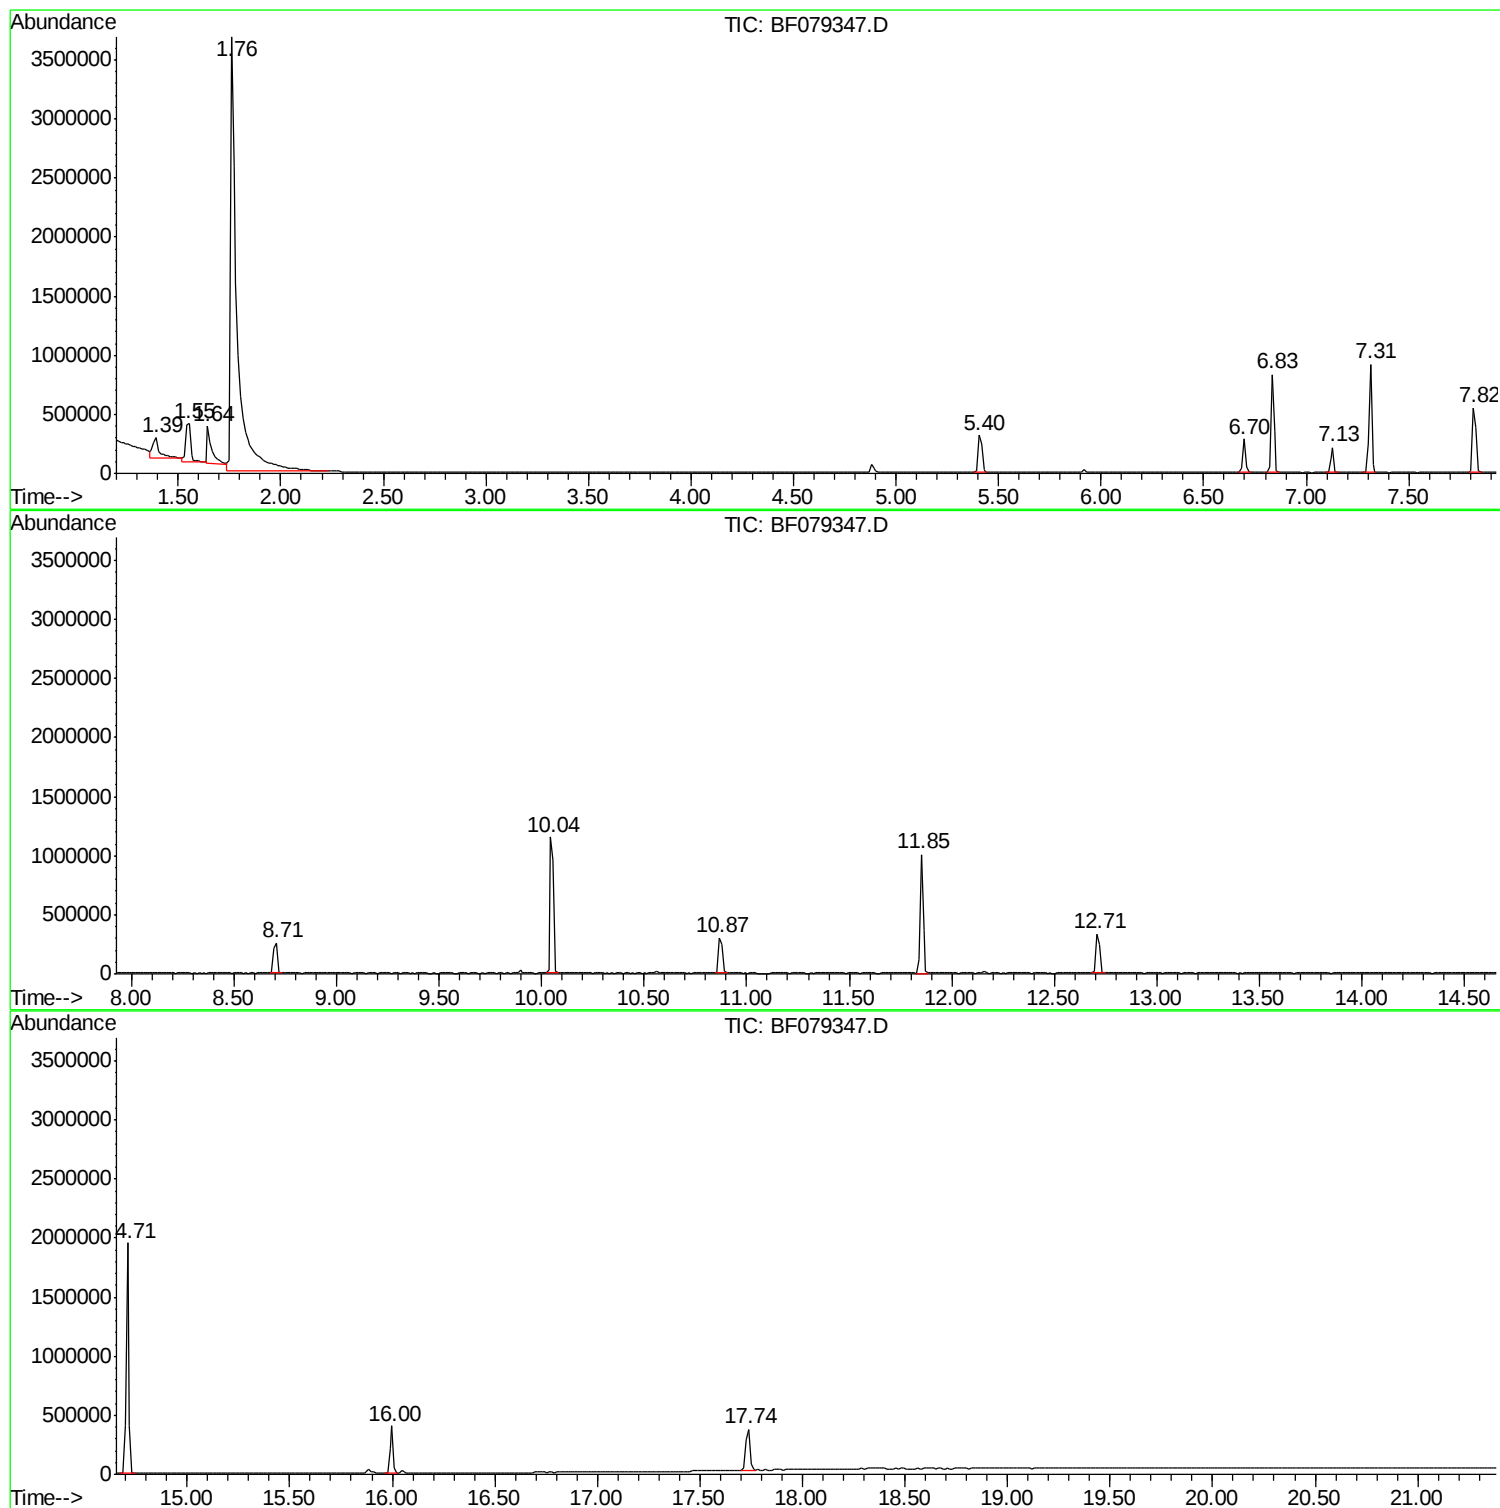

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051915\
Data File : BF079347.D
Acq On : 19 May 2015 17:43
Operator : TP/IZ
Sample : G2265-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HW-12-5-14-15










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.55	45.03 ng	546620	1,4-Dichlorobenzene-d4	7.13

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		Silane, tetramethyl-	88	C4H12Si	000075-76-3	35
3		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4		1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9
5		N-Ethylformamide	73	C3H7NO	000627-45-2	9

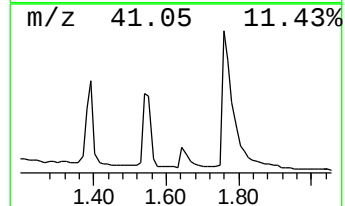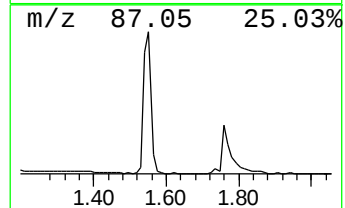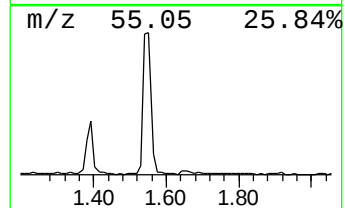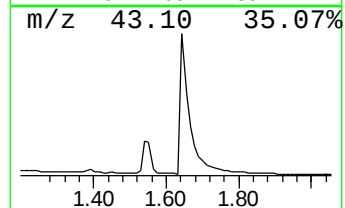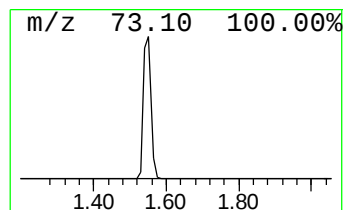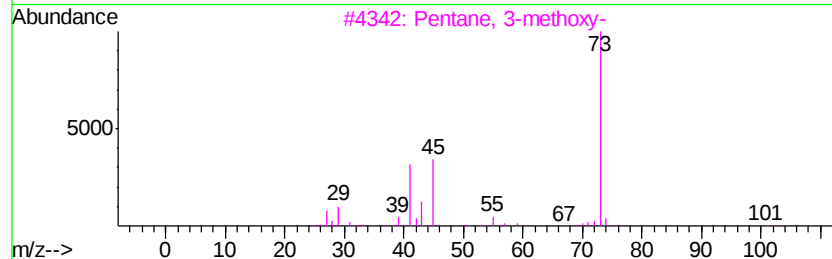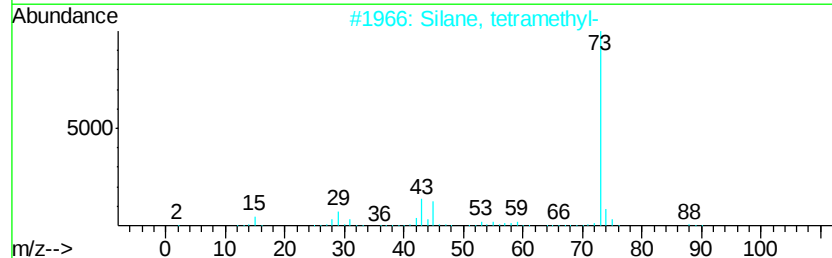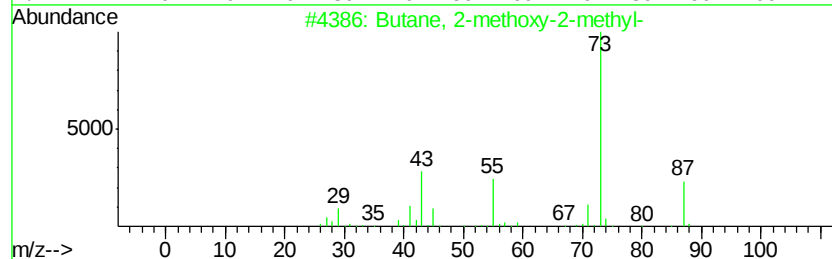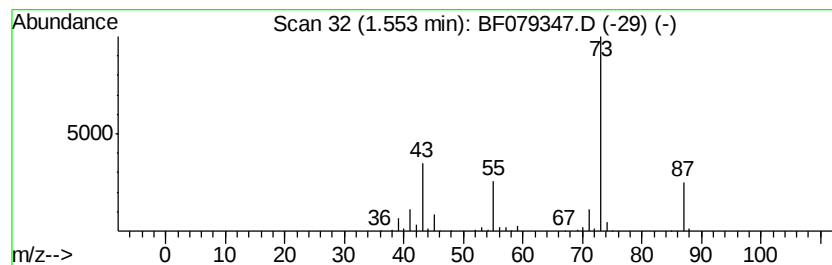

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051915\
Data File : BF079347.D
Acq On : 19 May 2015 17:43
Operator : TP/IZ
Sample : G2265-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HW-12-5-14-15










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 unknown6.83 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.83	70.74 ng	858709	1,4-Dichlorobenzene-d4	7.13

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27	
2	5-Aminoindole	132	C8H8N2	005192-03-0	12	
3	Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	10	
4	Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9	
5	4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9	

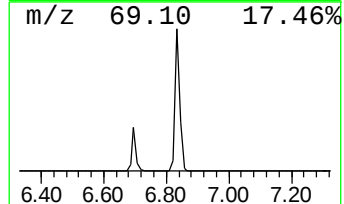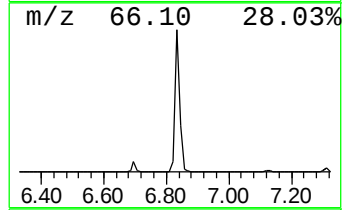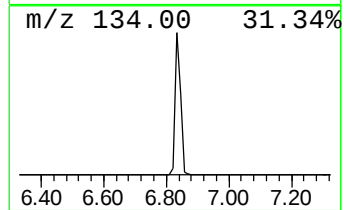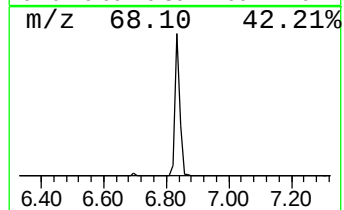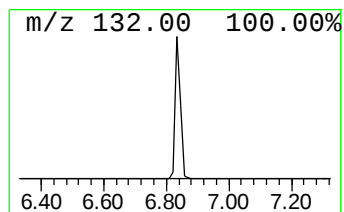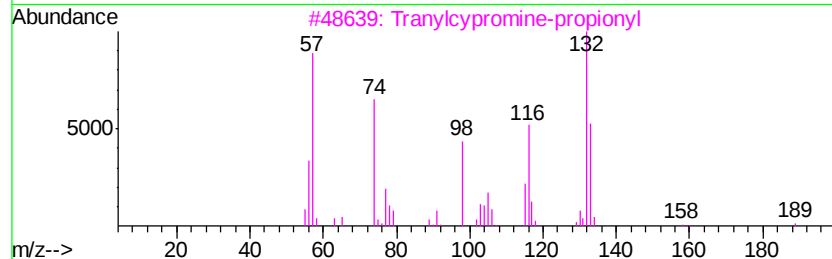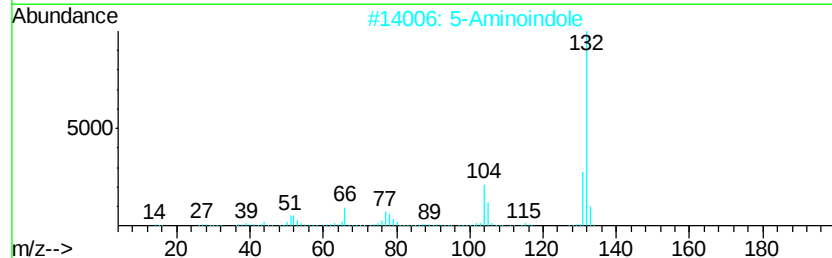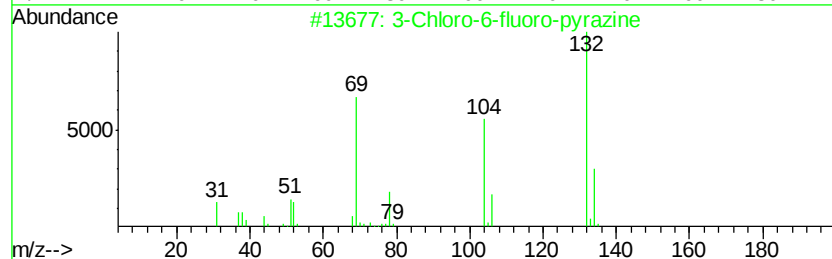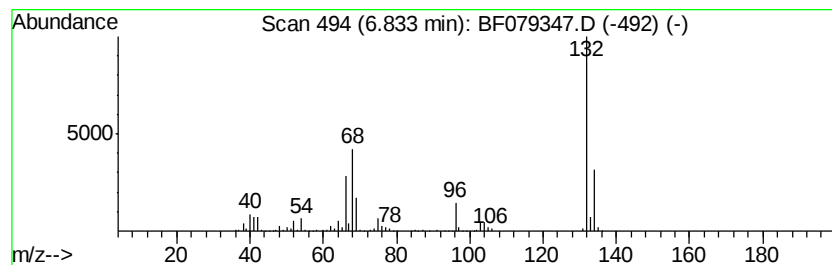

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051915\
Data File : BF079347.D
Acq On : 19 May 2015 17:43
Operator : TP/IZ
Sample : G2265-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HW-12-5-14-15

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	1.55	45.0	ng	546620	1	7.13	242762	20.0
unknown6.83	6.83	70.7	ng	858709	1	7.13	242762	20.0