

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051915\
 Data File : BF079349.D
 Acq On : 19 May 2015 18:41
 Operator : TP/IZ
 Sample : G2265-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HW-10-5-14-15

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.393	15	18	29	rVB	156080	443319	5.01%	2.261%
2	1.541	29	31	34	rVB	325529	428809	4.85%	2.187%
3	1.644	39	40	48	rVV	305867	497499	5.62%	2.538%
4	1.758	48	50	92	rVB	3757703	8846173	100.00%	45.122%
5	5.404	367	369	372	rBV	293732	372865	4.21%	1.902%
6	6.696	480	482	486	rBV	234397	239688	2.71%	1.223%
7	6.833	492	494	497	rBV	683083	784176	8.86%	4.000%
8	7.130	518	520	522	rBV	208607	231838	2.62%	1.183%
9	7.313	534	536	538	rBV	840736	764102	8.64%	3.897%
10	7.816	578	580	583	rBV	511647	610896	6.91%	3.116%
11	8.708	655	658	660	rBV	266022	321607	3.64%	1.640%
12	10.045	773	775	778	rBV	1086398	1422032	16.08%	7.253%
13	10.868	845	847	850	rVB	280901	374004	4.23%	1.908%
14	11.851	931	933	936	rBV	966621	1011908	11.44%	5.161%
15	12.708	1006	1008	1011	rBV	337785	404115	4.57%	2.061%
16	14.708	1180	1183	1186	rBV	1835711	1862915	21.06%	9.502%
17	16.000	1293	1296	1299	rVV	434922	489549	5.53%	2.497%
18	17.737	1445	1448	1451	rBV	414790	499478	5.65%	2.548%


Sum of corrected areas: 19604973

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051915\
Data File : BF079349.D
Acq On : 19 May 2015 18:41
Operator : TP/IZ
Sample : G2265-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HW-10-5-14-15

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

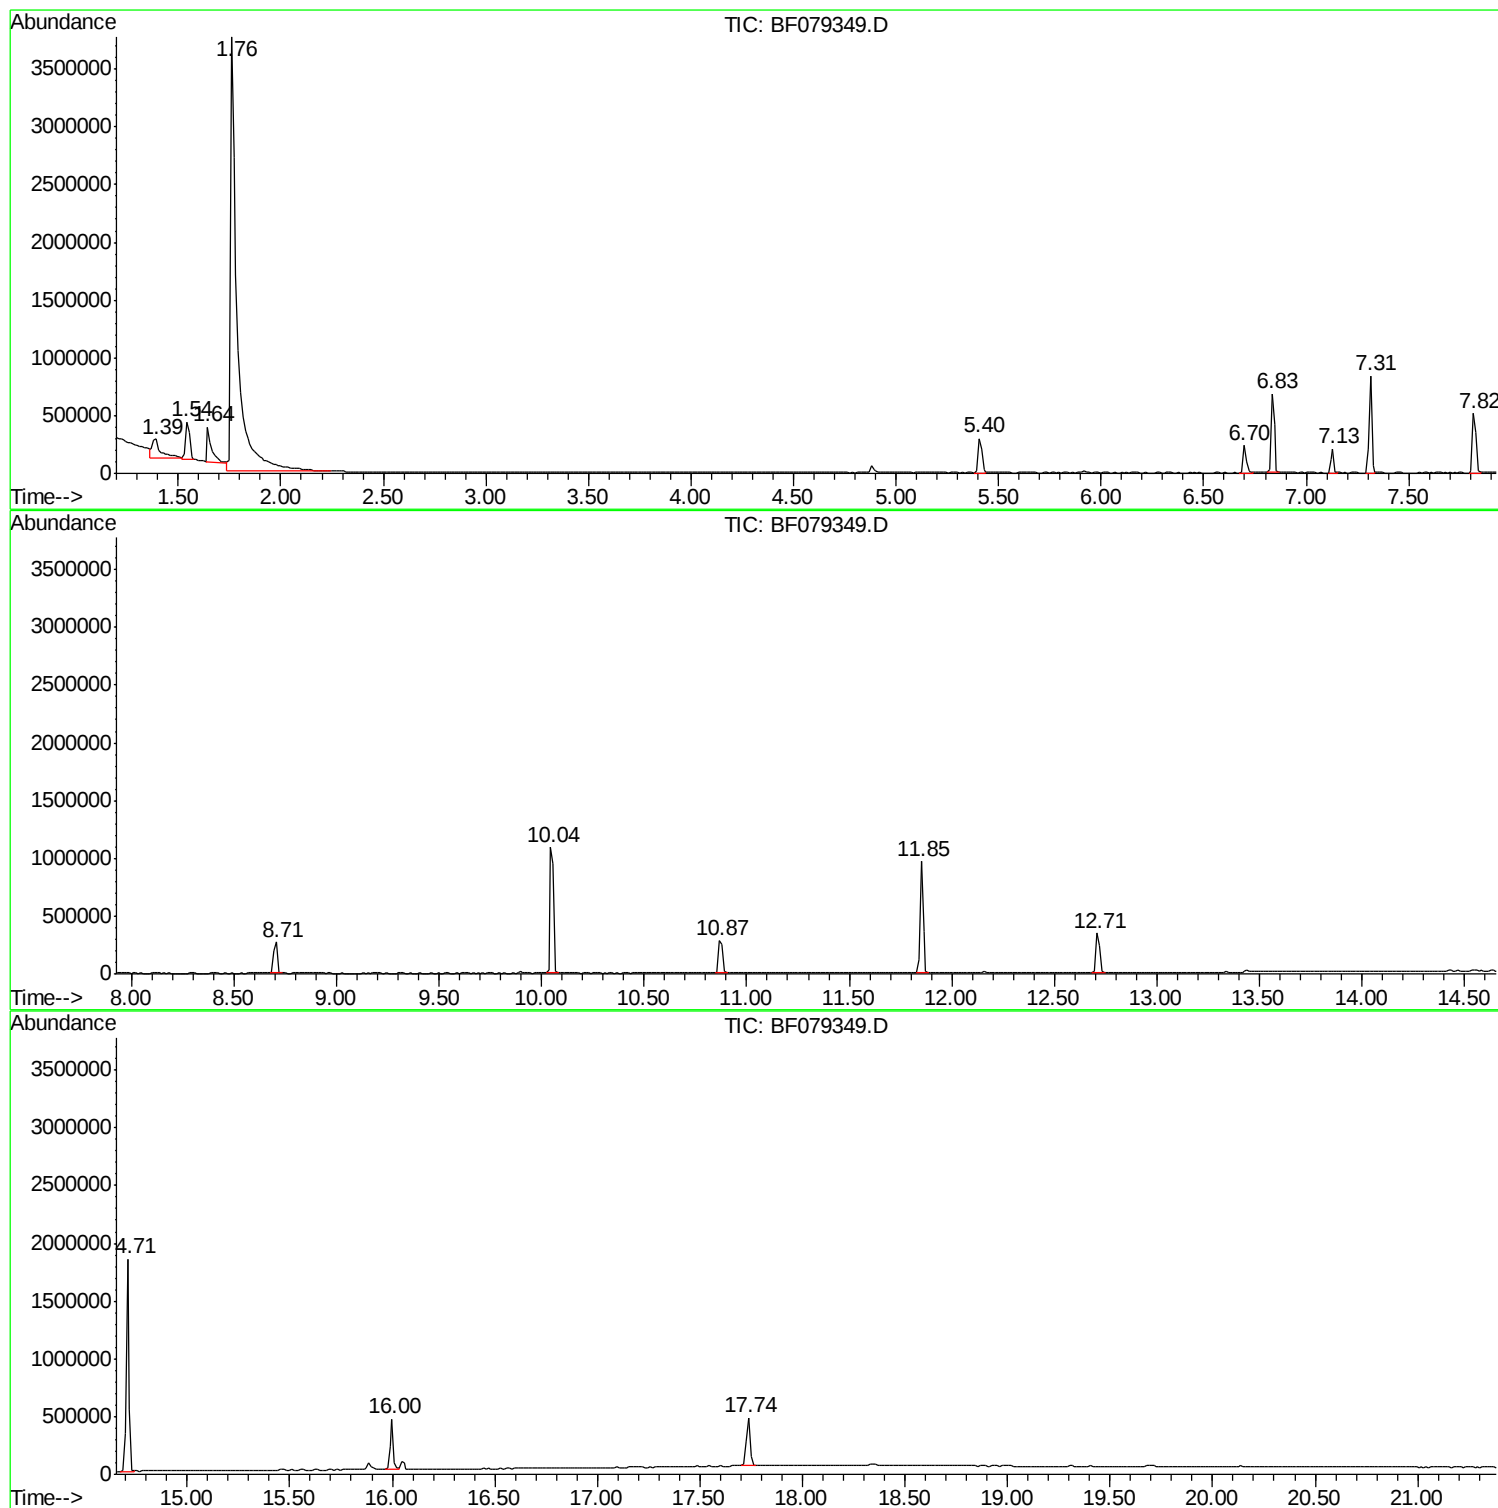

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051915\
Data File : BF079349.D
Acq On : 19 May 2015 18:41
Operator : TP/IZ
Sample : G2265-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HW-10-5-14-15










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.54	36.99 ng	428809	1,4-Dichlorobenzene-d4	7.13

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	37
3		2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	16
4		Silane, tetramethyl-	88	C4H12Si	000075-76-3	12
5		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12

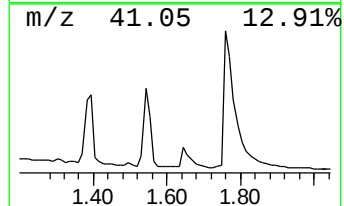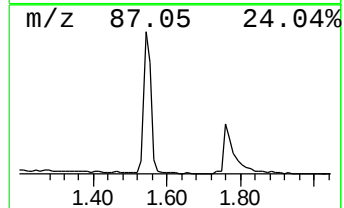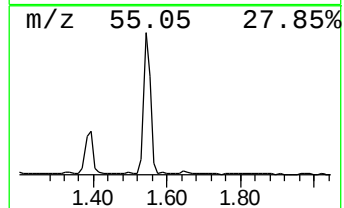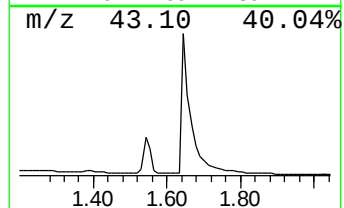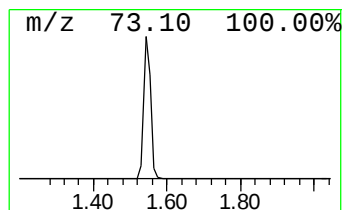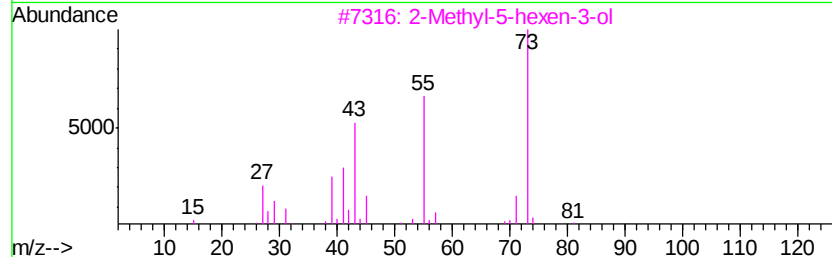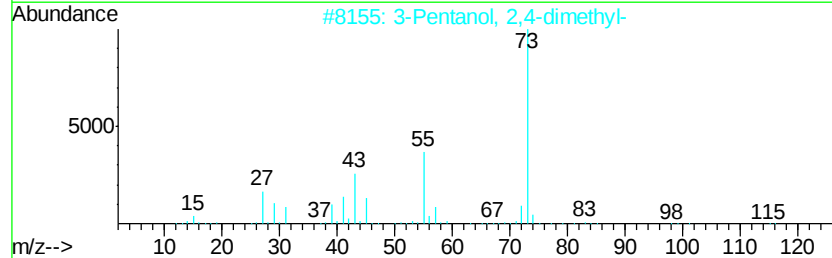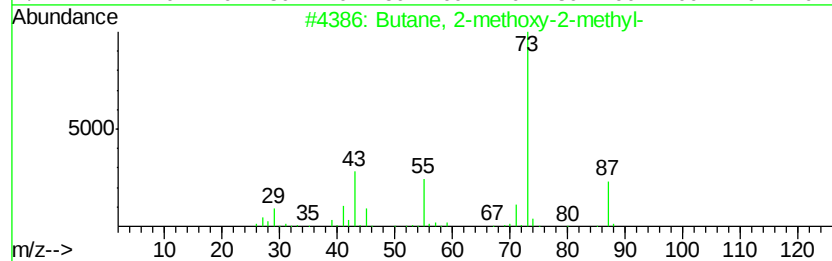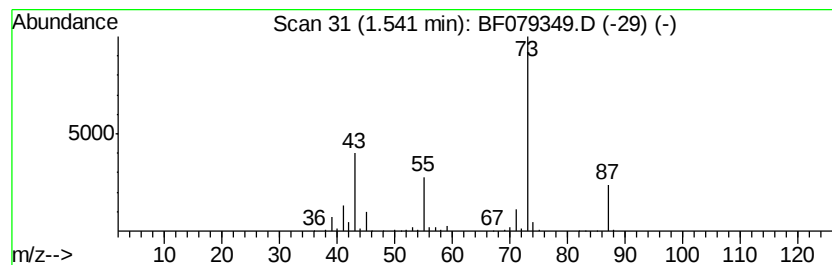

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051915\
Data File : BF079349.D
Acq On : 19 May 2015 18:41
Operator : TP/IZ
Sample : G2265-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HW-10-5-14-15








Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 unknown6.83 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.83	67.65 ng	784176	1,4-Dichlorobenzene-d4	7.13

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

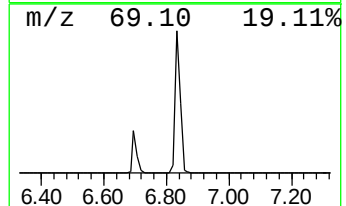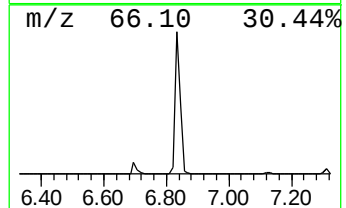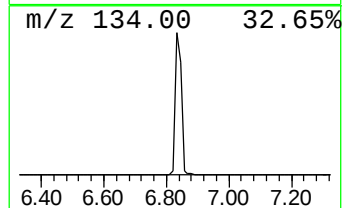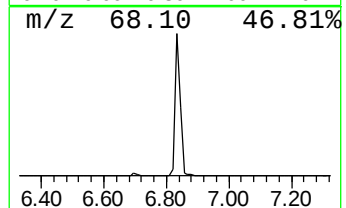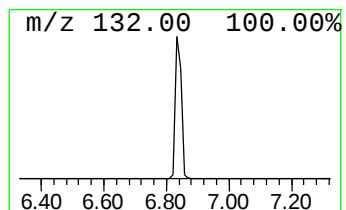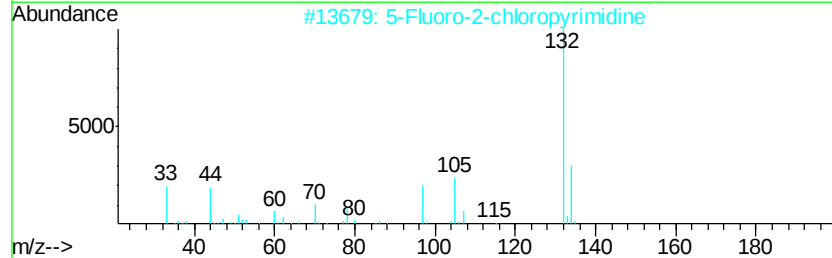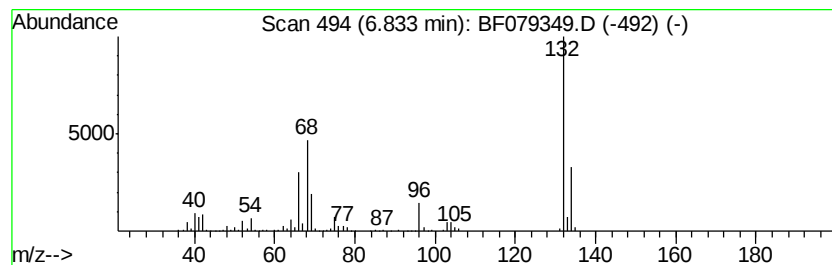

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051915\
Data File : BF079349.D
Acq On : 19 May 2015 18:41
Operator : TP/IZ
Sample : G2265-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HW-10-5-14-15

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	1.54	37.0	ng	428809	1	7.13	231838	20.0
unknown6.83	6.83	67.7	ng	784176	1	7.13	231838	20.0