


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051915\
Data File : BF079339.D
Acq On : 19 May 2015 11:48
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 20 05:08:22 2015

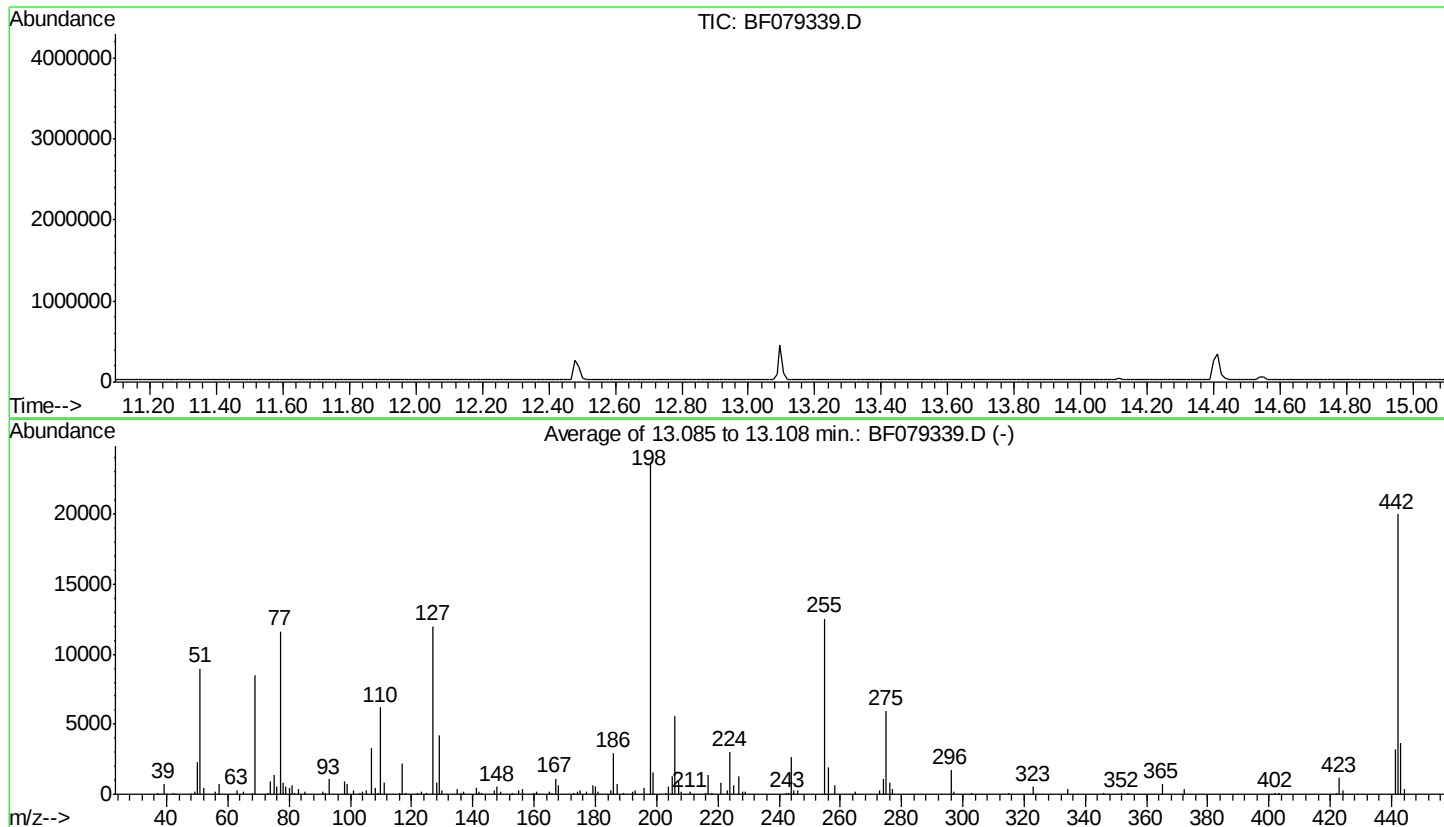

AutoFind: Scans 1041, 1042, 1043; Background Corrected with Scan 1038

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	8989	PASS
68	69	0.00	2	1.6	139	PASS
69	198	0.00	100	35.8	8474	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	12013	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23677	PASS
199	198	5	9	6.7	1598	PASS
275	198	10	60	25.1	5952	PASS
365	198	1	100	3.2	750	PASS
441	442	0.01	24	16.1	3221	PASS
442	198	50	100	84.5	20000	PASS
443	442	15	24	18.4	3684	PASS