
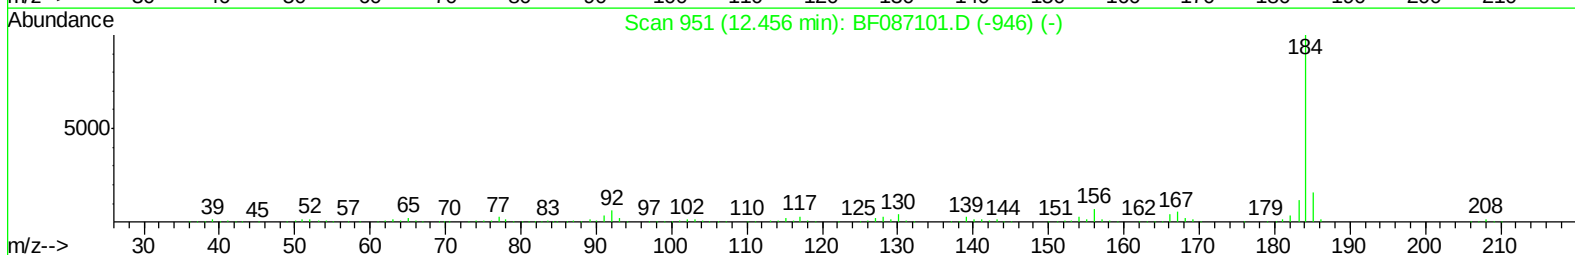
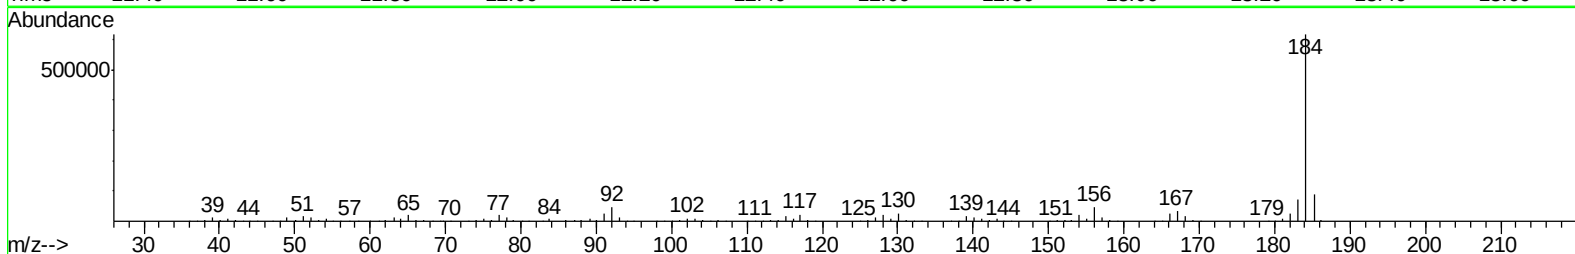


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051916\
Data File : BF087184.D
Acq On : 19 May 2016 12:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 08:12:17 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 16:55:01 2016
Response via : Initial Calibration

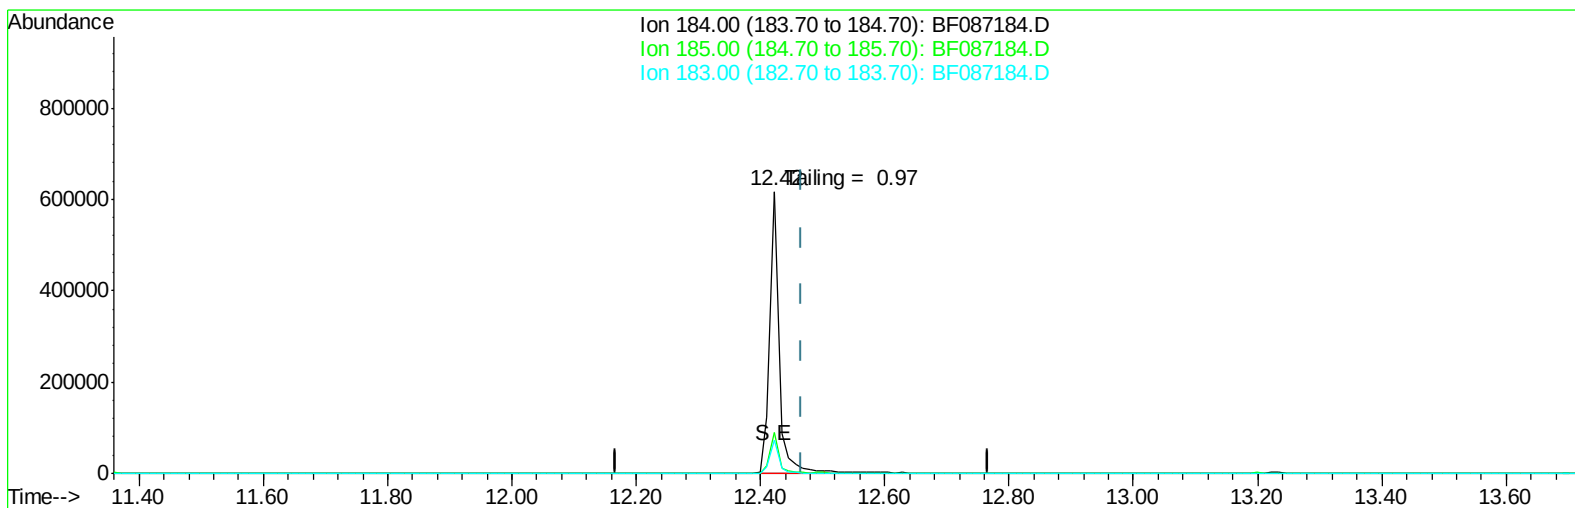

TIC: BF087184.D

(76) Benzidine




12.422min (-0.045) 0.00ng

response 653874

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.35
183.00	12.20	11.97
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051916\
Data File : BF087184.D
Acq On : 19 May 2016 12:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 20 08:12:17 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 16:55:01 2016
Response via : Initial Calibration

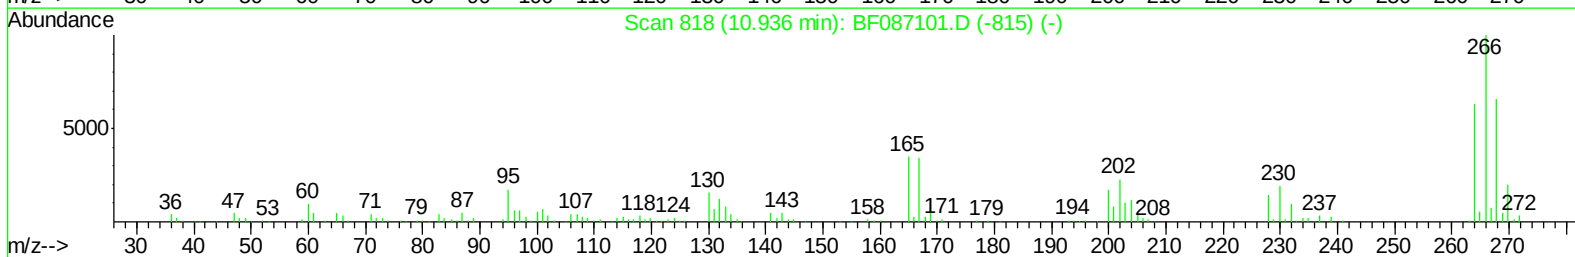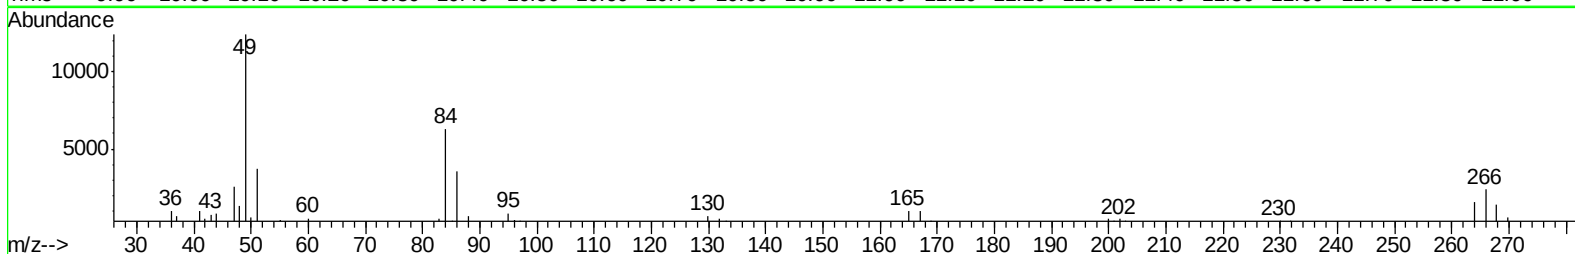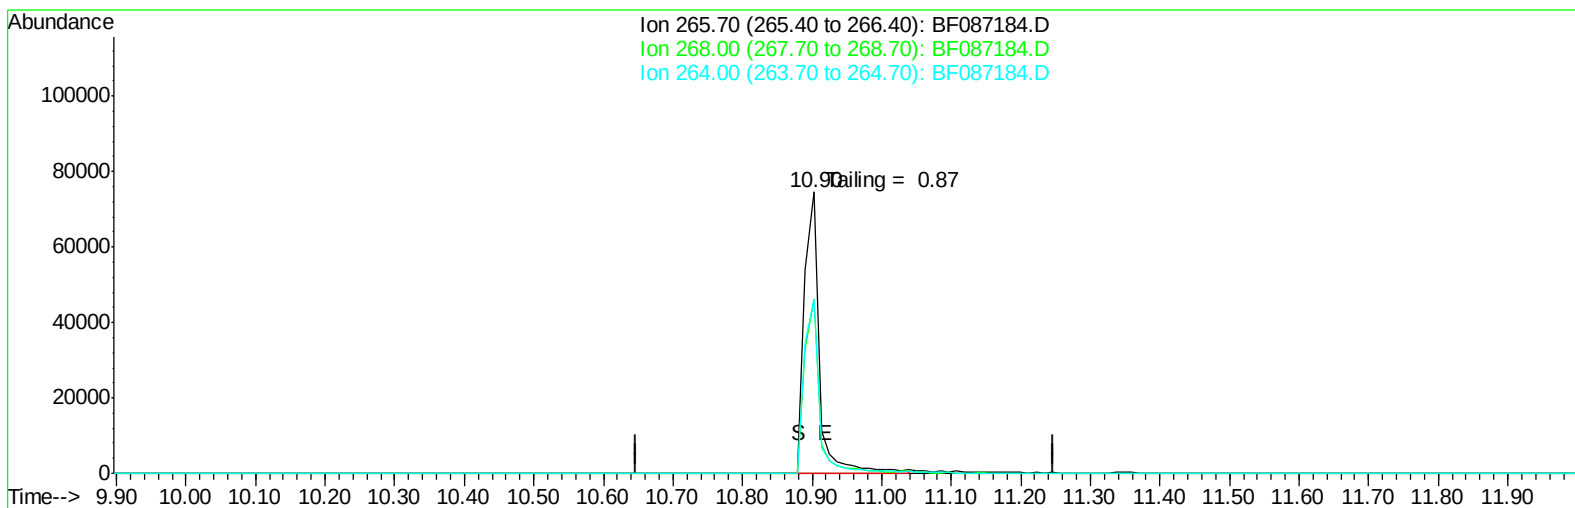

TIC: BF087184.D

(69) Pentachlorophenol (C)

10.948min (-10.948) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	64.40	0.00#
264.00	66.10	0.00#
0.00	0.00	0.00