

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051916\
 Data File : BF087215.D
 Acq On : 20 May 2016 6:38
 Operator : UM/SJ
 Sample : H3132-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB-BWR-BB-R10-C5-2(0-19FT)

Quant Time: May 20 08:00:47 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 16:55:01 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.57	152	124180	20.00	ng	-0.03
21) Naphthalene-d8	7.85	136	514011	20.00	ng	-0.05
38) Acenaphthene-d10	9.60	164	234762	20.00	ng	-0.05
63) Phenanthrene-d10	11.07	188	368069	20.00	ng	-0.05
75) Chrysene-d12	13.70	240	267456	20.00	ng	-0.06
86) Perylene-d12	15.06	264	225847	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	962321	130.25	ng	-0.03
7) Phenol-d6	6.24	99	1161336	117.20	ng	-0.05
23) Nitrobenzene-d5	7.14	82	847099	82.13	ng	-0.05
41) 2,4,6-Tribromophenol	10.40	330	311261	119.98	ng	-0.05
44) 2-Fluorobiphenyl	8.94	172	1483456	104.65	ng	-0.05
78) Terphenyl-d14	12.66	244	1034740	87.52	ng	-0.05


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051916\
Data File : BF087215.D
Acq On : 20 May 2016 6:38
Operator : UM/SJ
Sample : H3132-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-BWR-BB-R10-C5-2(0-19FT)

Quant Time: May 20 08:00:47 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 16:55:01 2016
Response via : Initial Calibration

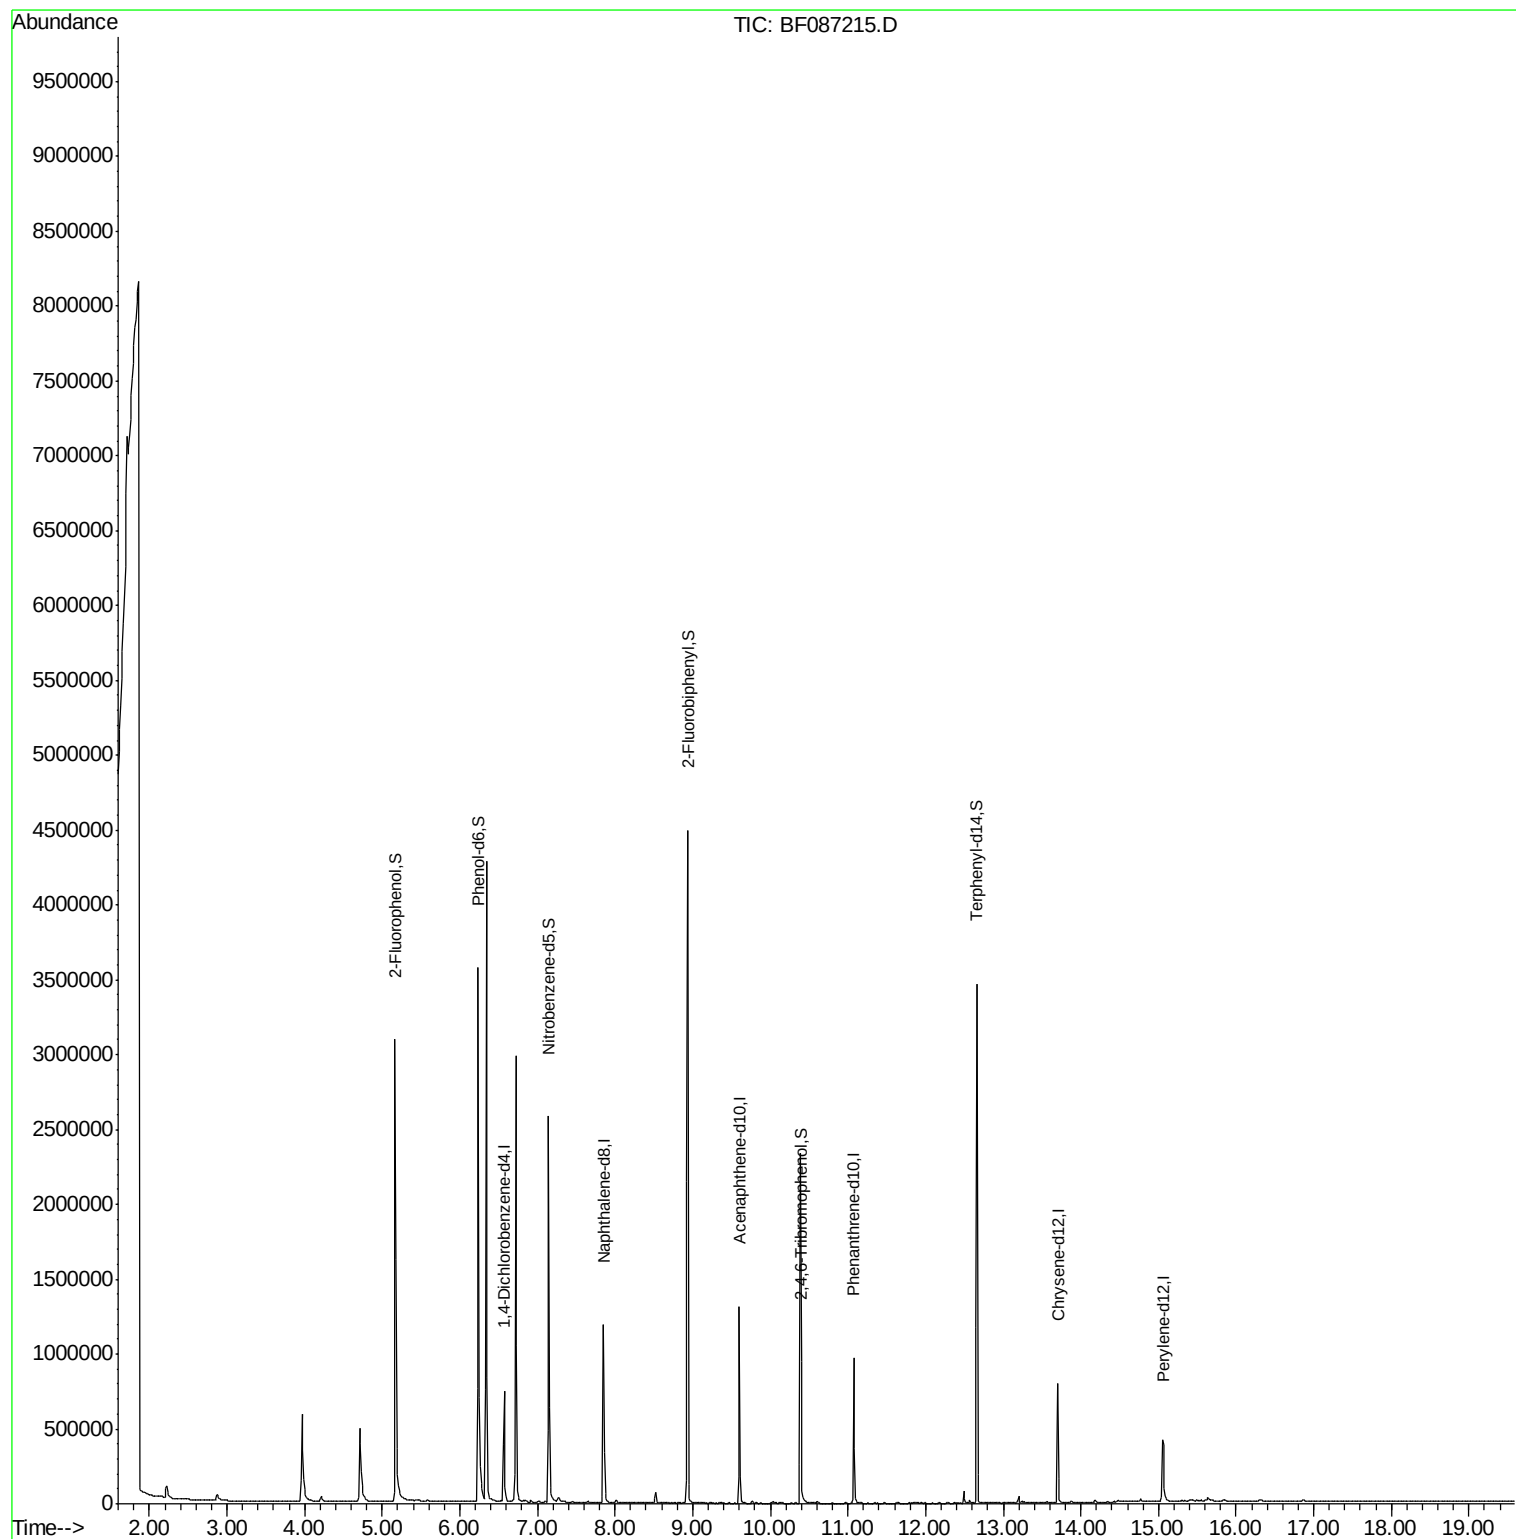

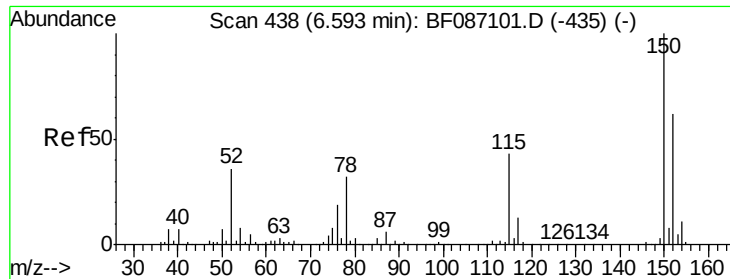

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.57 min Scan# 436

Delta R.T. -0.03 min

Lab File: BF087215.D

Acq: 20 May 2016 6:38

Instrument :

BNA_F

ClientSampleId :

FB-BWR-BB-R10-C5-2(0-19FT)


Tgt Ion:152 Resp: 124180

Ion Ratio Lower Upper

152 100

150 154.8 125.8 188.6


115 60.1 51.5 77.3

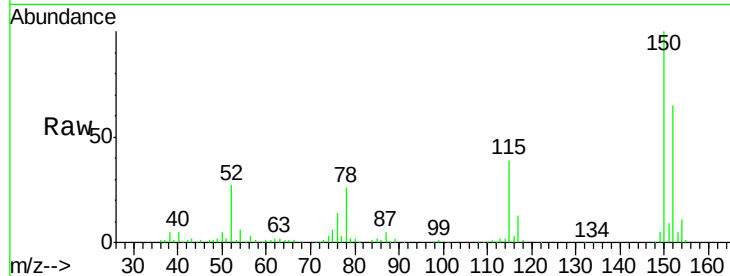


Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

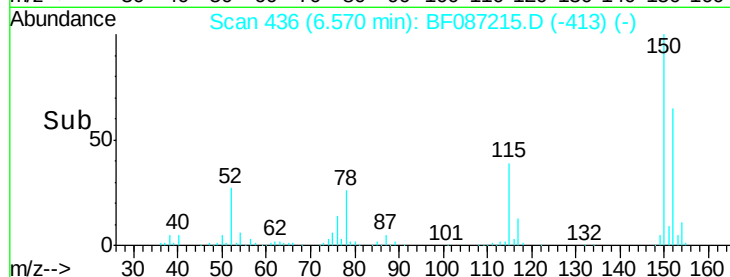

Time-->

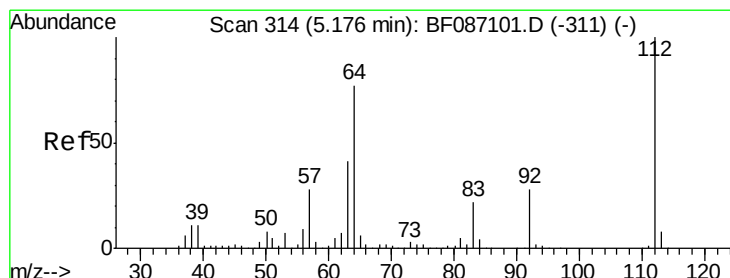

#5

2-Fluorophenol

Concen: 130.25 ng

RT: 5.16 min Scan# 313

Delta R.T. -0.03 min

Lab File: BF087215.D

Acq: 20 May 2016 6:38


Tgt Ion:112 Resp: 962321

Ion Ratio Lower Upper

112 100

64 79.1 52.1 78.1#


63 43.2 25.7 38.5#

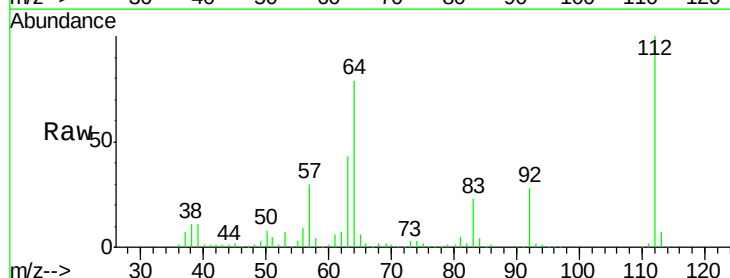


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

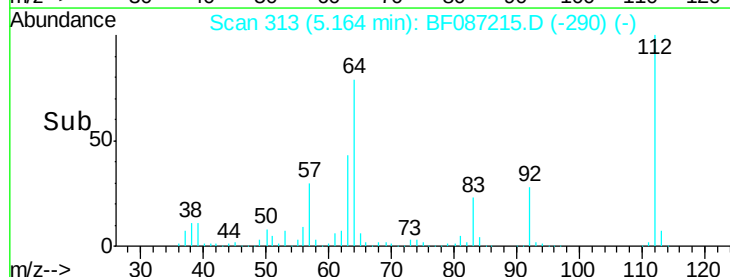

Time-->

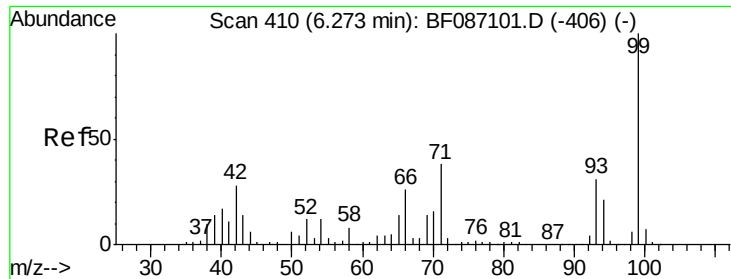

#7

Phenol-d6

Concen: 117.20 ng

RT: 6.24 min Scan# 407

Delta R.T. -0.05 min

Lab File: BF087215.D

Acq: 20 May 2016 6:38

Instrument :

BNA_F

ClientSampleId :

FB-BWR-BB-R10-C5-2(0-19FT)


Tgt Ion: 99 Resp: 1161336

Ion Ratio Lower Upper

99 100

42 30.4 13.6 20.4#




71 40.4 24.6 36.8#

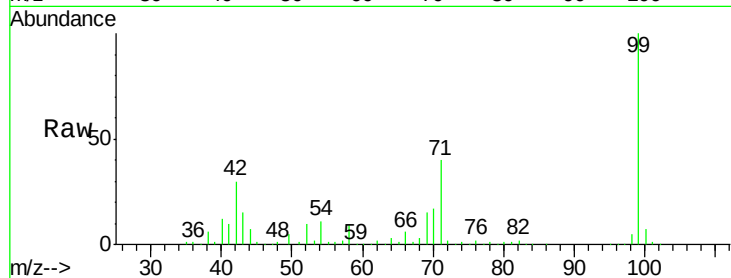

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

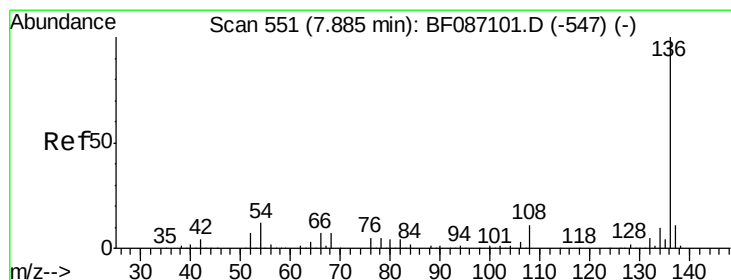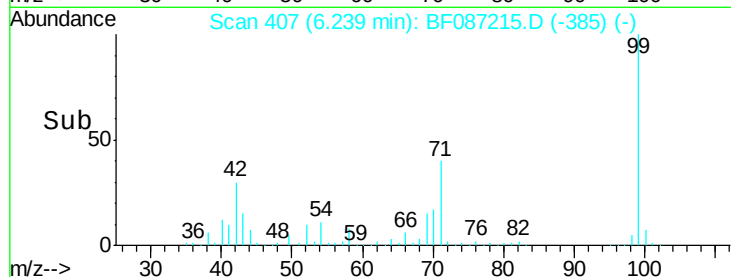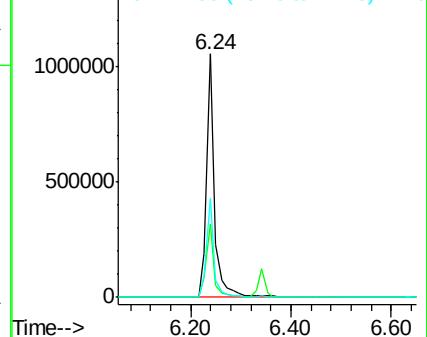

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.85 min Scan# 548

Delta R.T. -0.05 min

Lab File: BF087215.D

Acq: 20 May 2016 6:38

Tgt Ion: 136 Resp: 514011


Ion Ratio Lower Upper

136 100

137 11.3 8.8 13.2

54 13.4 5.0 7.4#

68 6.8 4.4 6.6#


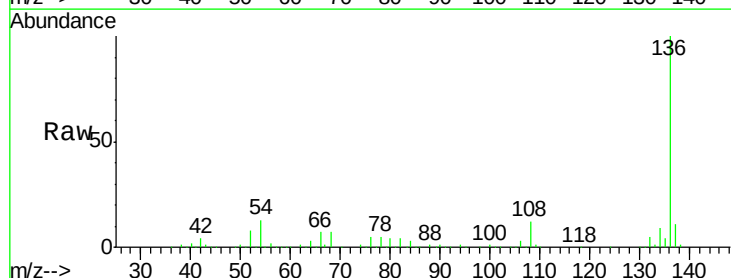



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



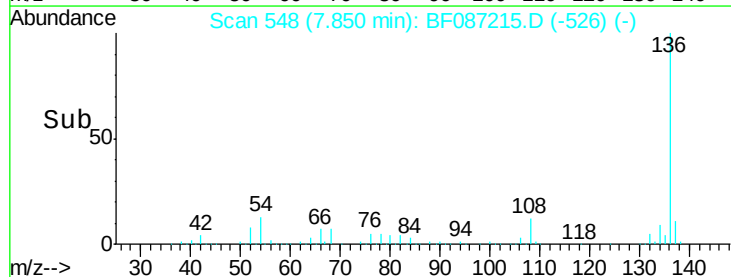
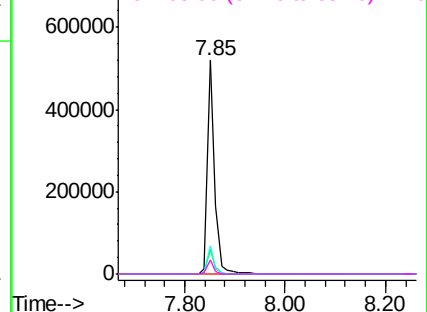


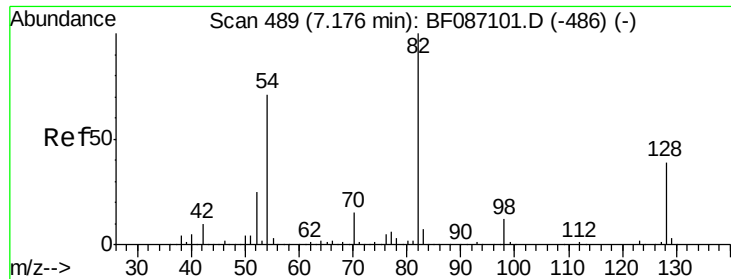

#23
 Nitrobenzene-d5
 Concen: 82.13 ng
 RT: 7.14 min Scan# 486
 Delta R.T. -0.05 min
 Lab File: BF087215.D
 Acq: 20 May 2016 6:38




Instrument :
 BNA_F
 ClientSampleId :
 FB-BWR-BB-R10-C5-2(0-19FT)


Tgt Ion: 82 Resp: 847099
 Ion Ratio Lower Upper
 82 100
 128 37.9 40.6 61.0#
 54 71.7 38.1 57.1#

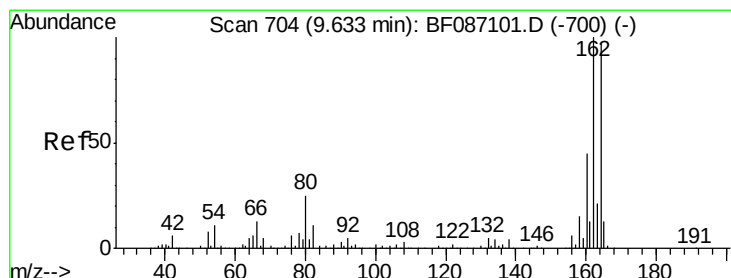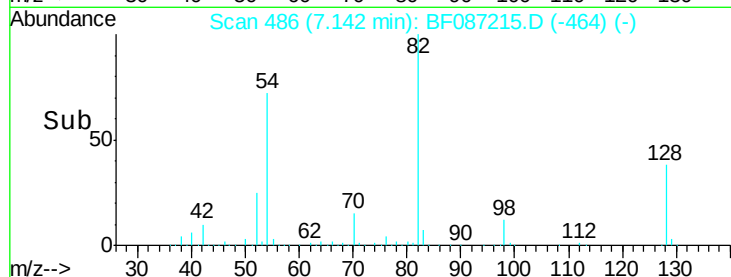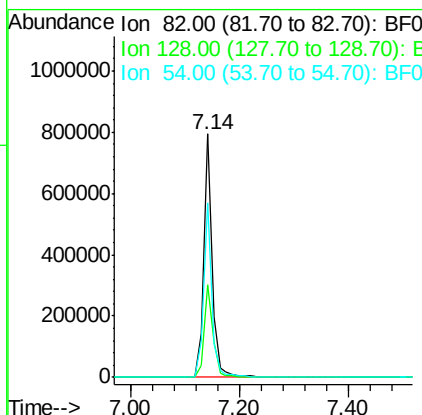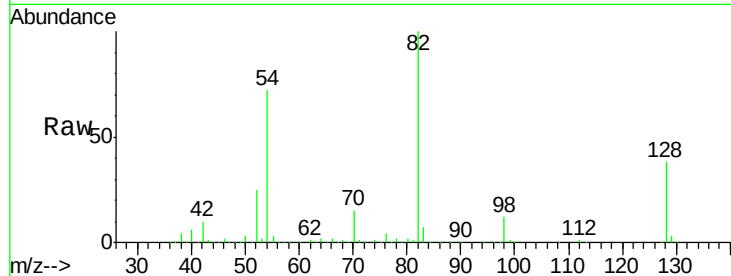

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.60 min Scan# 701
 Delta R.T. -0.05 min
 Lab File: BF087215.D
 Acq: 20 May 2016 6:38

Tgt Ion: 164 Resp: 234762
 Ion Ratio Lower Upper
 164 100
 162 104.1 82.8 124.2
 160 47.0 36.9 55.3


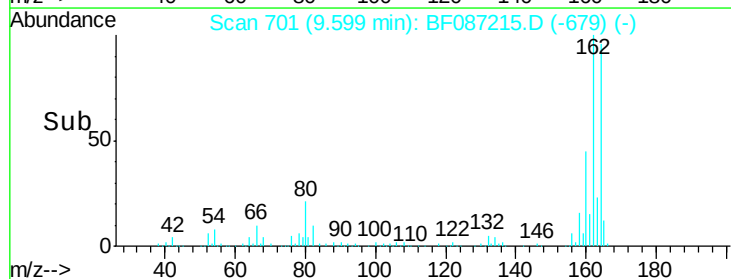
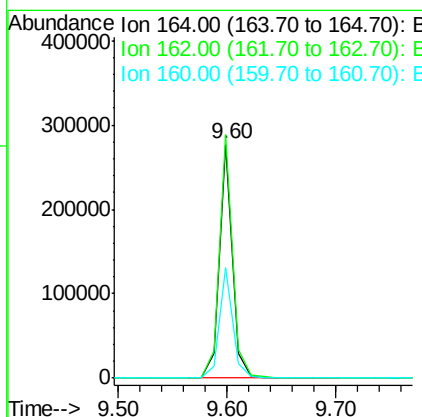
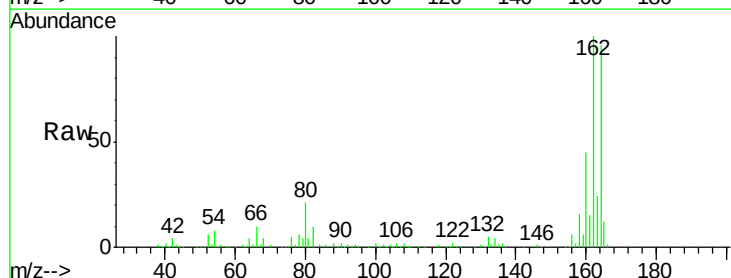


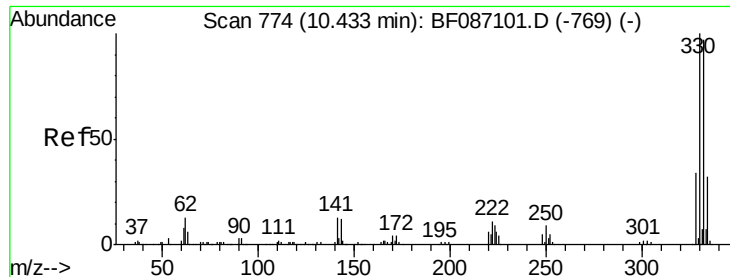

#41
 2,4,6-Tribromophenol
 Concen: 119.98 ng
 RT: 10.40 min Scan# 771
 Delta R.T. -0.05 min
 Lab File: BF087215.D
 Acq: 20 May 2016 6:38




Instrument :
 BNA_F
 ClientSampleId :
 FB-BWR-BB-R10-C5-2(0-19FT)


Tgt Ion:330 Resp: 311261
 Ion Ratio Lower Upper
 330 100
 332 96.5 79.0 118.4
 141 33.8 31.2 46.8

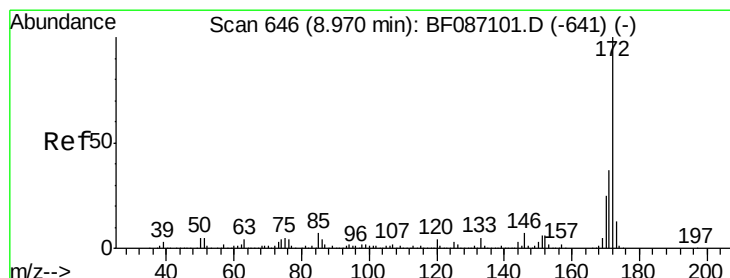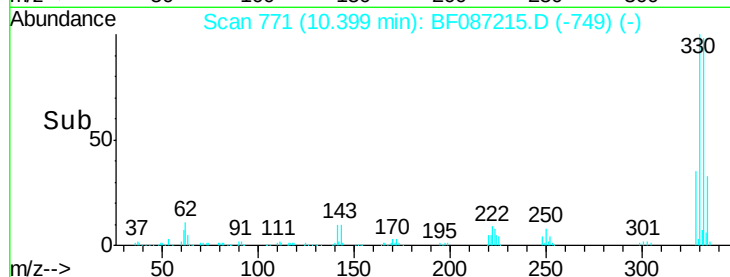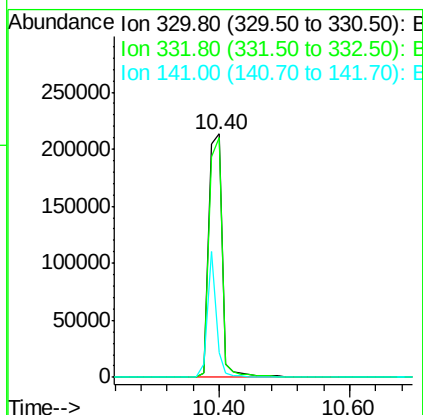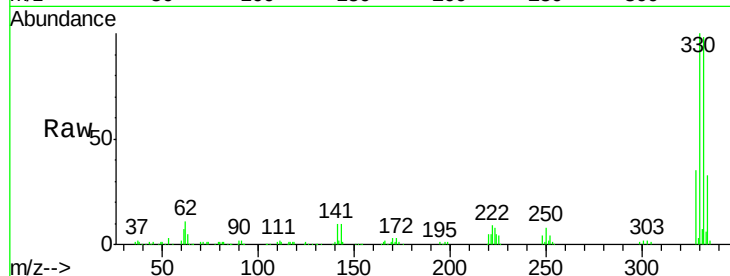

#44
 2-Fluorobiphenyl
 Concen: 104.65 ng
 RT: 8.94 min Scan# 643
 Delta R.T. -0.05 min
 Lab File: BF087215.D
 Acq: 20 May 2016 6:38

Tgt Ion:172 Resp: 1483456
 Ion Ratio Lower Upper
 172 100
 171 36.8 29.0 43.6
 170 24.9 19.8 29.8


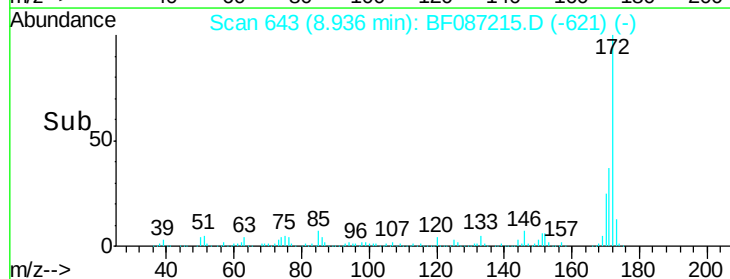
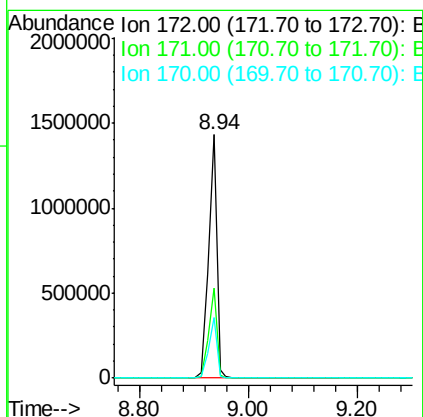
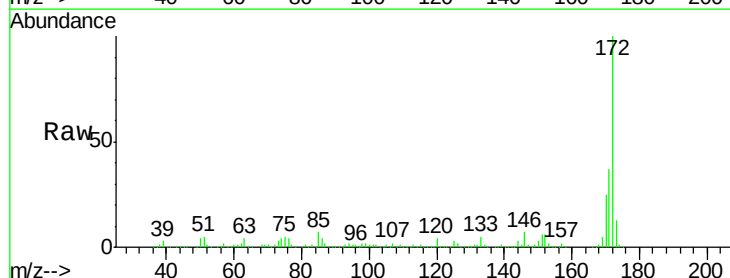


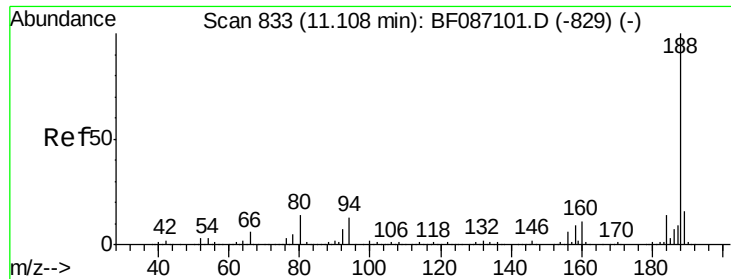

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.07 min Scan# 830
Delta R.T. -0.05 min
Lab File: BF087215.D
Acq: 20 May 2016 6:38




Instrument :
BNA_F
ClientSampleId :
FB-BWR-BB-R10-C5-2(0-19FT)


Tgt Ion:188 Resp: 368069
Ion Ratio Lower Upper
188 100
94 12.4 6.8 10.2#
80 13.9 7.1 10.7#

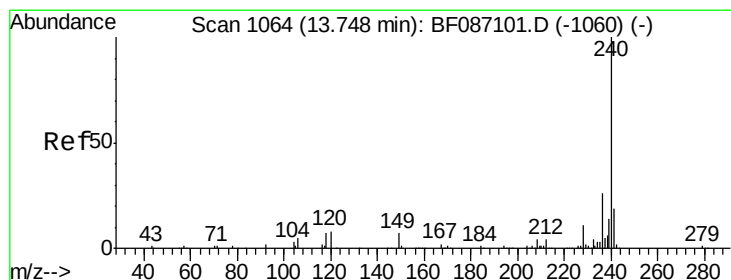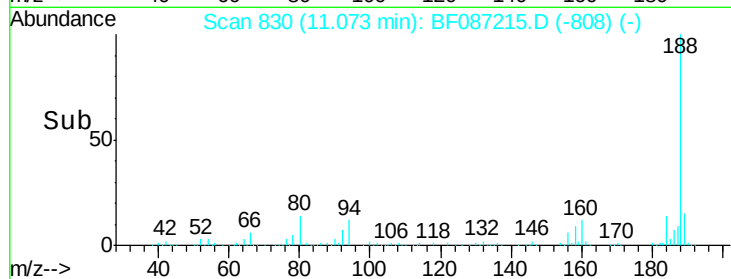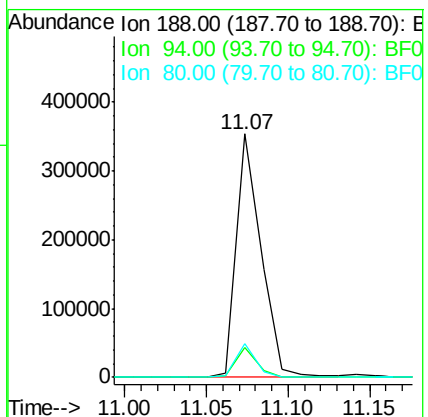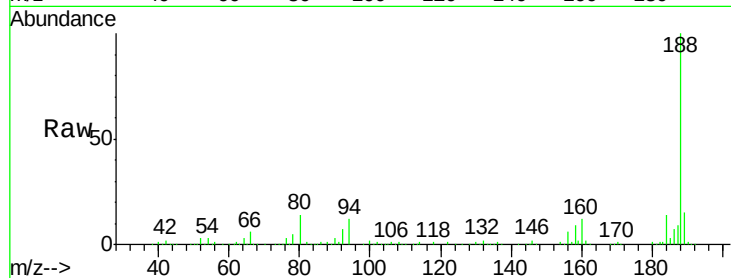

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.70 min Scan# 1060
Delta R.T. -0.06 min
Lab File: BF087215.D
Acq: 20 May 2016 6:38

Tgt Ion:240 Resp: 267456
Ion Ratio Lower Upper
240 100
120 12.0 11.2 16.8
236 26.1 21.2 31.8

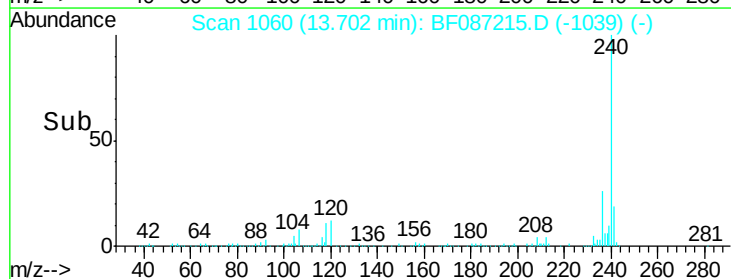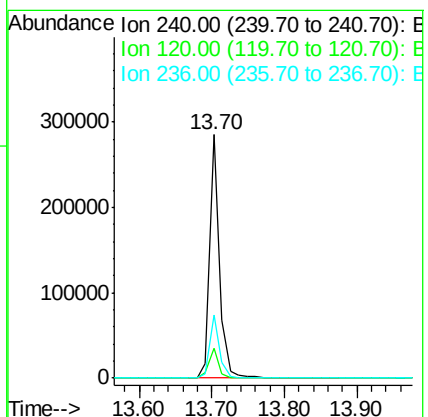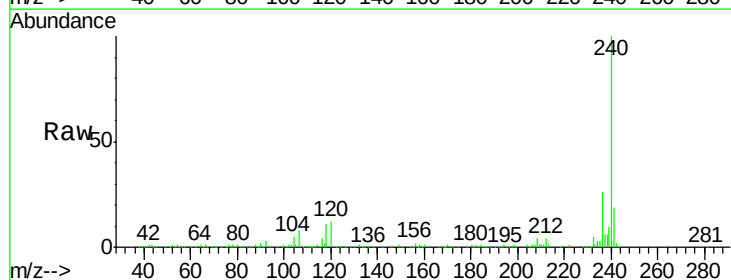

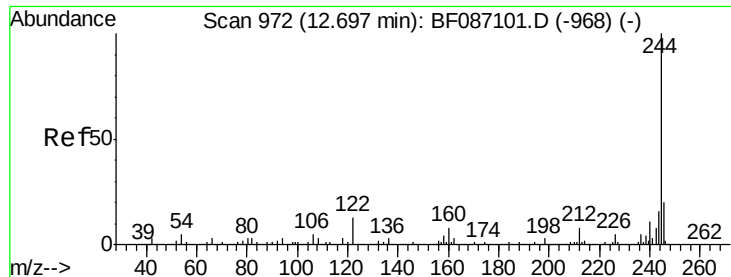

#78

Terphenyl-d14

Concen: 87.52 ng

RT: 12.66 min Scan# 969

Delta R.T. -0.05 min

Lab File: BF087215.D

Acq: 20 May 2016 6:38

Instrument :

BNA_F

ClientSampleId :

FB-BWR-BB-R10-C5-2(0-19FT)


Tgt Ion:244 Resp: 1034740

Ion Ratio Lower Upper

244 100

212 7.9 6.2 9.2




122 12.0 12.0 18.0#

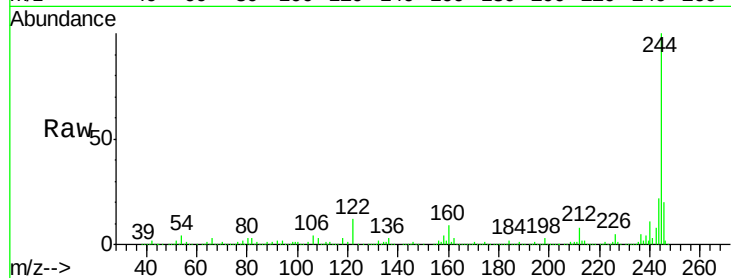

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

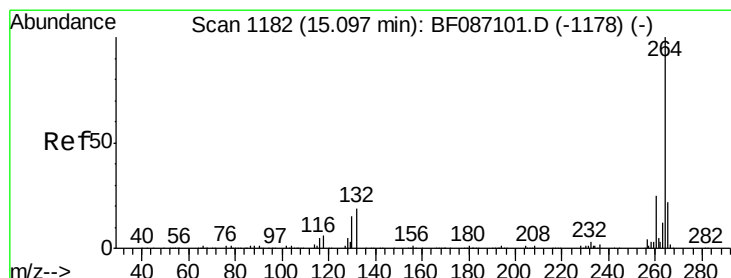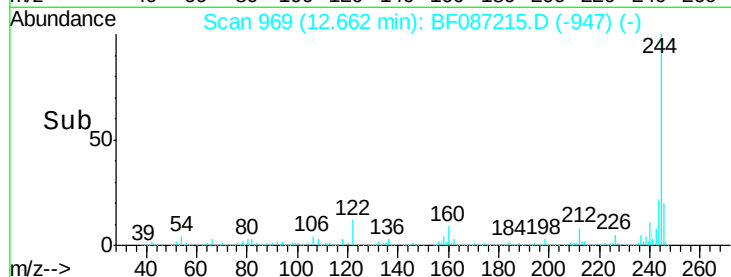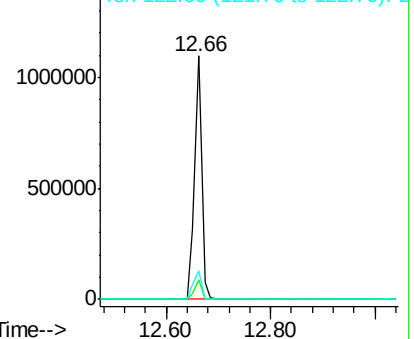

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.06 min Scan# 1179

Delta R.T. -0.05 min

Lab File: BF087215.D

Acq: 20 May 2016 6:38


Tgt Ion:264 Resp: 225847

Ion Ratio Lower Upper

264 100

260 23.8 19.5 29.3

265 21.2 17.3 25.9

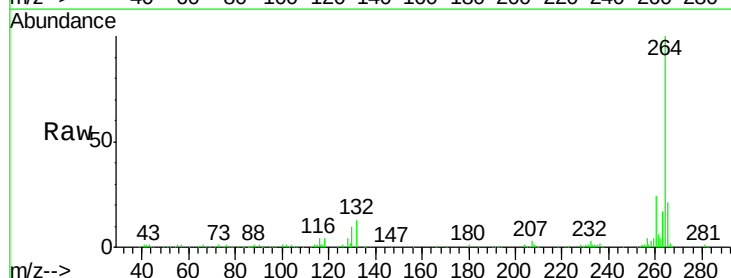

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

