


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051916\
 Data File : BF087184.D
 Acq On : 19 May 2016 12:36
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 17 16:55:01 2016

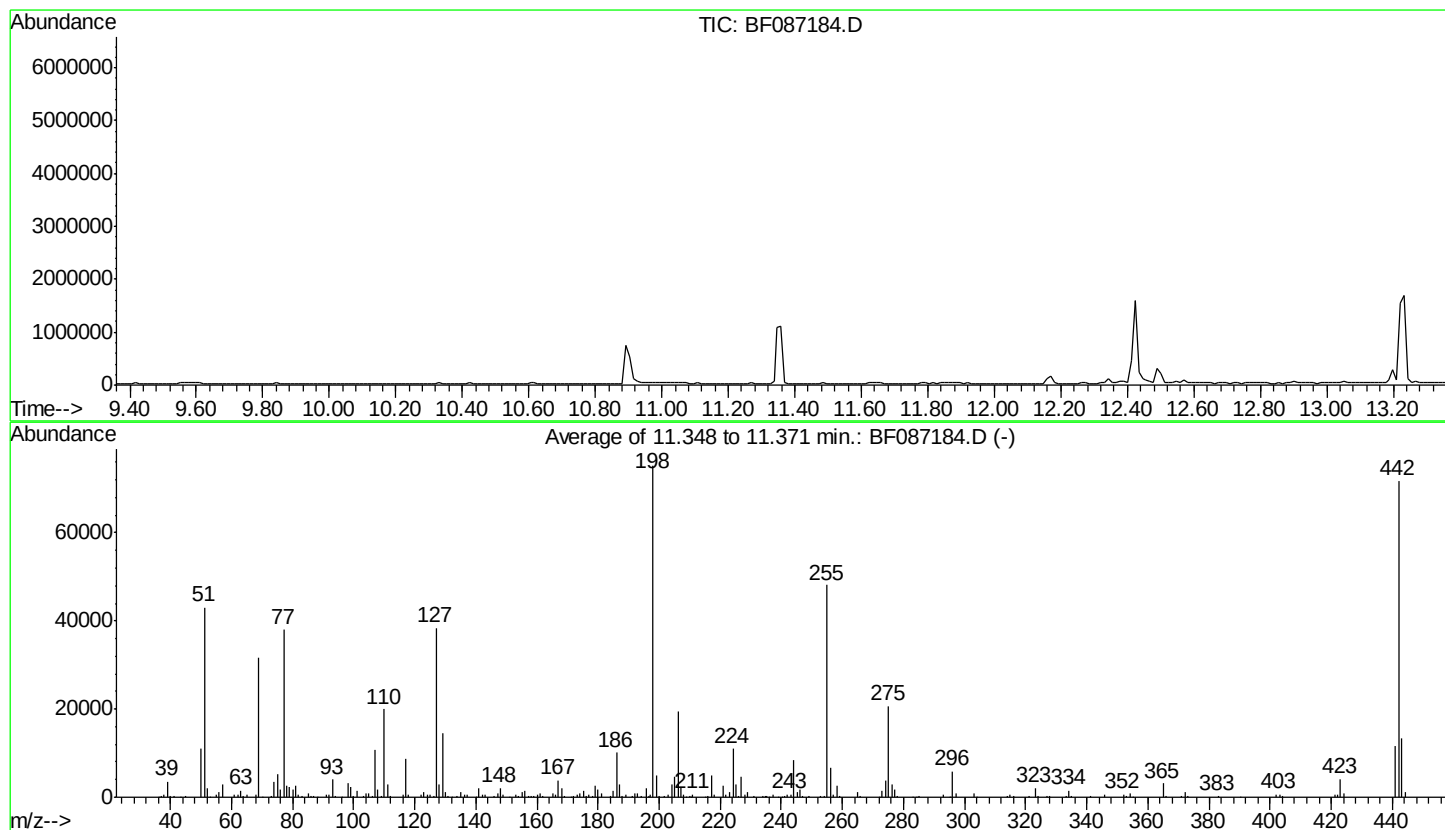

AutoFind: Scans 854, 855, 856; Background Corrected with Scan 850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.2	43011	PASS
68	69	0.00	2	1.9	614	PASS
69	198	0.00	100	42.1	31716	PASS
70	69	0.00	2	0.5	145	PASS
127	198	10	80	51.0	38360	PASS
197	198	0.00	2	0.8	579	PASS
198	198	100	100	100.0	75253	PASS
199	198	5	9	6.6	4988	PASS
275	198	10	60	27.6	20742	PASS
365	198	1	100	4.1	3109	PASS
441	442	0.01	24	16.1	11541	PASS
442	198	50	100	95.4	71768	PASS
443	442	15	24	18.6	13334	PASS