


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051916\
 Data File : BF087205.D
 Acq On : 20 May 2016 1:48
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 17 16:55:01 2016

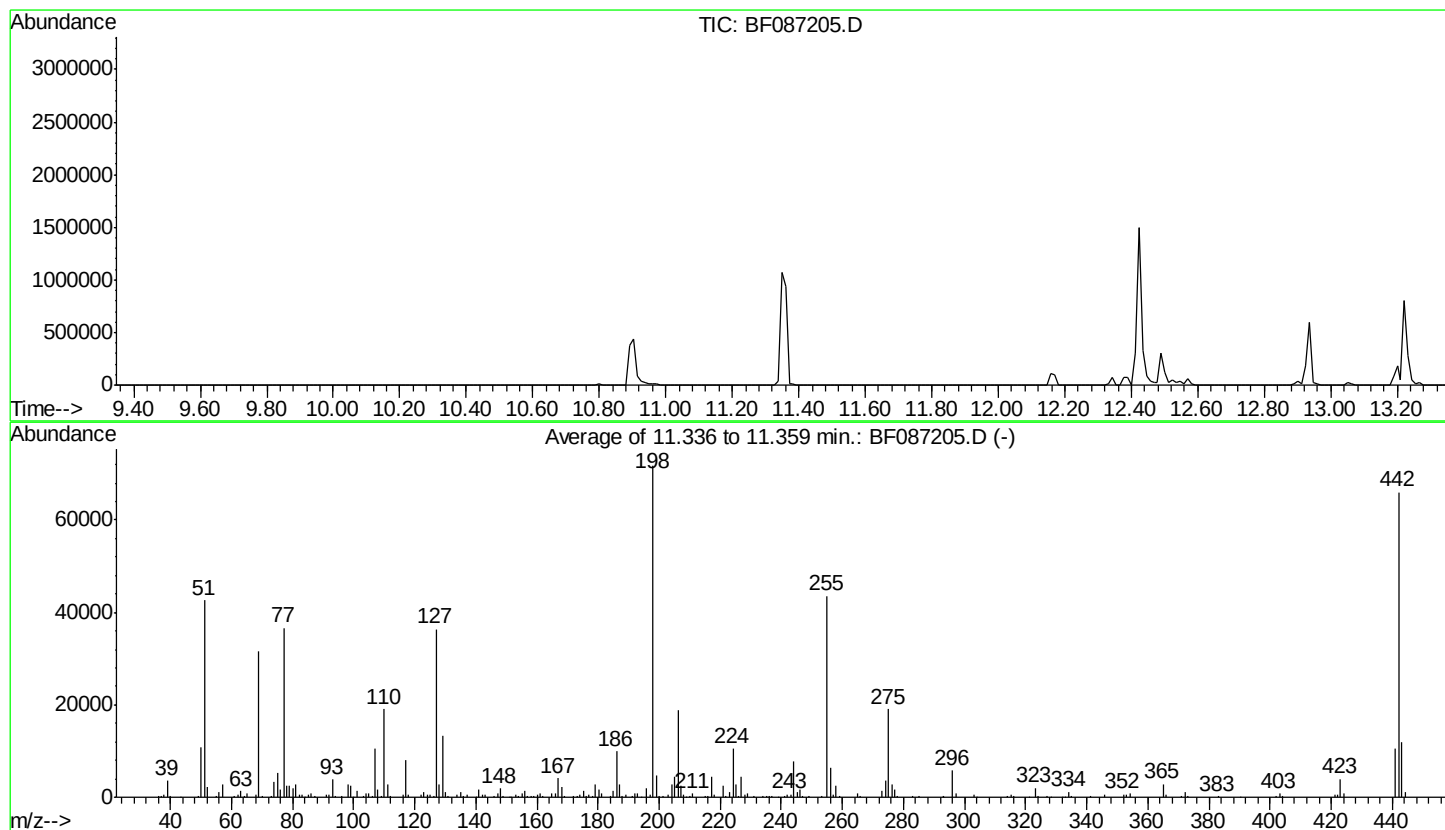

AutoFind: Scans 853, 854, 855; Background Corrected with Scan 850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.3	42587	PASS
68	69	0.00	2	2.0	644	PASS
69	198	0.00	100	44.0	31549	PASS
70	69	0.00	2	0.5	151	PASS
127	198	10	80	50.6	36294	PASS
197	198	0.00	2	0.8	554	PASS
198	198	100	100	100.0	71761	PASS
199	198	5	9	6.5	4643	PASS
275	198	10	60	26.5	18989	PASS
365	198	1	100	4.0	2857	PASS
441	442	0.01	24	15.8	10460	PASS
442	198	50	100	92.0	66029	PASS
443	442	15	24	18.2	12035	PASS